

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
 Data File : PL076361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 12:39
 Operator : AR\AJ
 Sample : PB146127BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 23:55:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.646	4.626	12819103	30852275	17.794	15.259
28)	SA Decachlor...	11.638	10.367	13319755	27773788	22.577	16.552 #
Target Compounds							
2)	A alpha-BHC	6.200f	0.000	79722	0	0.085	N.D. #
9)	A Endosulfan I	8.508f	0.000	338138	0	0.501	N.D. #
10)	B gamma-Chl...	0.000	7.334	0	576243	N.D.	0.289 #
15)	B Endosulfa...	9.296	0.000	1025593	0	1.717	N.D. #
17)	MA 4,4'-DDT	9.517	0.000	509958	0	0.858	N.D. #
19)	B Endosulfa...	0.000	8.730f	0	494993	N.D.	0.311 #
20)	A Methoxychlor	0.000	9.063f	0	51117	N.D.	0.060 #
21)	B Endrin ke...	10.181	0.000	3457511	0	5.114	N.D. #
25)	Chlordane-3	0.000	7.334	0	576243	N.D.	3.403 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
Data File : PL076361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 12:39
Operator : AR\AJ
Sample : PB146127BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 23:55:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

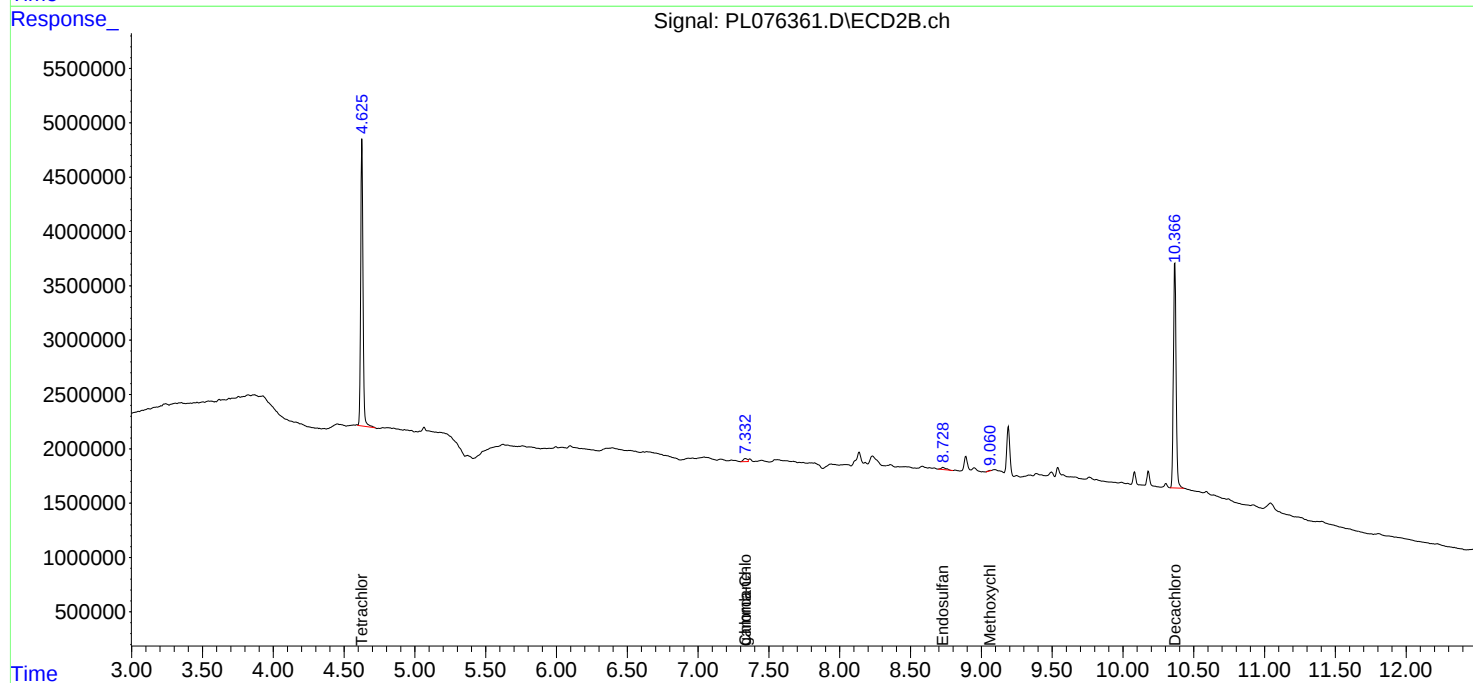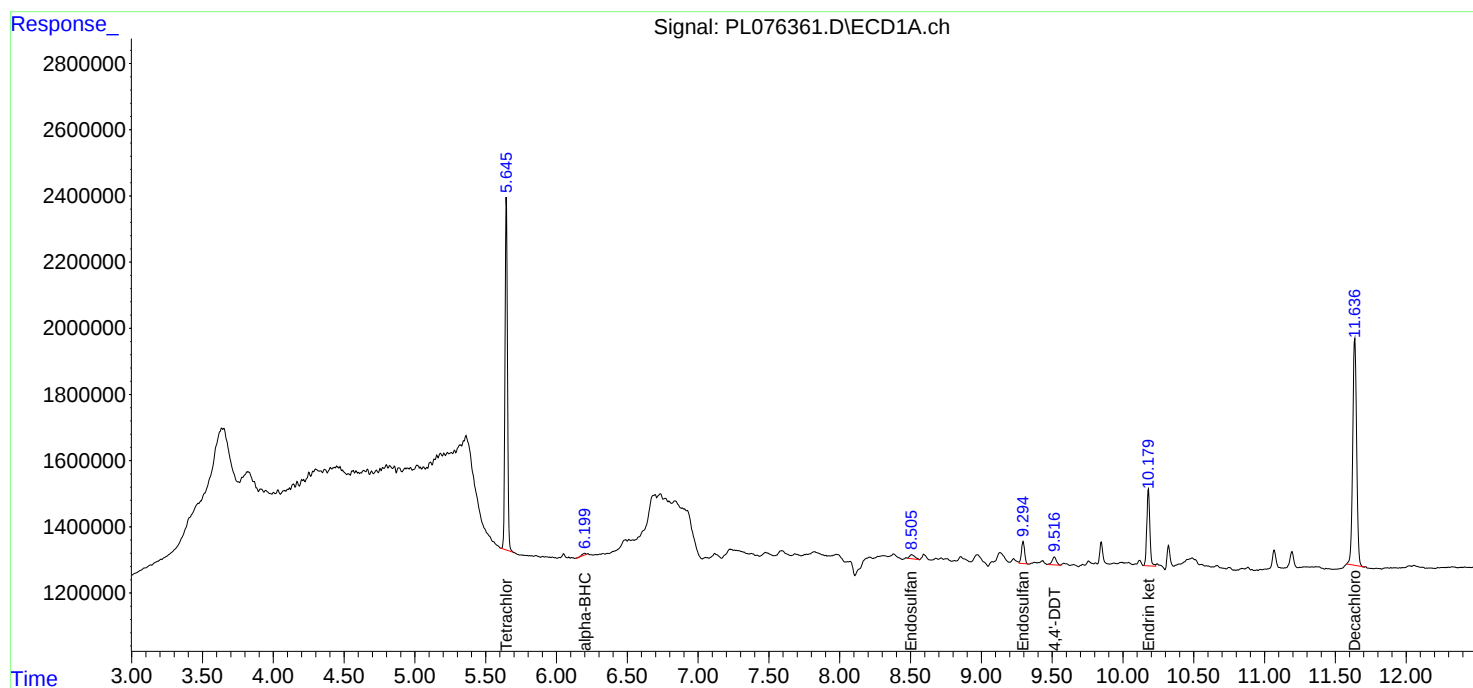


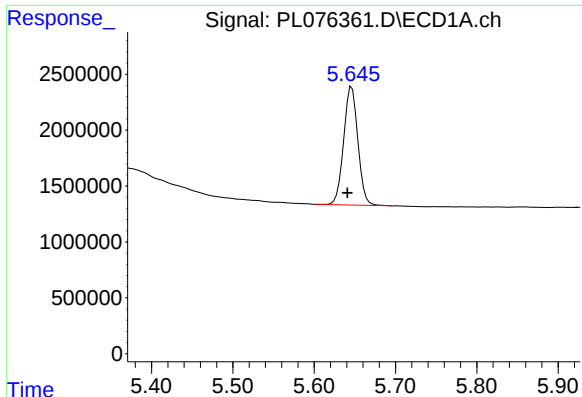

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: 0.005 min
Response: 12819103
Conc: 17.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

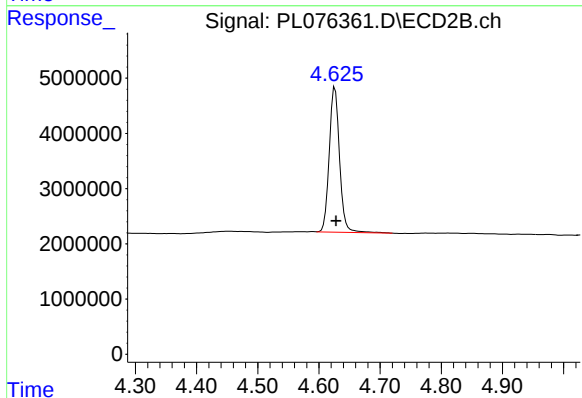


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: -0.002 min
Response: 30852275
Conc: 15.26 ng/ml

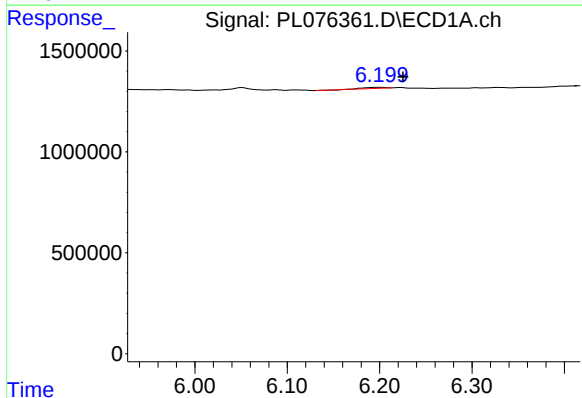


#2 alpha-BHC

R.T.: 6.200 min
Delta R.T.: -0.025 min
Response: 79722
Conc: 0.09 ng/ml

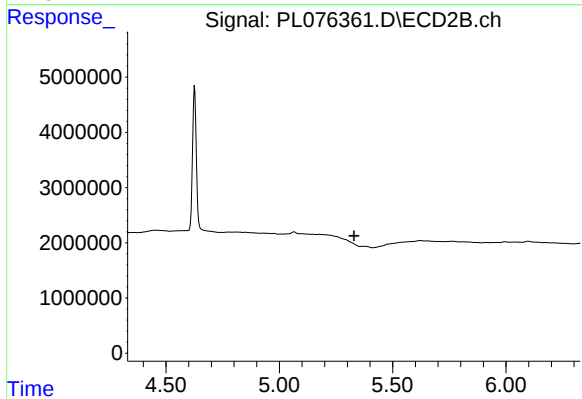

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 5.329 min
Response: 0
Conc: N.D.

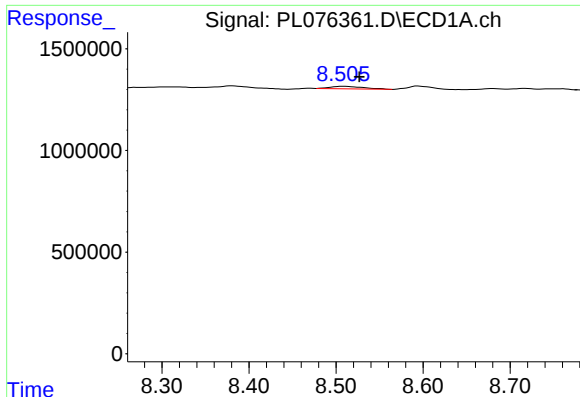

#9 Endosulfan I


R.T.: 8.508 min
Delta R.T.: -0.019 min
Response: 338138
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

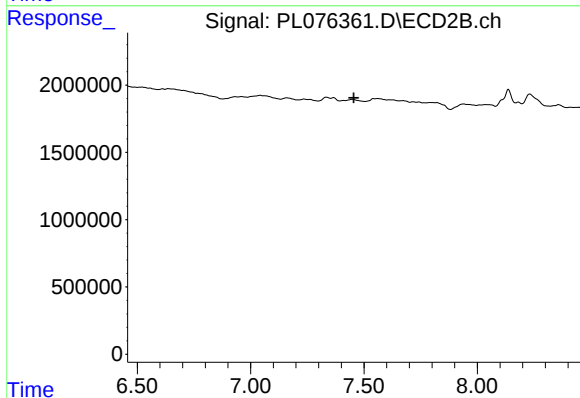


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.455 min
Response: 0
Conc: N.D.

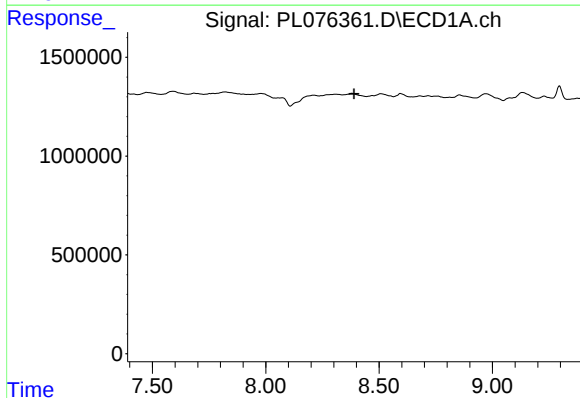


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.389 min
Response: 0
Conc: N.D.

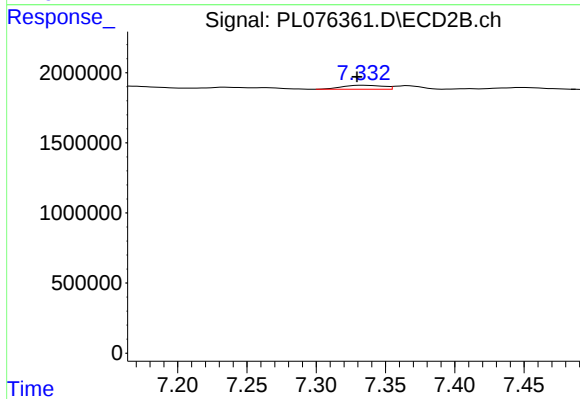

#10 gamma-Chlordane


R.T.: 7.334 min
Delta R.T.: 0.004 min
Response: 576243
Conc: 0.29 ng/ml

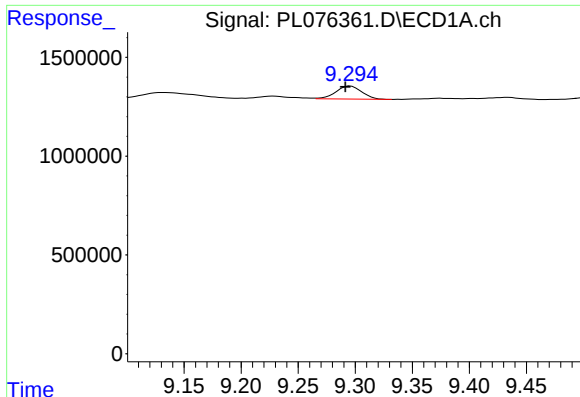

#15 Endosulfan II


R.T.: 9.296 min
Delta R.T.: 0.004 min
Response: 1025593
Conc: 1.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

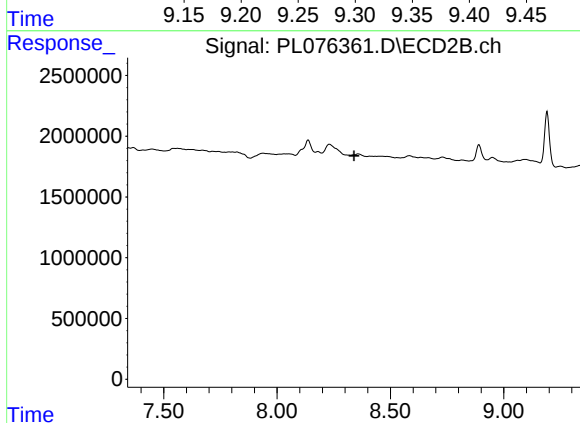


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.340 min
Response: 0
Conc: N.D.

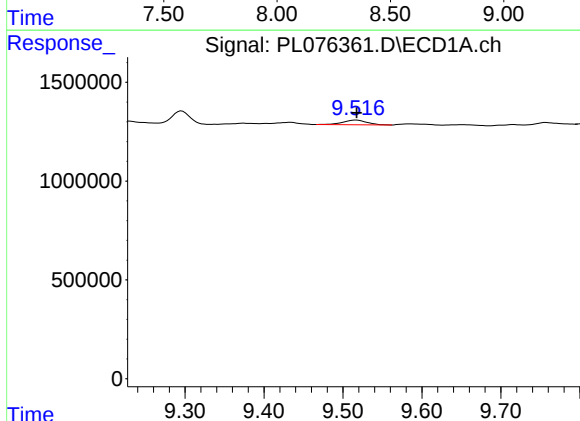


#17 4,4'-DDT

R.T.: 9.517 min
Delta R.T.: 0.000 min
Response: 509958
Conc: 0.86 ng/ml

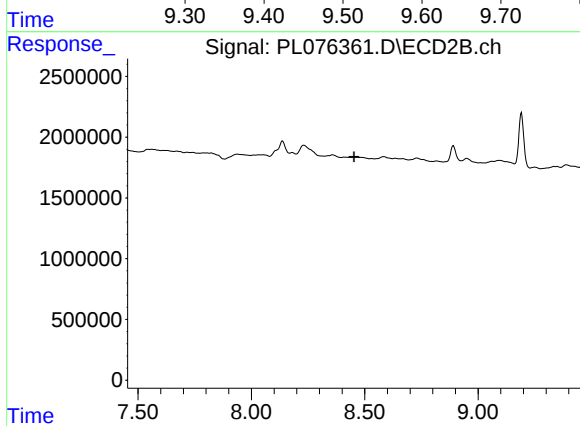

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 8.454 min
Response: 0
Conc: N.D.

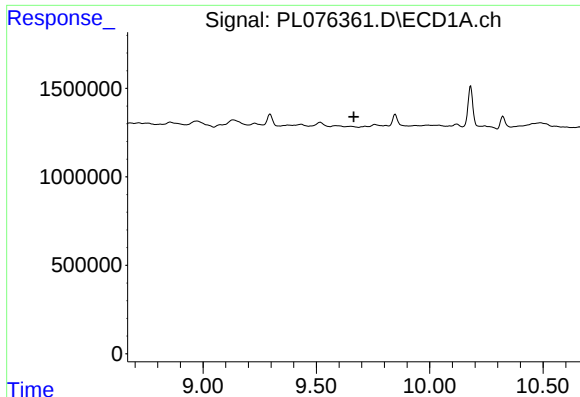

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 9.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

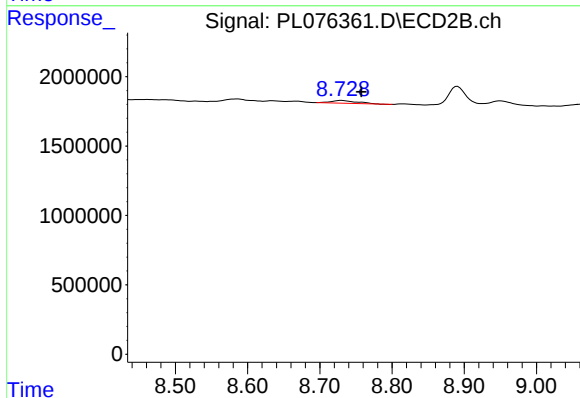


#19 Endosulfan Sulfate

R.T.: 8.730 min
Delta R.T.: -0.028 min
Response: 494993
Conc: 0.31 ng/ml

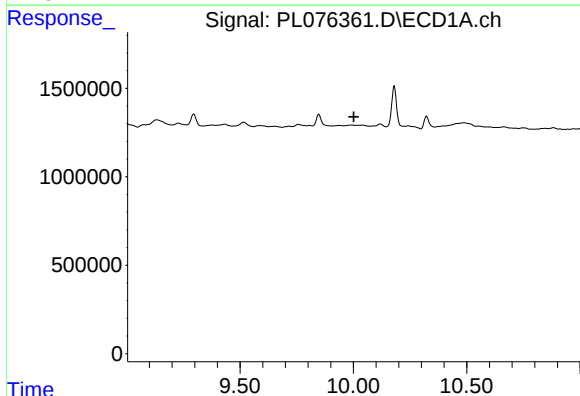


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 10.002 min
Response: 0
Conc: N.D.

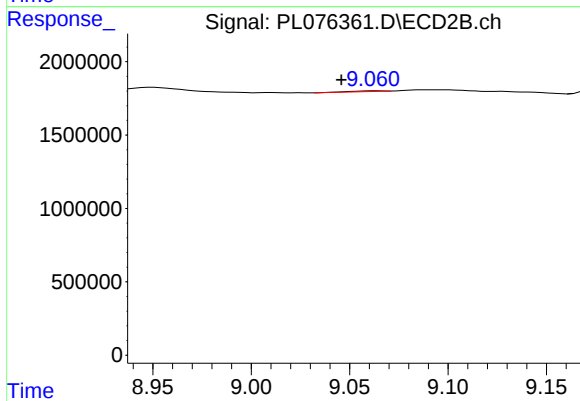

#20 Methoxychlor


R.T.: 9.063 min
Delta R.T.: 0.017 min
Response: 51117
Conc: 0.06 ng/ml

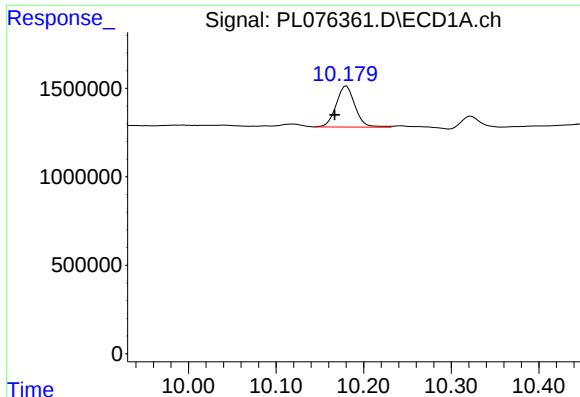

#21 Endrin ketone


R.T.: 10.181 min
Delta R.T.: 0.014 min
Response: 3457511
Conc: 5.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

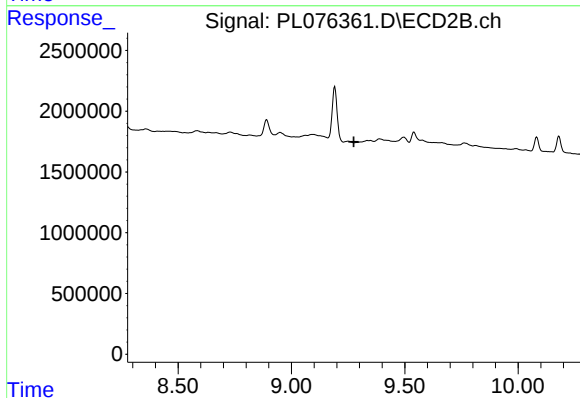


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.275 min
Response: 0
Conc: N.D.

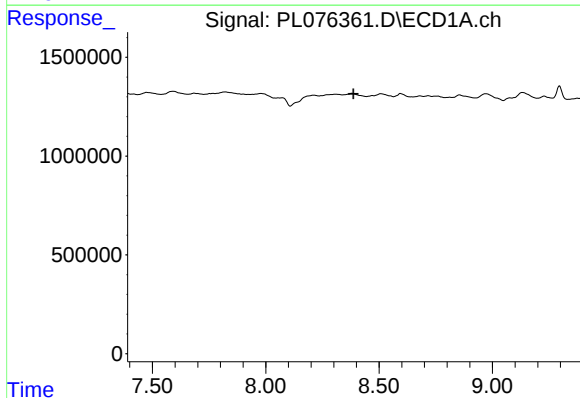


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.388 min
Response: 0
Conc: N.D.

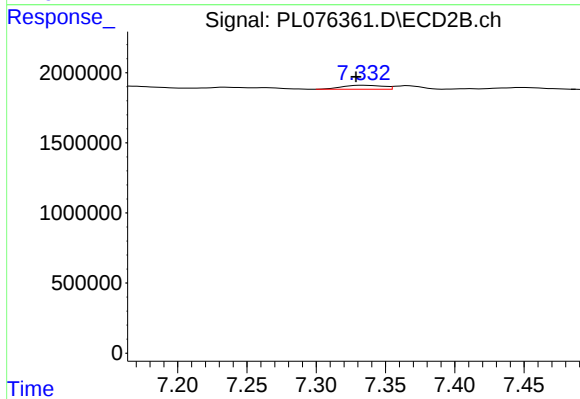

#25 Chlordane-3


R.T.: 7.334 min
Delta R.T.: 0.005 min
Response: 576243
Conc: 3.40 ng/ml

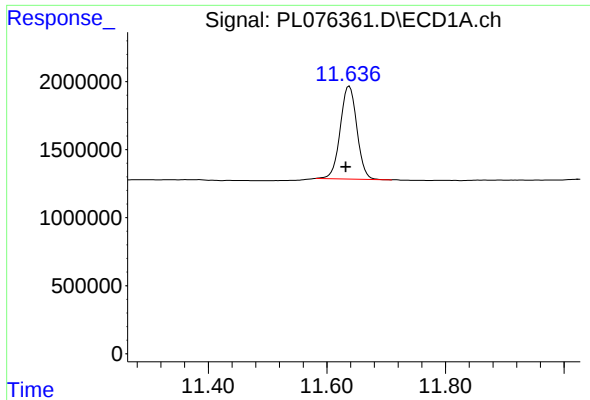

#28 Decachlorobiphenyl

R.T.: 11.638 min
Delta R.T.: 0.006 min
Response: 13319755
Conc: 22.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

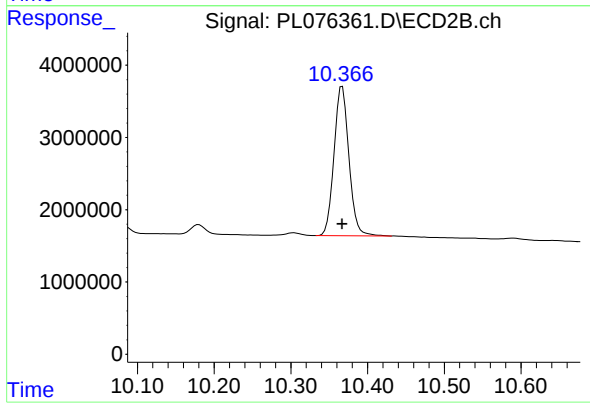

#28 Decachlorobiphenyl

R.T.: 10.367 min
Delta R.T.: 0.000 min
Response: 27773788
Conc: 16.55 ng/ml