

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
 Data File : PL076363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 14:27
 Operator : AR\AJ
 Sample : N3645-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-08-070822

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/12/2022
 Supervised By : Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:47:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.638	4.625	7082385	20475396	9.831m	10.127m
28) SA Decachlor...	11.628	10.361	6663557	14589487	11.295	8.695

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
Data File : PL076363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 14:27
Operator : AR\AJ
Sample : N3645-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-08-070822


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/12/2022
Supervised By : Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:47:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

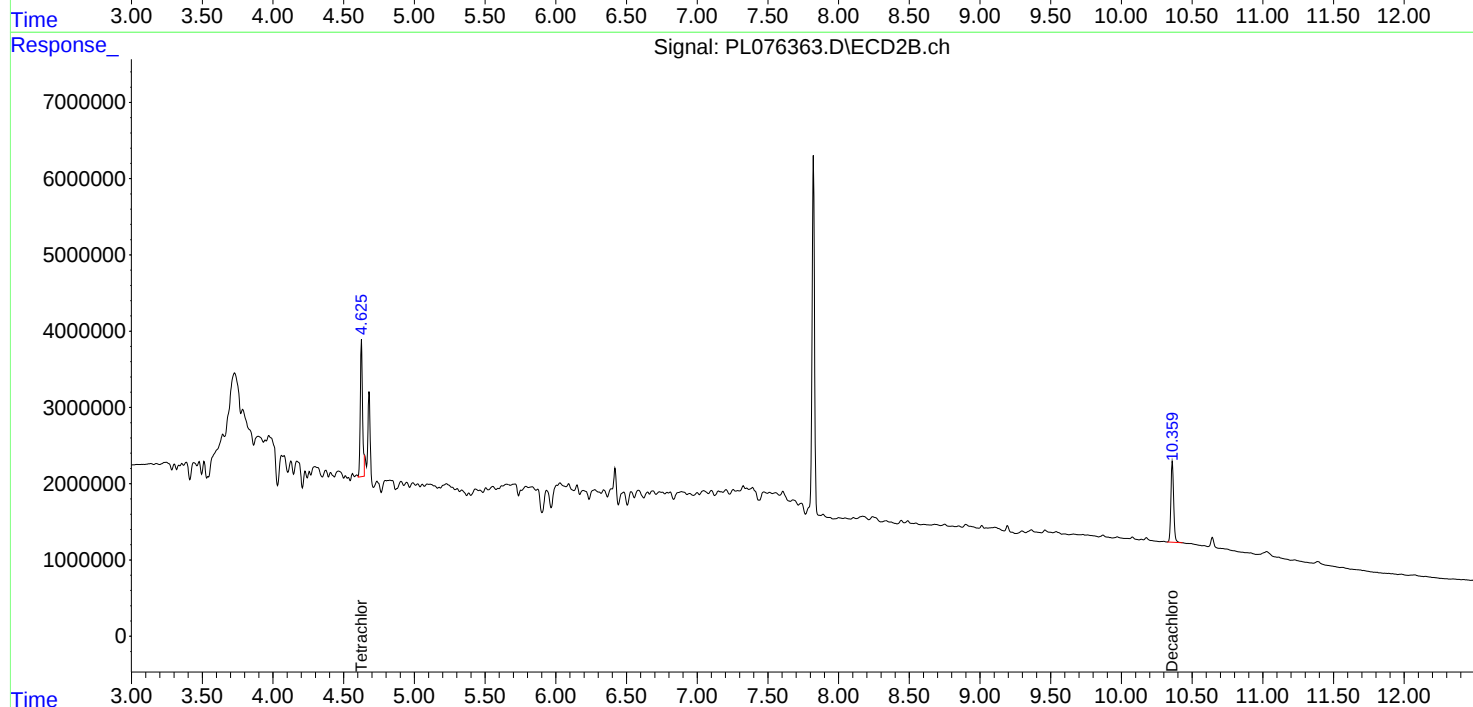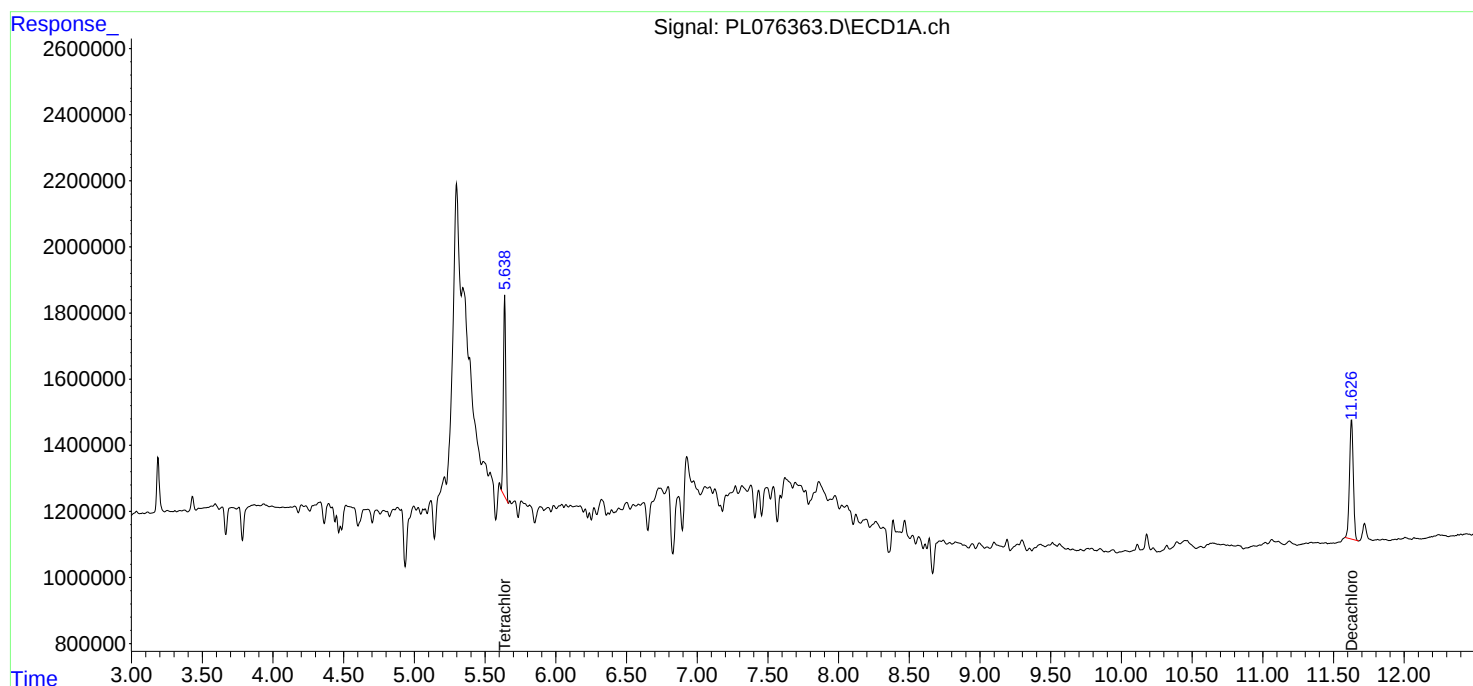

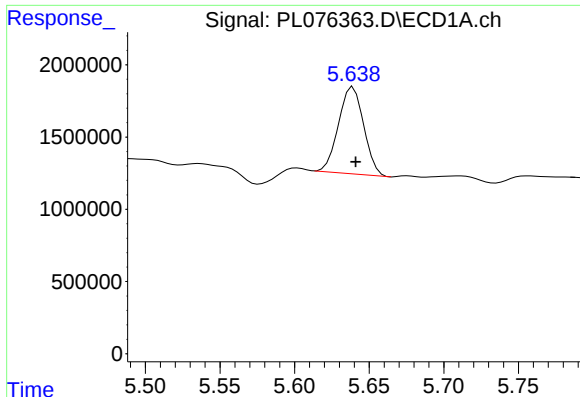


#1 Tetrachloro-m-xylene

R.T.: 5.638 min
Delta R.T.: -0.003 min
Response: 7082385
Conc: 9.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-08-070822


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

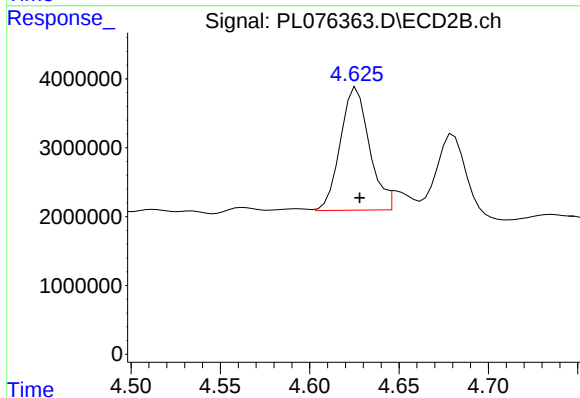


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: -0.003 min
Response: 20475396
Conc: 10.13 ng/ml m

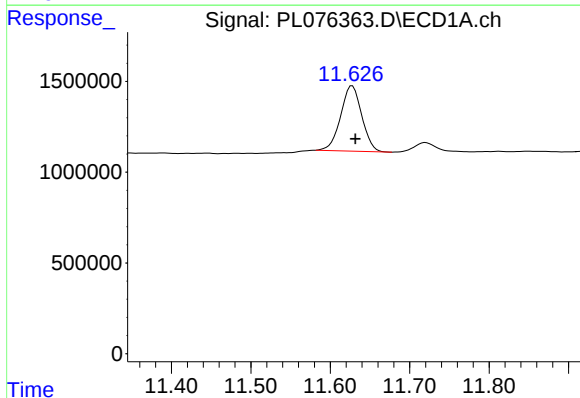

#28 Decachlorobiphenyl

R.T.: 11.628 min
Delta R.T.: -0.004 min
Response: 6663557
Conc: 11.29 ng/ml

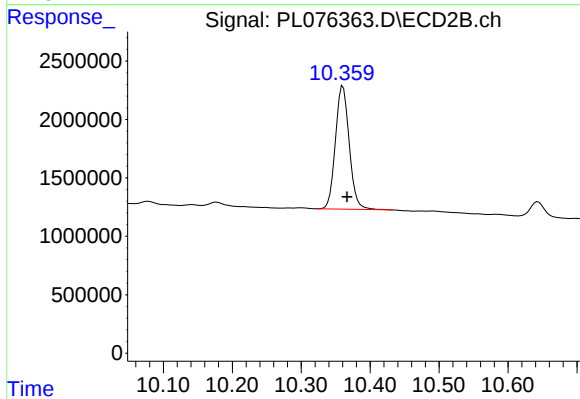

#28 Decachlorobiphenyl

R.T.: 10.361 min
Delta R.T.: -0.006 min
Response: 14589487
Conc: 8.69 ng/ml