

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
 Data File : PL076369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2022 16:07
 Operator : AR\AJ
 Sample : N3644-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-070822

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/12/2022
 Supervised By : Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 00:00:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.640	4.633	690353	983201	0.958m	0.486m#
28) SA Decachlor...	11.634	10.365	829987	1100525	1.407	0.656 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071122\
Data File : PL076369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2022 16:07
Operator : AR\AJ
Sample : N3644-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-03-070822


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/12/2022
Supervised By : Ankita Jodhani 07/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 00:00:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

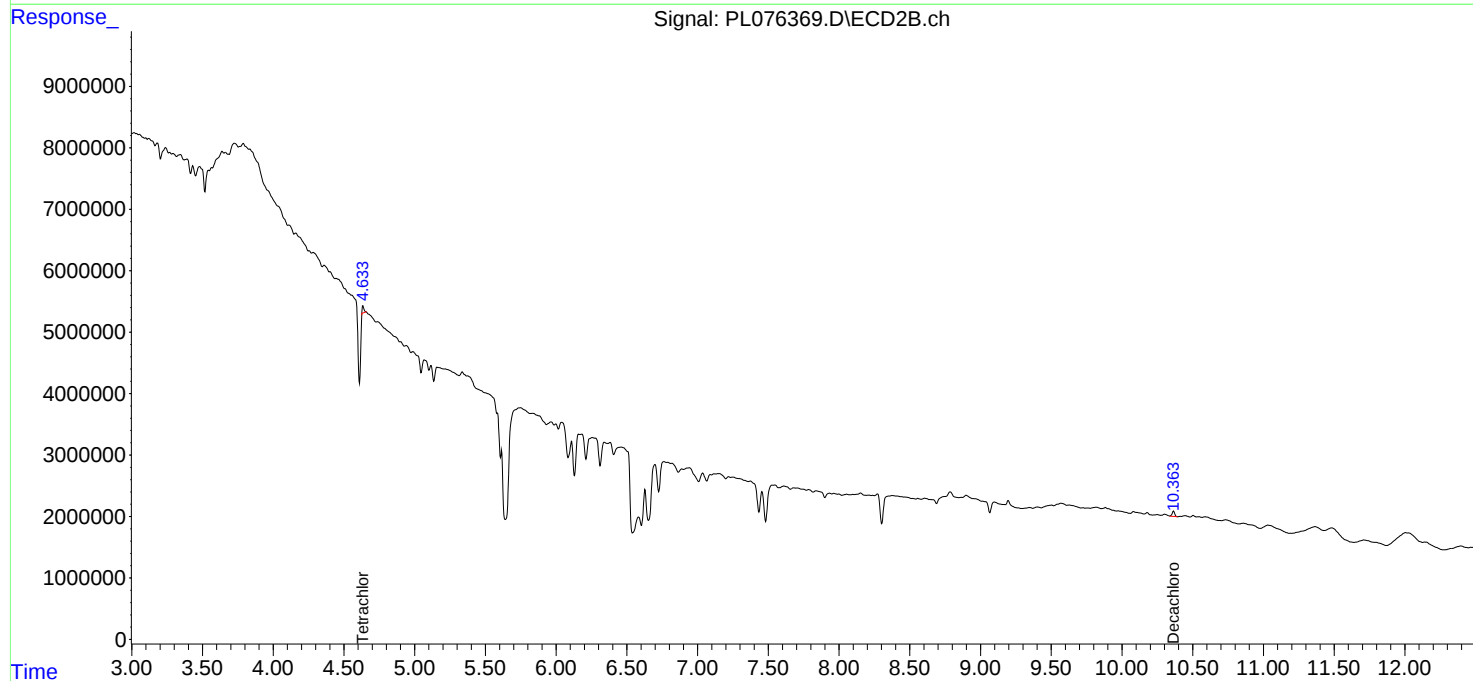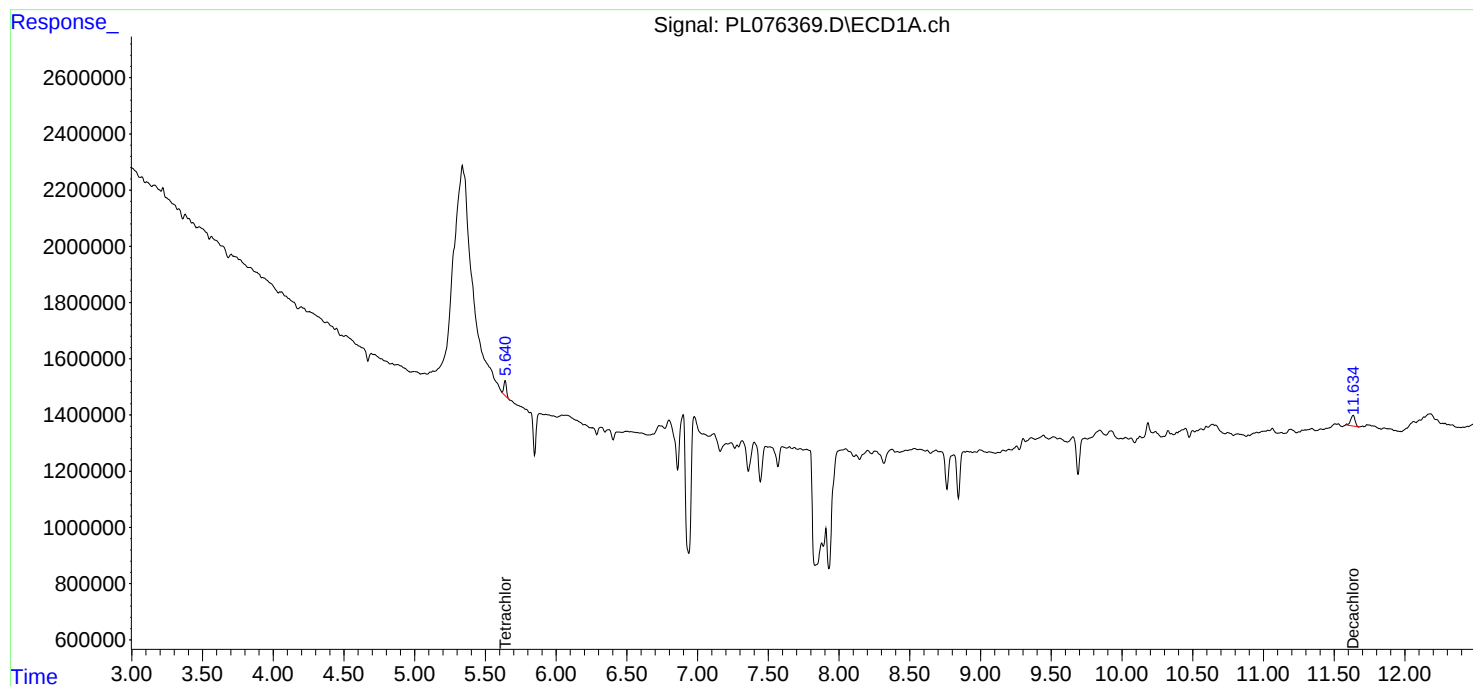

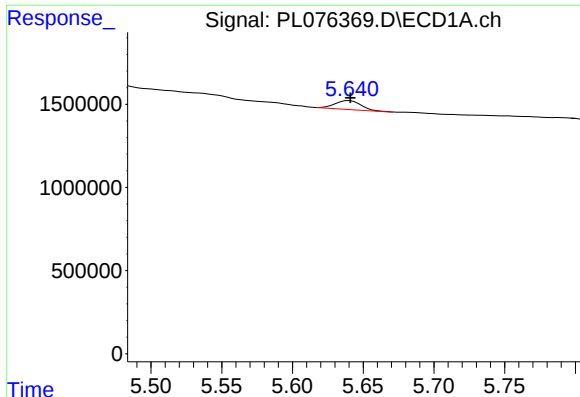


#1 Tetrachloro-m-xylene

R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 690353
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-070822


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/12/2022
Supervised By :Ankita Jodhani 07/12/2022

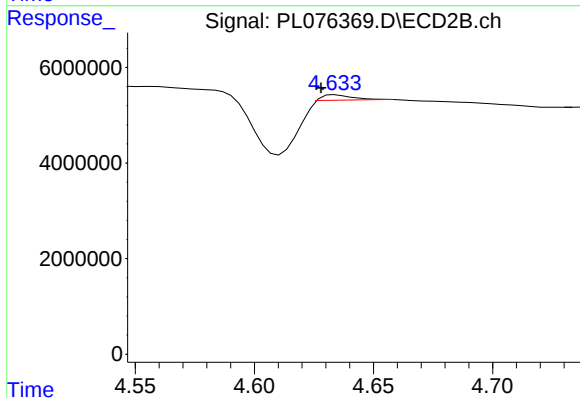


#1 Tetrachloro-m-xylene

R.T.: 4.633 min
Delta R.T.: 0.005 min
Response: 983201
Conc: 0.49 ng/ml m

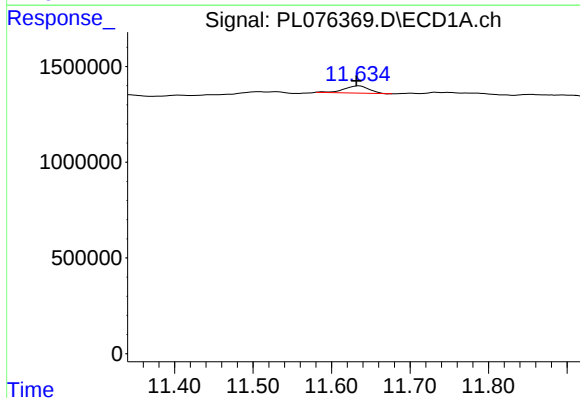

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.002 min
Response: 829987
Conc: 1.41 ng/ml

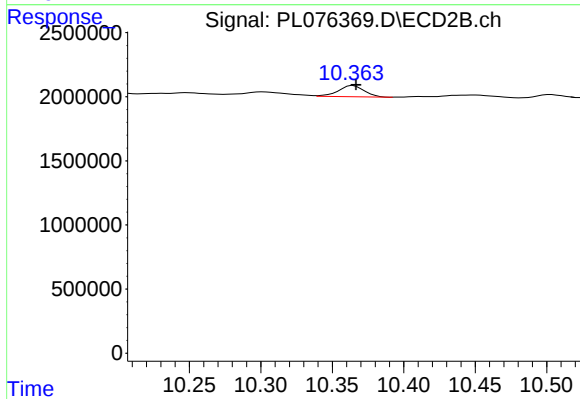

#28 Decachlorobiphenyl

R.T.: 10.365 min
Delta R.T.: -0.002 min
Response: 1100525
Conc: 0.66 ng/ml