

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071124\
 Data File : PL090484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2024 11:52
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/12/2024
 Supervised By :Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 01:00:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 25 11:05:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.789	41955922	32115008	18.486m	20.303m
28) SA Decachlor...	9.061	7.934	39696268	28136613	25.740m	18.862m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071124\
Data File : PL090484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2024 11:52
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/12/2024
Supervised By :Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 01:00:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
Quant Title : GC Extractables
QLast Update : Tue Jun 25 11:05:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

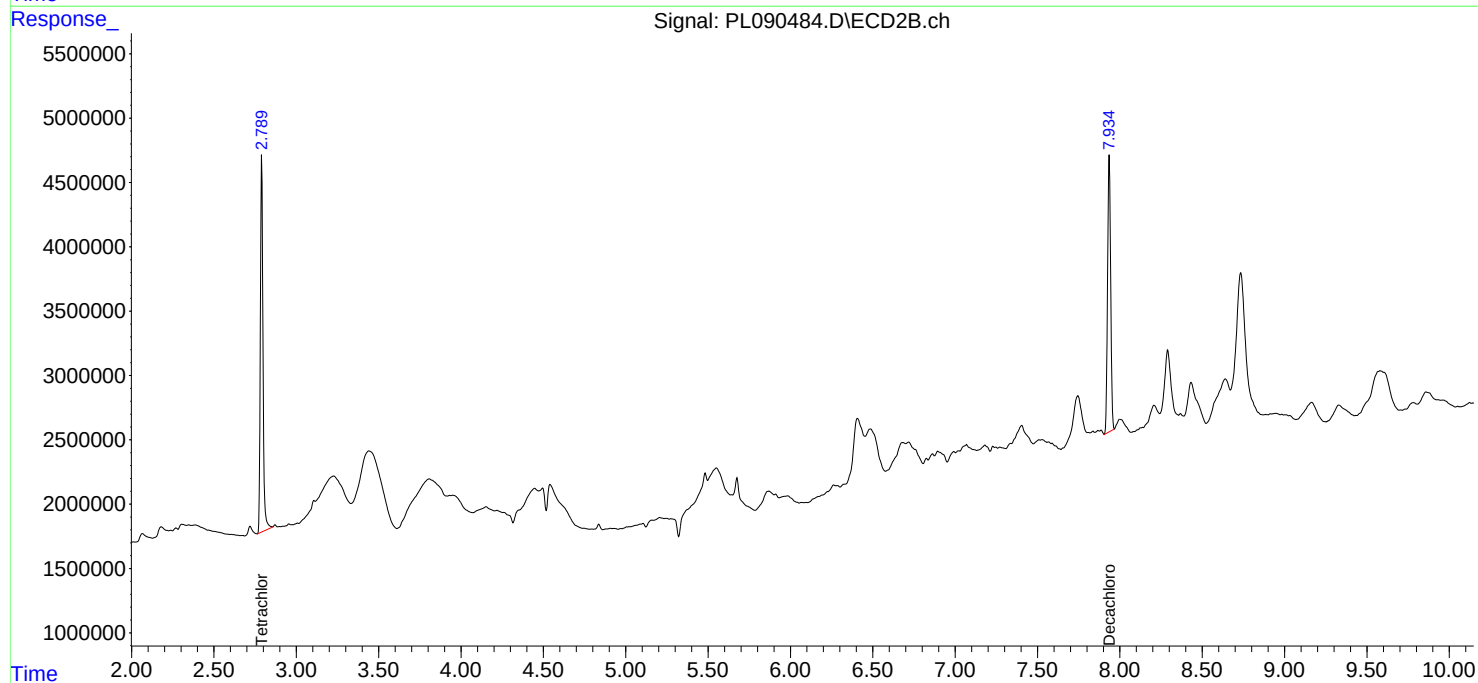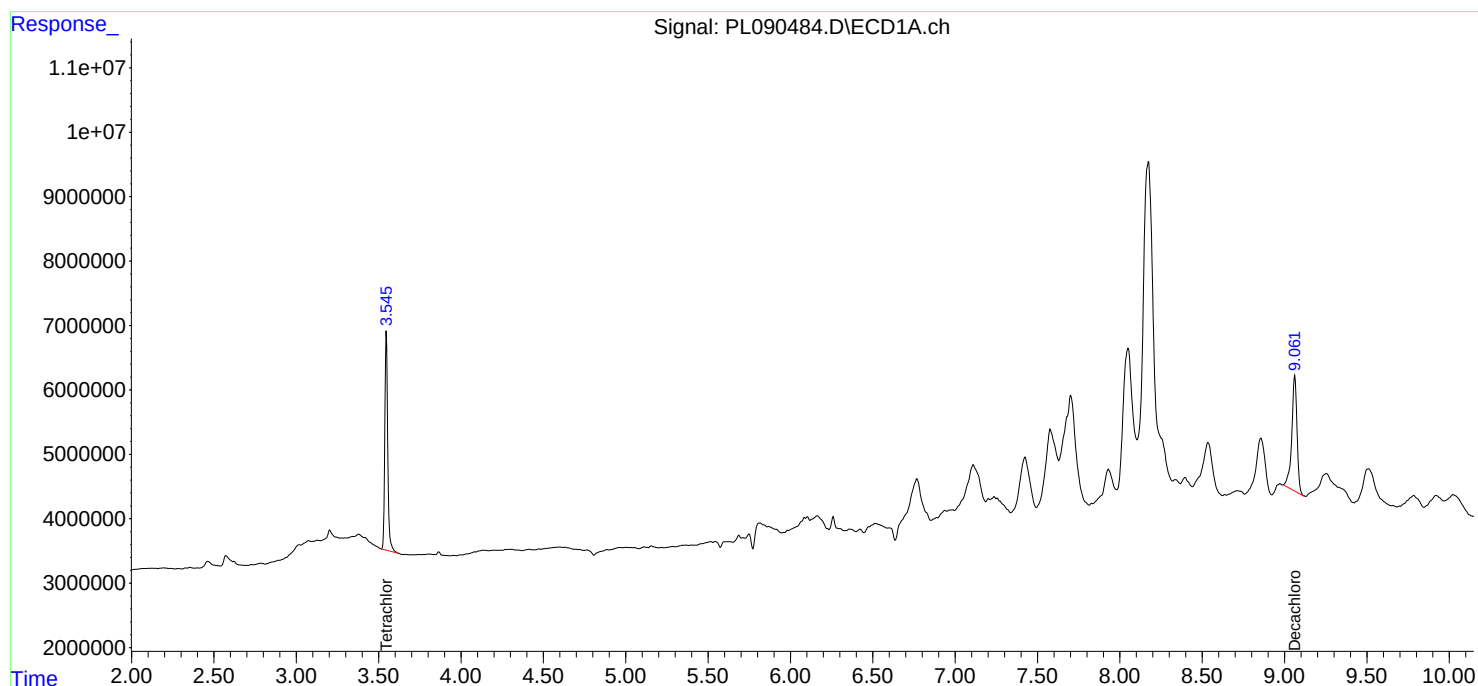

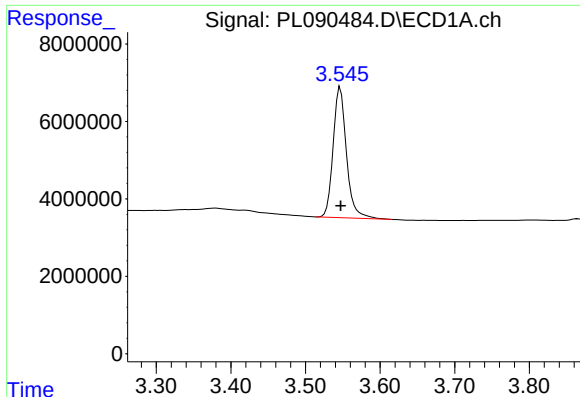


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.002 min
Response: 41955922
Conc: 18.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/12/2024
Supervised By :Ankita Jodhani 07/12/2024

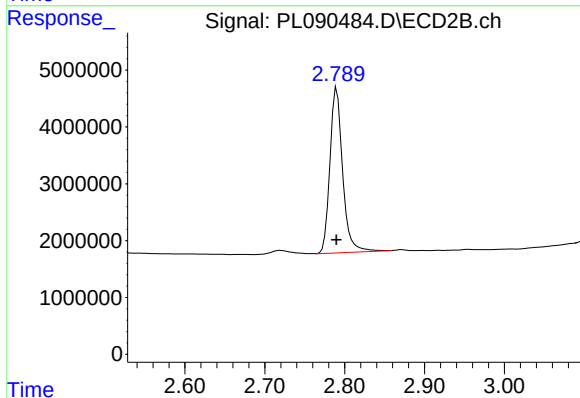


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 32115008
Conc: 20.30 ng/ml m

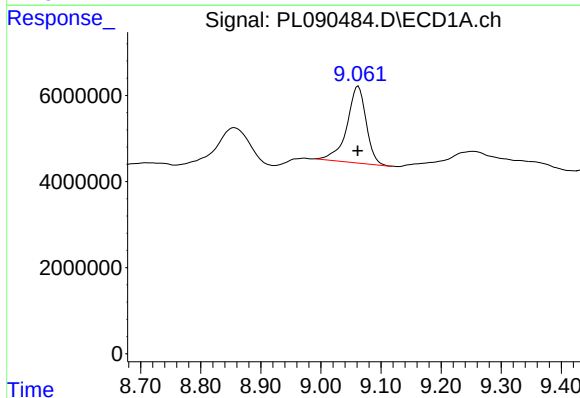

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 39696268
Conc: 25.74 ng/ml m

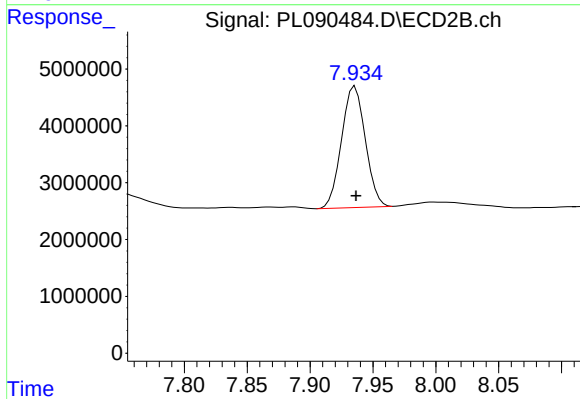

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: -0.002 min
Response: 28136613
Conc: 18.86 ng/ml m