

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071124\
 Data File : PL090495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2024 18:08
 Operator : AR\AJ
 Sample : P3193-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FILL-MATERIAL-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/12/2024
 Supervised By :Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 01:32:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 25 11:05:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.783	40576351	31650188	17.878m	20.010m
28) SA Decachlor...	9.051	7.927	26894687	26855276	17.439m	18.003m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071124\
Data File : PL090495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2024 18:08
Operator : AR\AJ
Sample : P3193-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FILL-MATERIAL-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/12/2024
Supervised By : Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 01:32:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
Quant Title : GC Extractables
QLast Update : Tue Jun 25 11:05:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

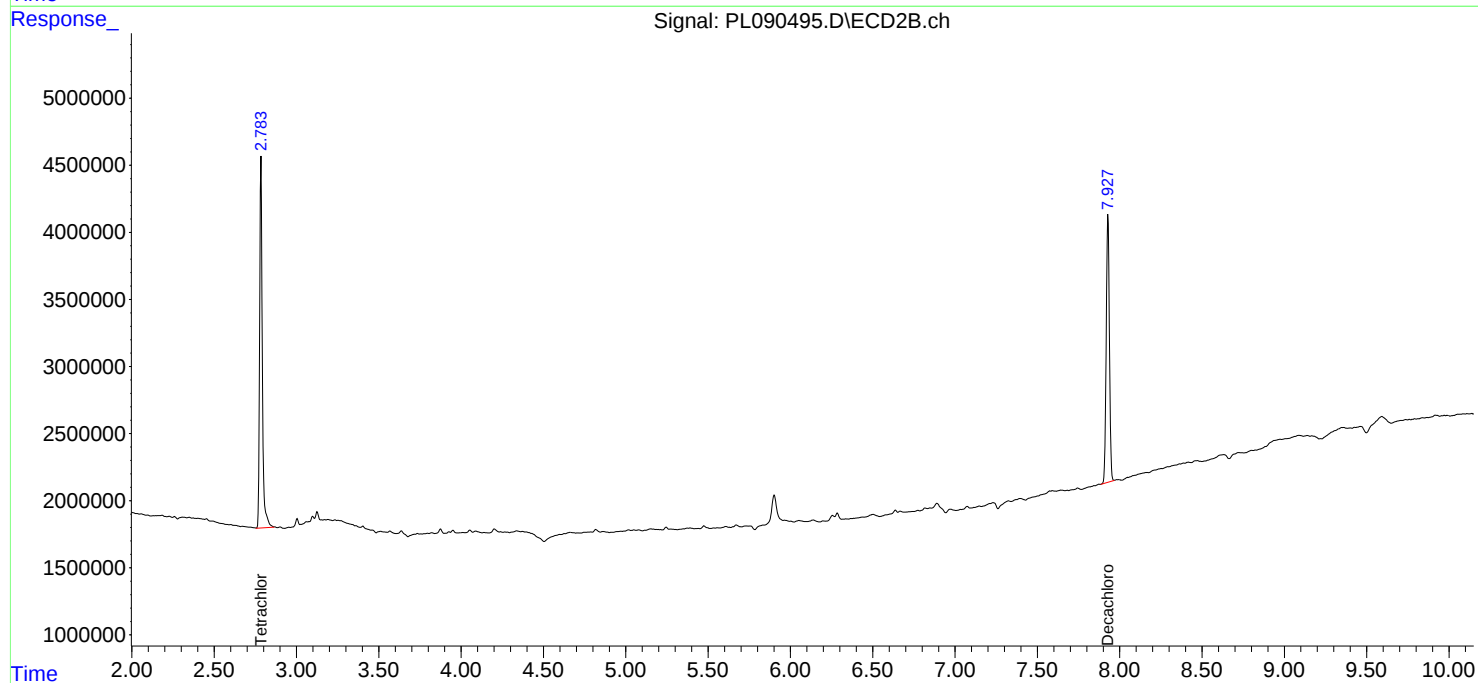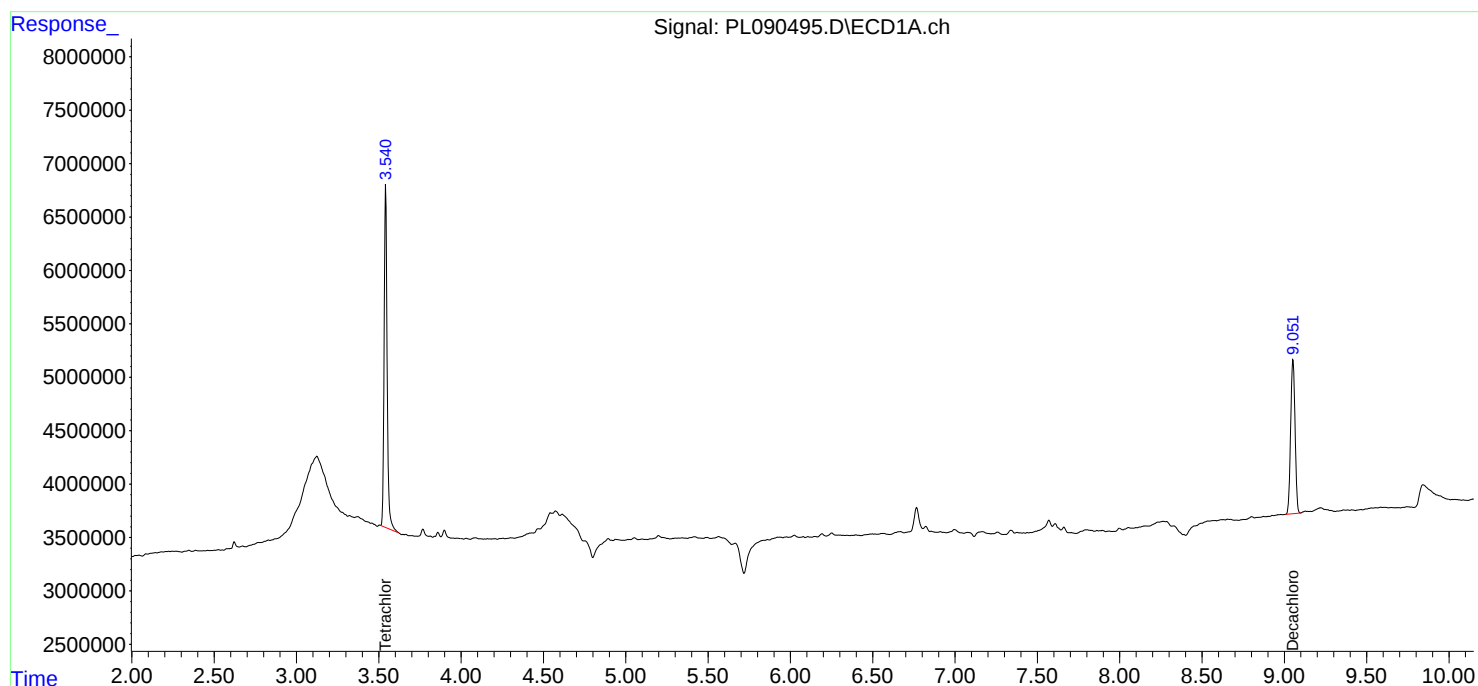

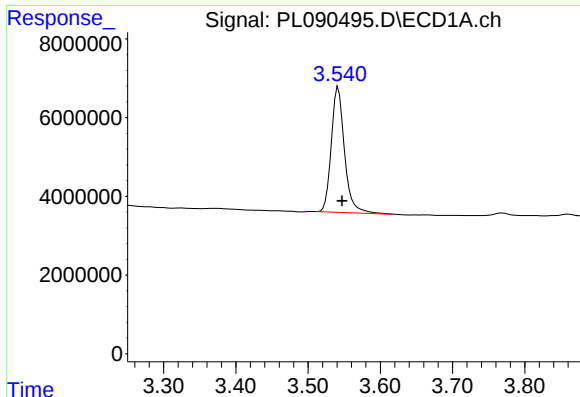


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.007 min
Response: 40576351
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
FILL-MATERIAL-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/12/2024
Supervised By :Ankita Jodhani 07/12/2024

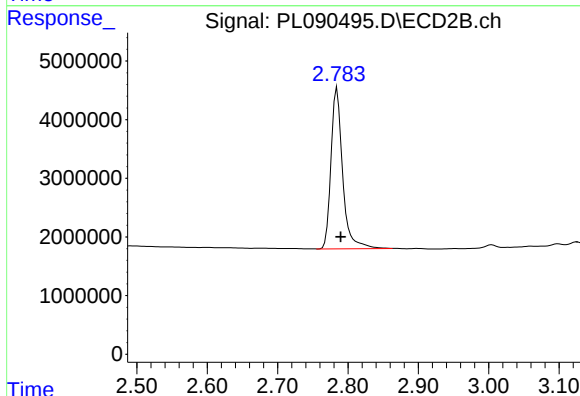


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: -0.007 min
Response: 31650188
Conc: 20.01 ng/ml m

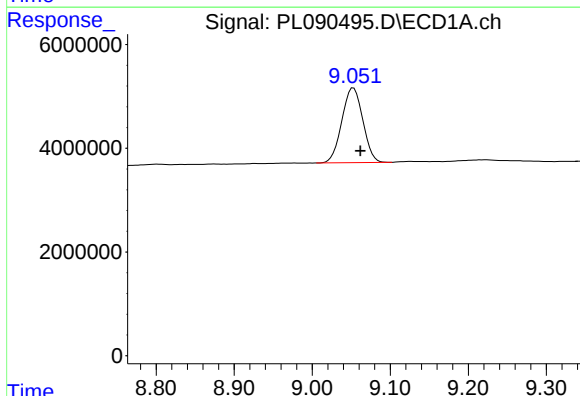

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.010 min
Response: 26894687
Conc: 17.44 ng/ml m

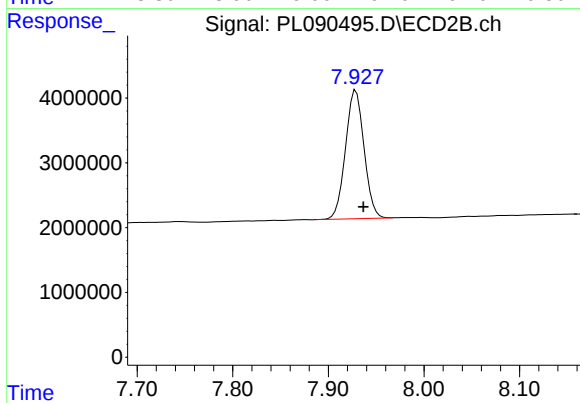

#28 Decachlorobiphenyl

R.T.: 7.927 min
Delta R.T.: -0.009 min
Response: 26855276
Conc: 18.00 ng/ml m