

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071125\
 Data File : PL096338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jul 2025 08:58
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 22:48:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.659	0.000	69755806	0	16.812	N.D. #
10) B	gamma-Chl...	5.891f	0.000	12469160	0	2.818	N.D. #
13) MA	Dieldrin	0.000	5.428	0	7032020	N.D.	1.031 #
14) MA	Endrin	0.000	5.718	0	8724813	N.D.	1.431 #
15) B	Endosulfa...	6.749	0.000	4918097	0	1.417	N.D. #
25)	Chlordane-3	5.891f	0.000	12469160	0	16.924	N.D. #
27)	Chlordane-5	6.839	0.000	1262462	0	8.364	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071125\
Data File : PL096338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jul 2025 08:58
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 22:48:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

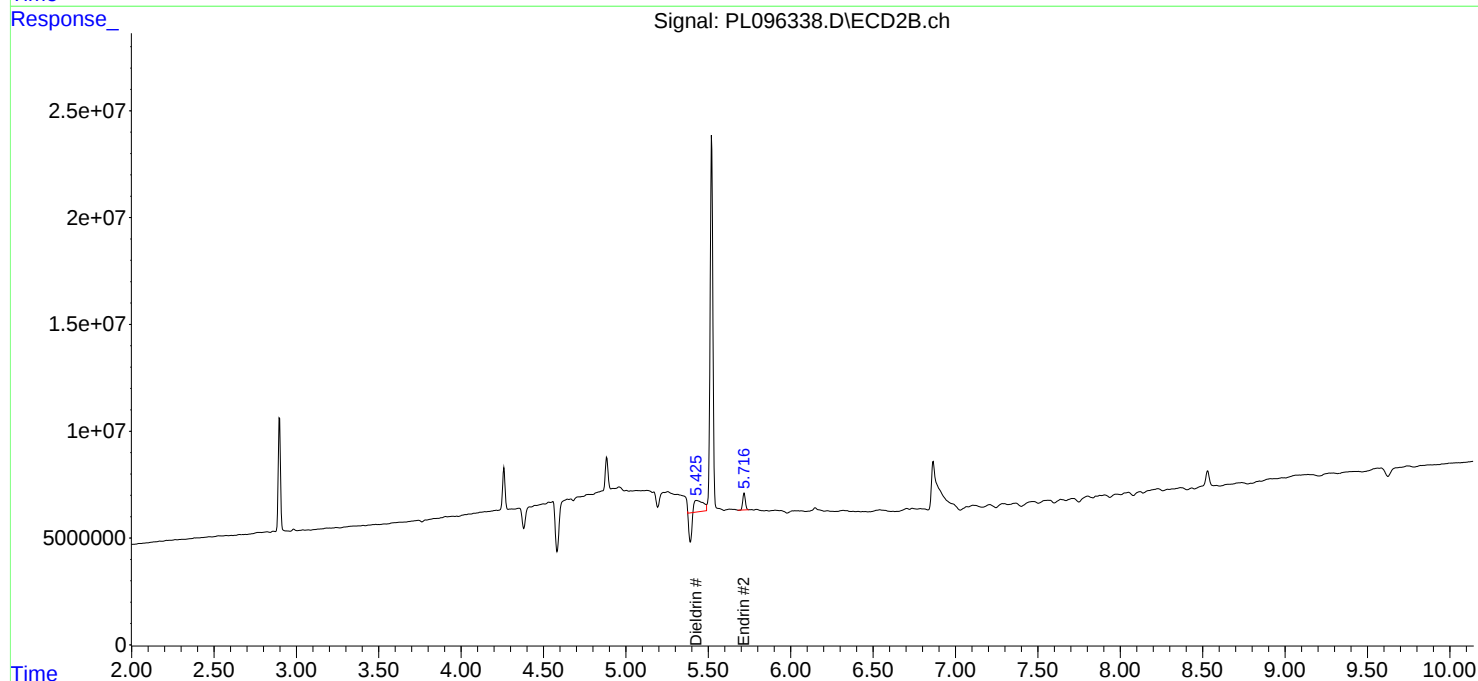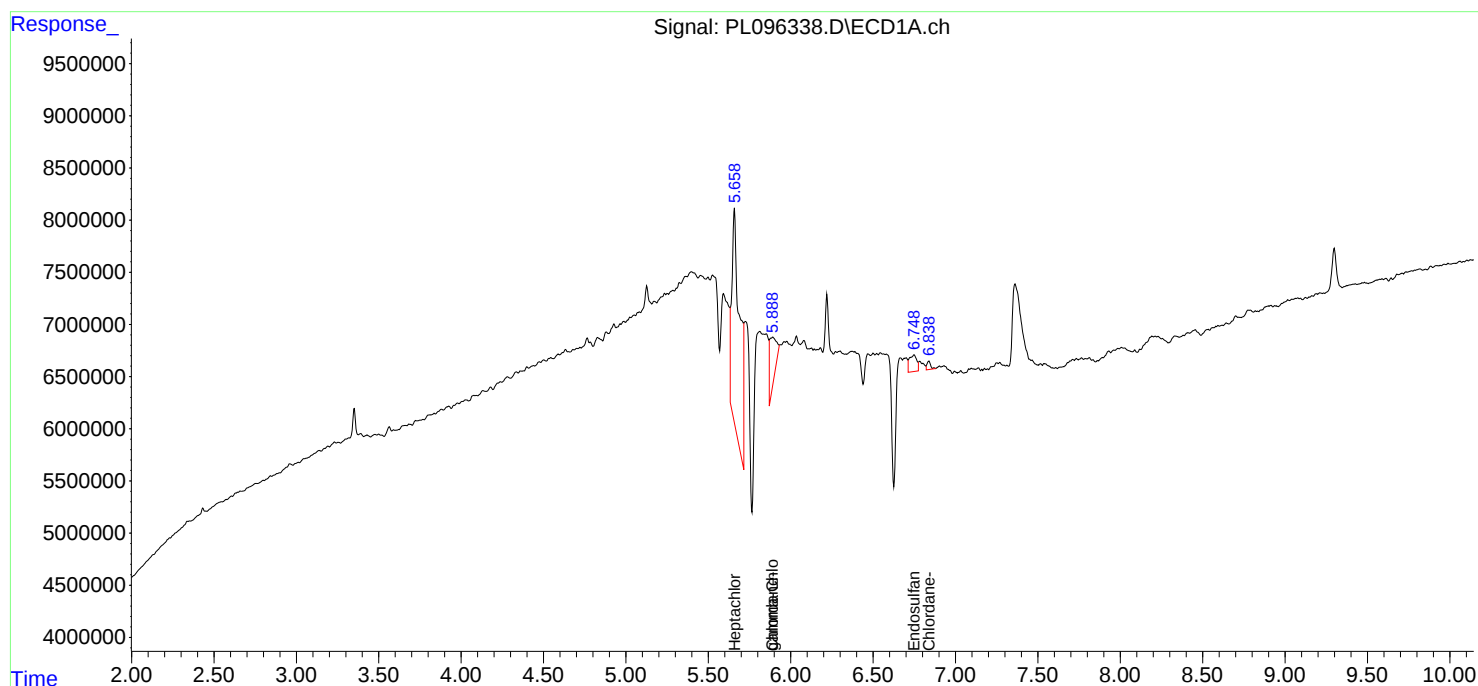


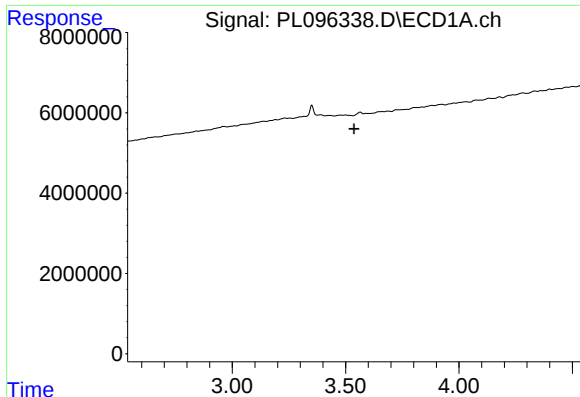

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

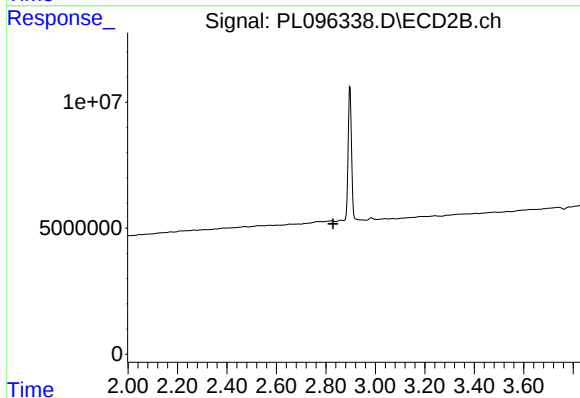

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 2.828 min
Response: 0
Conc: N.D.

#8 Heptachlor epoxide

R.T.: 5.659 min
Delta R.T.: -0.007 min
Response: 69755806
Conc: 16.81 ng/ml

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

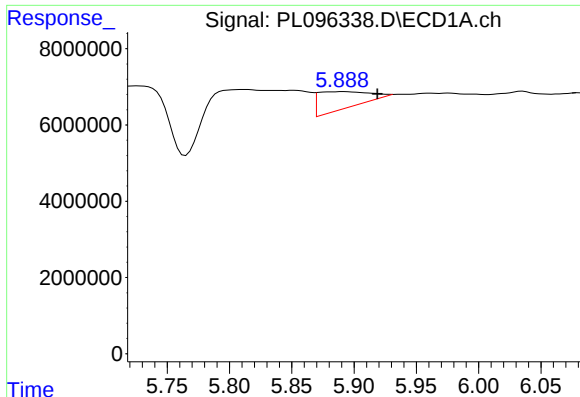

#10 gamma-Chlordane


R.T.: 5.891 min
Delta R.T.: -0.027 min
Response: 12469160
Conc: 2.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

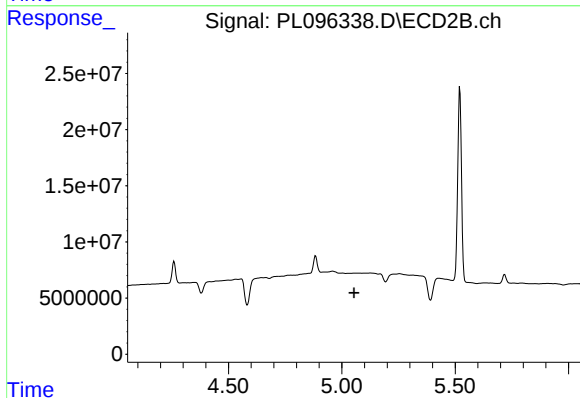


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

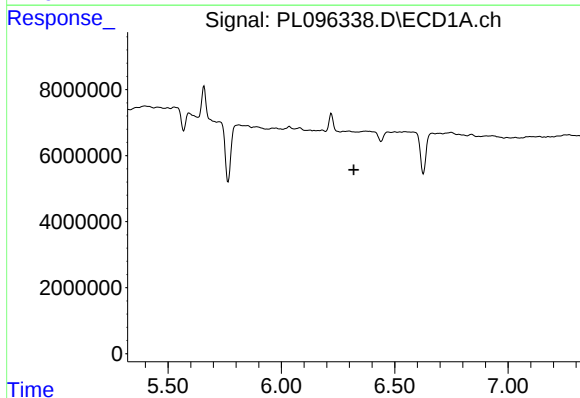


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

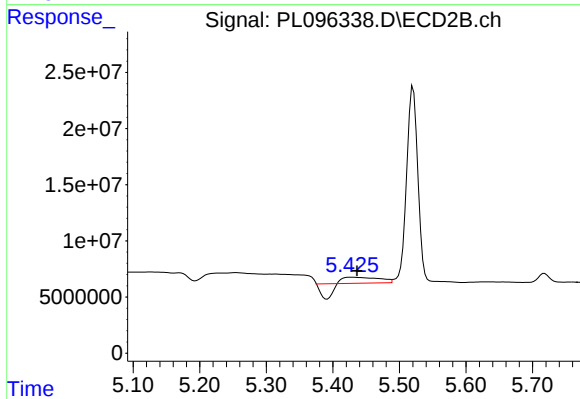

#13 Dieldrin


R.T.: 5.428 min
Delta R.T.: -0.008 min
Response: 7032020
Conc: 1.03 ng/ml

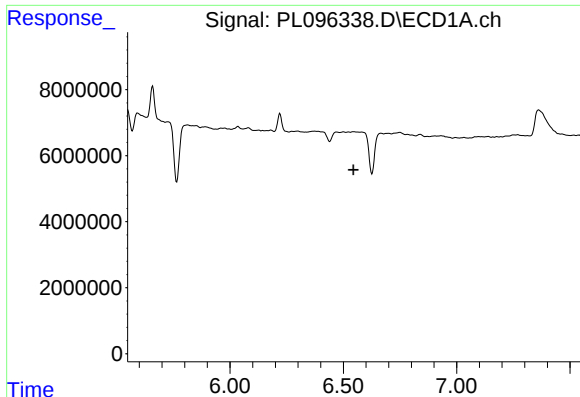

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.545 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

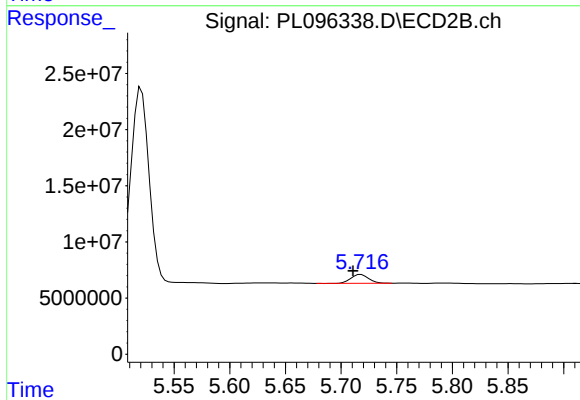


#14 Endrin

R.T.: 5.718 min
Delta R.T.: 0.007 min
Response: 8724813
Conc: 1.43 ng/ml

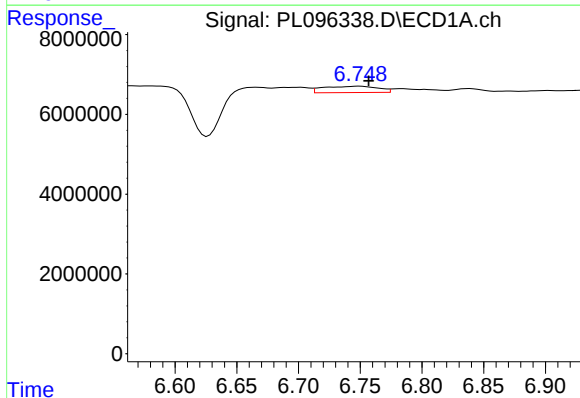


#15 Endosulfan II

R.T.: 6.749 min
Delta R.T.: -0.008 min
Response: 4918097
Conc: 1.42 ng/ml

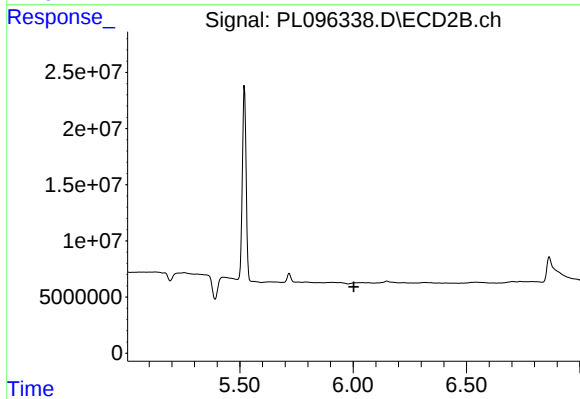

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.003 min
Response: 0
Conc: N.D.

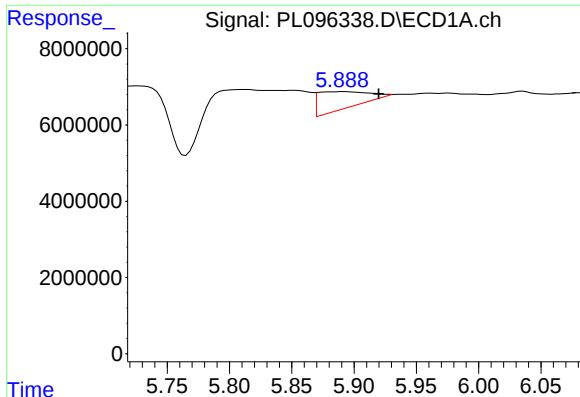

#25 Chlordane-3


R.T.: 5.891 min
Delta R.T.: -0.029 min
Response: 12469160
Conc: 16.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

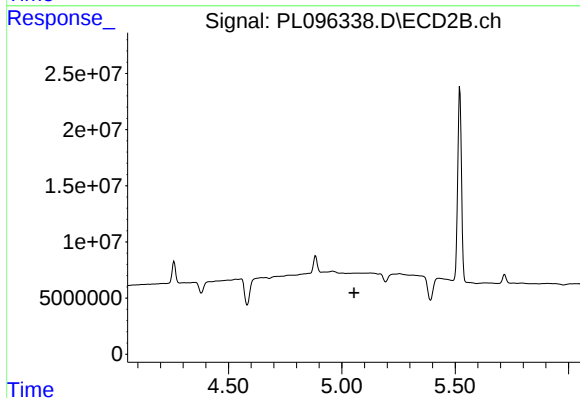


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

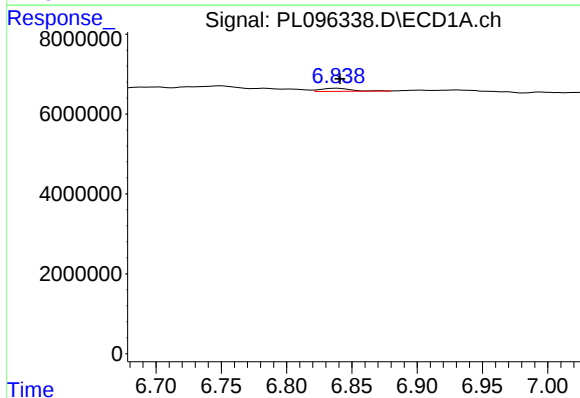


#27 Chlordane-5

R.T.: 6.839 min
Delta R.T.: -0.002 min
Response: 1262462
Conc: 8.36 ng/ml

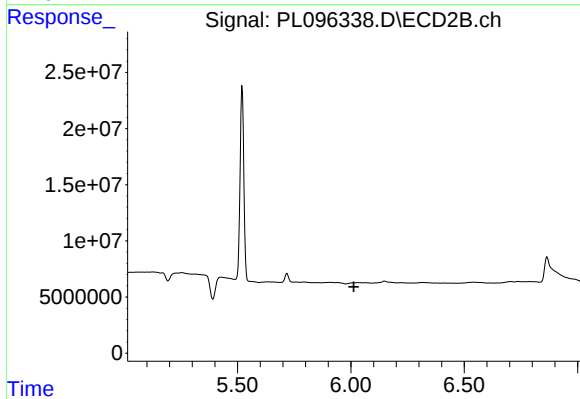

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.013 min
Response: 0
Conc: N.D.

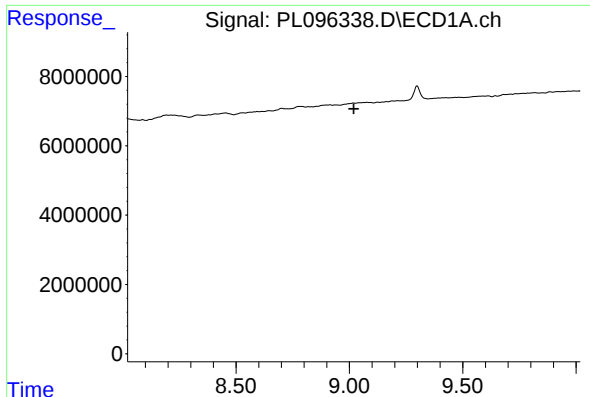

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.020 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

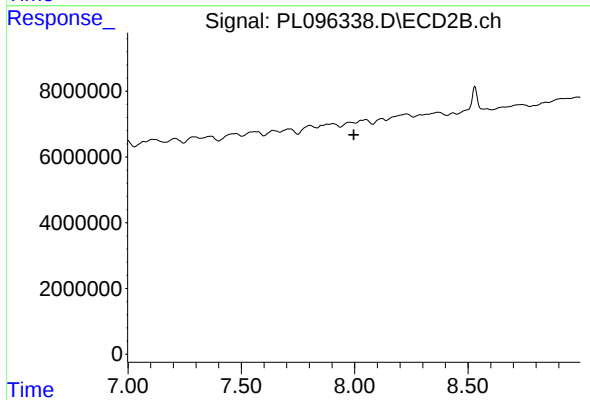

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.997 min
Response: 0
Conc: N.D.