

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071018\
 Data File : PL037846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2018 17:41
 Operator : AJ\SJ
 Sample : PB110960TB
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 07:06:21 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	141.5E6	57603662	17.884	20.820
28)	SA Decachlor...	8.011	8.947	135.1E6	51202730	22.394	25.809
Target Compounds							
3)	MA gamma-BHC...	4.012f	0.000	5168815	0	0.501	N.D. #
9)	A Endosulfan I	5.366	0.000	7964662	0	0.941	N.D. #
10)	B gamma-Chl...	5.163f	0.000	67289394	0	7.184	N.D. #
19)	B Endosulfa...	6.503	0.000	7071936	0	1.057	N.D. #
24)	Chlordane-2	4.645	0.000	9008256	0	25.304	N.D. #
25)	Chlordane-3	5.163	0.000	67289394	0	63.306	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071018\
Data File : PL037846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2018 17:41
Operator : AJ\SJ
Sample : PB110960TB
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 07:06:21 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

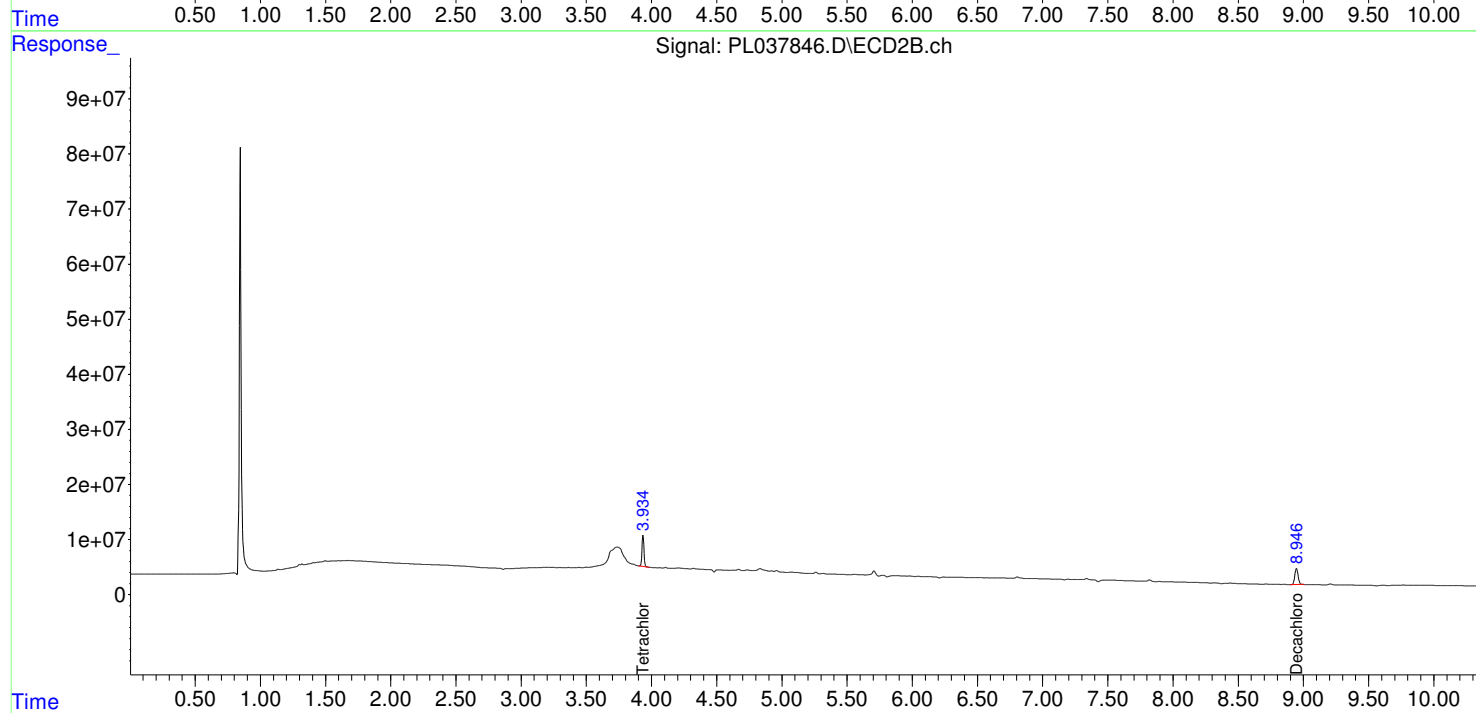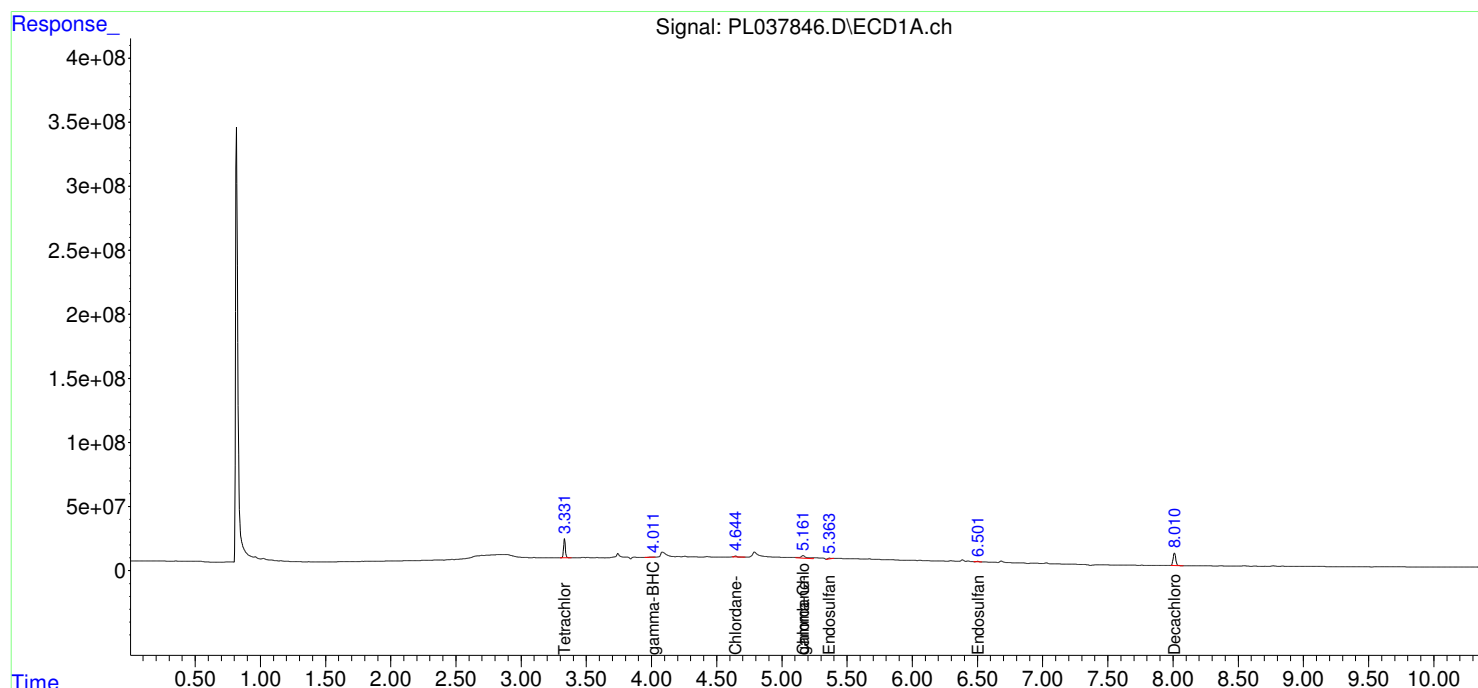


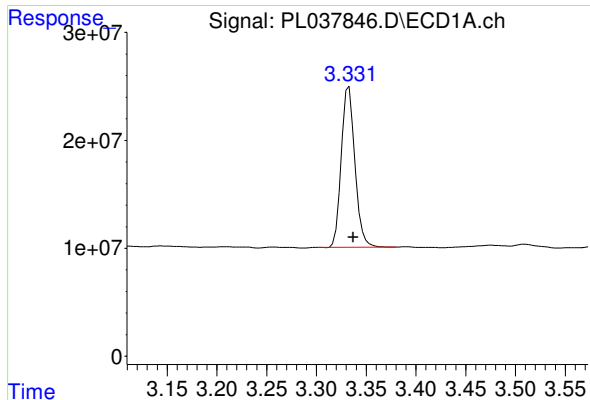

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 141470962
Conc: 17.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

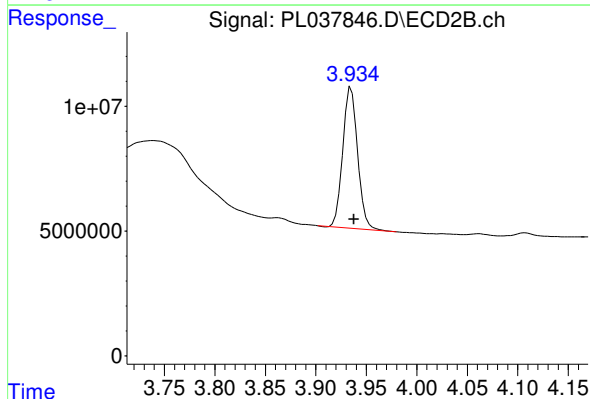


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 57603662
Conc: 20.82 ng/ml

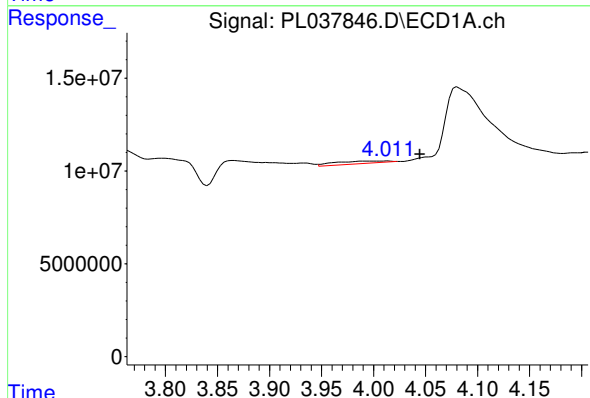


#3 gamma-BHC (Lindane)

R.T.: 4.012 min
Delta R.T.: -0.032 min
Response: 5168815
Conc: 0.50 ng/ml

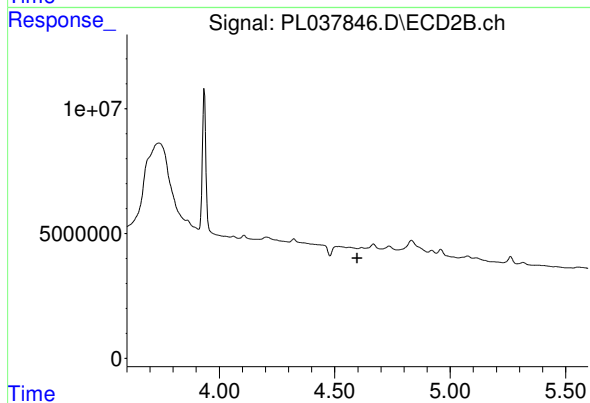

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

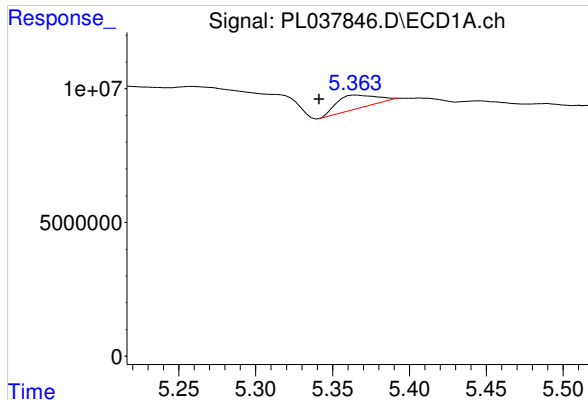

#9 Endosulfan I


R.T.: 5.366 min
Delta R.T.: 0.025 min
Response: 7964662
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

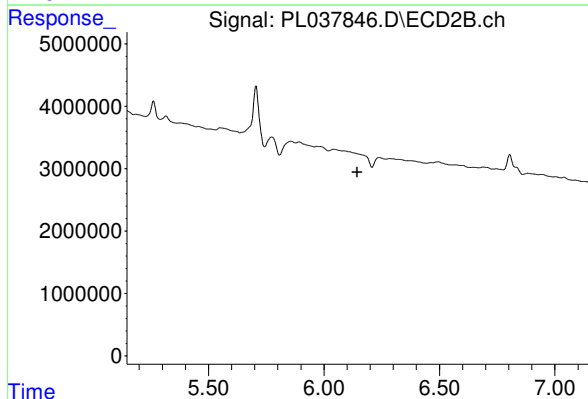


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.144 min
Response: 0
Conc: N.D.

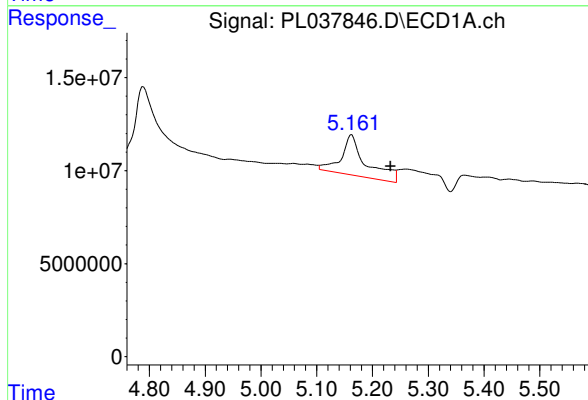


#10 gamma-Chlordane

R.T.: 5.163 min
Delta R.T.: -0.070 min
Response: 67289394
Conc: 7.18 ng/ml

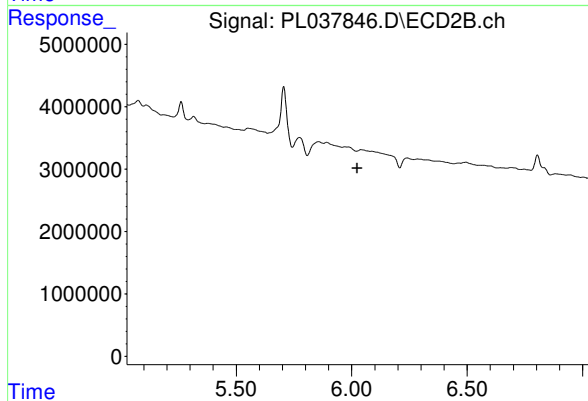

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.023 min
Response: 0
Conc: N.D.

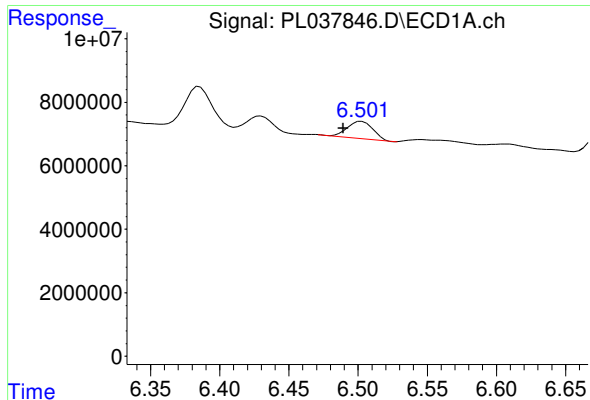

#19 Endosulfan Sulfate


R.T.: 6.503 min
Delta R.T.: 0.013 min
Response: 7071936
Conc: 1.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

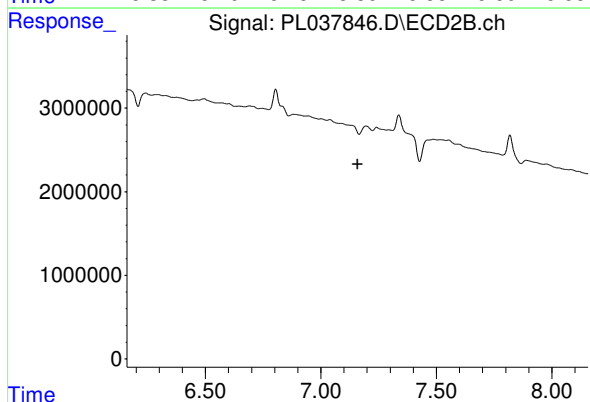


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.159 min
Response: 0
Conc: N.D.

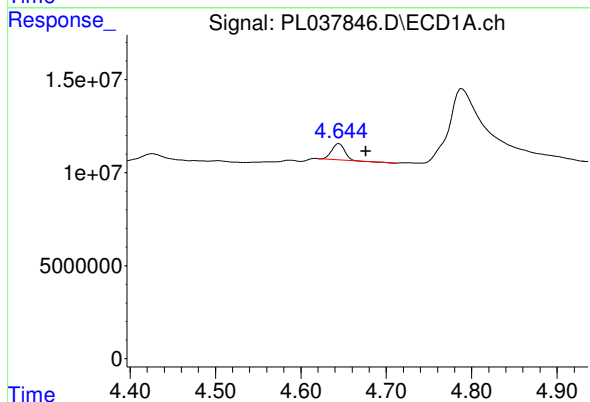


#24 Chlordane-2

R.T.: 4.645 min
Delta R.T.: -0.031 min
Response: 9008256
Conc: 25.30 ng/ml

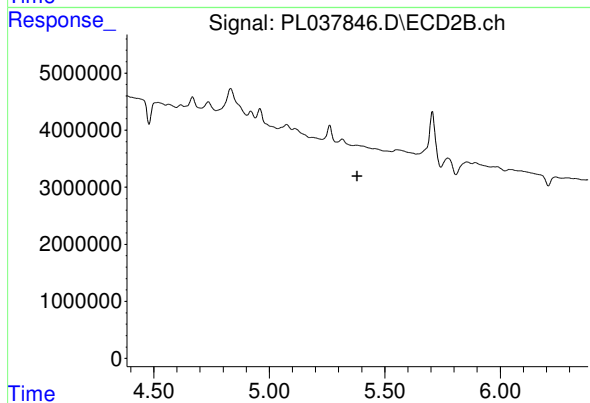

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

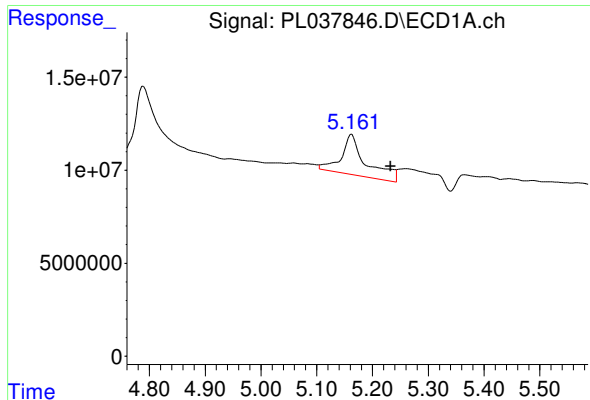

#25 Chlordane-3


R.T.: 5.163 min
Delta R.T.: -0.070 min
Response: 67289394
Conc: 63.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

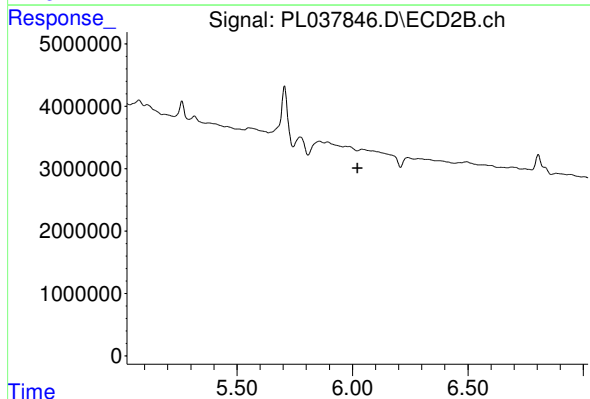


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

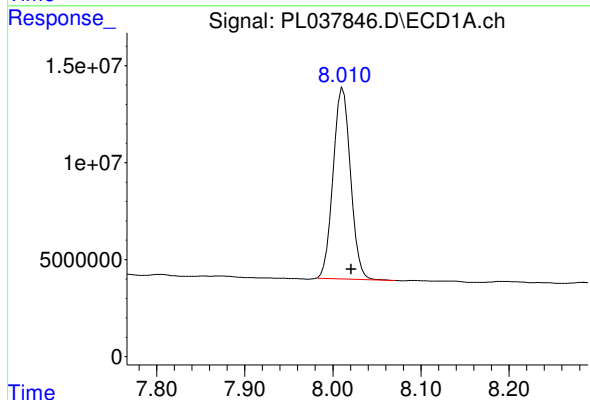

#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.009 min
Response: 135125239
Conc: 22.39 ng/ml

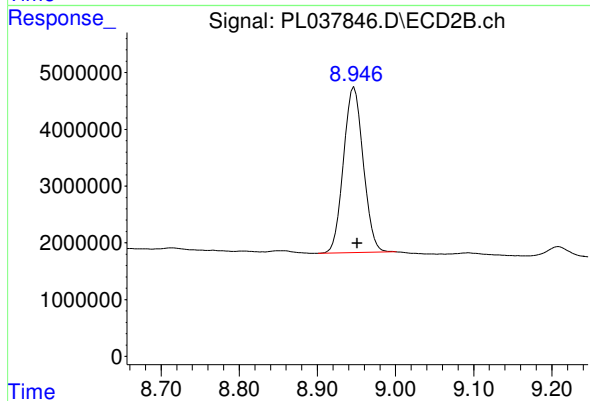

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 51202730
Conc: 25.81 ng/ml