

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071018\
 Data File : PL037853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2018 19:20
 Operator : AJ\SJ
 Sample : J3914-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 07:06:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.936	120.8E6	50021856	15.271	18.080
28)	SA Decachlor...	8.012	8.948	106.8E6	40474429	17.699	20.401
Target Compounds							
9)	A Endosulfan I	5.363	0.000	6140001	0	0.726	N.D. #
24)	Chlordane-2	4.645	0.000	5760318	0	16.181	N.D. #
25)	Chlordane-3	5.162	0.000	122.8E6	0	115.520	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071018\
Data File : PL037853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2018 19:20
Operator : AJ\SJ
Sample : J3914-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 07:06:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

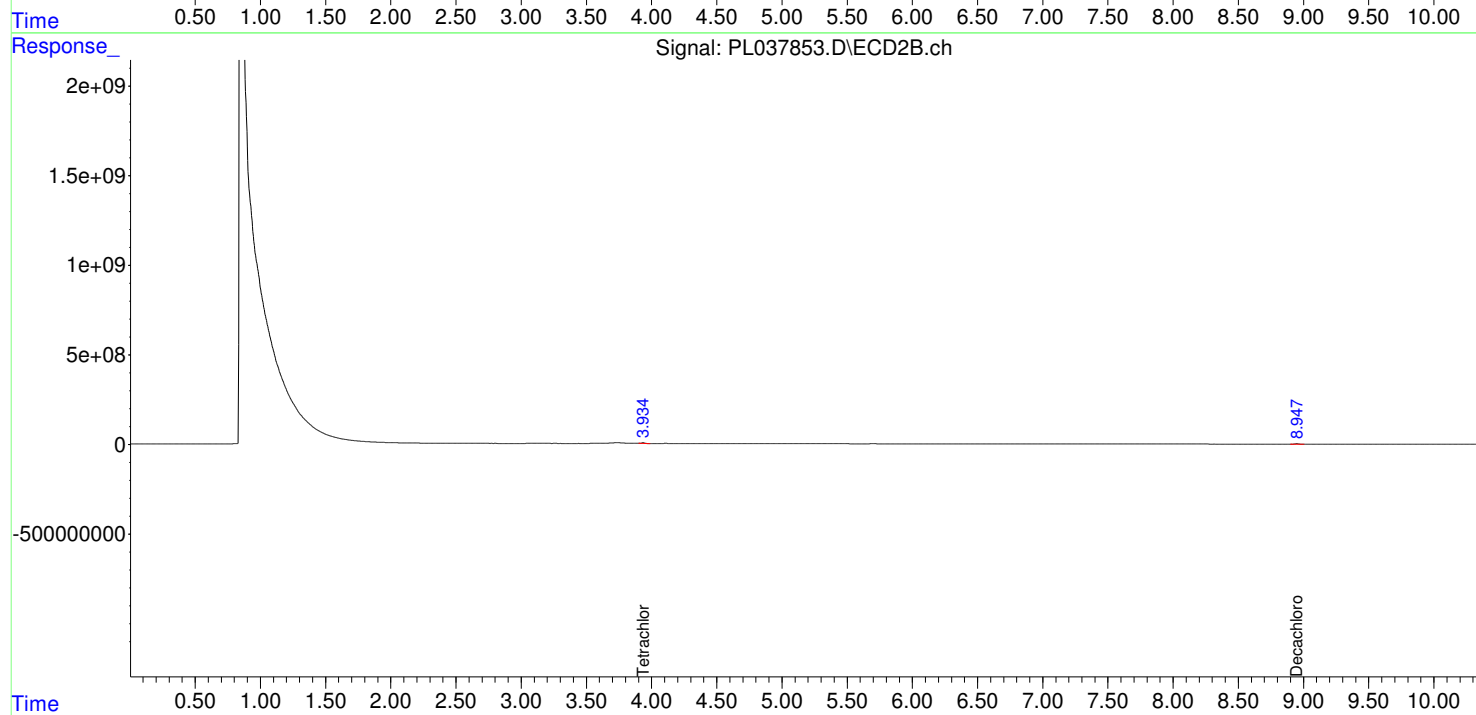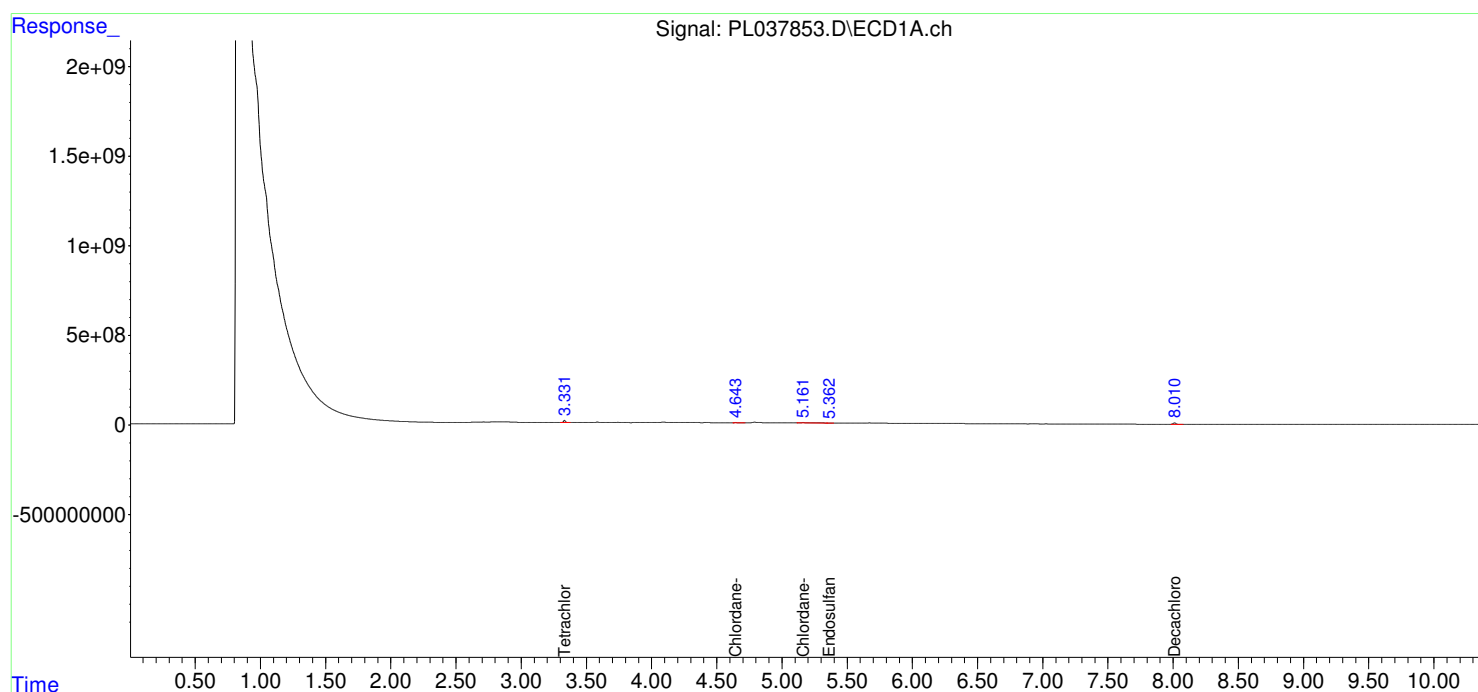


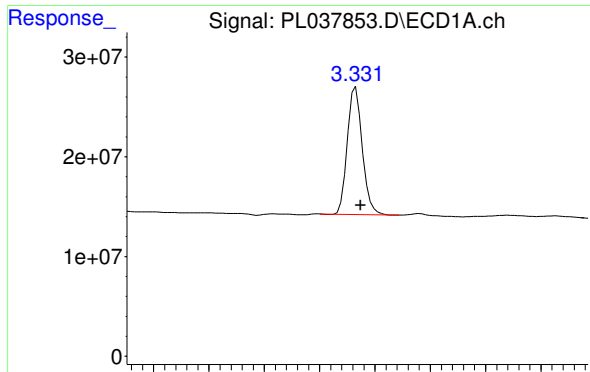

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 120794901
Conc: 15.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

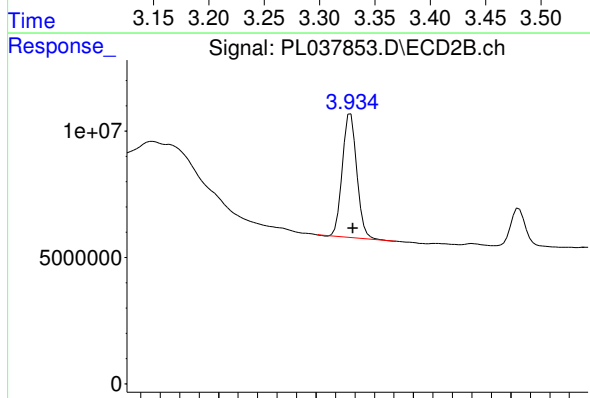


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 50021856
Conc: 18.08 ng/ml

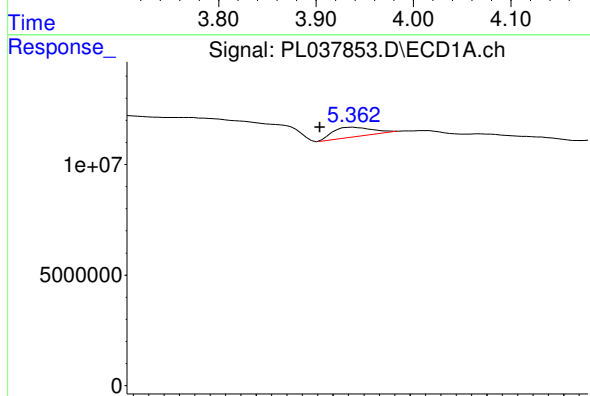


#9 Endosulfan I

R.T.: 5.363 min
Delta R.T.: 0.022 min
Response: 6140001
Conc: 0.73 ng/ml

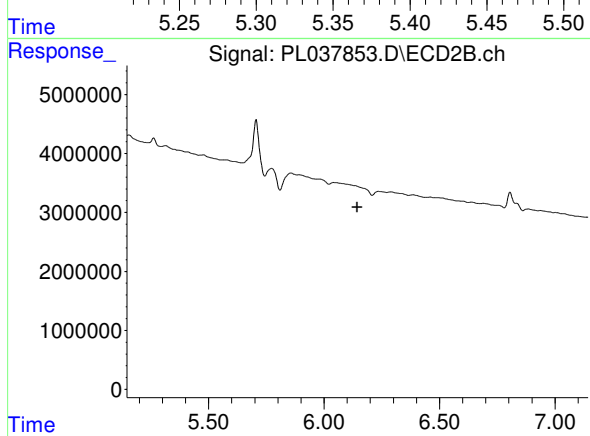

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.144 min
Response: 0
Conc: N.D.

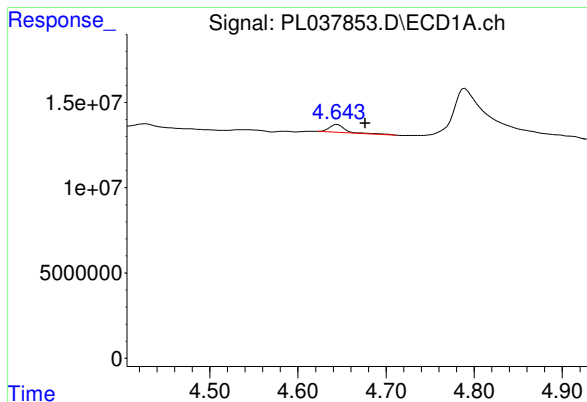

#24 Chlordane-2


R.T.: 4.645 min
Delta R.T.: -0.032 min
Response: 5760318
Conc: 16.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

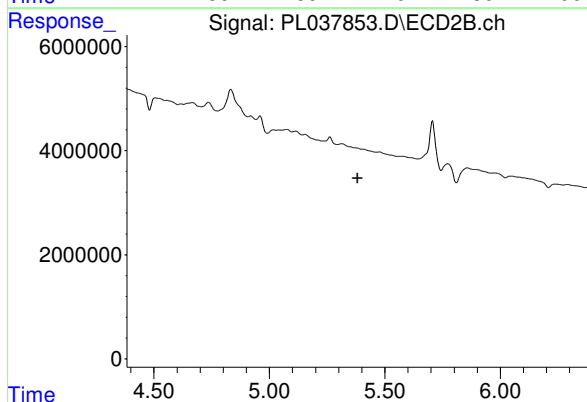


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.382 min
Response: 0
Conc: N.D.

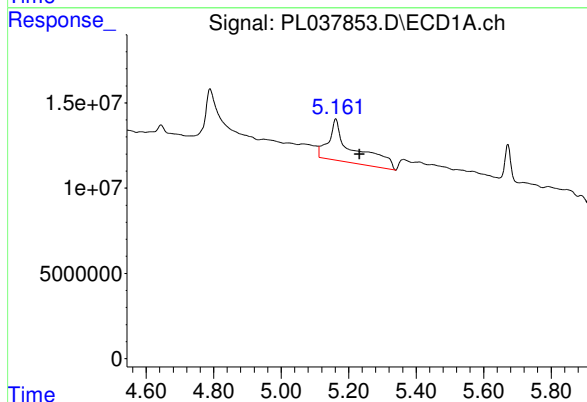


#25 Chlordane-3

R.T.: 5.162 min
Delta R.T.: -0.070 min
Response: 122788896
Conc: 115.52 ng/ml

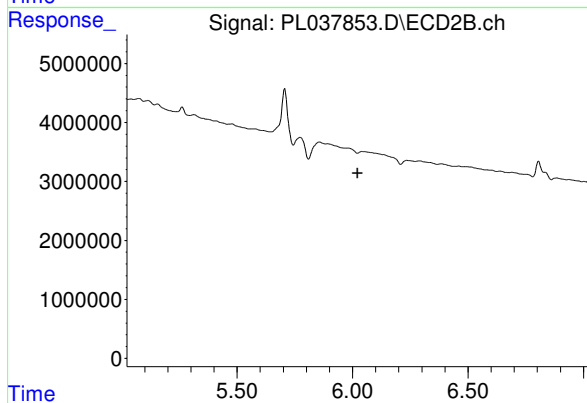

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

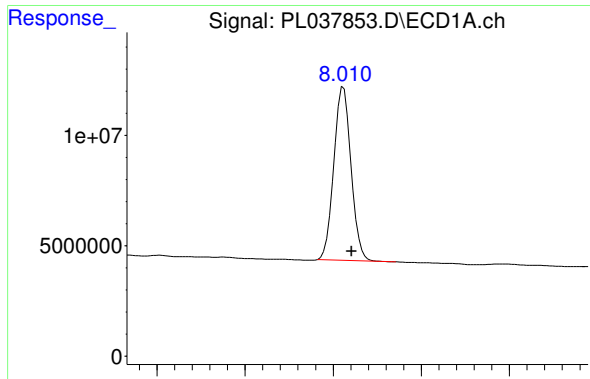

#28 Decachlorobiphenyl

R.T.: 8.012 min
Delta R.T.: -0.009 min
Response: 106796231
Conc: 17.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

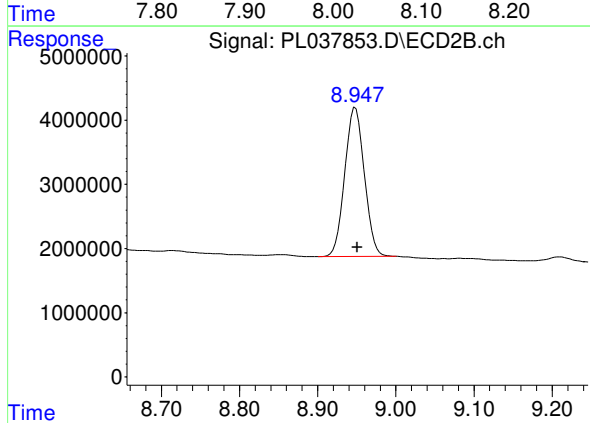

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 40474429
Conc: 20.40 ng/ml