

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071018\
 Data File : PL037857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2018 20:16
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 07:07:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.333	3.936	125.9E6	49466680	15.921	17.879
28) SA Decachlor...	8.012	8.949	128.9E6	48092768	21.370	24.241
Target Compounds						
6) B beta-BHC	4.251f	0.000	6963013	0	1.527	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071018\
Data File : PL037857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2018 20:16
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 07:07:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

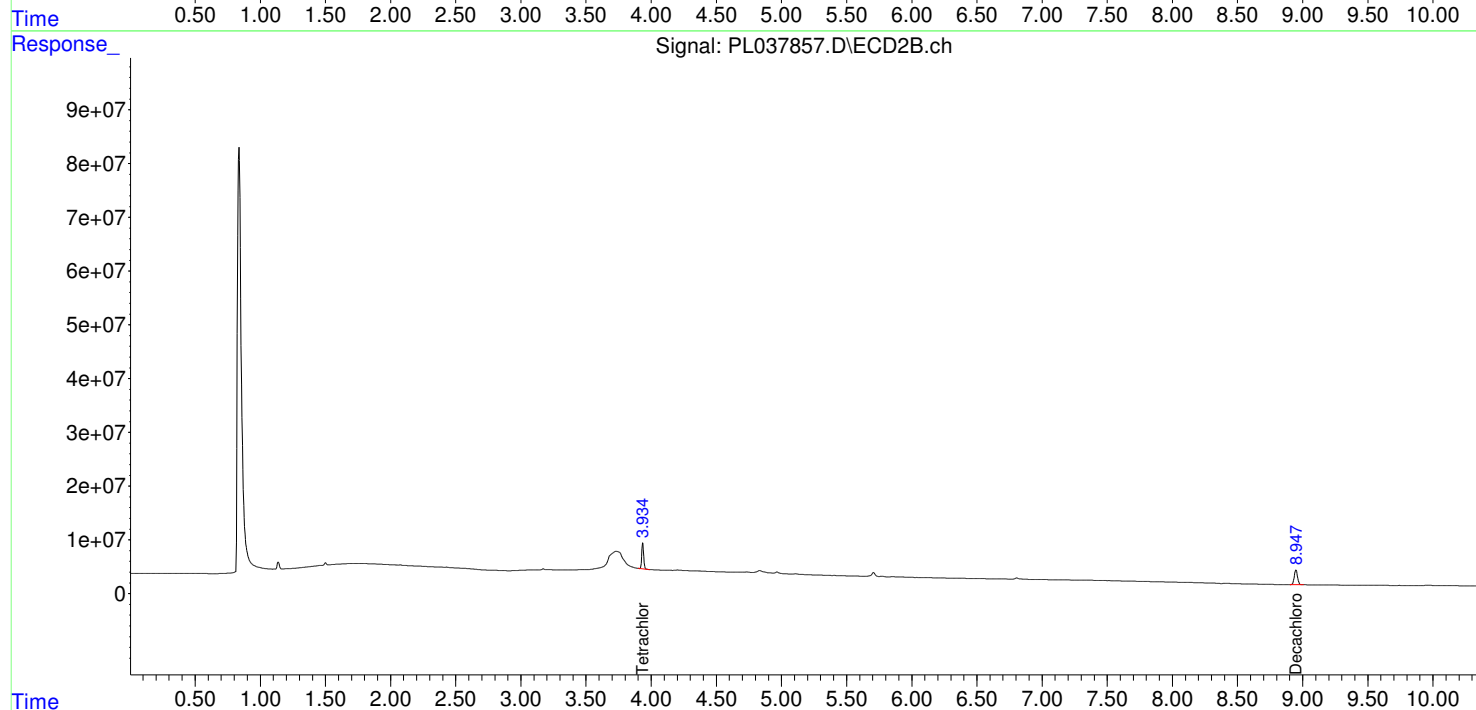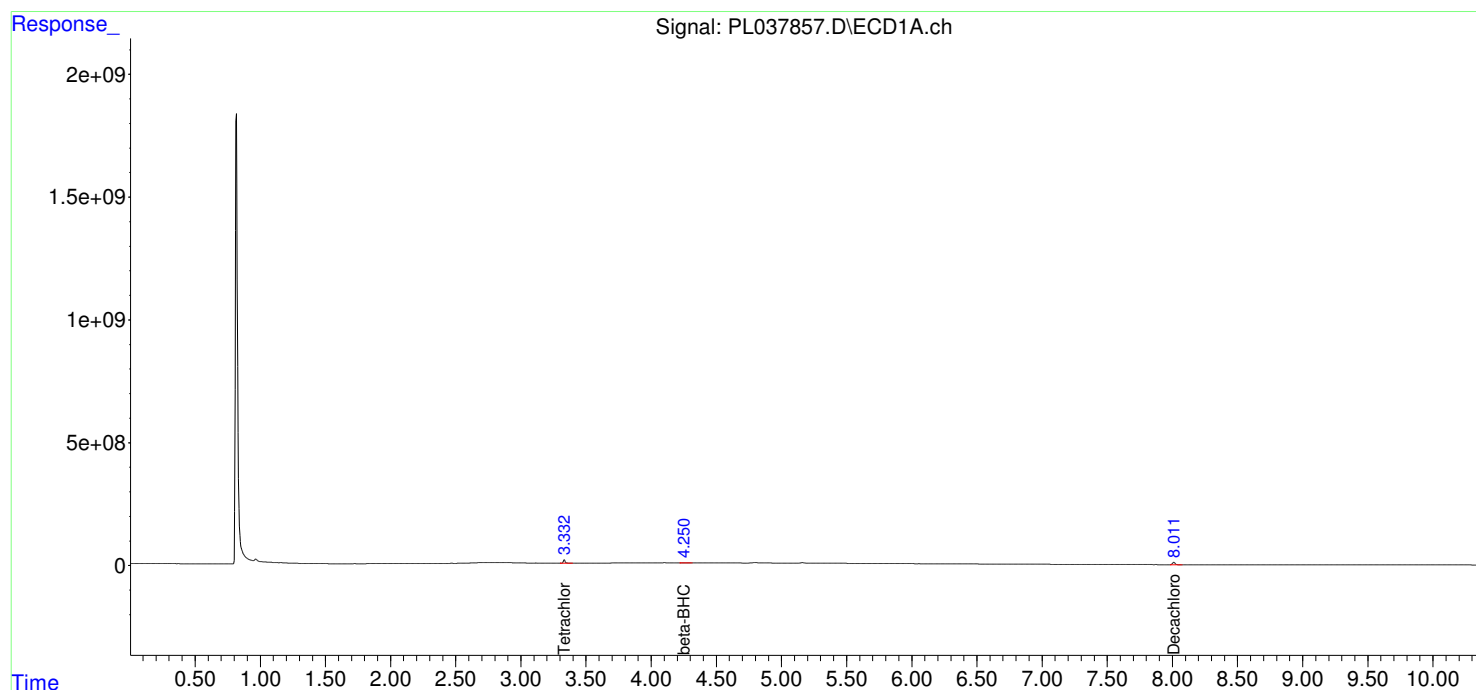


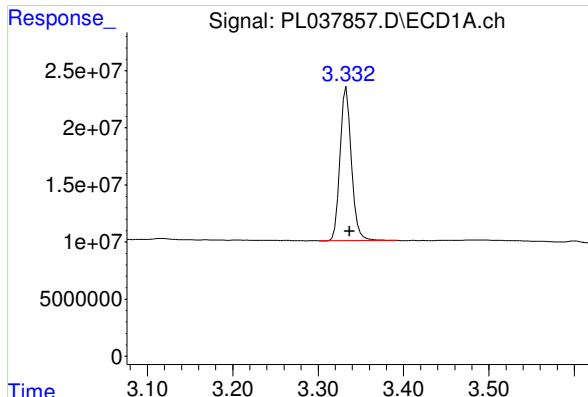

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 125941018
Conc: 15.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

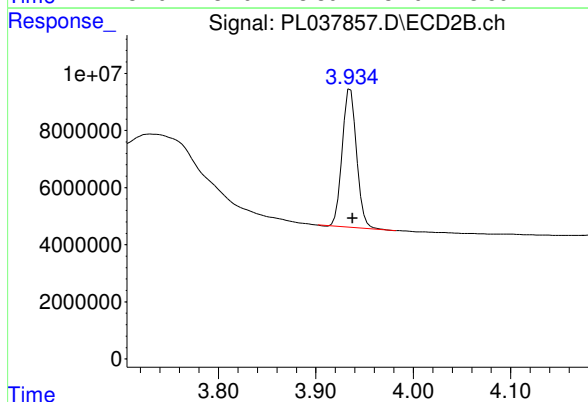


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 49466680
Conc: 17.88 ng/ml

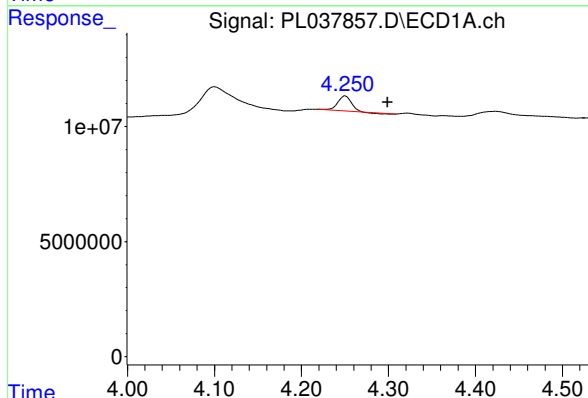


#6 beta-BHC

R.T.: 4.251 min
Delta R.T.: -0.048 min
Response: 6963013
Conc: 1.53 ng/ml

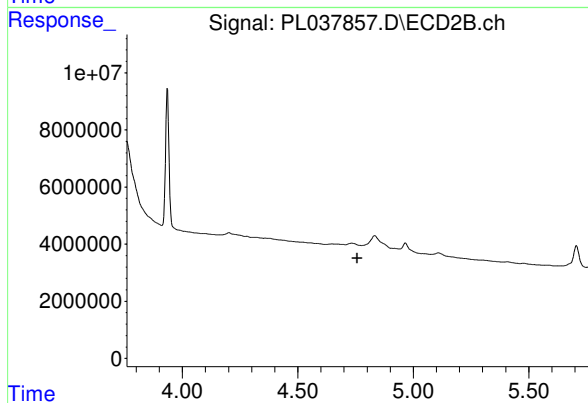

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.758 min
Response: 0
Conc: N.D.

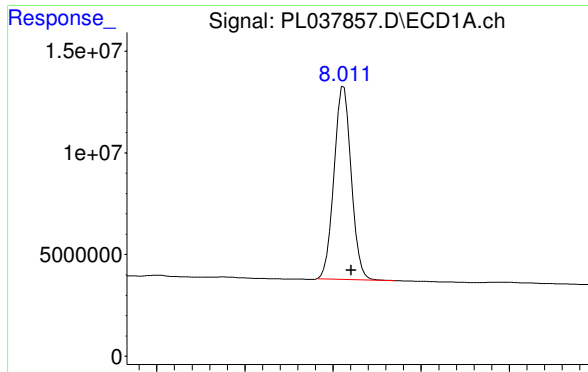

#28 Decachlorobiphenyl

R.T.: 8.012 min
Delta R.T.: -0.009 min
Response: 128946667
Conc: 21.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

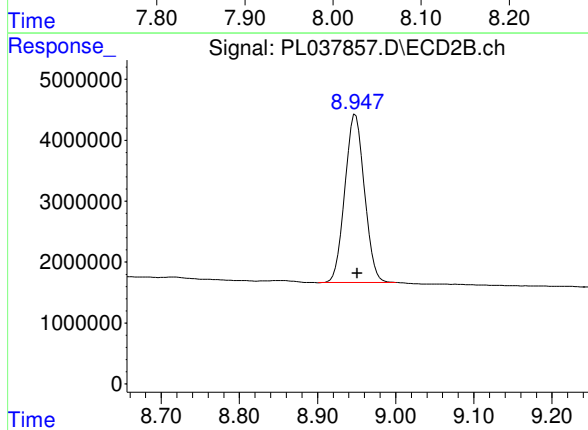

#28 Decachlorobiphenyl

R.T.: 8.949 min
Delta R.T.: -0.002 min
Response: 48092768
Conc: 24.24 ng/ml