

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071218\
 Data File : PL037903.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 08:33
 Operator : AJ\SJ
 Sample : J3918-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:24:14 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.333	3.935	152.0E6	62247634	19.219	22.499
28)	SA Decachlor...	8.008	8.946	140.0E6	55069736	23.207	27.758
Target Compounds							
3)	MA gamma-BHC...	4.092f	0.000	28189979	0	2.733	N.D. #
6)	B beta-BHC	4.250f	0.000	14171893	0	3.107	N.D. #
7)	B delta-BHC	0.000	4.965	0	7910801	N.D.	2.805 #
23)	Chlordane-1	4.250	4.965	14171893	7910801	46.155	65.835 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071218\
Data File : PL037903.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 08:33
Operator : AJ\SJ
Sample : J3918-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:24:14 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

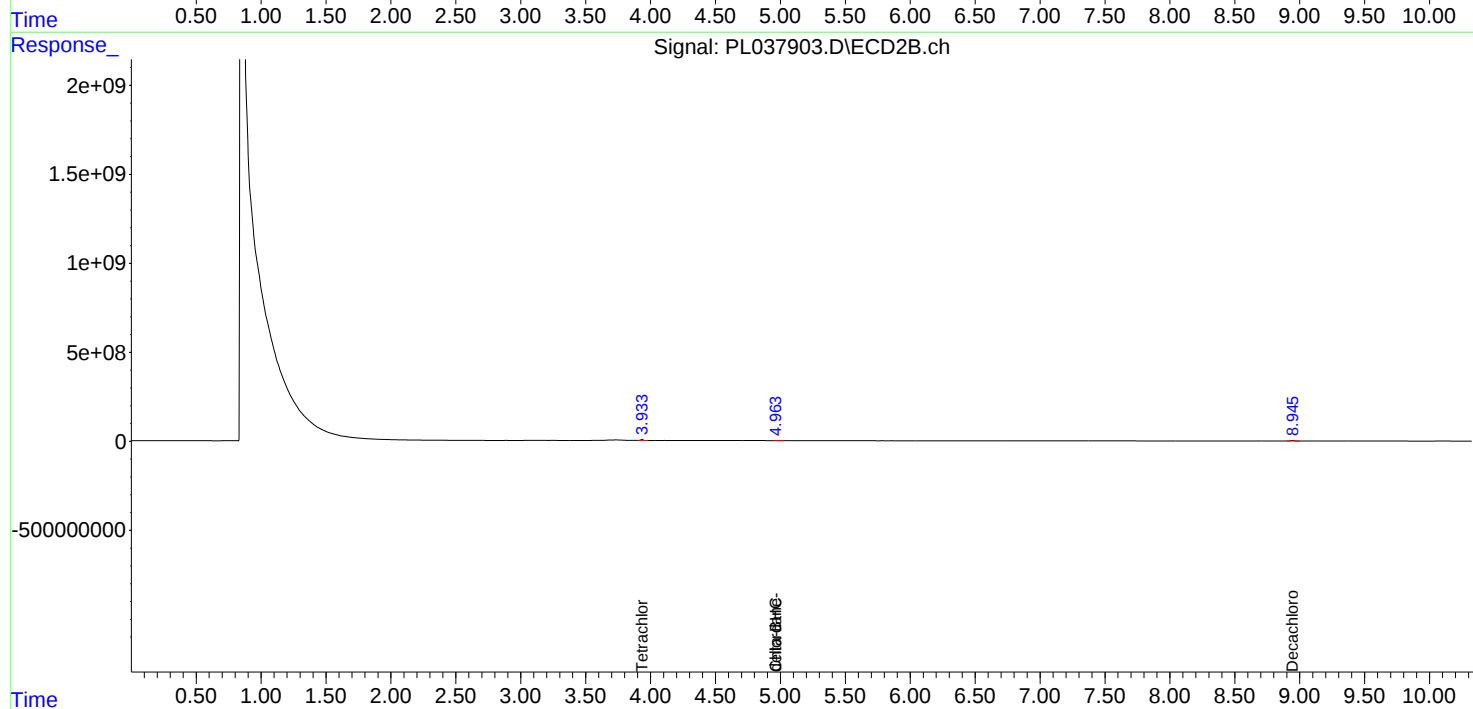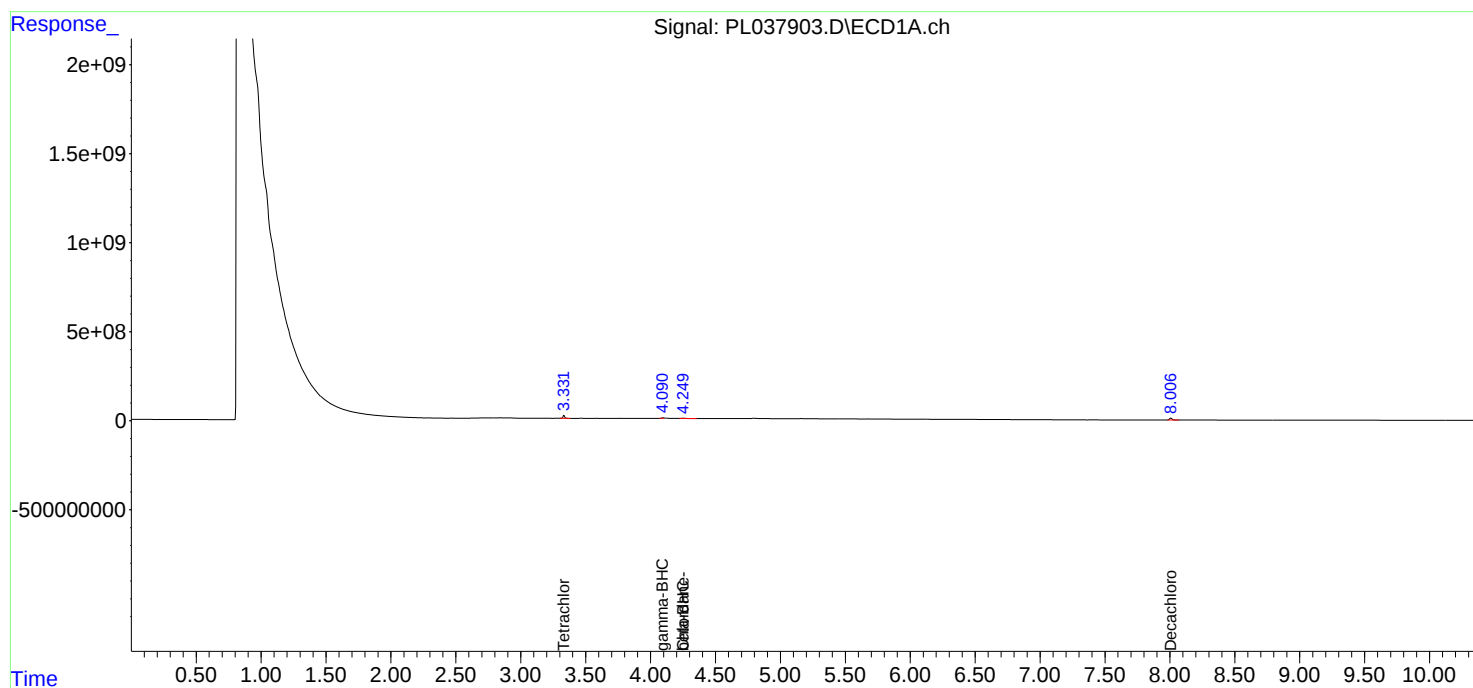


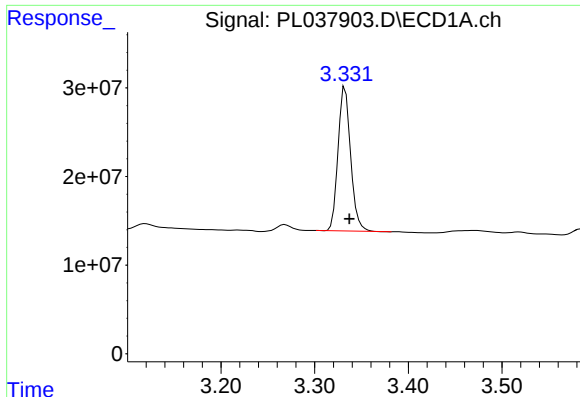

#1 Tetrachloro-m-xylene


R.T.: 3.333 min
Delta R.T.: -0.004 min
Response: 152030014
Conc: 19.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

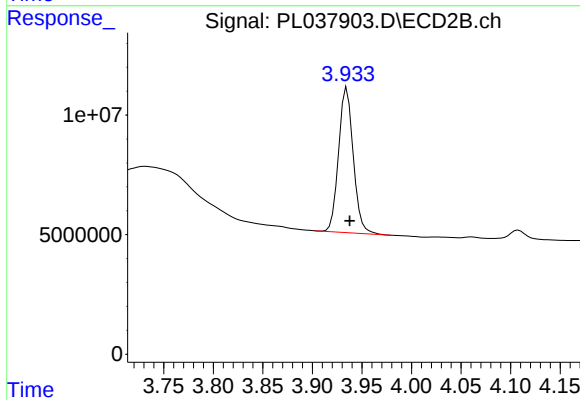


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 62247634
Conc: 22.50 ng/ml

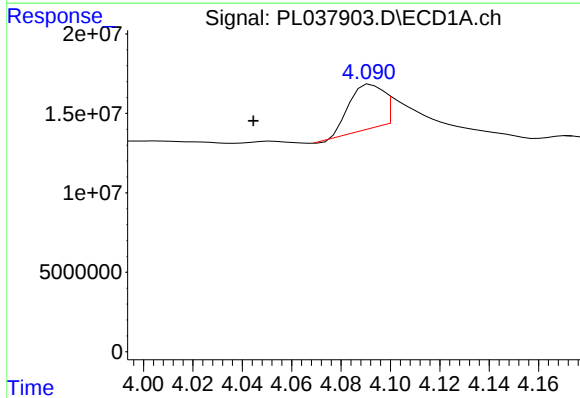


#3 gamma-BHC (Lindane)

R.T.: 4.092 min
Delta R.T.: 0.048 min
Response: 28189979
Conc: 2.73 ng/ml

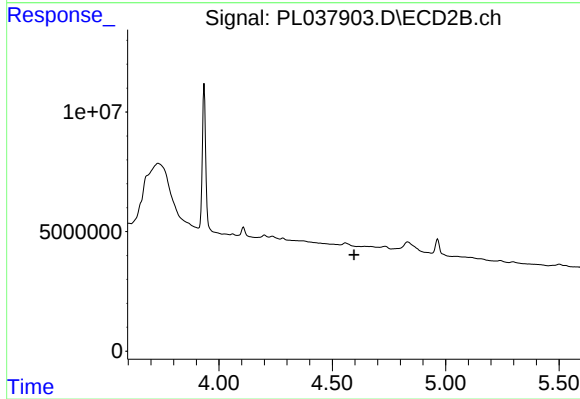

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

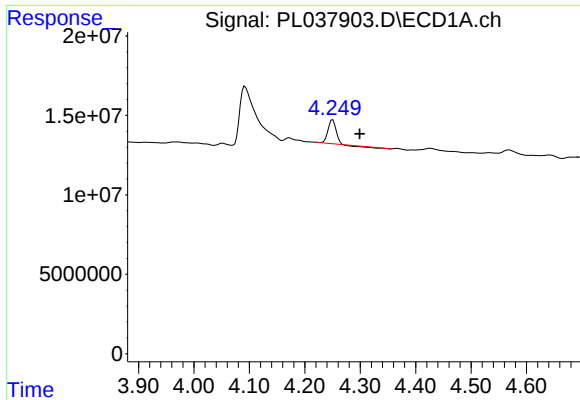

#6 beta-BHC


R.T.: 4.250 min
Delta R.T.: -0.049 min
Response: 14171893
Conc: 3.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

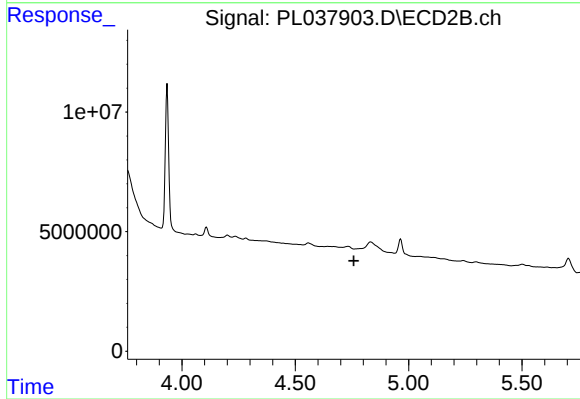


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

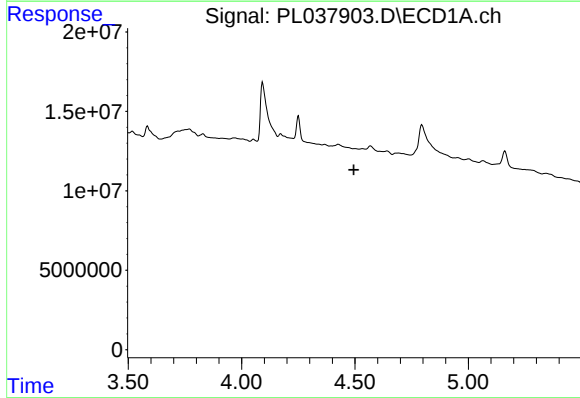


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.494 min
Response: 0
Conc: N.D.

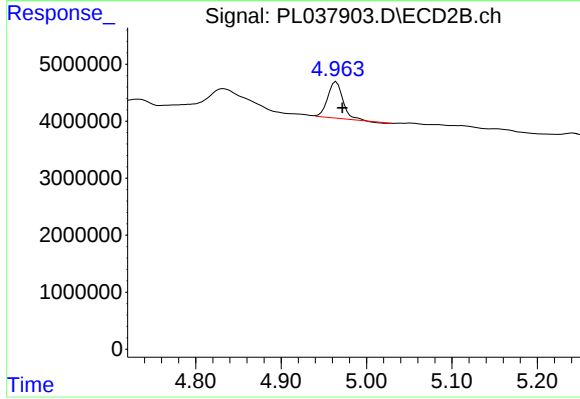

#7 delta-BHC


R.T.: 4.965 min
Delta R.T.: -0.007 min
Response: 7910801
Conc: 2.80 ng/ml

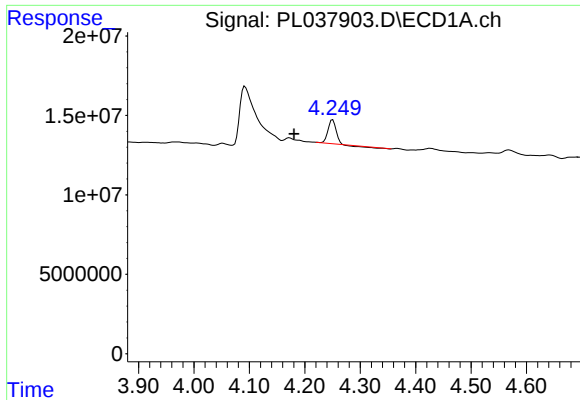

#23 Chlordane-1


R.T.: 4.250 min
Delta R.T.: 0.070 min
Response: 14171893
Conc: 46.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

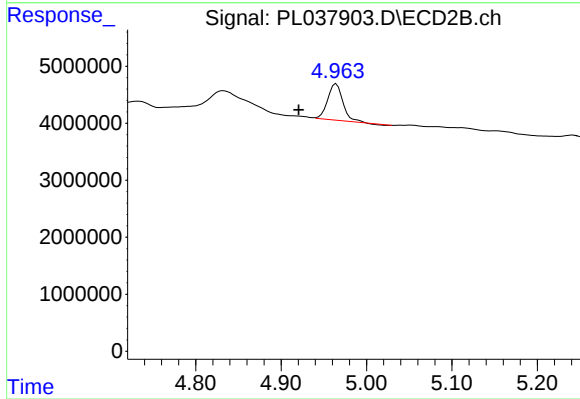


#23 Chlordane-1

R.T.: 4.965 min
Delta R.T.: 0.044 min
Response: 7910801
Conc: 65.84 ng/ml

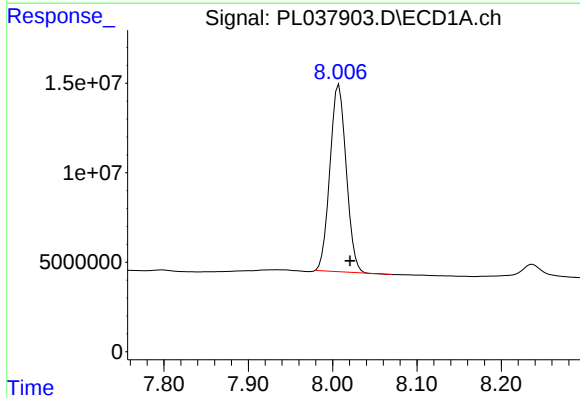

#28 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: -0.013 min
Response: 140030436
Conc: 23.21 ng/ml

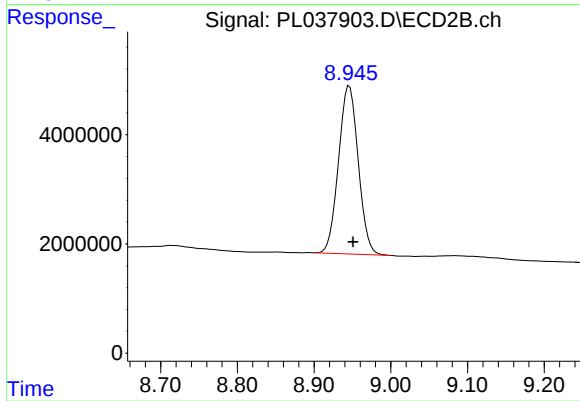

#28 Decachlorobiphenyl

R.T.: 8.946 min
Delta R.T.: -0.005 min
Response: 55069736
Conc: 27.76 ng/ml