

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071218\
 Data File : PL037916.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 11:36
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:26:25 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	3.935	120.9E6	47676862	15.280	17.232
28)	SA Decachlor...	8.008	8.945	108.7E6	43791901	18.010	22.073
Target Compounds							
4)	MA Heptachlor	0.000	5.052f	0	6113247	N.D.	1.769 #
6)	B beta-BHC	4.250f	0.000	11036814	0	2.420	N.D. #
7)	B delta-BHC	4.506	0.000	15470220	0	1.462	N.D. #
8)	B Heptachlo...	0.000	5.779	0	30772243	N.D.	10.795 #
13)	MA Dieldrin	5.533f	0.000	6207460	0	0.701	N.D. #
14)	MA Endrin	5.845	0.000	50935235	0	6.466	N.D. #
21)	B Endrin ke...	6.931f	0.000	810.3E6	0	113.944	N.D. #
23)	Chlordane-1	4.250	0.000	11036814	0	35.944	N.D. #
24)	Chlordane-2	0.000	5.315	0	35261939	N.D.	278.639 #
27)	Chlordane-5	5.845	0.000	50935235	0	389.210	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071218\
Data File : PL037916.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 11:36
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:26:25 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

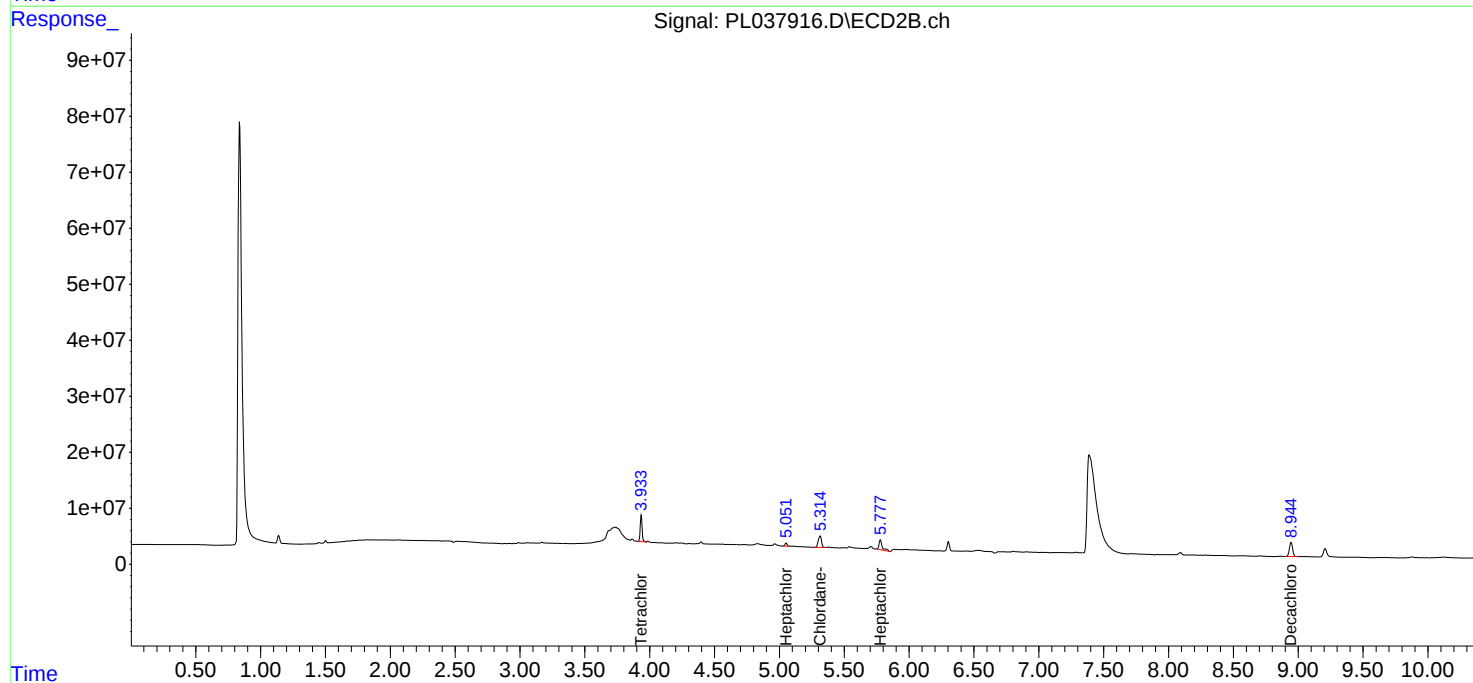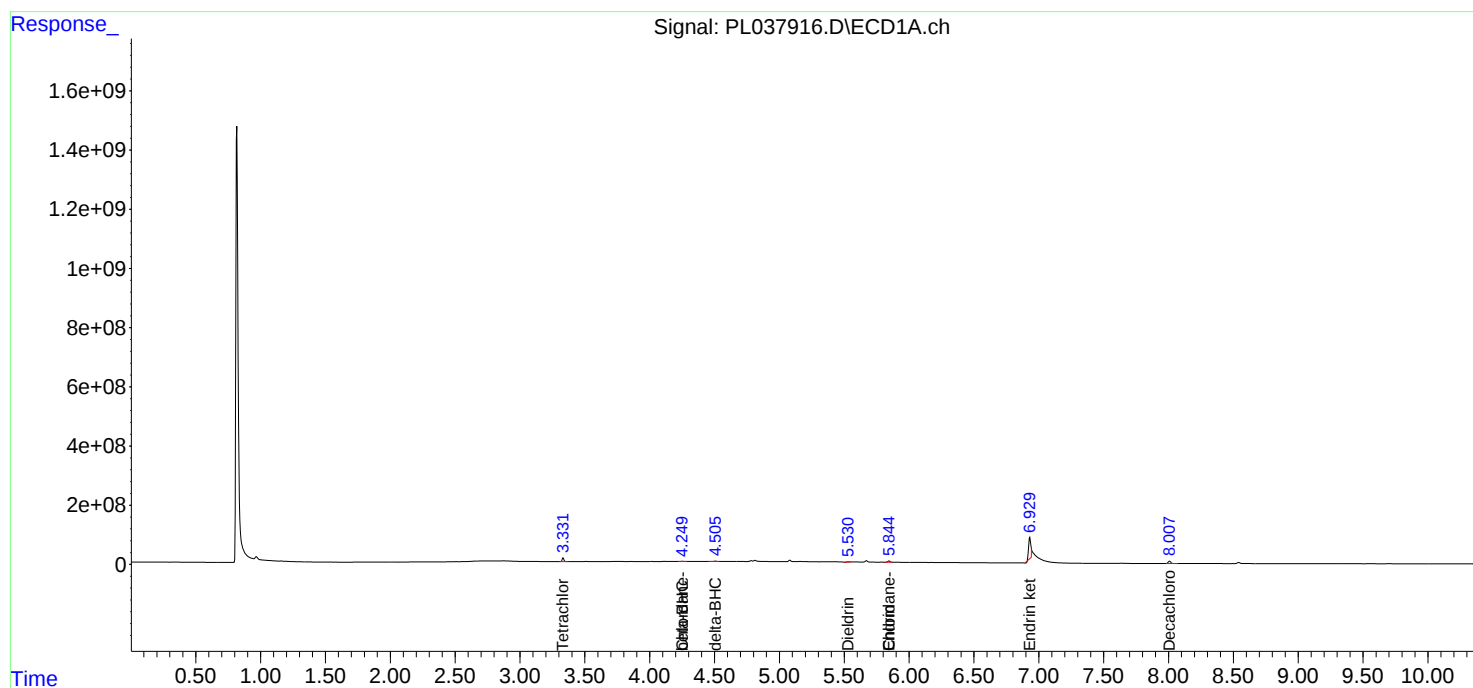


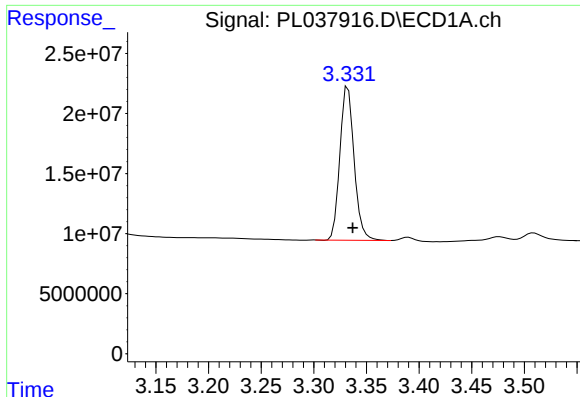

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.005 min
Response: 120870215
Conc: 15.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

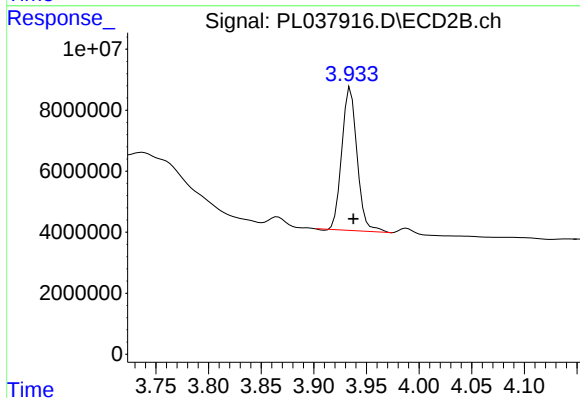


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 47676862
Conc: 17.23 ng/ml

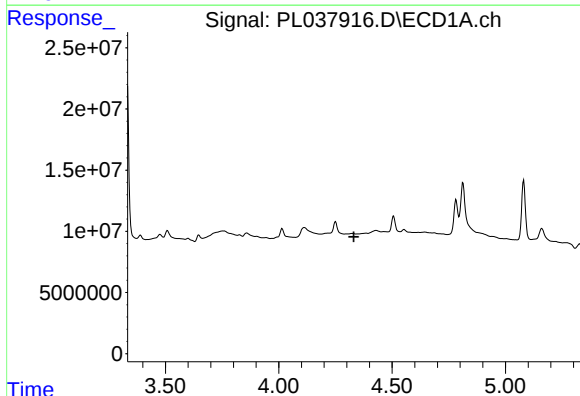


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.330 min
Response: 0
Conc: N.D.

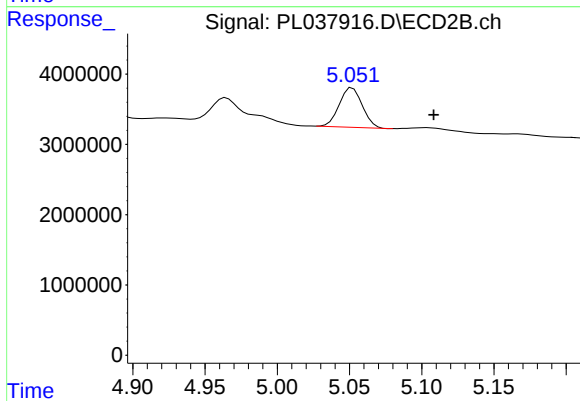

#4 Heptachlor


R.T.: 5.052 min
Delta R.T.: -0.056 min
Response: 6113247
Conc: 1.77 ng/ml

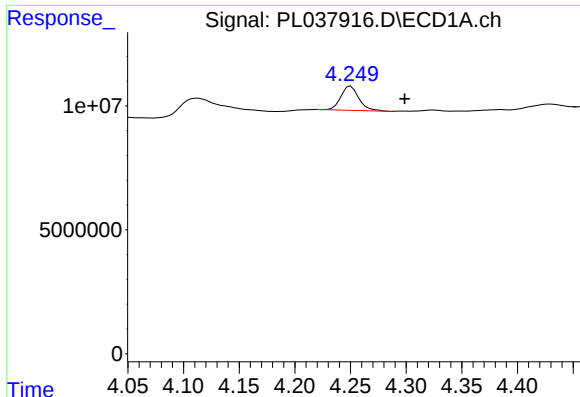

#6 beta-BHC


R.T.: 4.250 min
Delta R.T.: -0.049 min
Response: 11036814
Conc: 2.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

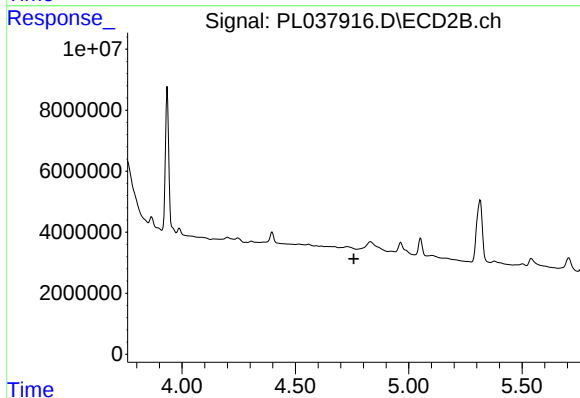


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

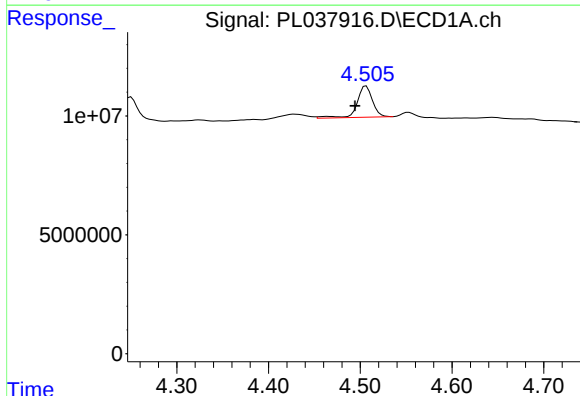


#7 delta-BHC

R.T.: 4.506 min
Delta R.T.: 0.012 min
Response: 15470220
Conc: 1.46 ng/ml

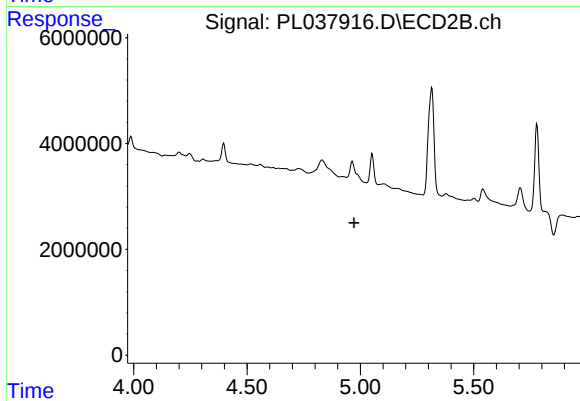

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

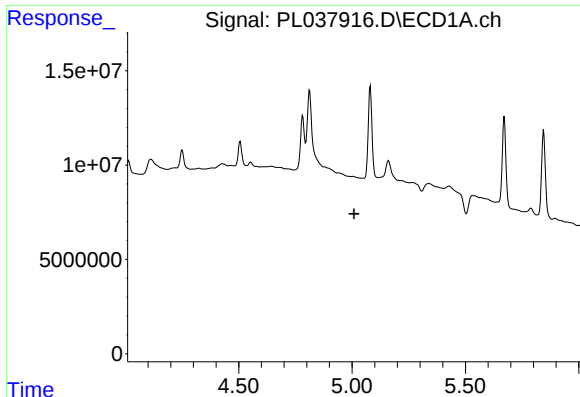

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

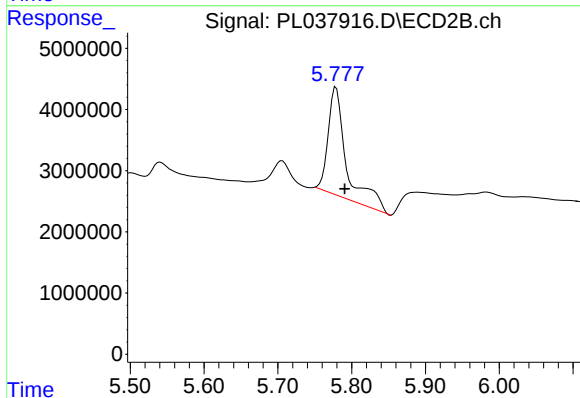


#8 Heptachlor epoxide

R.T.: 5.779 min
Delta R.T.: -0.011 min
Response: 30772243
Conc: 10.79 ng/ml

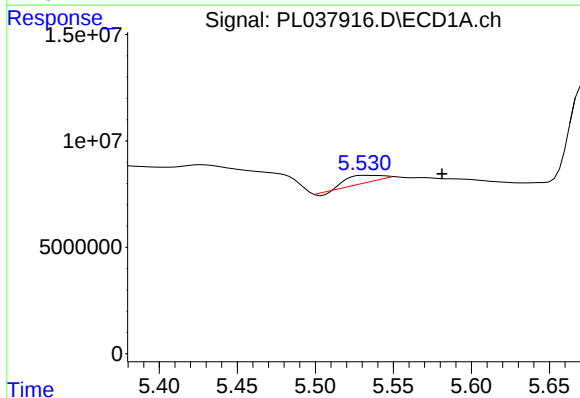


#13 Dieldrin

R.T.: 5.533 min
Delta R.T.: -0.048 min
Response: 6207460
Conc: 0.70 ng/ml

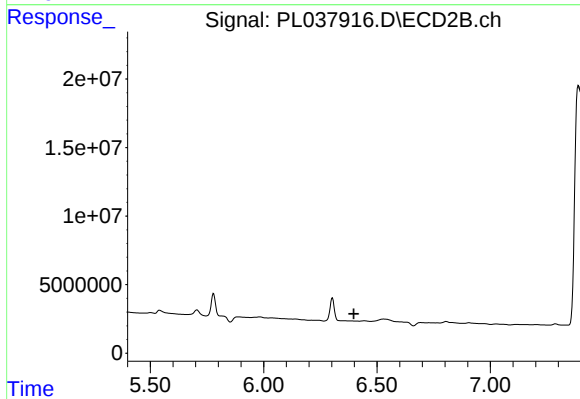

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

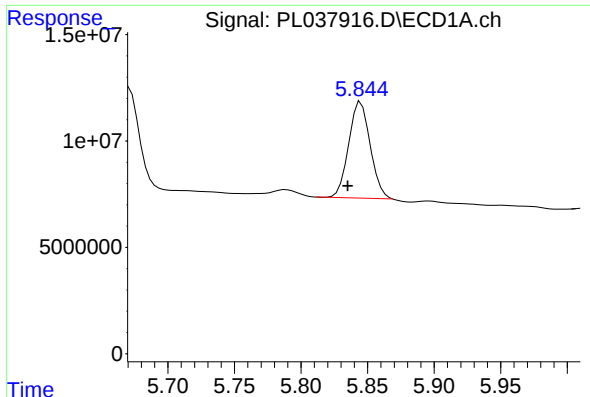

#14 Endrin


R.T.: 5.845 min
Delta R.T.: 0.010 min
Response: 50935235
Conc: 6.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

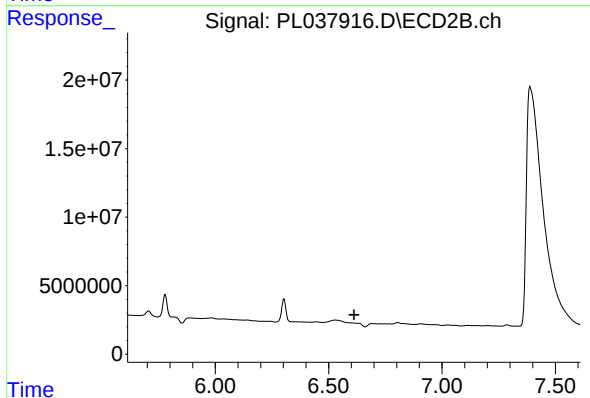


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

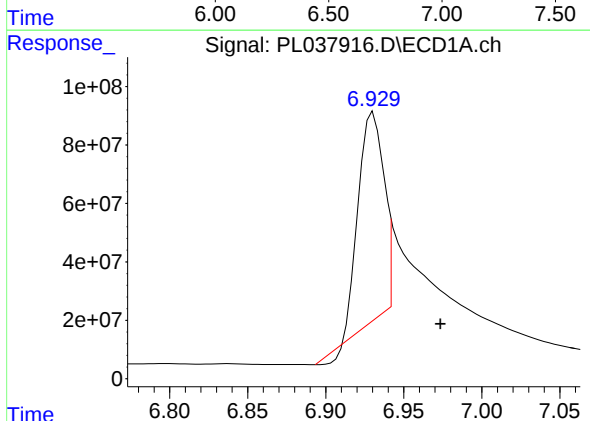


#21 Endrin ketone

R.T.: 6.931 min
Delta R.T.: -0.043 min
Response: 810333088
Conc: 113.94 ng/ml

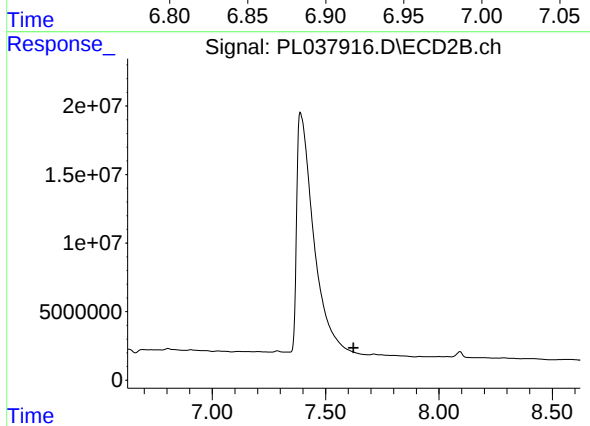

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

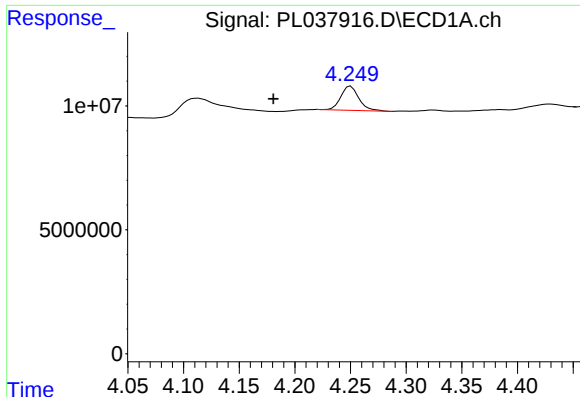

#23 Chlordane-1


R.T.: 4.250 min
Delta R.T.: 0.070 min
Response: 11036814
Conc: 35.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

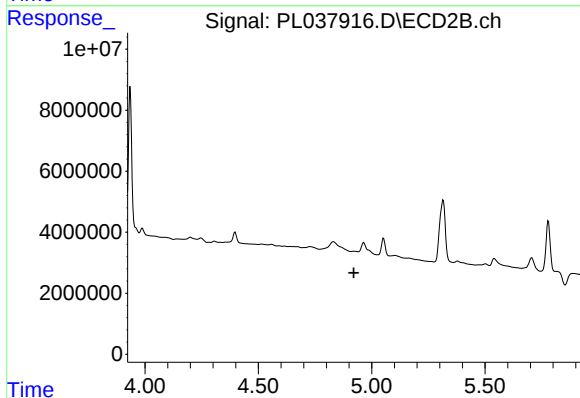


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

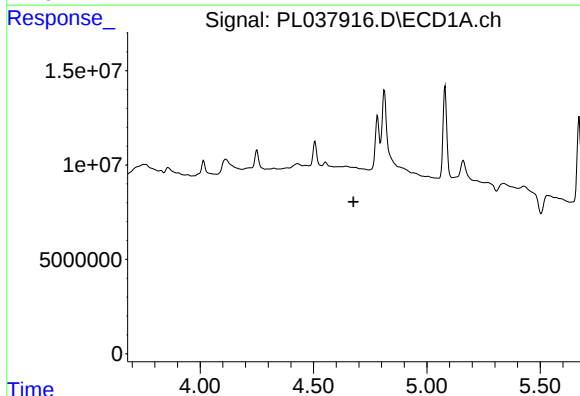


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

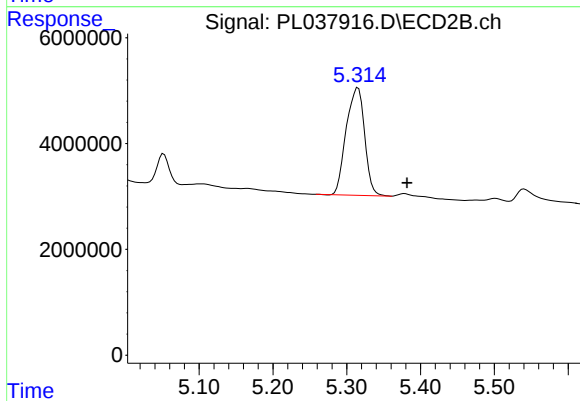

#24 Chlordane-2


R.T.: 5.315 min
Delta R.T.: -0.066 min
Response: 35261939
Conc: 278.64 ng/ml

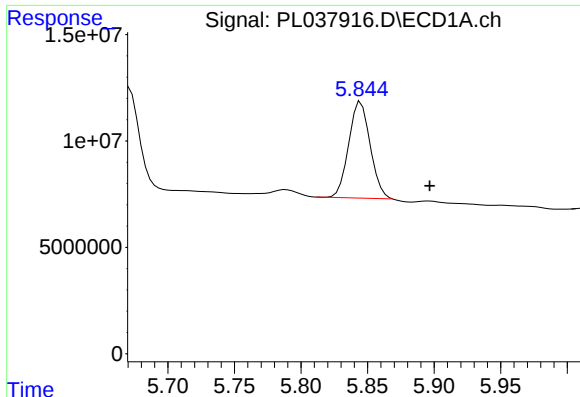

#27 Chlordane-5


R.T.: 5.845 min
Delta R.T.: -0.052 min
Response: 50935235
Conc: 389.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

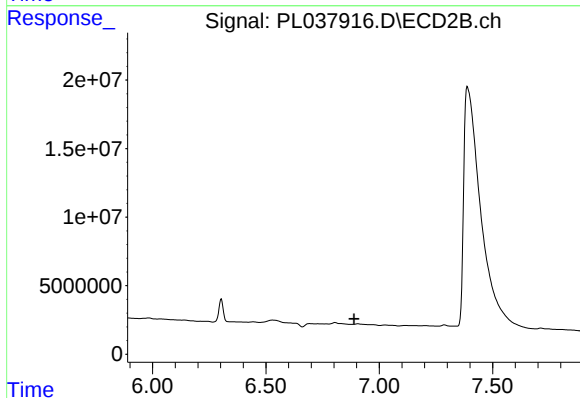


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.889 min
Response: 0
Conc: N.D.

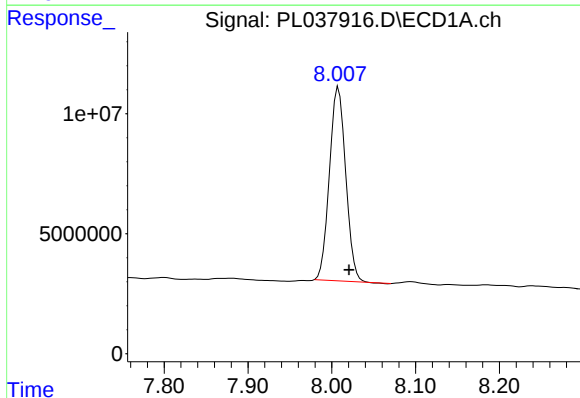

#28 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: -0.013 min
Response: 108674610
Conc: 18.01 ng/ml

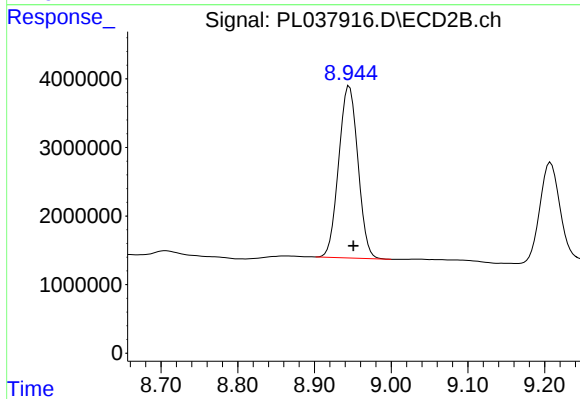

#28 Decachlorobiphenyl

R.T.: 8.945 min
Delta R.T.: -0.005 min
Response: 43791901
Conc: 22.07 ng/ml