

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071218\
 Data File : PL037921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2018 13:01
 Operator : AJ\SJ
 Sample : J3828-01 5X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:27:06 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	3.999f	0.000	20055335	0	1.944	N.D.	#
6) B	beta-BHC	4.250f	0.000	15848654	0	3.475	N.D.	#
12) B	4,4'-DDE	5.449	0.000	6673526	0	0.756	N.D.	#
23)	Chlordane-1	4.250	0.000	15848654	0	51.616	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071218\
Data File : PL037921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2018 13:01
Operator : AJ\SJ
Sample : J3828-01 5X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:27:06 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

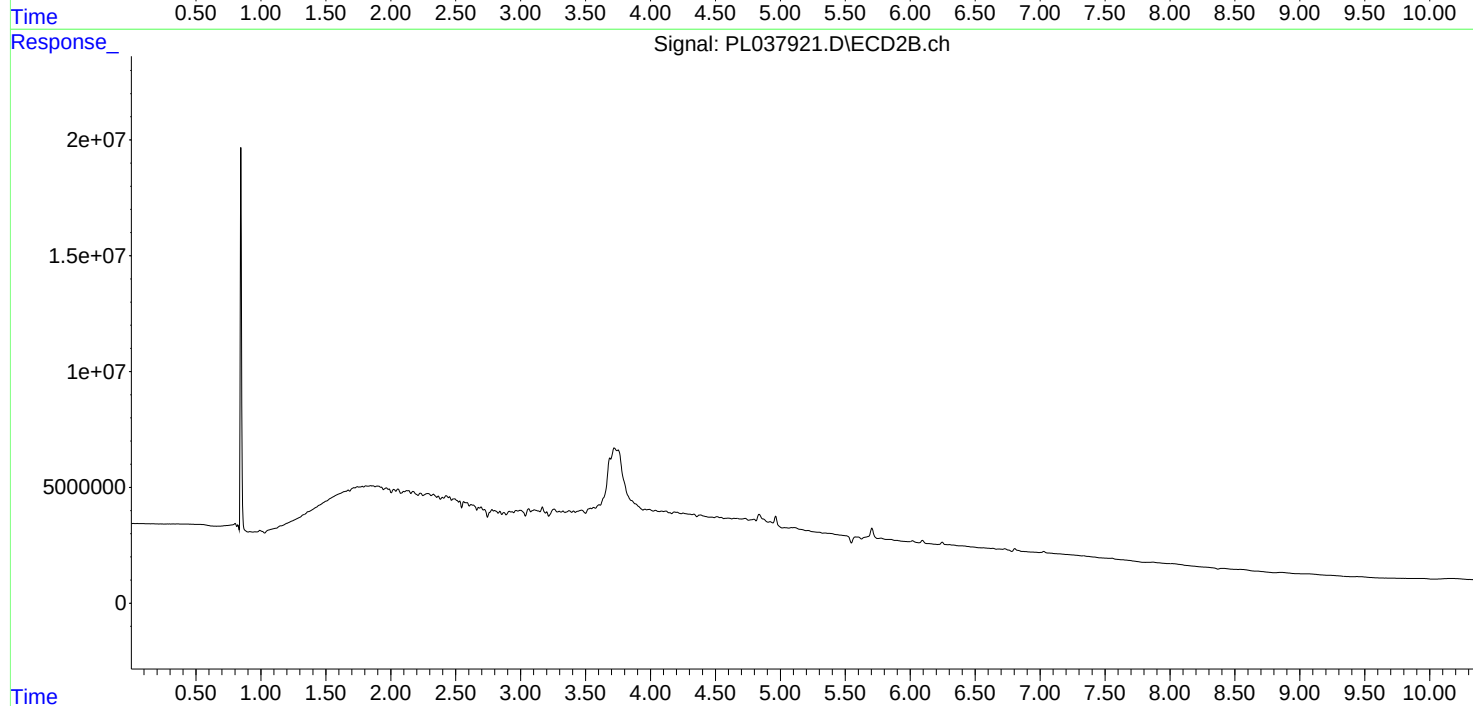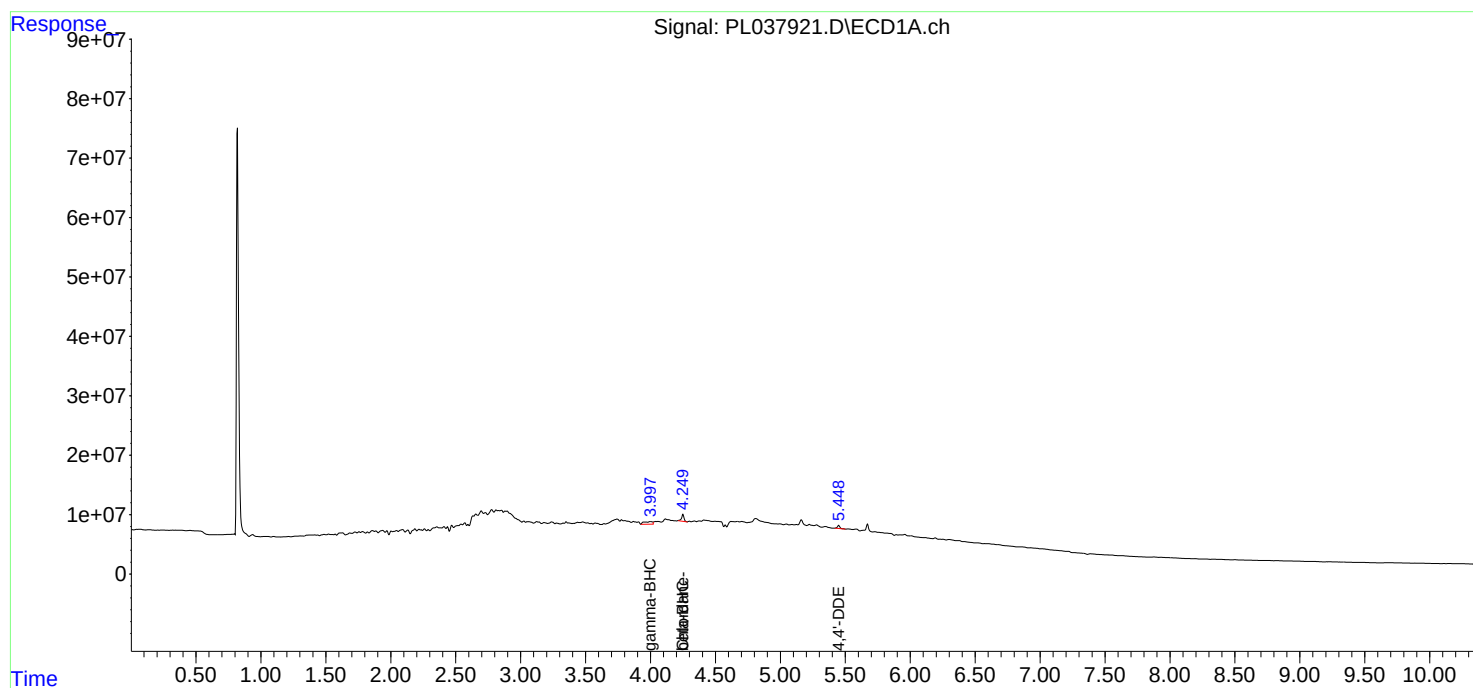


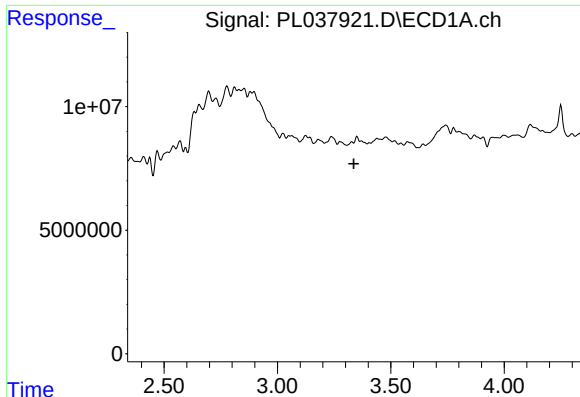

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.337 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

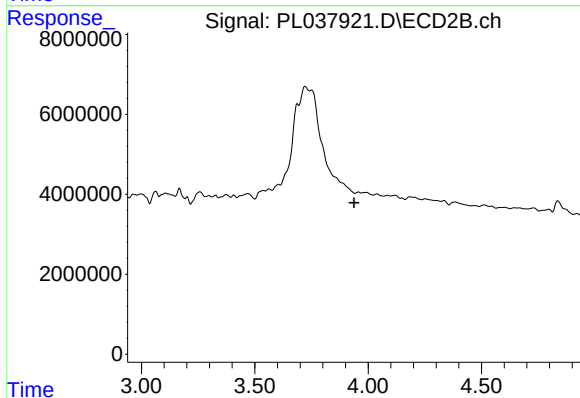


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.938 min
Response: 0
Conc: N.D.

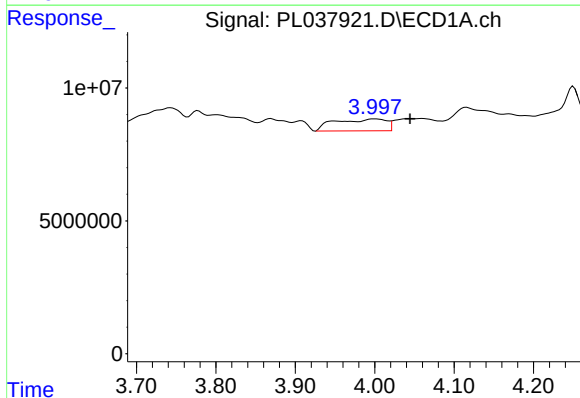


#3 gamma-BHC (Lindane)

R.T.: 3.999 min
Delta R.T.: -0.046 min
Response: 20055335
Conc: 1.94 ng/ml

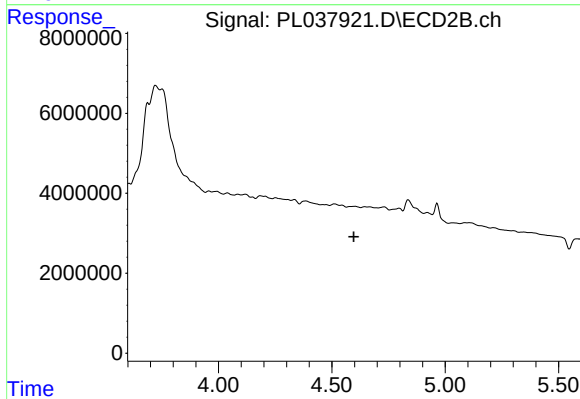

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.597 min
Response: 0
Conc: N.D.

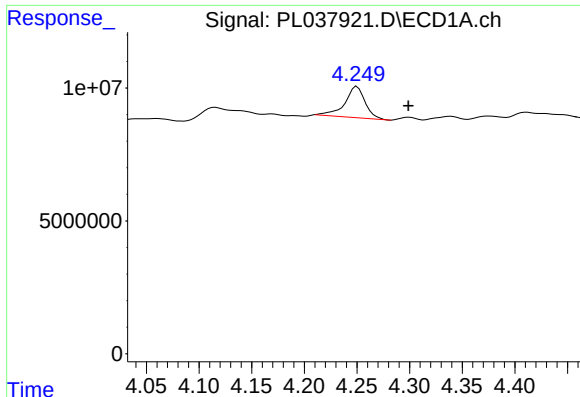

#6 beta-BHC


R.T.: 4.250 min
Delta R.T.: -0.049 min
Response: 15848654
Conc: 3.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

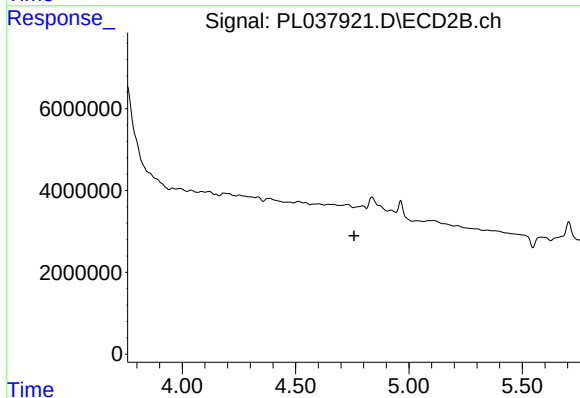


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

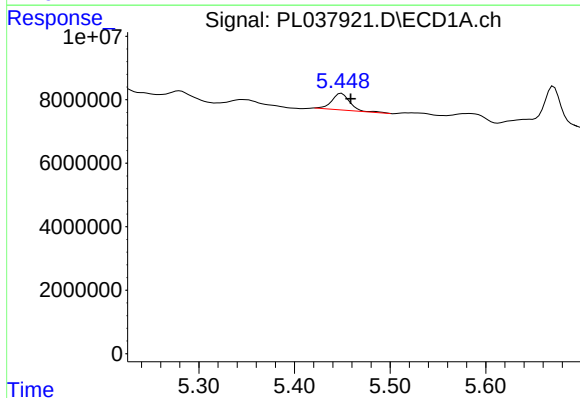


#12 4,4'-DDE

R.T.: 5.449 min
Delta R.T.: -0.010 min
Response: 6673526
Conc: 0.76 ng/ml

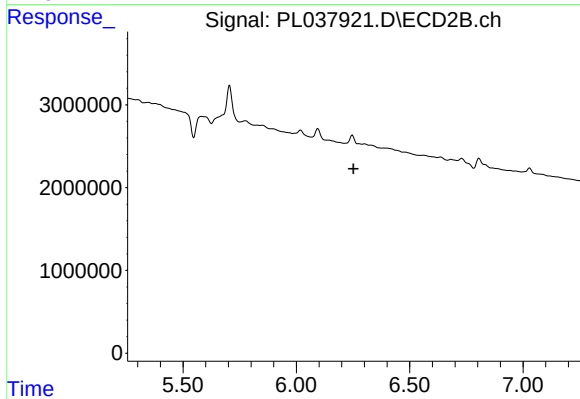

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.252 min
Response: 0
Conc: N.D.

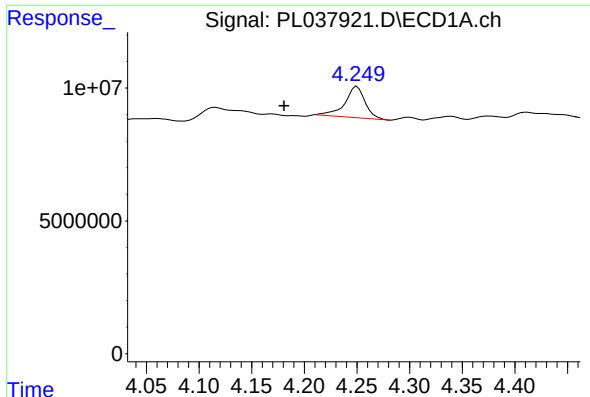

#23 Chlordane-1


R.T.: 4.250 min
Delta R.T.: 0.069 min
Response: 15848654
Conc: 51.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

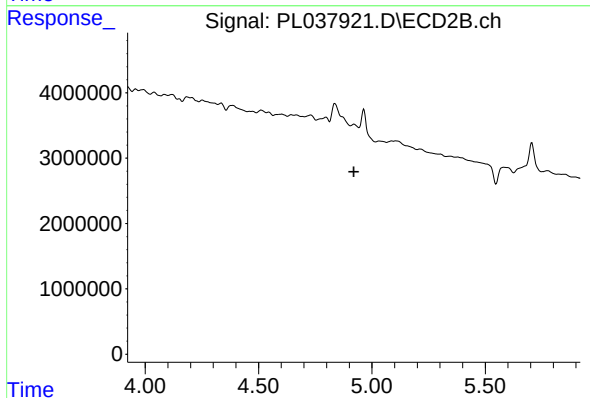


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

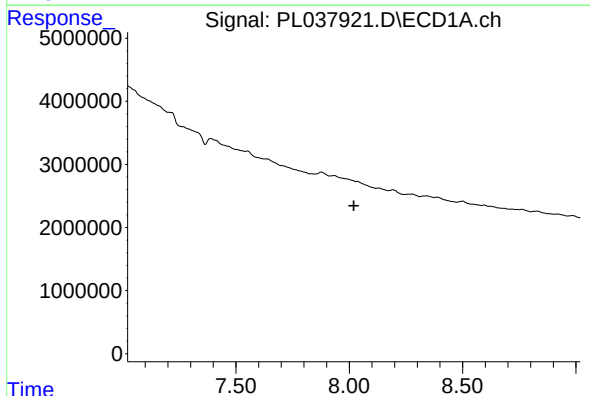

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.021 min
Response: 0
Conc: N.D.

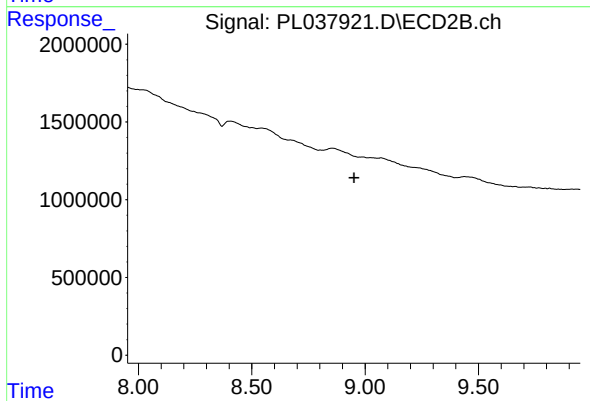

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.951 min
Response: 0
Conc: N.D.