

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
 Data File : PL050324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 10:03
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:11:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	0.000	5.792	0	25273934	N.D. 6.951 #
9) A	Endosulfan I	5.334	0.000	118.3E6	0	7.647 N.D. #
12) B	4,4'-DDE	5.455f	0.000	89789870	0	5.390 N.D. #
14) MA	Endrin	0.000	6.629	0	16047968	N.D. 5.083 #
17) MA	4,4'-DDT	6.159f	0.000	35945022	0	2.708 N.D. #
24)	Chlordane-2	4.679f	0.000	58743124	0	100.582 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
Data File : PL050324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 10:03
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:11:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

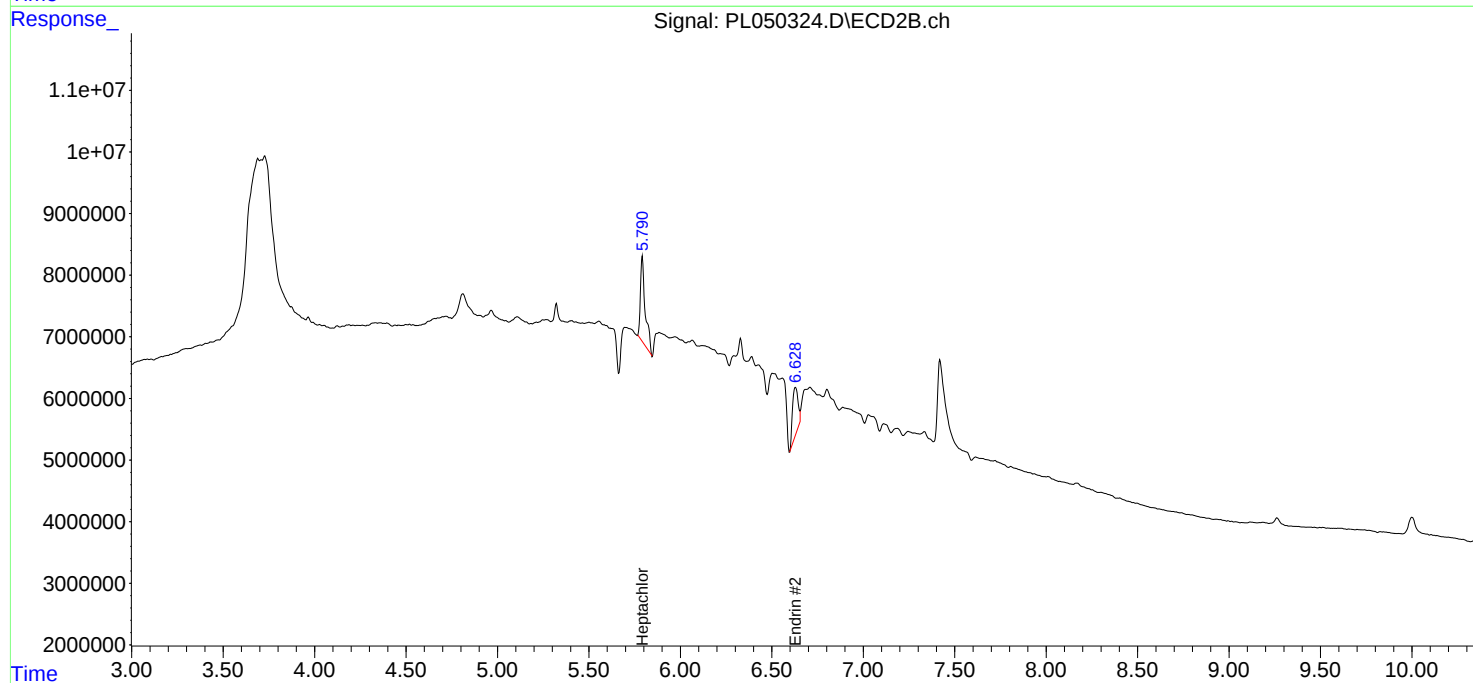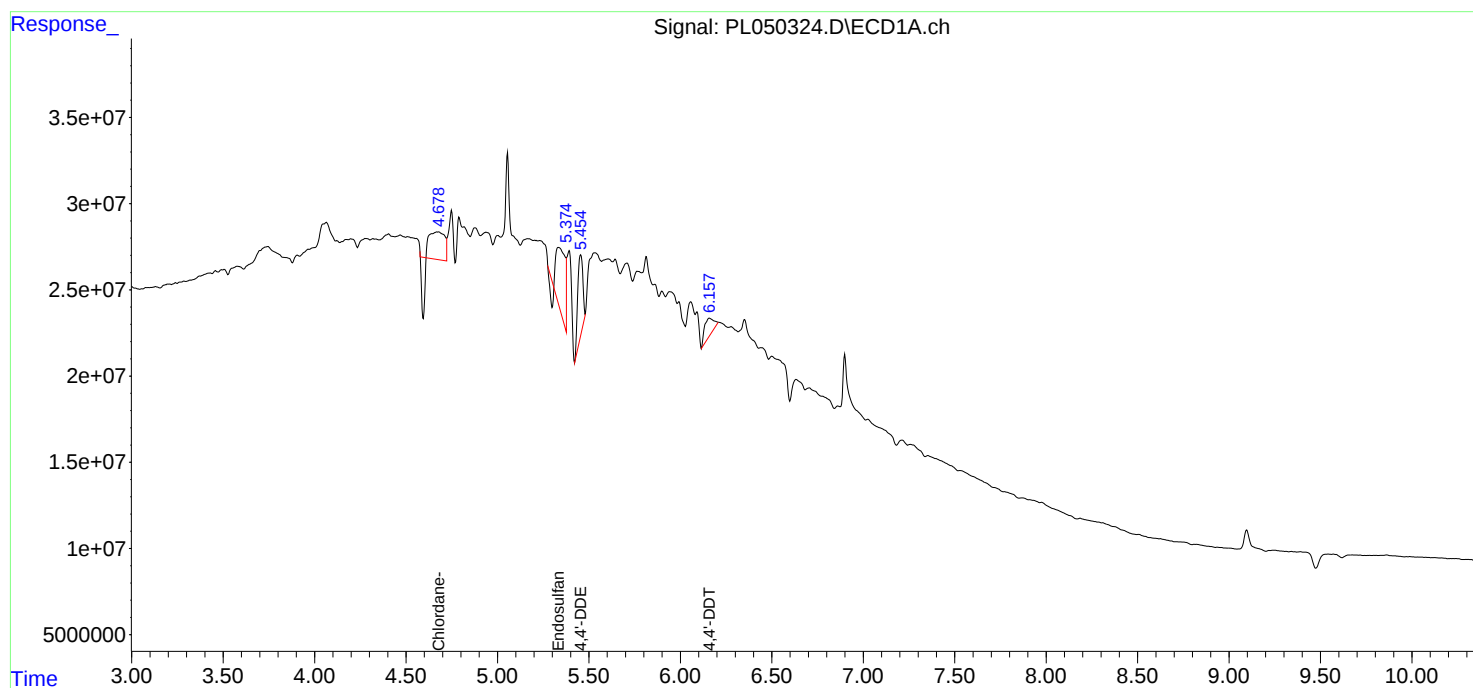


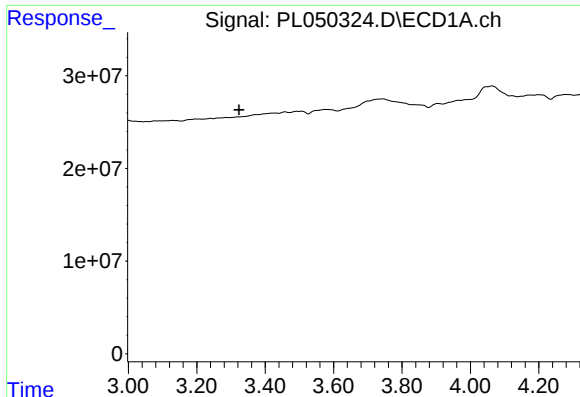

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.324 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

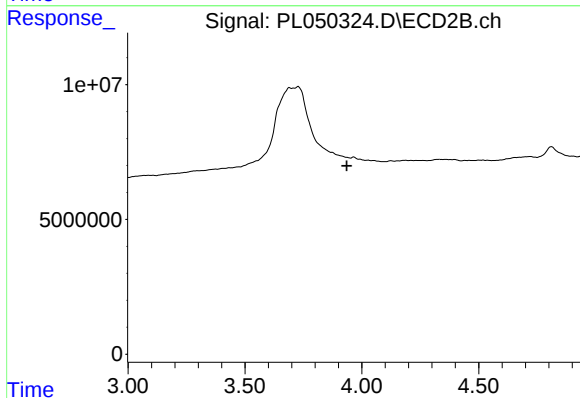


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.935 min
Response: 0
Conc: N.D.

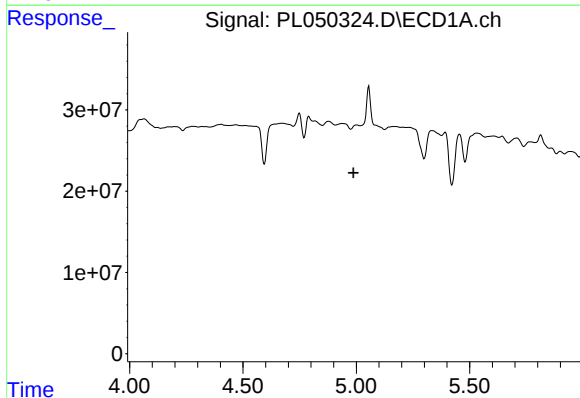


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

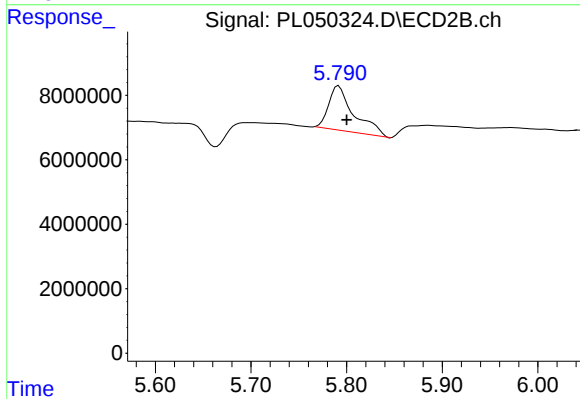

#8 Heptachlor epoxide


R.T.: 5.792 min
Delta R.T.: -0.008 min
Response: 25273934
Conc: 6.95 ng/ml

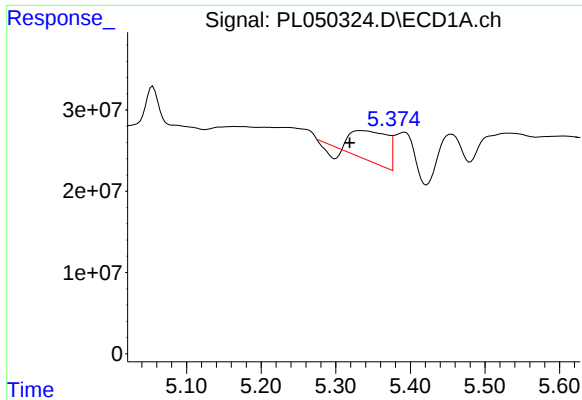

#9 Endosulfan I


R.T.: 5.334 min
Delta R.T.: 0.015 min
Response: 118312430
Conc: 7.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

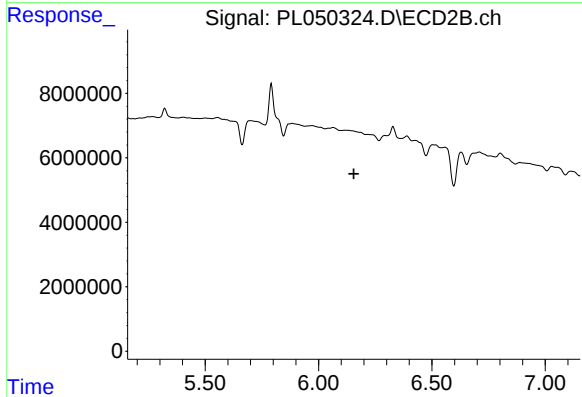


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

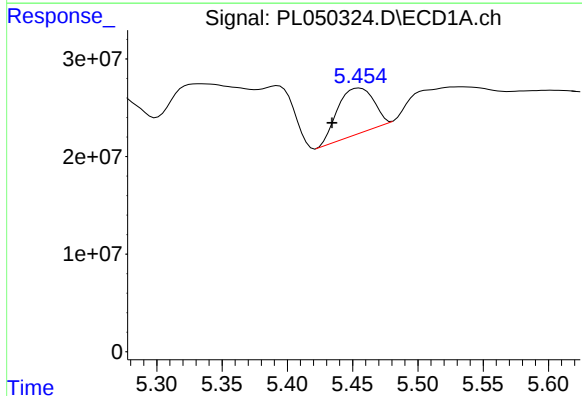


#12 4,4'-DDE

R.T.: 5.455 min
Delta R.T.: 0.021 min
Response: 89789870
Conc: 5.39 ng/ml

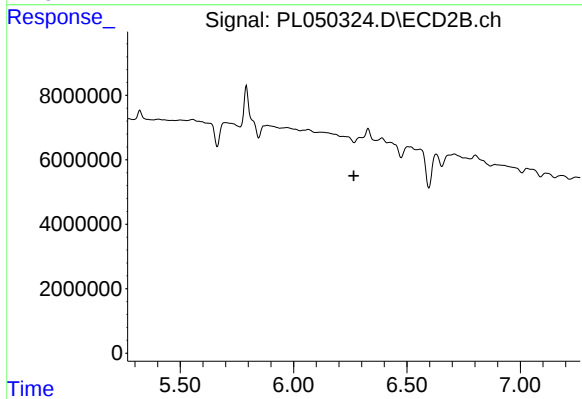

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

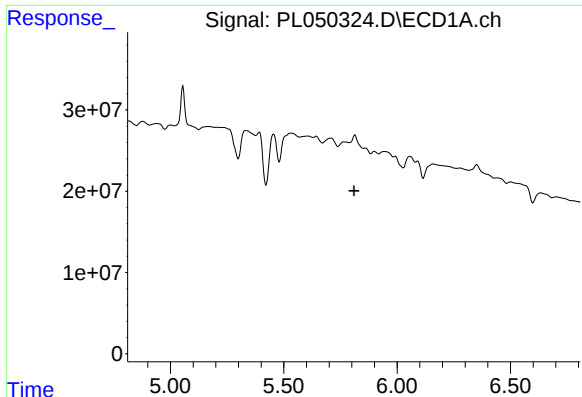

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.811 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

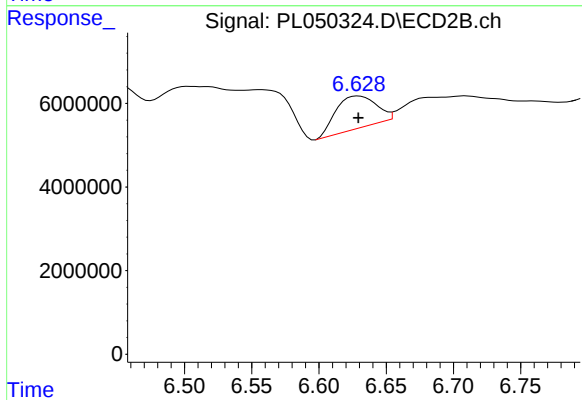


#14 Endrin

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 16047968
Conc: 5.08 ng/ml

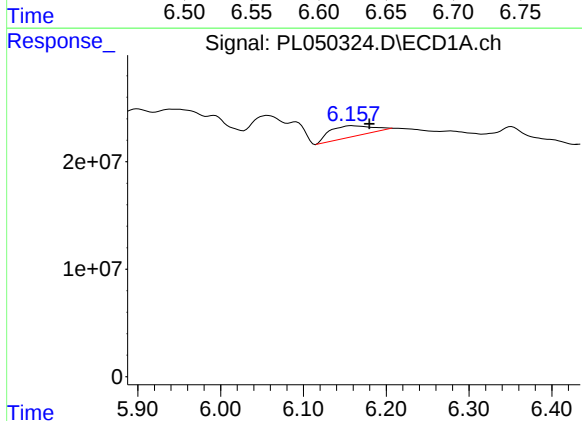


#17 4,4'-DDT

R.T.: 6.159 min
Delta R.T.: -0.021 min
Response: 35945022
Conc: 2.71 ng/ml

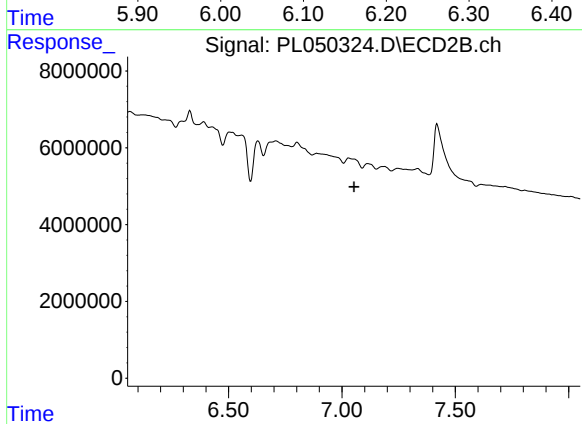

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.054 min
Response: 0
Conc: N.D.

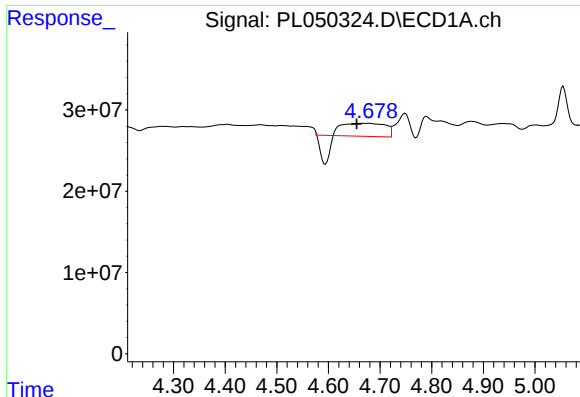

#24 Chlordane-2


R.T.: 4.679 min
Delta R.T.: 0.024 min
Response: 58743124
Conc: 100.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

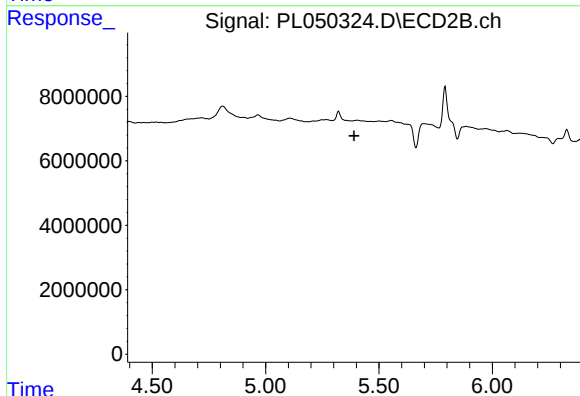


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.390 min
Response: 0
Conc: N.D.

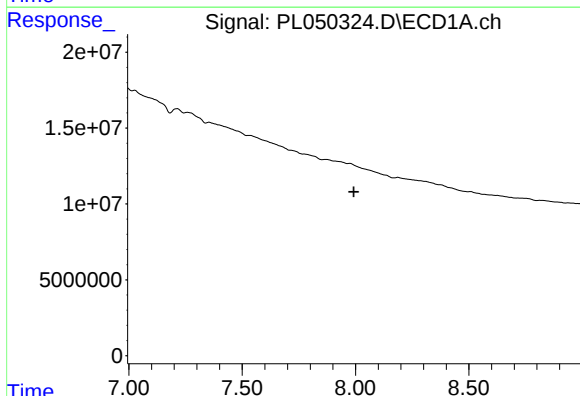

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

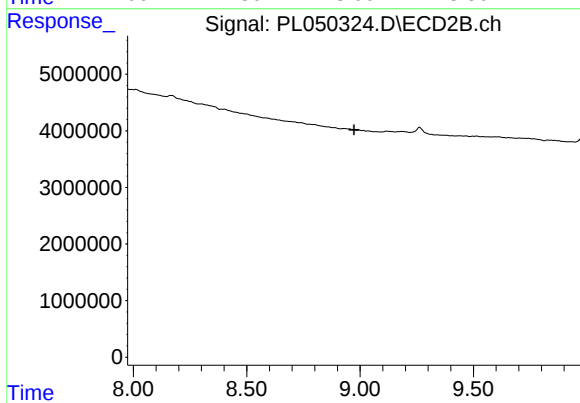

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.973 min
Response: 0
Conc: N.D.