

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
 Data File : PL050372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2019 01:59
 Operator : SM\AJ
 Sample : K3740-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 03:28:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.319	3.931	197.8E6	60650880	17.538	19.809
28) SA Decachlor...	7.981	8.962	154.3E6	44270270	12.147	13.187
Target Compounds						
4) MA Heptachlor	4.299	0.000	62068247	0	3.415	N.D. #
6) B beta-BHC	4.299f	0.000	62068247	0	8.485	N.D. #
7) B delta-BHC	0.000	4.975f	0	7928218	N.D.	2.013 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
Data File : PL050372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2019 01:59
Operator : SM\AJ
Sample : K3740-08
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-23

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 03:28:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

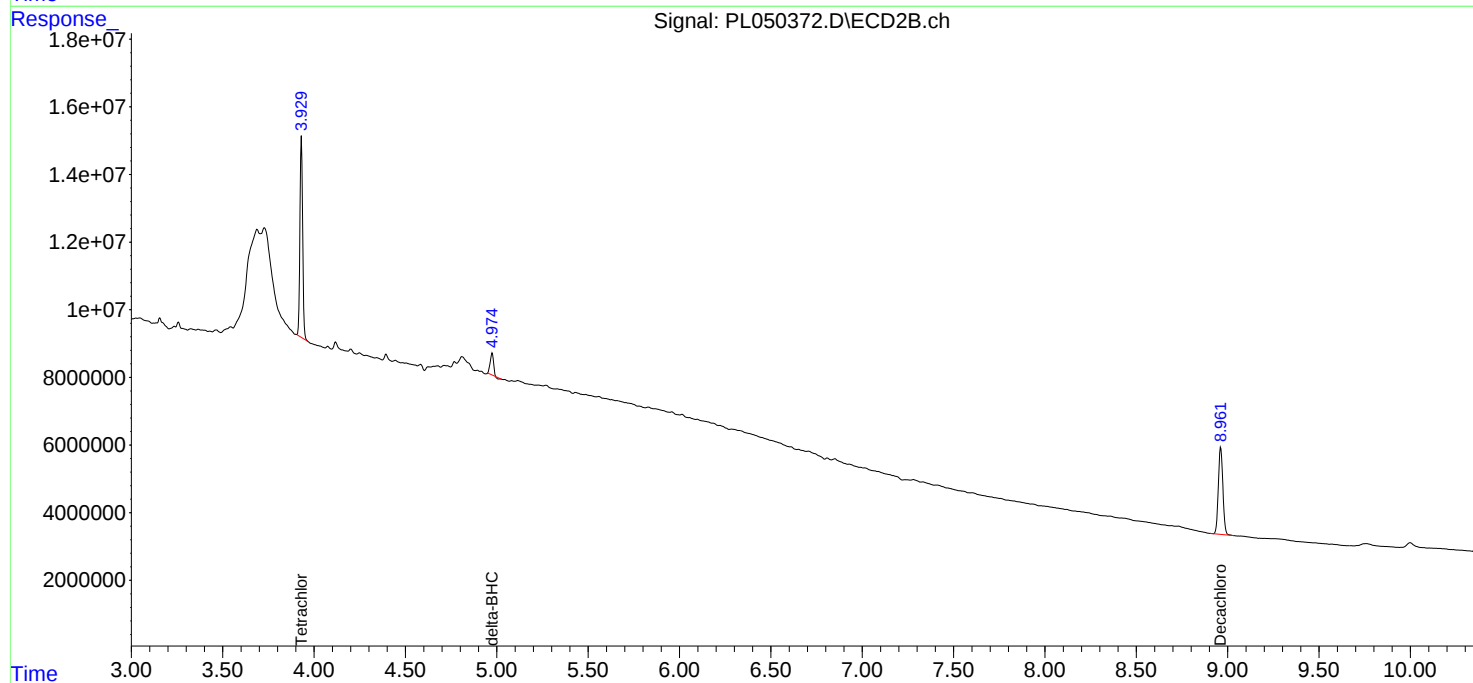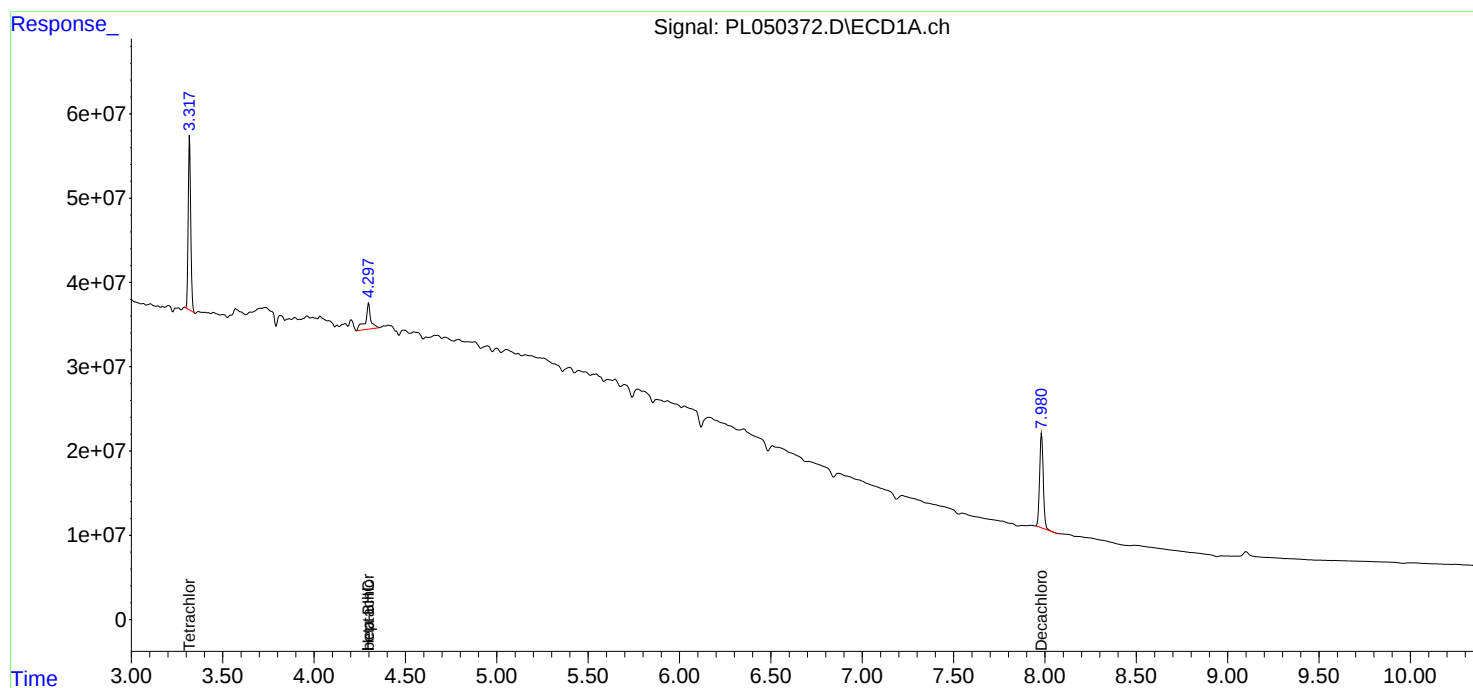


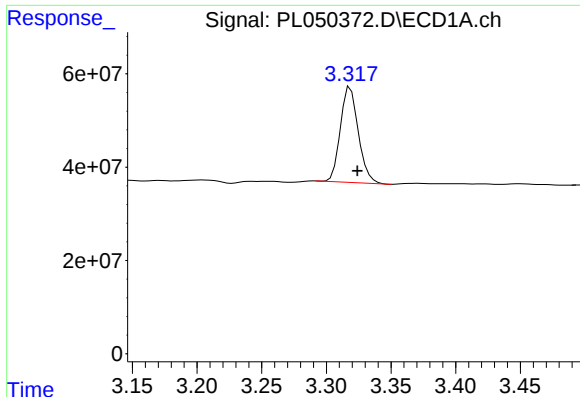

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: -0.005 min
Response: 197782652
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-23

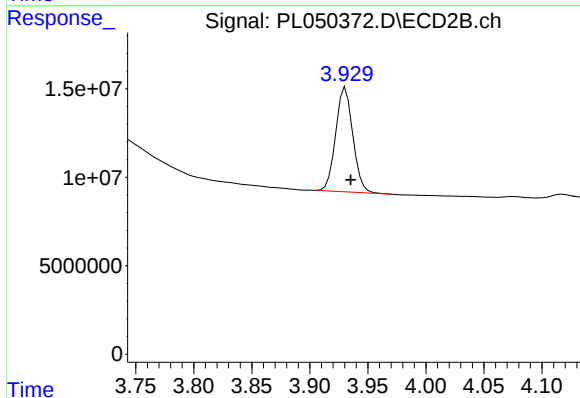


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.004 min
Response: 60650880
Conc: 19.81 ng/ml

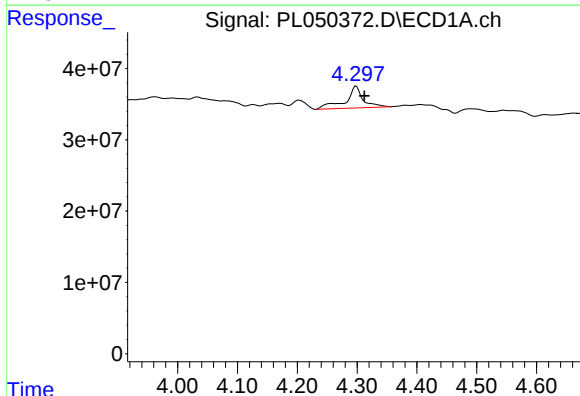


#4 Heptachlor

R.T.: 4.299 min
Delta R.T.: -0.014 min
Response: 62068247
Conc: 3.41 ng/ml

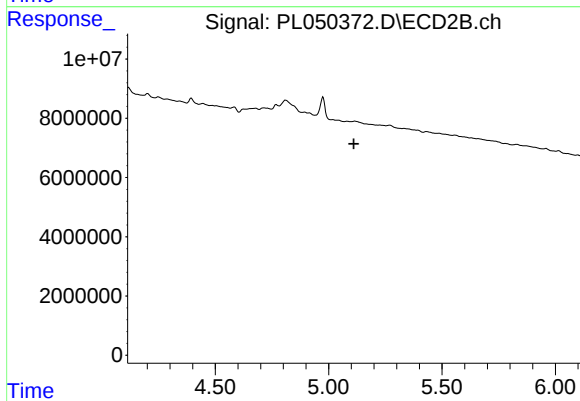

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.110 min
Response: 0
Conc: N.D.

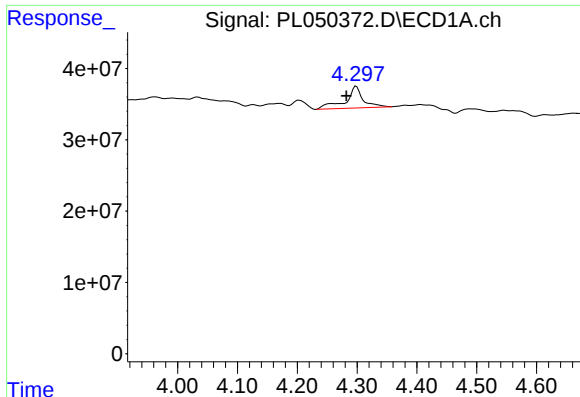

#6 beta-BHC


R.T.: 4.299 min
Delta R.T.: 0.016 min
Response: 62068247
Conc: 8.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-23

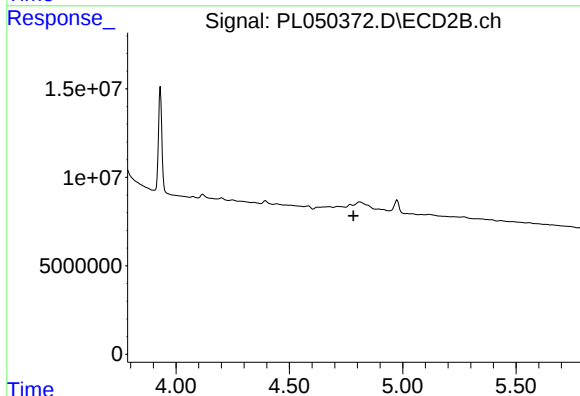


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.783 min
Response: 0
Conc: N.D.

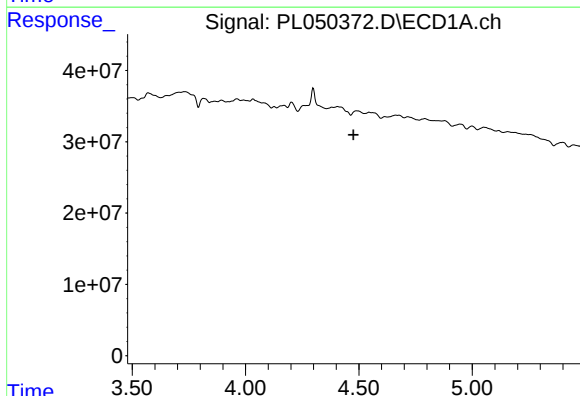


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.476 min
Response: 0
Conc: N.D.

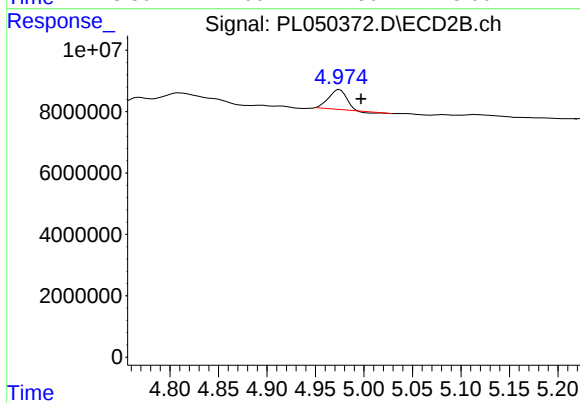

#7 delta-BHC


R.T.: 4.975 min
Delta R.T.: -0.022 min
Response: 7928218
Conc: 2.01 ng/ml

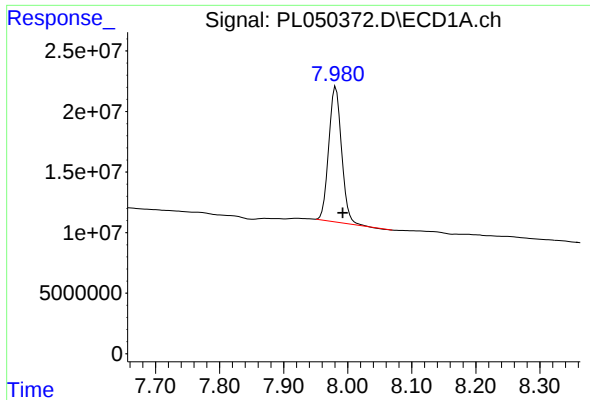

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.011 min
Response: 154346203
Conc: 12.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-23

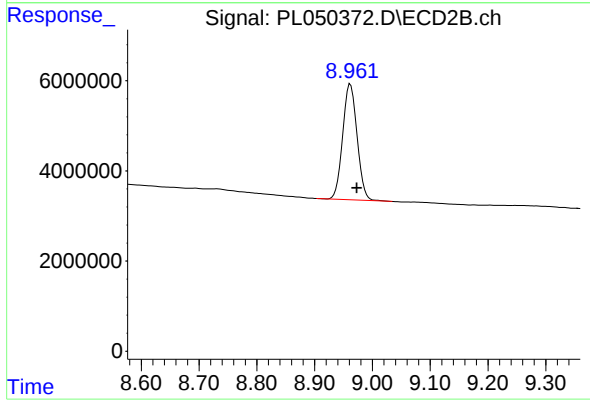

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: -0.011 min
Response: 44270270
Conc: 13.19 ng/ml