

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
 Data File : PL050347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 16:49
 Operator : SM\AJ
 Sample : K3618-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-071119

Manual Integrations
 APPROVED

Ankita
 7/16/2019 10:11:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:17:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.930	115.4E6	23531256	10.232m	7.686m
28)	SA Decachlor...	7.983	8.965	110.4E6	33627670	8.685m	10.017m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
Data File : PL050347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 16:49
Operator : SM\AJ
Sample : K3618-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HD-02-071119


Manual Integrations
APPROVED

Ankita
7/16/2019 10:11:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:17:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

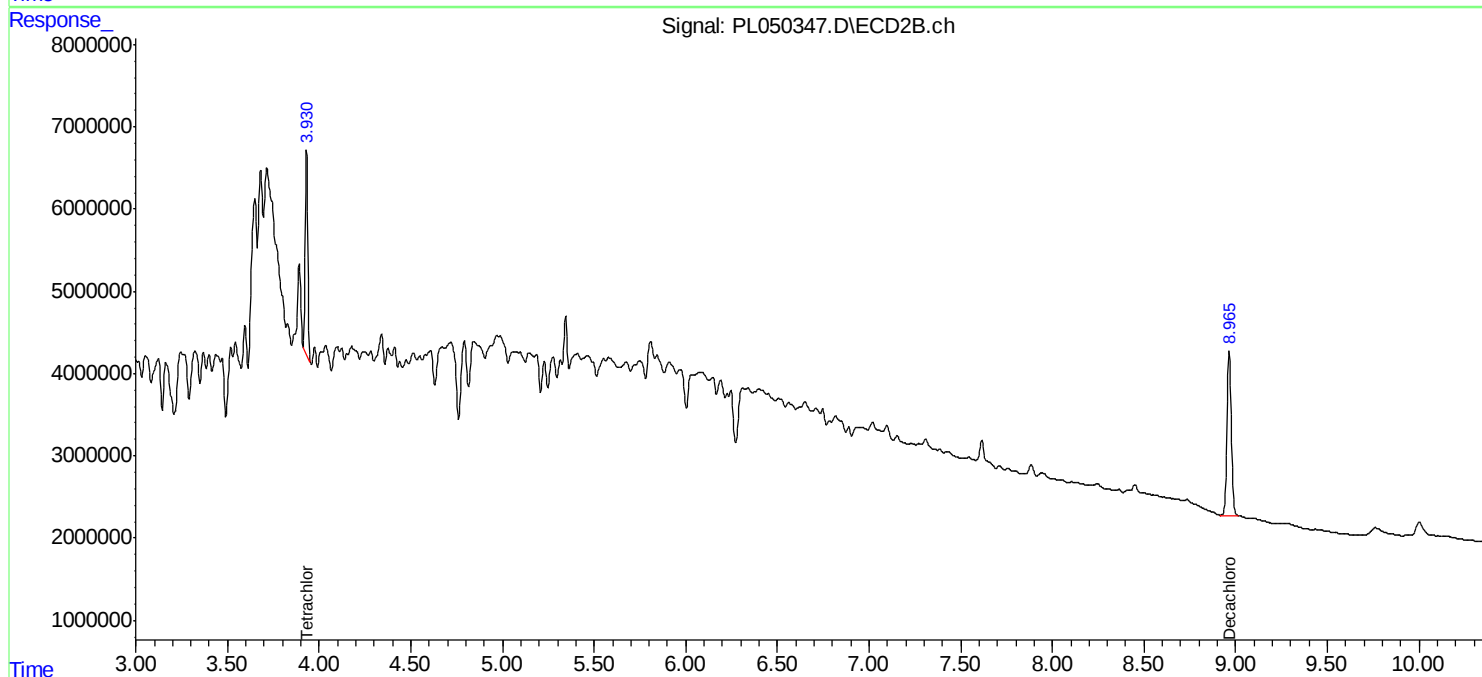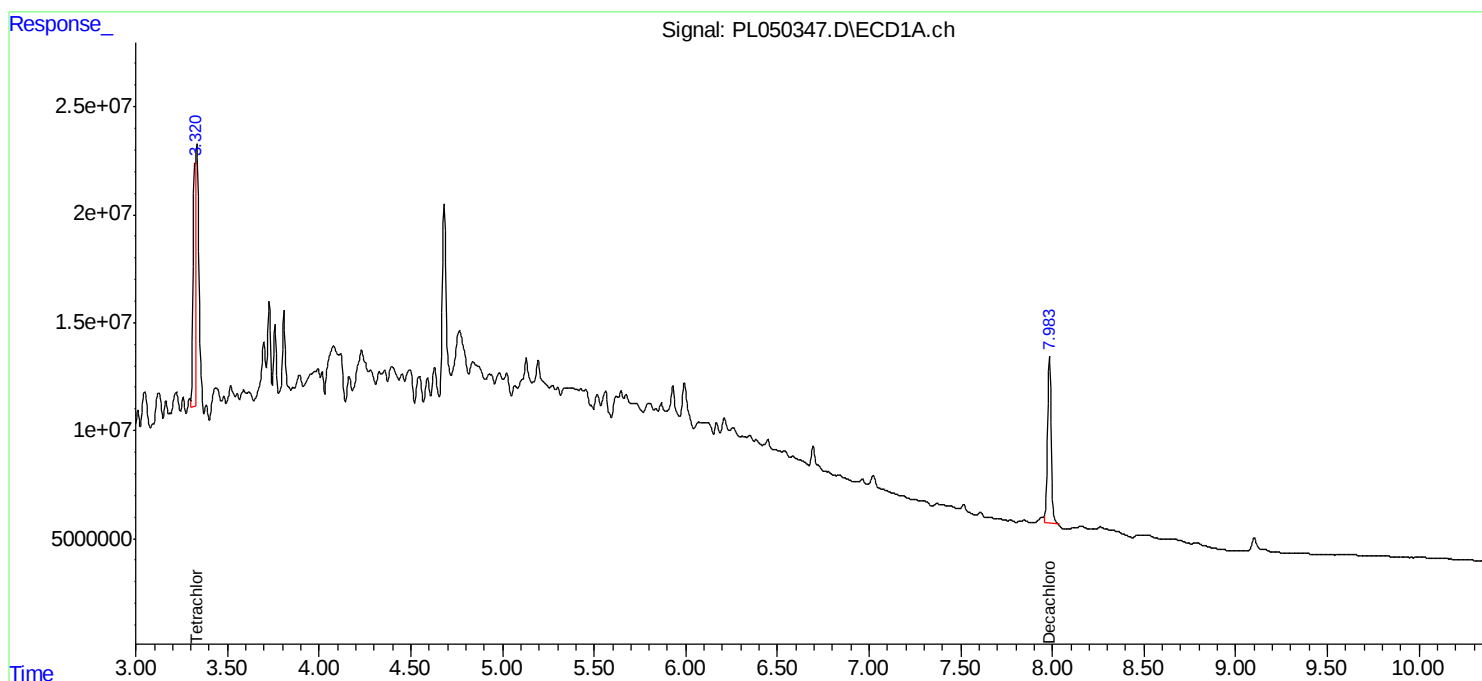

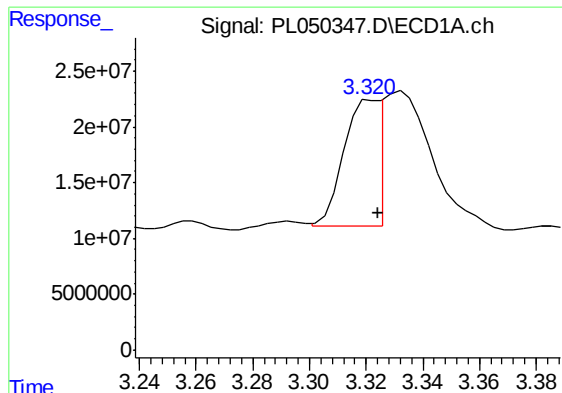


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 115390045
Conc: 10.23 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HD-02-071119


Manual Integrations
APPROVED

Ankita
7/16/2019 10:11:03 AM

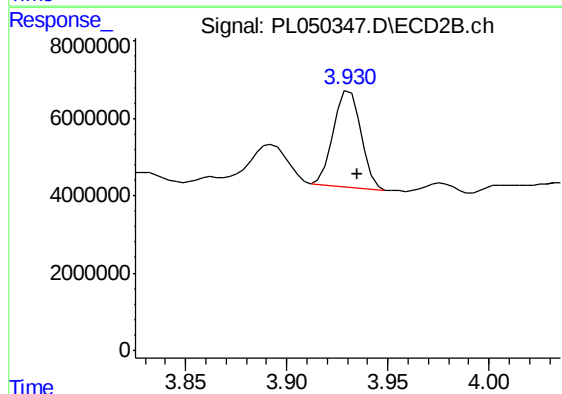


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: -0.006 min
Response: 23531256
Conc: 7.69 ng/ml m

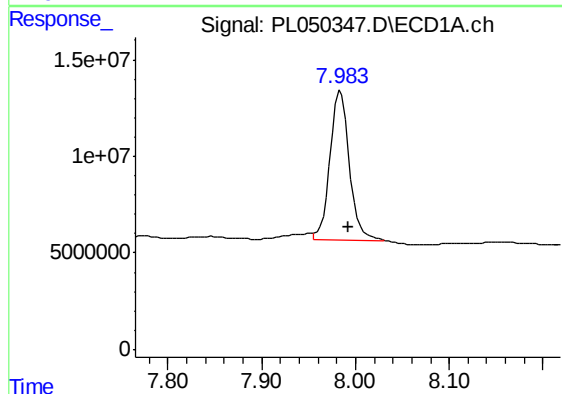

#28 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.010 min
Response: 110355651
Conc: 8.69 ng/ml m

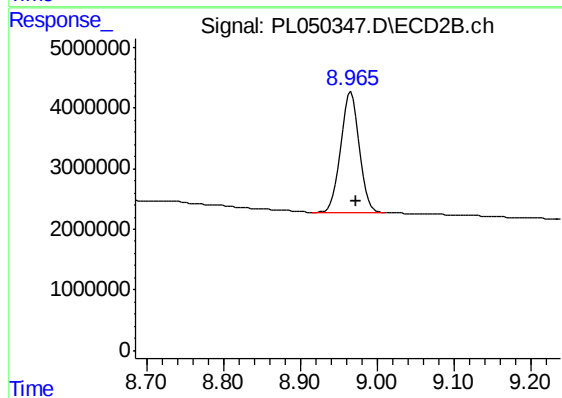

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 33627670
Conc: 10.02 ng/ml m