

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
 Data File : PL050363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2019 20:59
 Operator : SM\AJ
 Sample : K3621-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-071019-A

Manual Integrations
 APPROVED

Ankita
 7/16/2019 10:14:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 23:22:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.931	180.3E6	56624676	15.984	18.494
28)	SA Decachlor...	7.981	8.965	178.6E6	51861009	14.056m	15.448

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
Data File : PL050363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2019 20:59
Operator : SM\AJ
Sample : K3621-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-03-071019-A


Manual Integrations
APPROVED

Ankita
7/16/2019 10:14:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 23:22:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

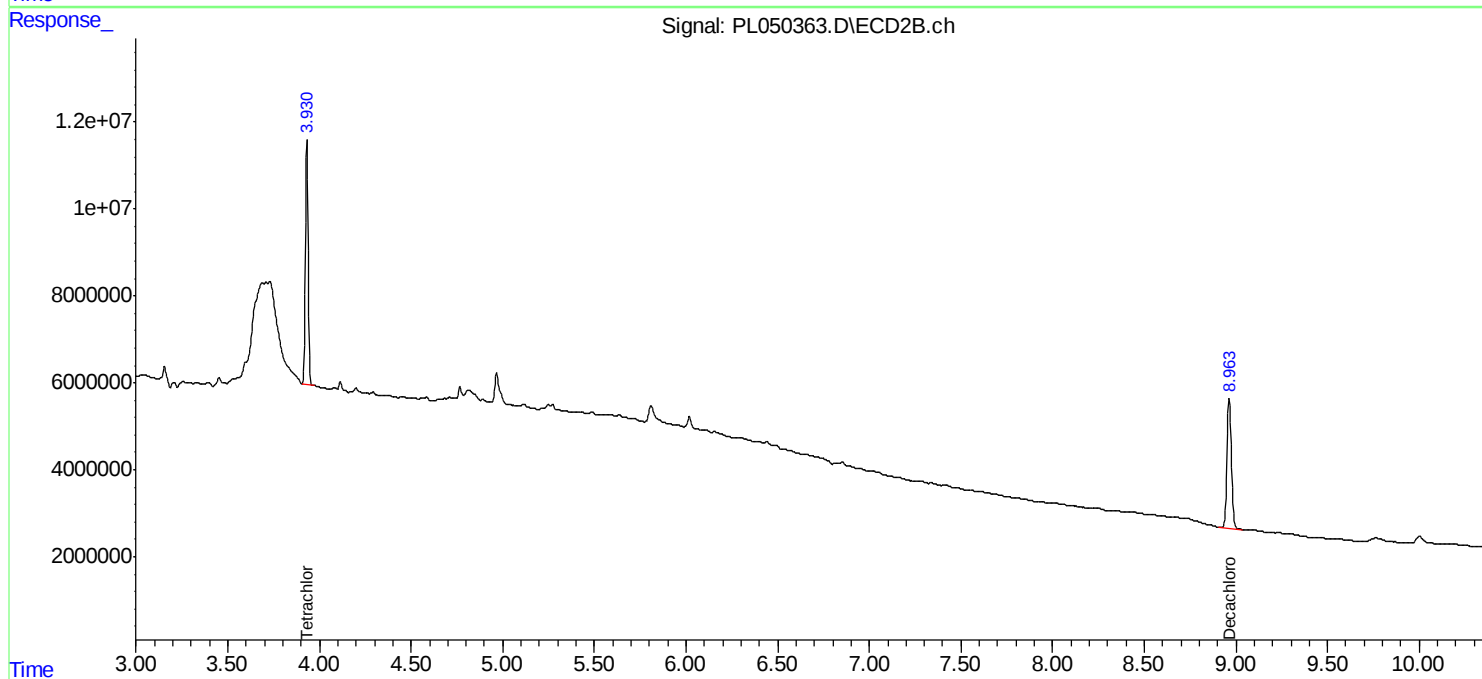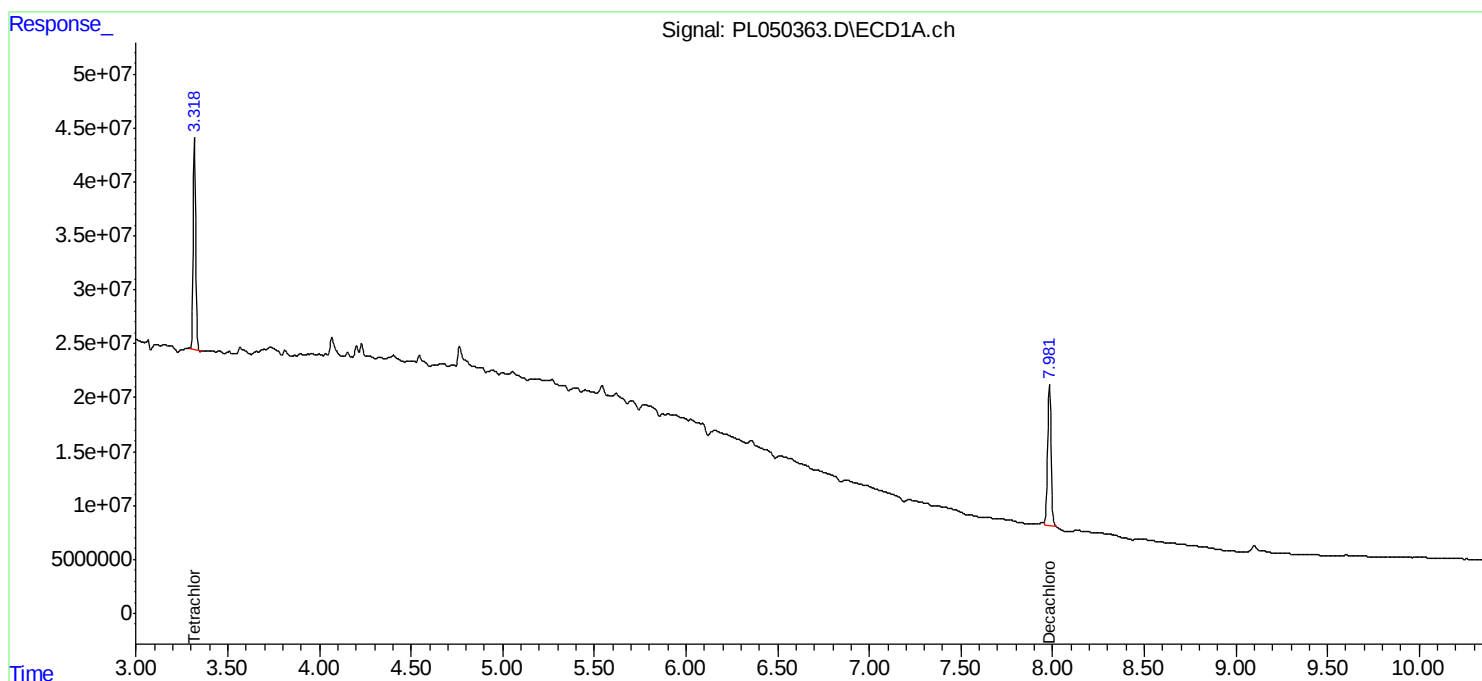

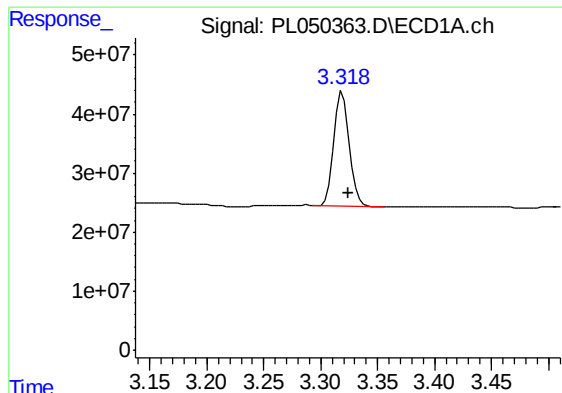


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.005 min
Response: 180259476
Conc: 15.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-03-071019-A


Manual Integrations
APPROVED

Ankita
7/16/2019 10:14:04 AM

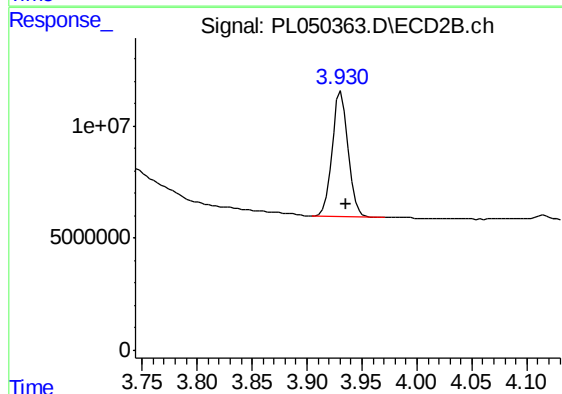


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.004 min
Response: 56624676
Conc: 18.49 ng/ml

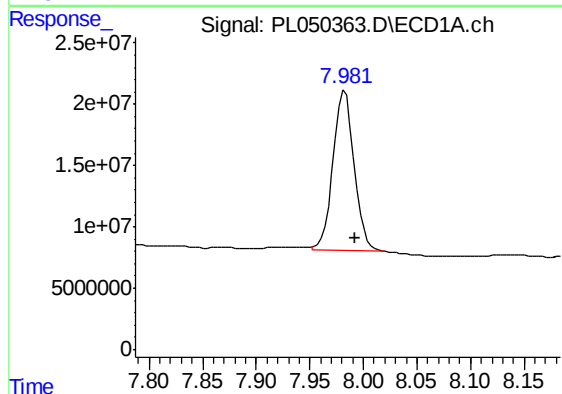

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.011 min
Response: 178595199
Conc: 14.06 ng/ml m

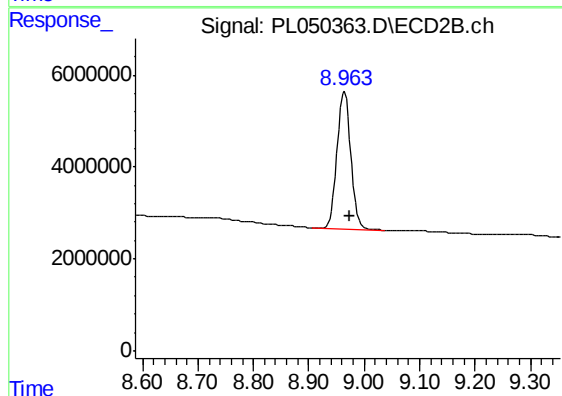

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 51861009
Conc: 15.45 ng/ml