

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
 Data File : PL050371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2019 01:45
 Operator : SM\AJ
 Sample : K3740-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-22

Manual Integrations
 APPROVED

Ankita
 7/16/2019 10:14:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 03:27:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.931	199.8E6	59431975	17.718	19.411
28)	SA Decachlor...	7.980	8.962	186.0E6	54057375	14.641m	16.103

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071219\
Data File : PL050371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2019 01:45
Operator : SM\AJ
Sample : K3740-07
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-22


Manual Integrations
APPROVED

Ankita
7/16/2019 10:14:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 03:27:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

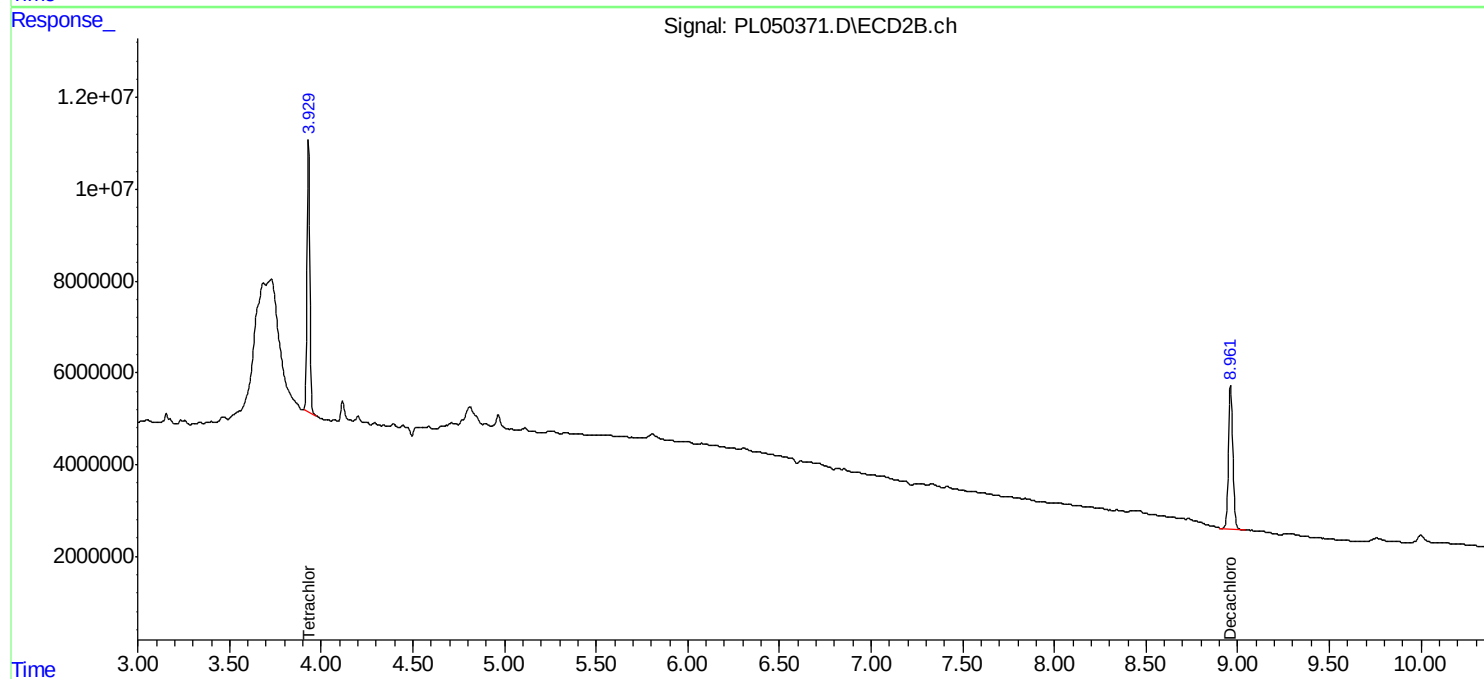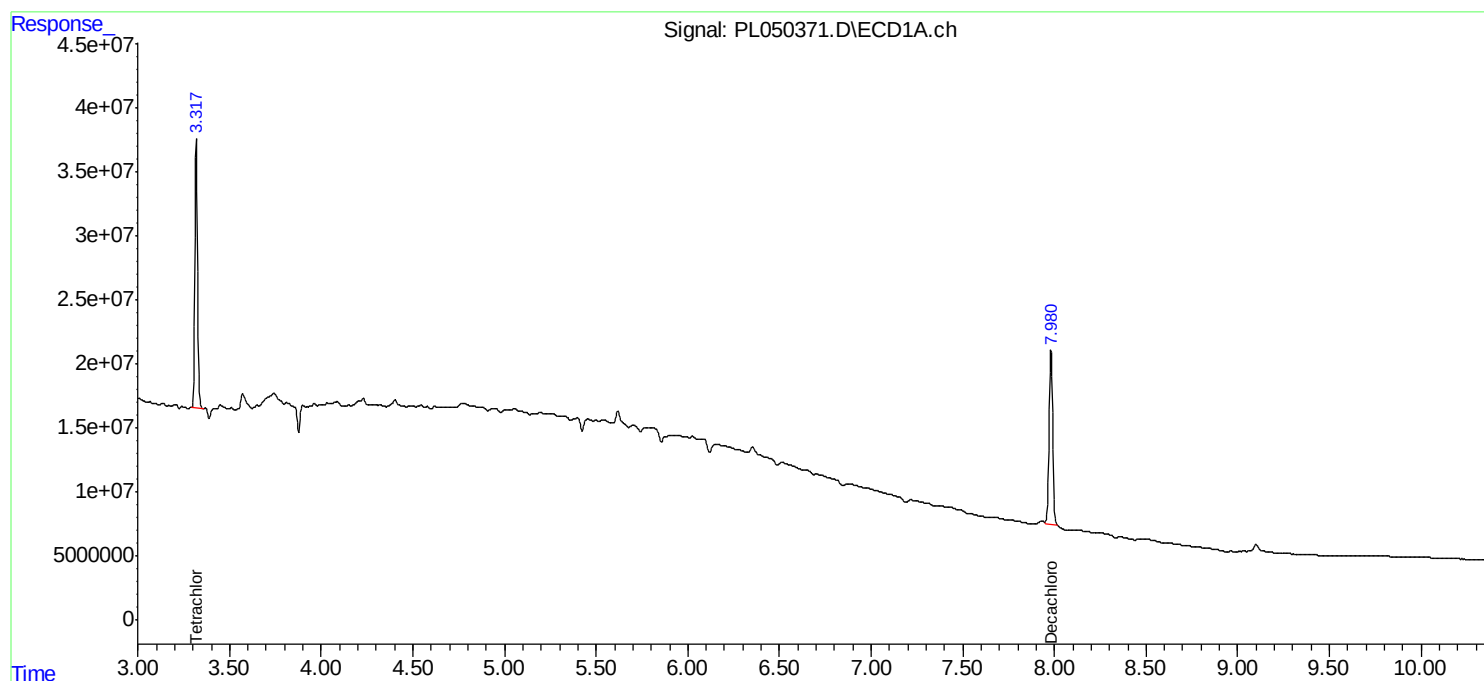

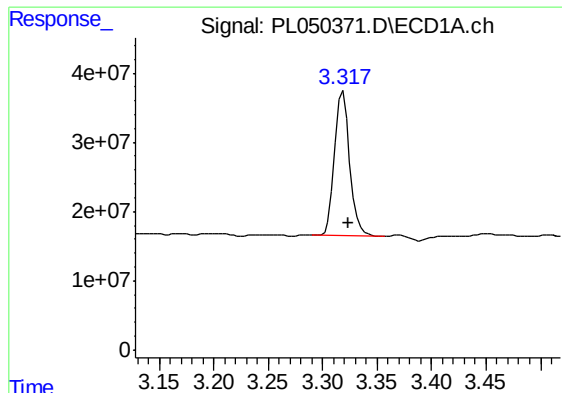


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: -0.005 min
Response: 199812543
Conc: 17.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-22


Manual Integrations
APPROVED

Ankita
7/16/2019 10:14:08 AM

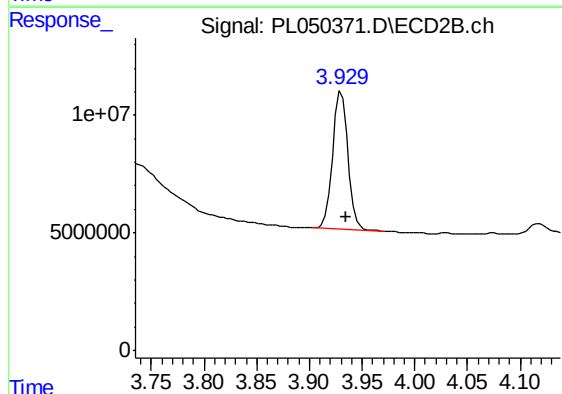


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.005 min
Response: 59431975
Conc: 19.41 ng/ml

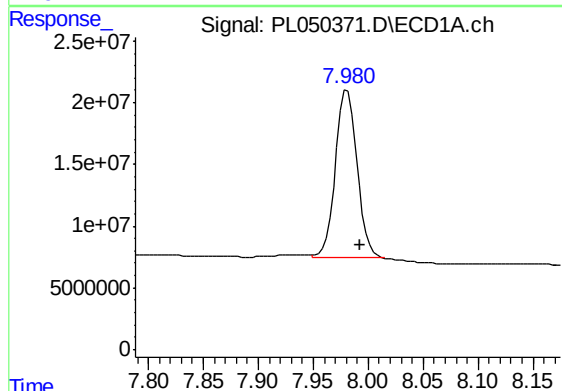

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.012 min
Response: 186039649
Conc: 14.64 ng/ml m

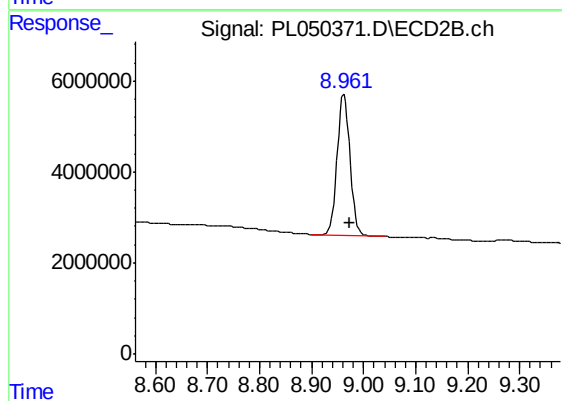

#28 Decachlorobiphenyl

R.T.: 8.962 min
Delta R.T.: -0.011 min
Response: 54057375
Conc: 16.10 ng/ml