

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
 Data File : PL068034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2021 14:55
 Operator : AR\AJ
 Sample : M2956-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 15:44:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 12 14:08:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.674	5.582	9202424	15158252	16.627	14.823
28)	SA Decachlor...	10.488	11.507	8743638	13703570	15.755	17.585
Target Compounds							
23)	Chlordane-1	5.992f	0.000	1122729	0	64.464	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
Data File : PL068034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2021 14:55
Operator : AR\AJ
Sample : M2956-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 15:44:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Mon Jul 12 14:08:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

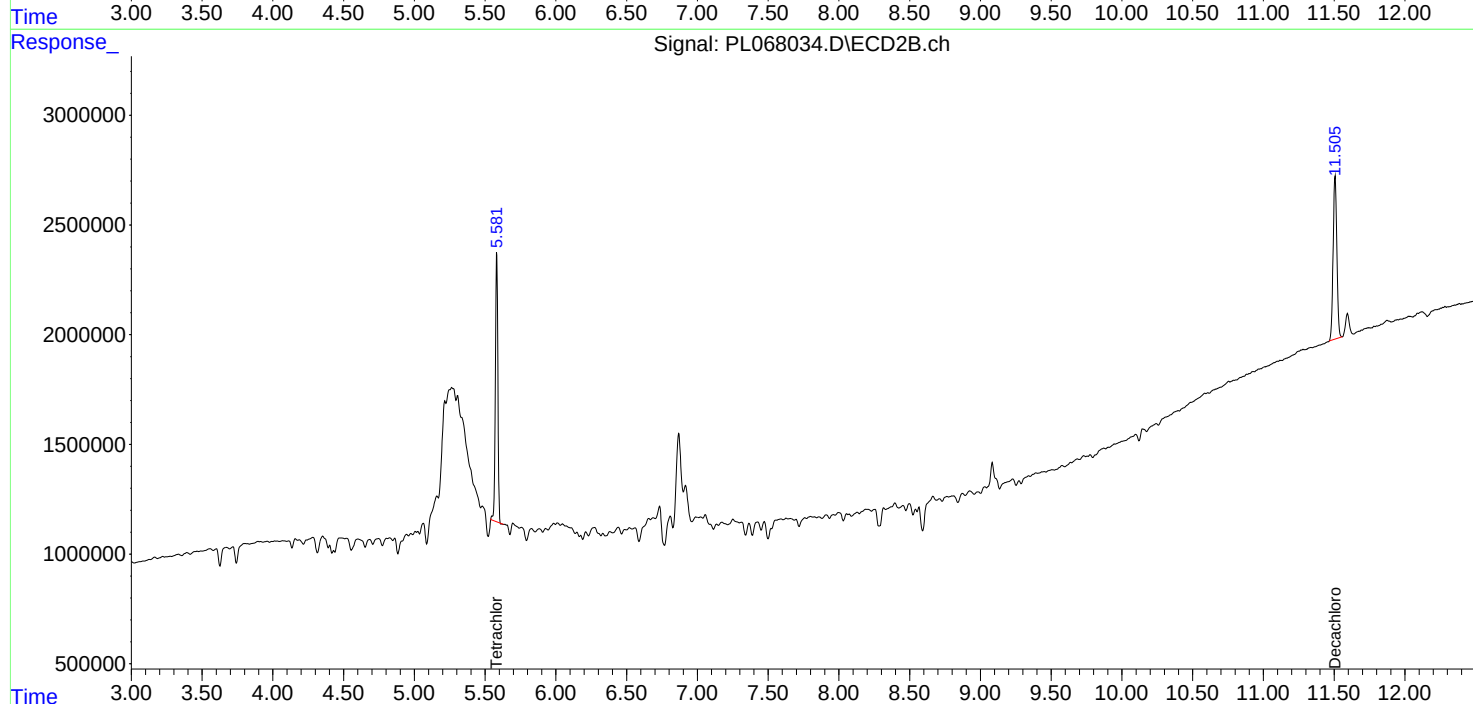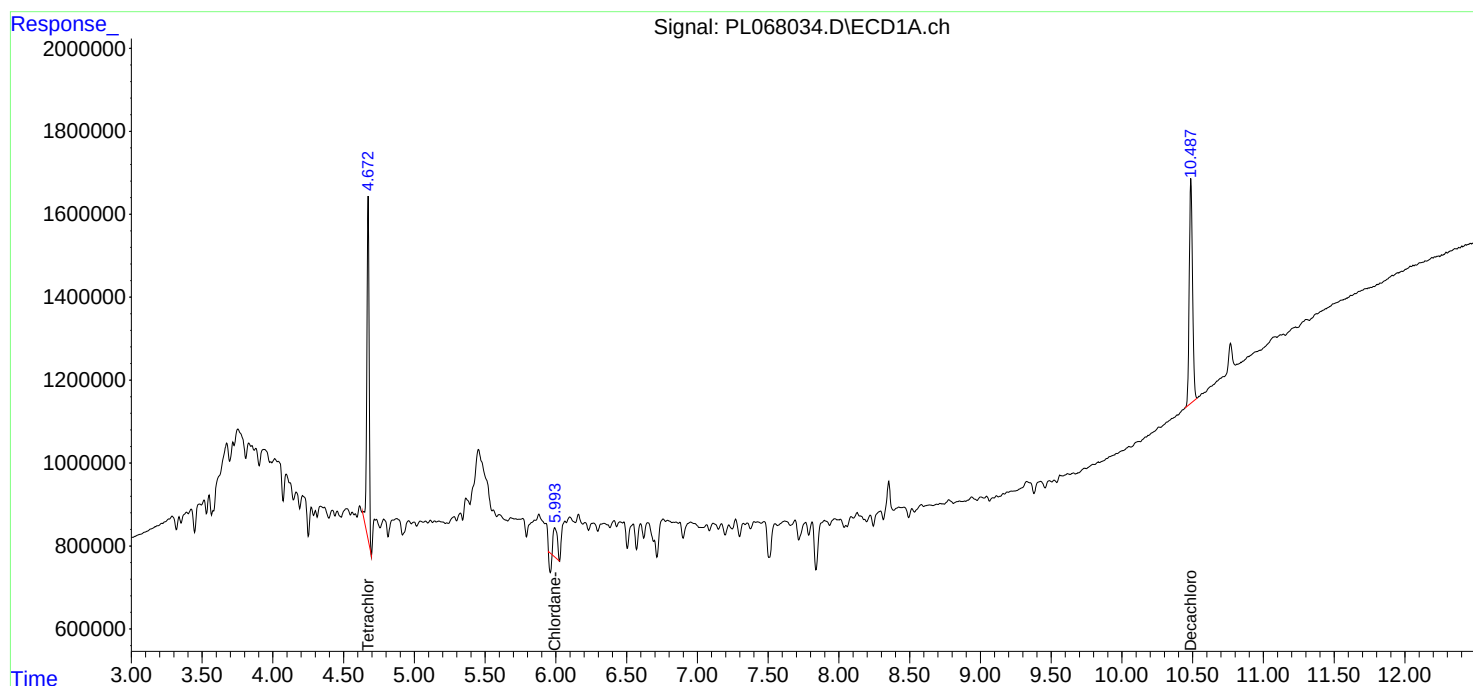


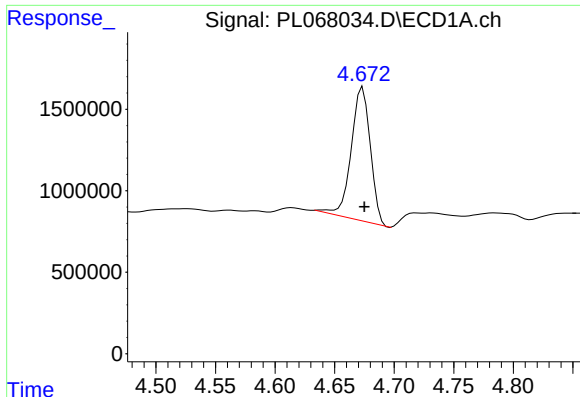

#1 Tetrachloro-m-xylene


R.T.: 4.674 min
Delta R.T.: -0.001 min
Response: 9202424
Conc: 16.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

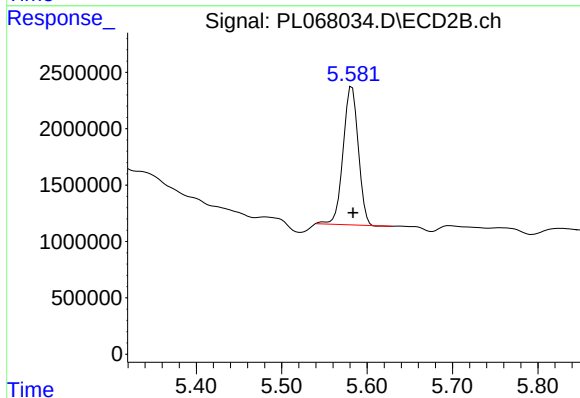


#1 Tetrachloro-m-xylene

R.T.: 5.582 min
Delta R.T.: -0.001 min
Response: 15158252
Conc: 14.82 ng/ml

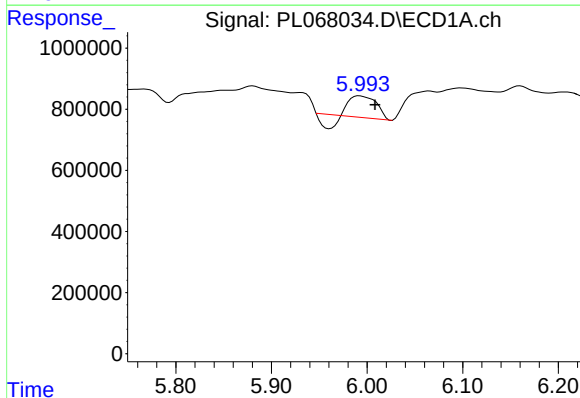


#23 Chlordane-1

R.T.: 5.992 min
Delta R.T.: -0.016 min
Response: 1122729
Conc: 64.46 ng/ml

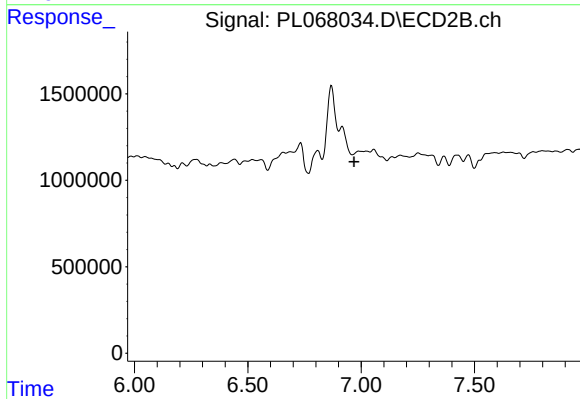

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 6.969 min
Response: 0
Conc: N.D.

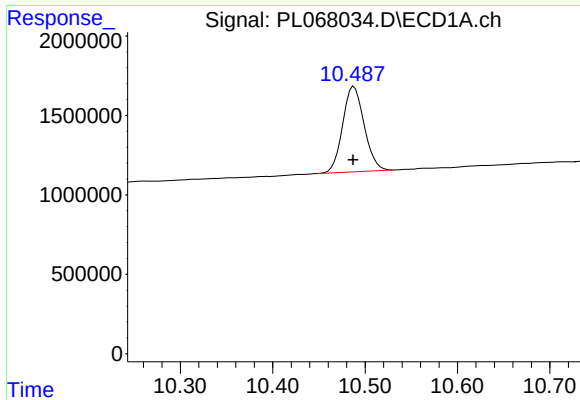

#28 Decachlorobiphenyl

R.T.: 10.488 min
Delta R.T.: 0.001 min
Response: 8743638
Conc: 15.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

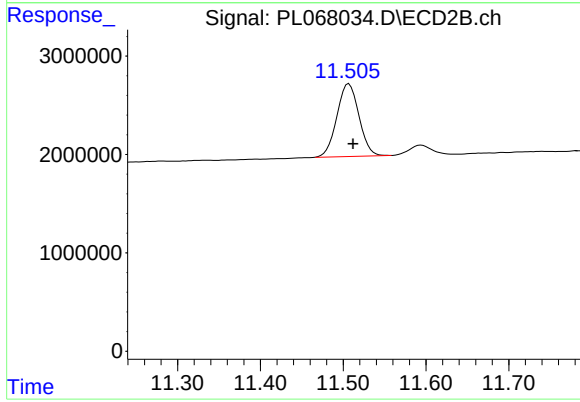

#28 Decachlorobiphenyl

R.T.: 11.507 min
Delta R.T.: -0.005 min
Response: 13703570
Conc: 17.59 ng/ml