

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
 Data File : PL068052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2021 19:56
 Operator : AR\AJ
 Sample : M2989-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 02:36:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 12 14:08:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.673	5.581	5711842	10212805	10.320	9.987
28)	SA Decachlor...	10.471f	11.505	4983136	8556742	8.979	10.981
Target Compounds							
10)	B gamma-Chl...	0.000	8.313	0	1417320	N.D.	1.383 #
11)	B alpha-Chl...	0.000	8.395	0	1985845	N.D.	1.954 #
25)	Chlordane-3	0.000	8.313	0	1417320	N.D.	10.096 #
26)	Chlordane-4	0.000	8.395	0	1985845	N.D.	11.771 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
Data File : PL068052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2021 19:56
Operator : AR\AJ
Sample : M2989-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 02:36:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Mon Jul 12 14:08:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

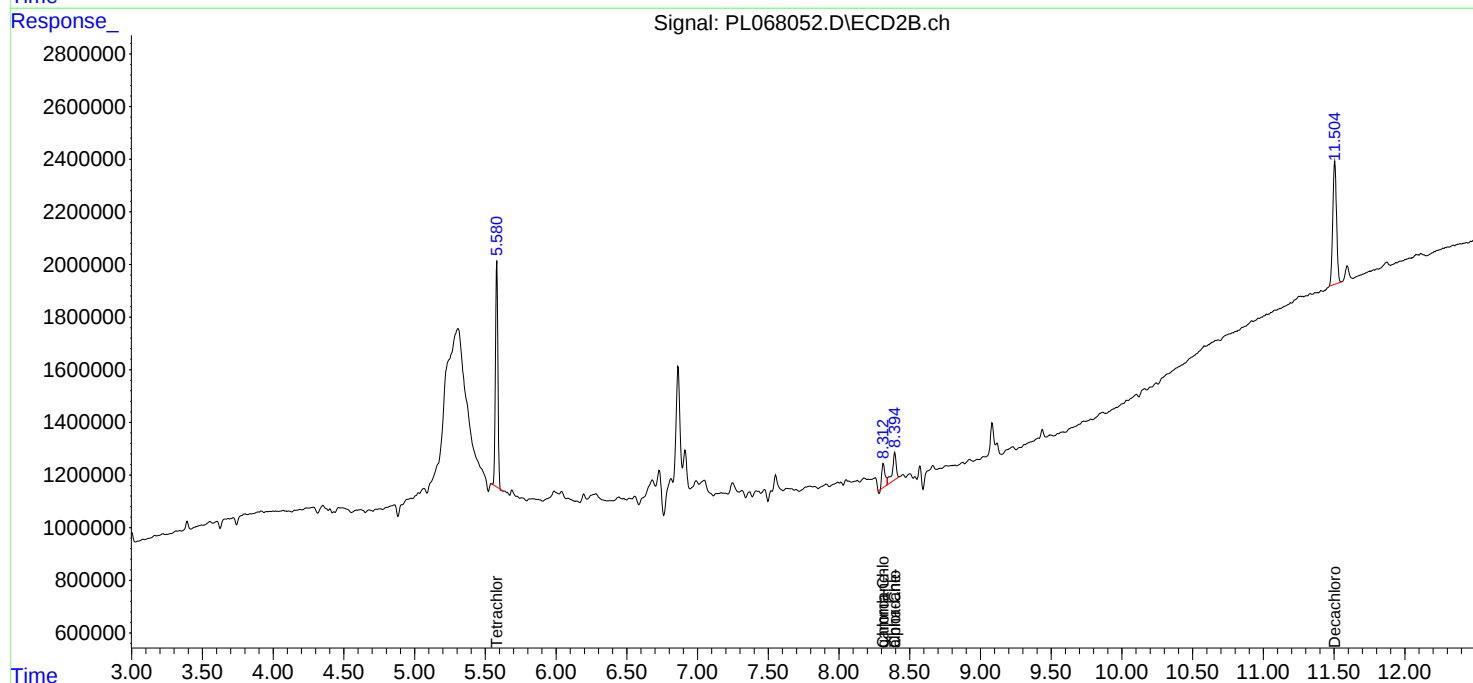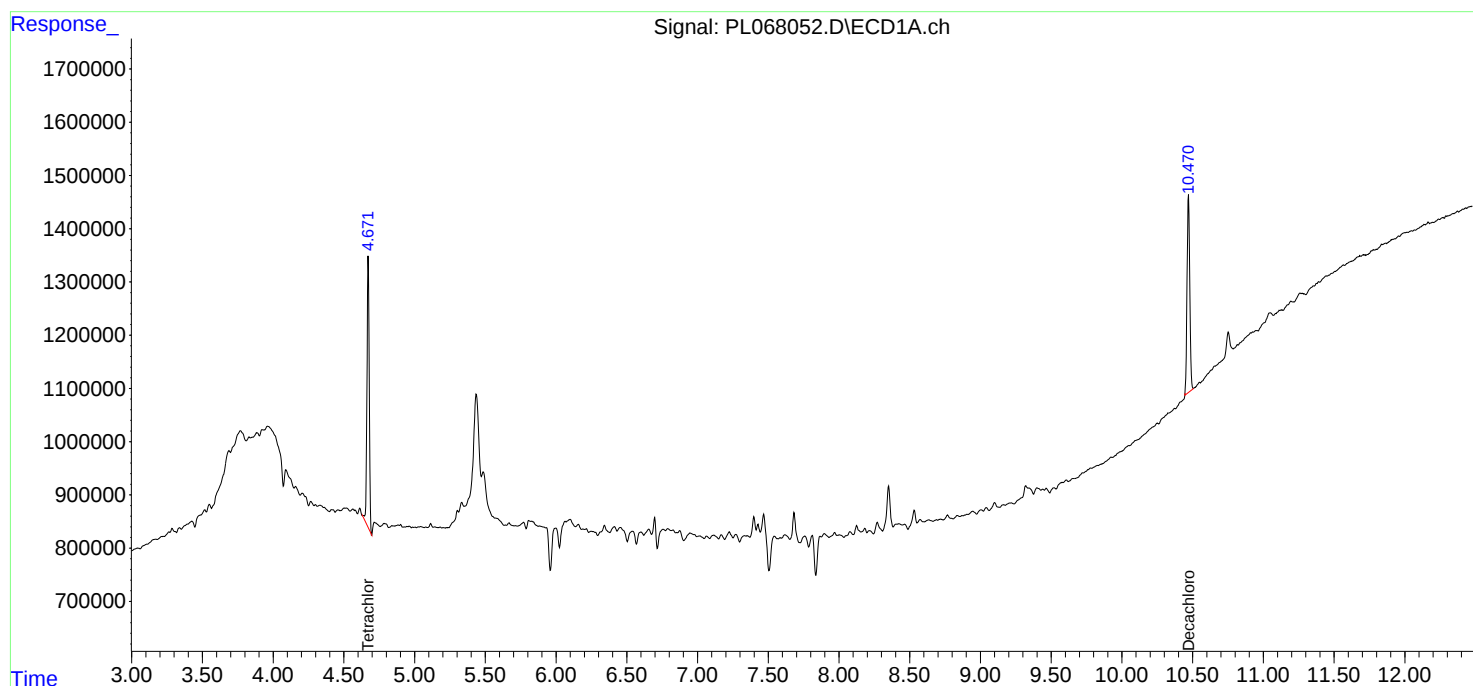


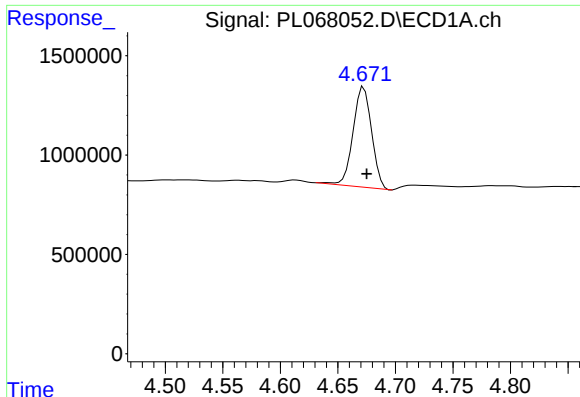

#1 Tetrachloro-m-xylene


R.T.: 4.673 min
Delta R.T.: -0.002 min
Response: 5711842
Conc: 10.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

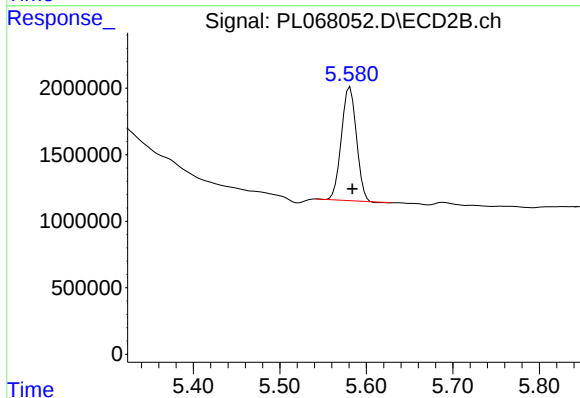


#1 Tetrachloro-m-xylene

R.T.: 5.581 min
Delta R.T.: -0.003 min
Response: 10212805
Conc: 9.99 ng/ml

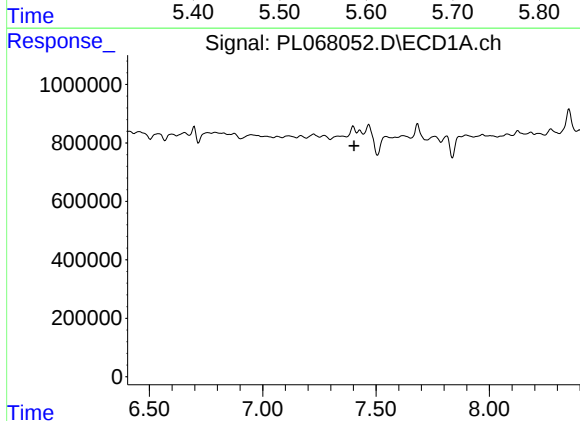


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.403 min
Response: 0
Conc: N.D.

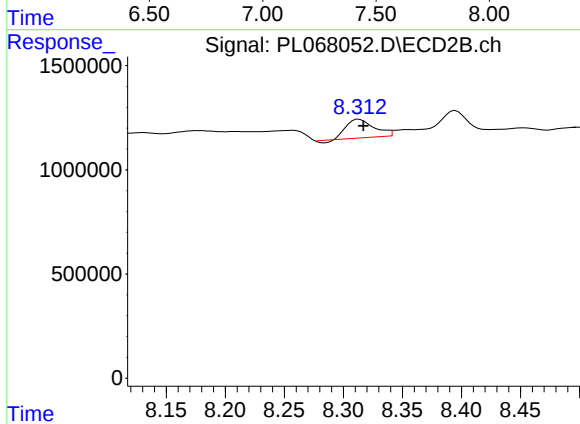

#10 gamma-Chlordane


R.T.: 8.313 min
Delta R.T.: -0.004 min
Response: 1417320
Conc: 1.38 ng/ml

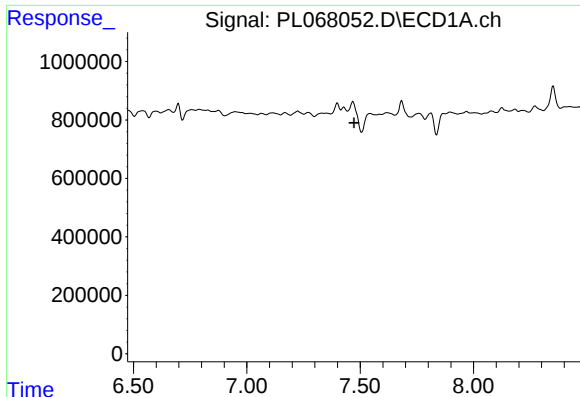

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.473 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

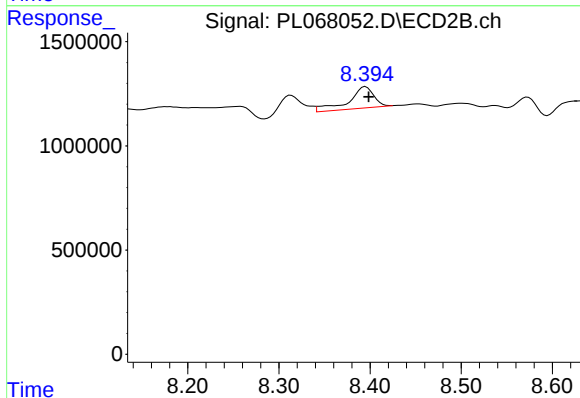


#11 alpha-Chlordane

R.T.: 8.395 min
Delta R.T.: -0.003 min
Response: 1985845
Conc: 1.95 ng/ml

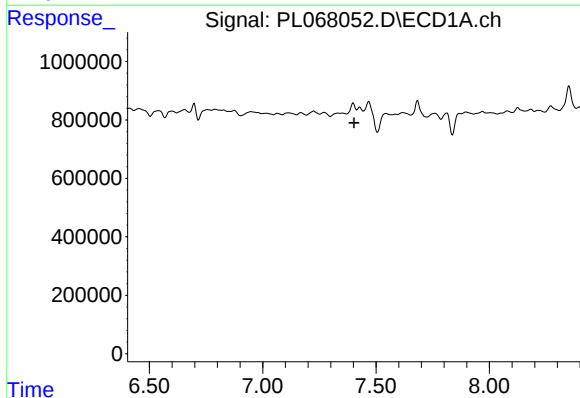


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.403 min
Response: 0
Conc: N.D.

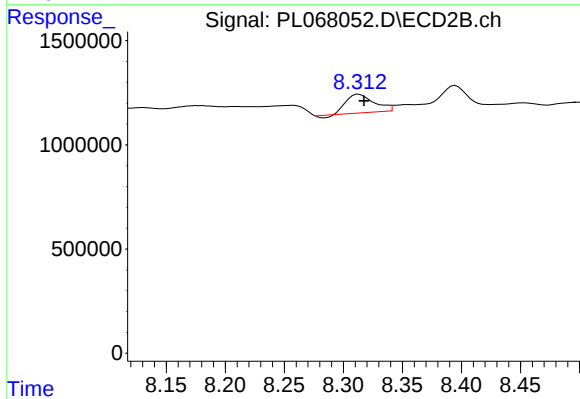

#25 Chlordane-3


R.T.: 8.313 min
Delta R.T.: -0.004 min
Response: 1417320
Conc: 10.10 ng/ml

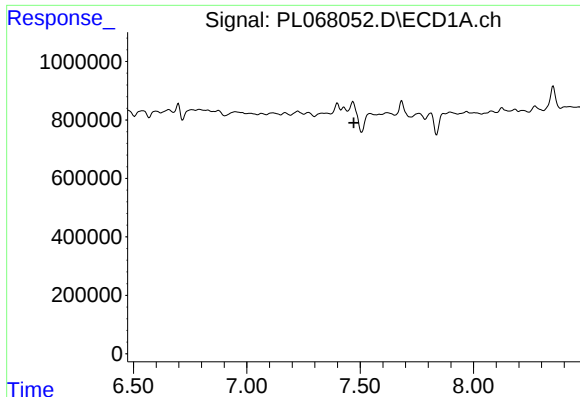

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

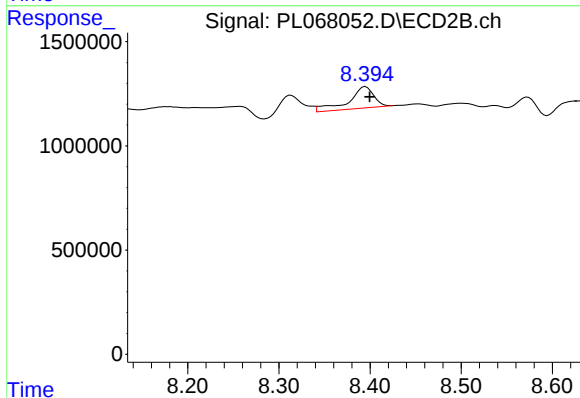


#26 Chlordane-4

R.T.: 8.395 min
Delta R.T.: -0.005 min
Response: 1985845
Conc: 11.77 ng/ml

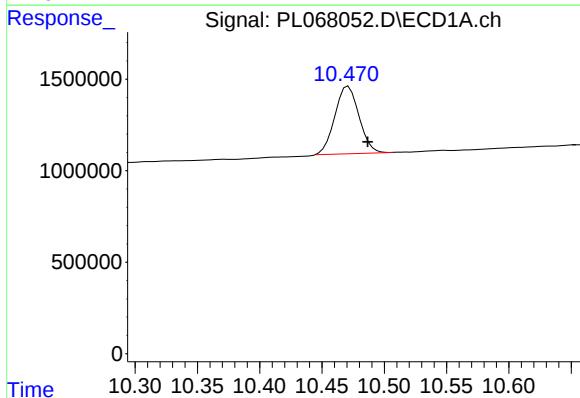

#28 Decachlorobiphenyl

R.T.: 10.471 min
Delta R.T.: -0.016 min
Response: 4983136
Conc: 8.98 ng/ml

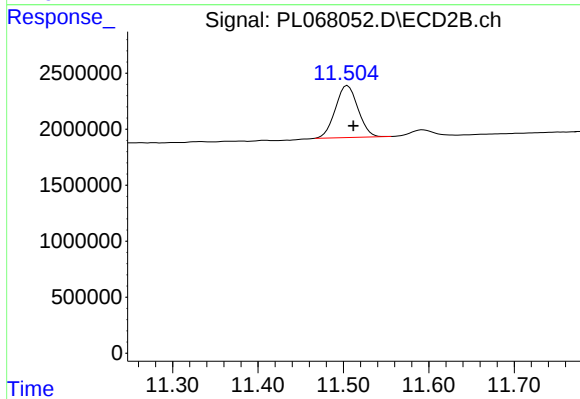

#28 Decachlorobiphenyl

R.T.: 11.505 min
Delta R.T.: -0.007 min
Response: 8556742
Conc: 10.98 ng/ml