

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
 Data File : PL068071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2021 01:30
 Operator : AR\AJ
 Sample : M3001-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 02:41:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 12 14:08:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.674	5.582	5532853	10335218	9.997	10.106
28)	SA Decachlor...	10.473	11.505	7281630	11733699	13.121	15.058
Target Compounds							
11)	B alpha-Chl...	0.000	8.397	0	1930965	N.D.	1.900 #
22)	Mirex	0.000	10.561	0	7364027	N.D.	10.922 #
26)	Chlordane-4	0.000	8.397	0	1930965	N.D.	11.446 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
Data File : PL068071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2021 01:30
Operator : AR\AJ
Sample : M3001-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 02:41:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Mon Jul 12 14:08:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

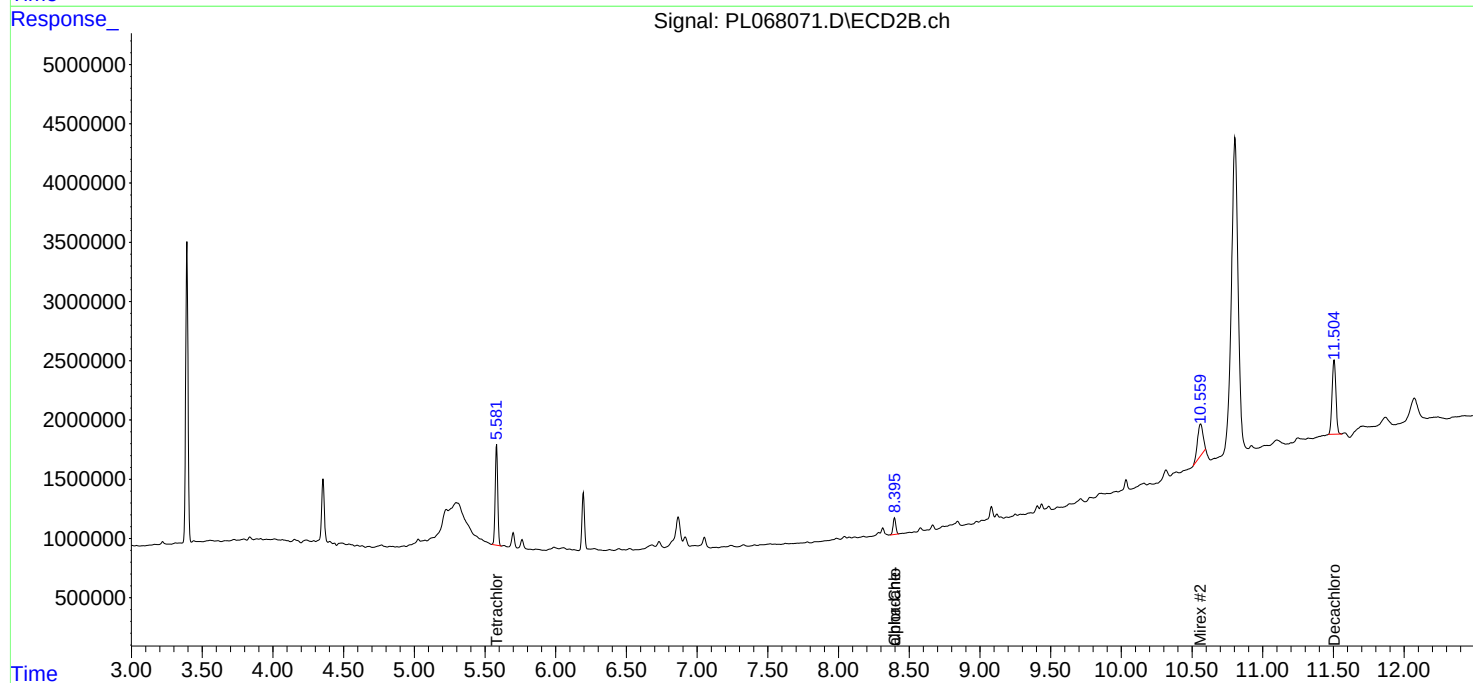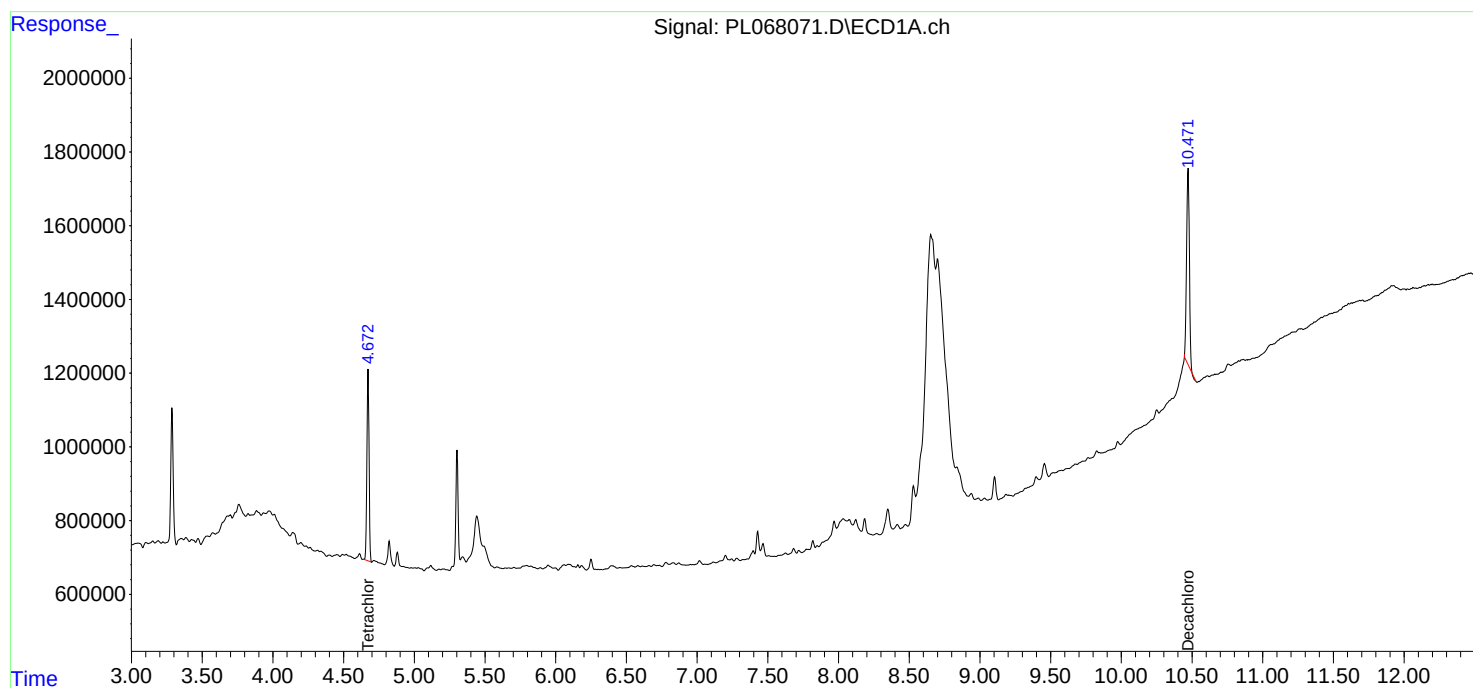


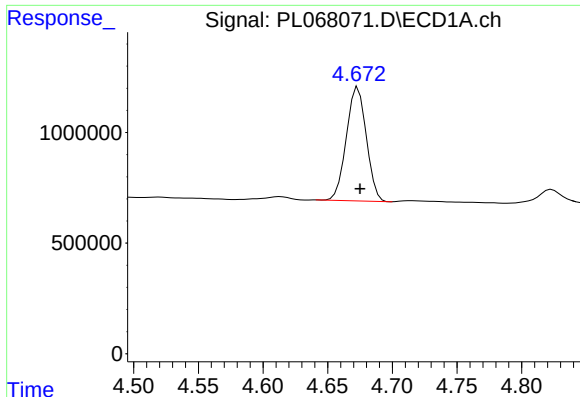

#1 Tetrachloro-m-xylene


R.T.: 4.674 min
Delta R.T.: -0.001 min
Response: 5532853
Conc: 10.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

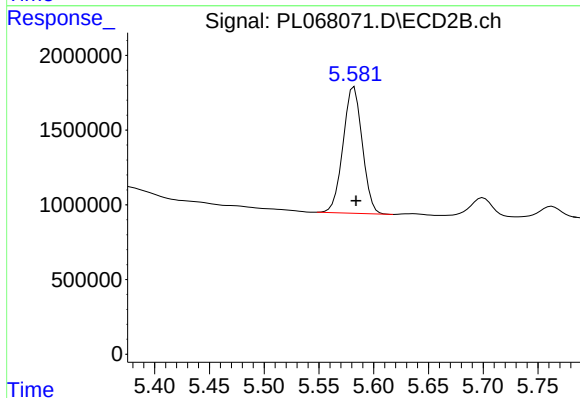


#1 Tetrachloro-m-xylene

R.T.: 5.582 min
Delta R.T.: -0.002 min
Response: 10335218
Conc: 10.11 ng/ml

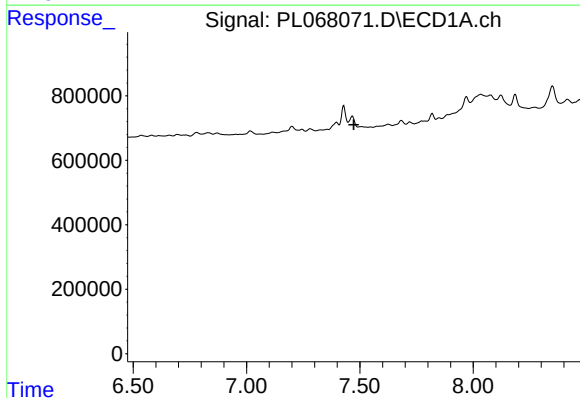


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.473 min
Response: 0
Conc: N.D.

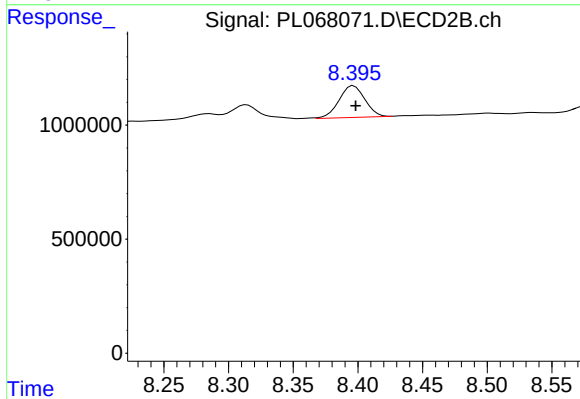

#11 alpha-Chlordane


R.T.: 8.397 min
Delta R.T.: -0.002 min
Response: 1930965
Conc: 1.90 ng/ml

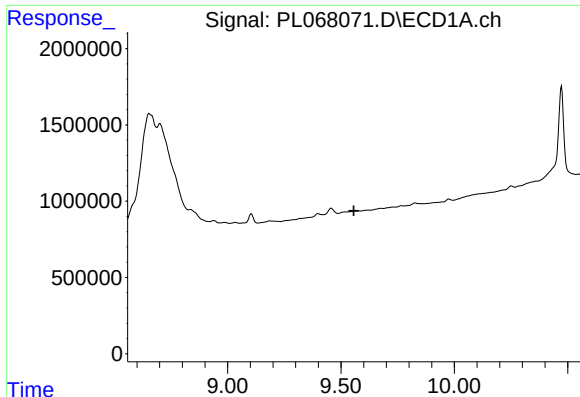

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.557 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

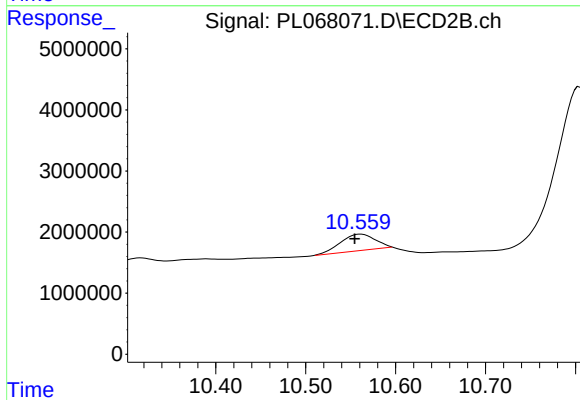


#22 Mirex

R.T.: 10.561 min
Delta R.T.: 0.007 min
Response: 7364027
Conc: 10.92 ng/ml

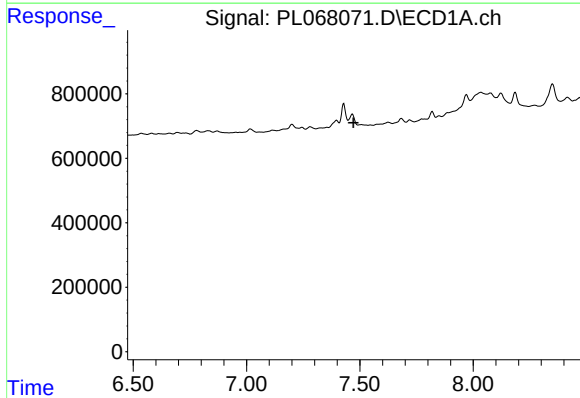


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.472 min
Response: 0
Conc: N.D.

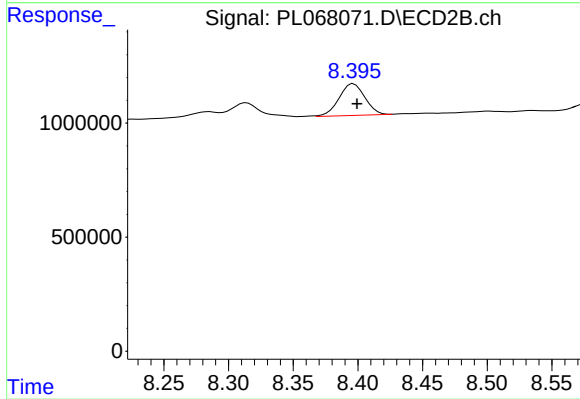

#26 Chlordane-4


R.T.: 8.397 min
Delta R.T.: -0.003 min
Response: 1930965
Conc: 11.45 ng/ml

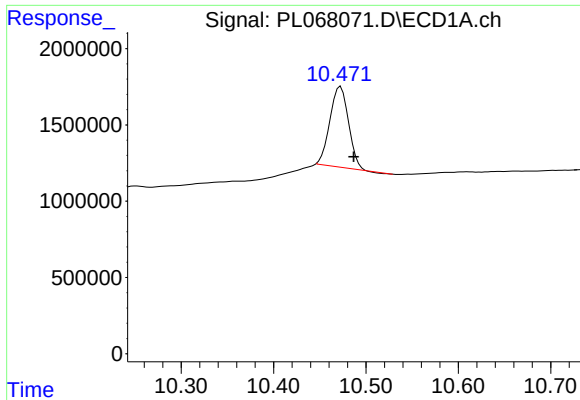

#28 Decachlorobiphenyl

R.T.: 10.473 min
Delta R.T.: -0.014 min
Response: 7281630
Conc: 13.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

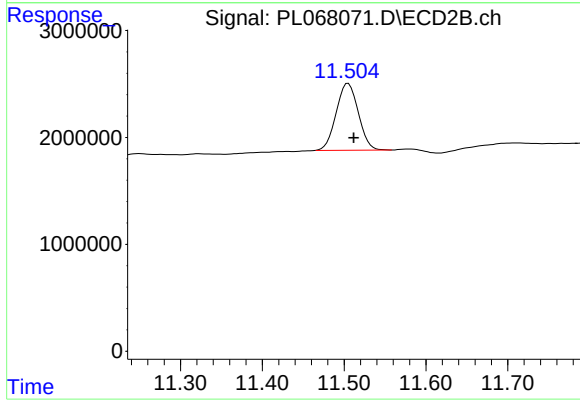

#28 Decachlorobiphenyl

R.T.: 11.505 min
Delta R.T.: -0.007 min
Response: 11733699
Conc: 15.06 ng/ml