

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
 Data File : PL068073.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2021 02:04
 Operator : AR\AJ
 Sample : M3006-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 02:41:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 12 14:08:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.672	5.582	7287018	13819127	13.166	13.513
28)	SA Decachlor...	10.472	11.504	7040265	11474714	12.686	14.725
Target Compounds							
11)	B alpha-Chl...	0.000	8.395	0	1839353	N.D.	1.810 #
26)	Chlordane-4	0.000	8.395	0	1839353	N.D.	10.903 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
Data File : PL068073.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2021 02:04
Operator : AR\AJ
Sample : M3006-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 02:41:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Mon Jul 12 14:08:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

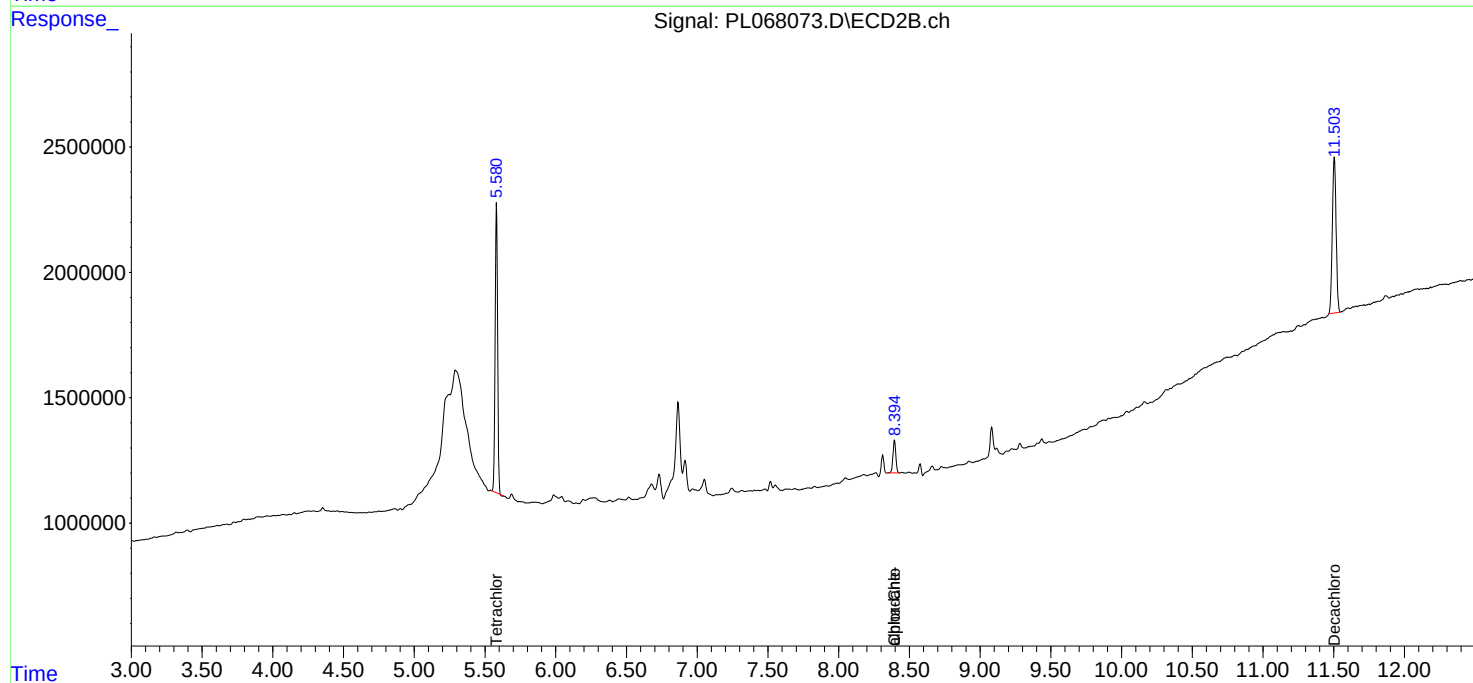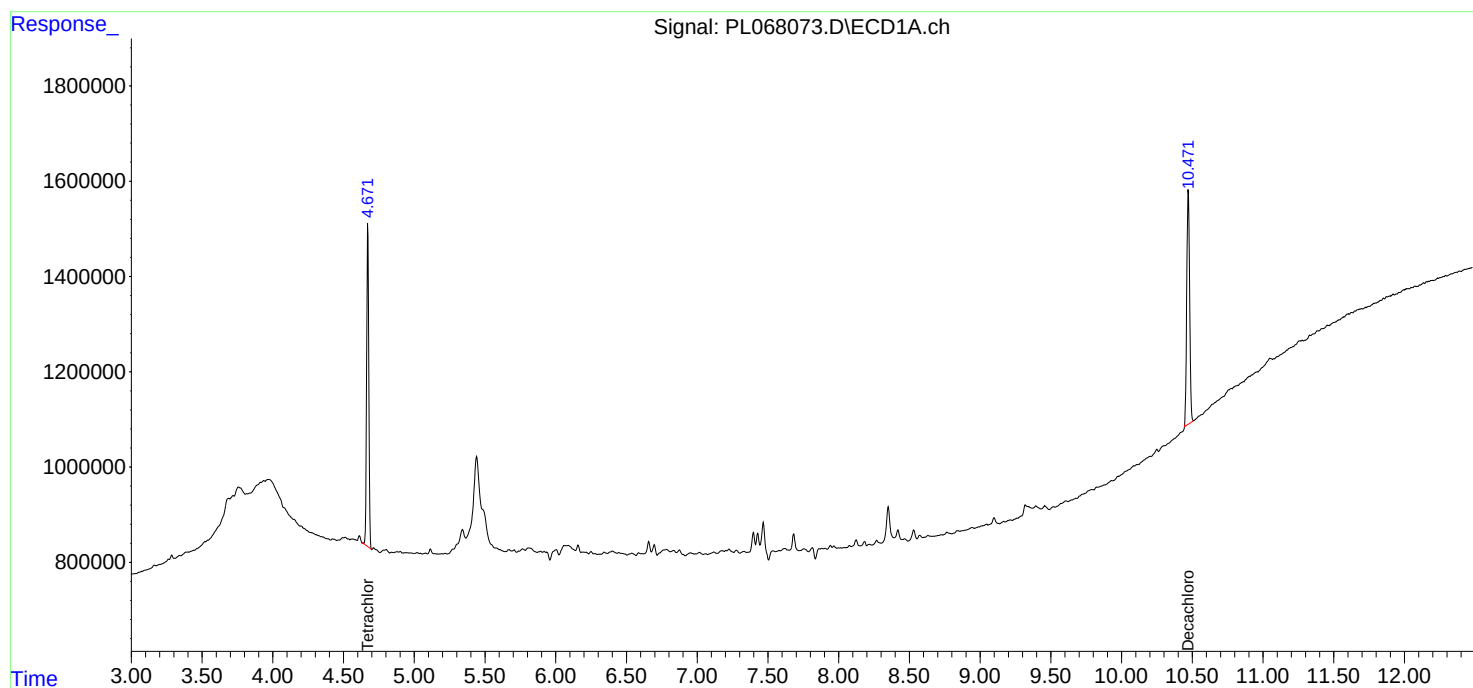


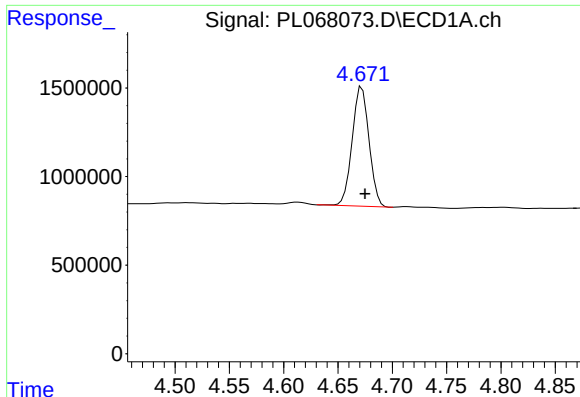

#1 Tetrachloro-m-xylene


R.T.: 4.672 min
Delta R.T.: -0.003 min
Response: 7287018
Conc: 13.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

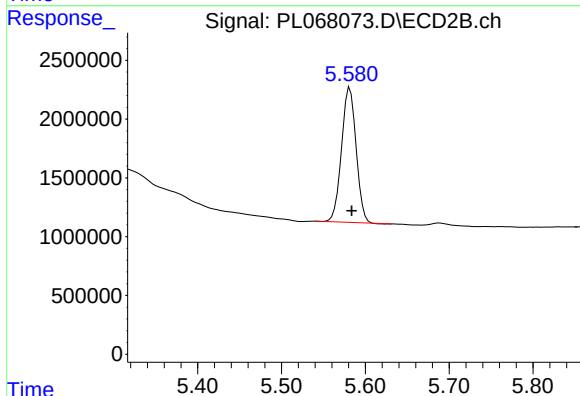


#1 Tetrachloro-m-xylene

R.T.: 5.582 min
Delta R.T.: -0.002 min
Response: 13819127
Conc: 13.51 ng/ml

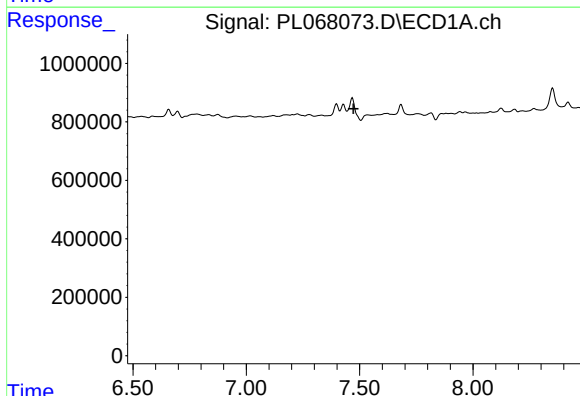


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.473 min
Response: 0
Conc: N.D.

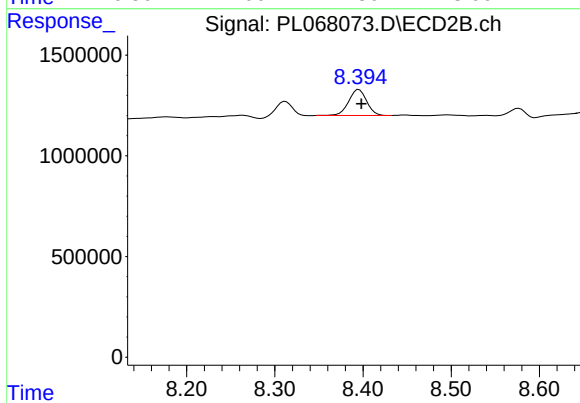

#11 alpha-Chlordane


R.T.: 8.395 min
Delta R.T.: -0.003 min
Response: 1839353
Conc: 1.81 ng/ml

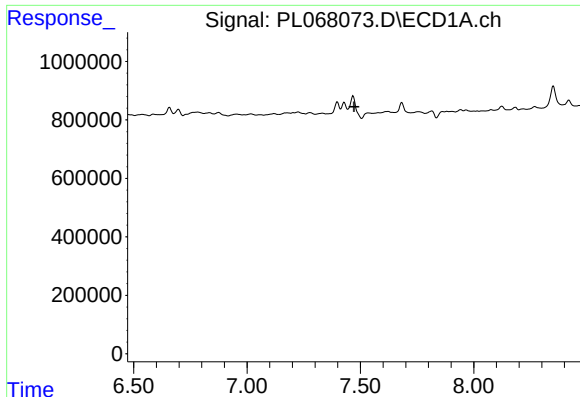

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

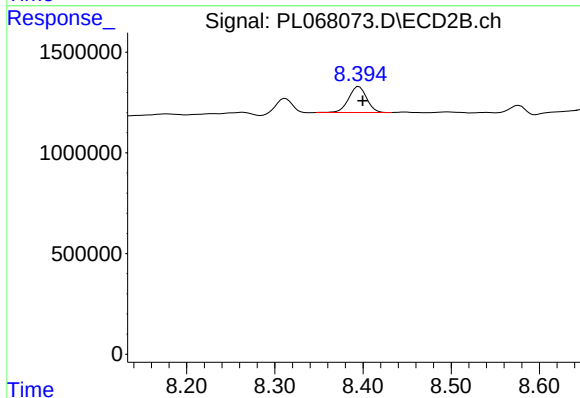


#26 Chlordane-4

R.T.: 8.395 min
Delta R.T.: -0.004 min
Response: 1839353
Conc: 10.90 ng/ml

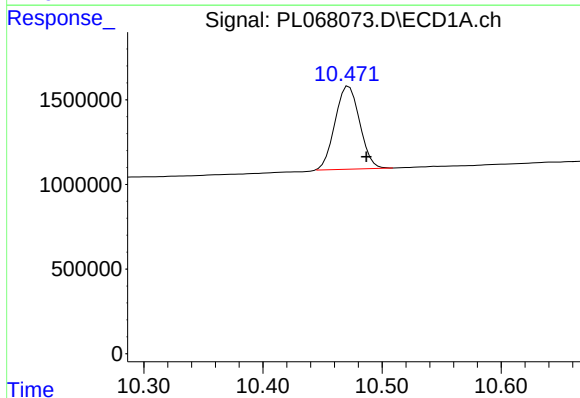

#28 Decachlorobiphenyl

R.T.: 10.472 min
Delta R.T.: -0.015 min
Response: 7040265
Conc: 12.69 ng/ml

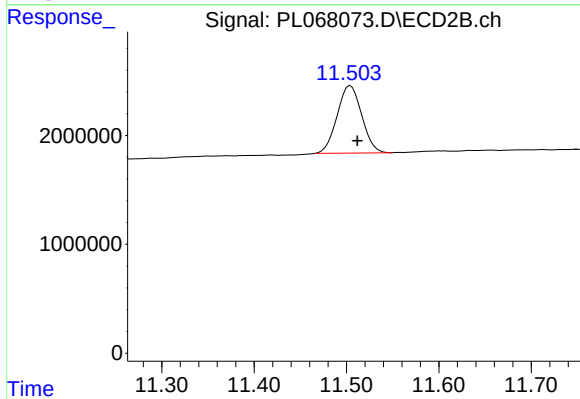

#28 Decachlorobiphenyl

R.T.: 11.504 min
Delta R.T.: -0.007 min
Response: 11474714
Conc: 14.73 ng/ml