

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
 Data File : PL068028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2021 12:00
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 14:06:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 12 14:06:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.675	5.584	33446099	52526807	50.000	50.000
28)	SA Decachlor...	10.489	11.512	28190349	39434535	50.000	50.000
Target Compounds							
23)	Chlordane-1	6.008	6.969	8708156	18272212	500.000	500.000
24)	Chlordane-2	6.698	7.559	11773288	19814773	500.000	500.000
25)	Chlordane-3	7.403	8.317	32077625	70195256	500.000	500.000
26)	Chlordane-4	7.472	8.400	33671607	84353184	500.000	500.000
27)	Chlordane-5	8.426	9.288	11316556	15255259	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
Data File : PL068028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2021 12:00
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 14:06:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Mon Jul 12 14:06:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

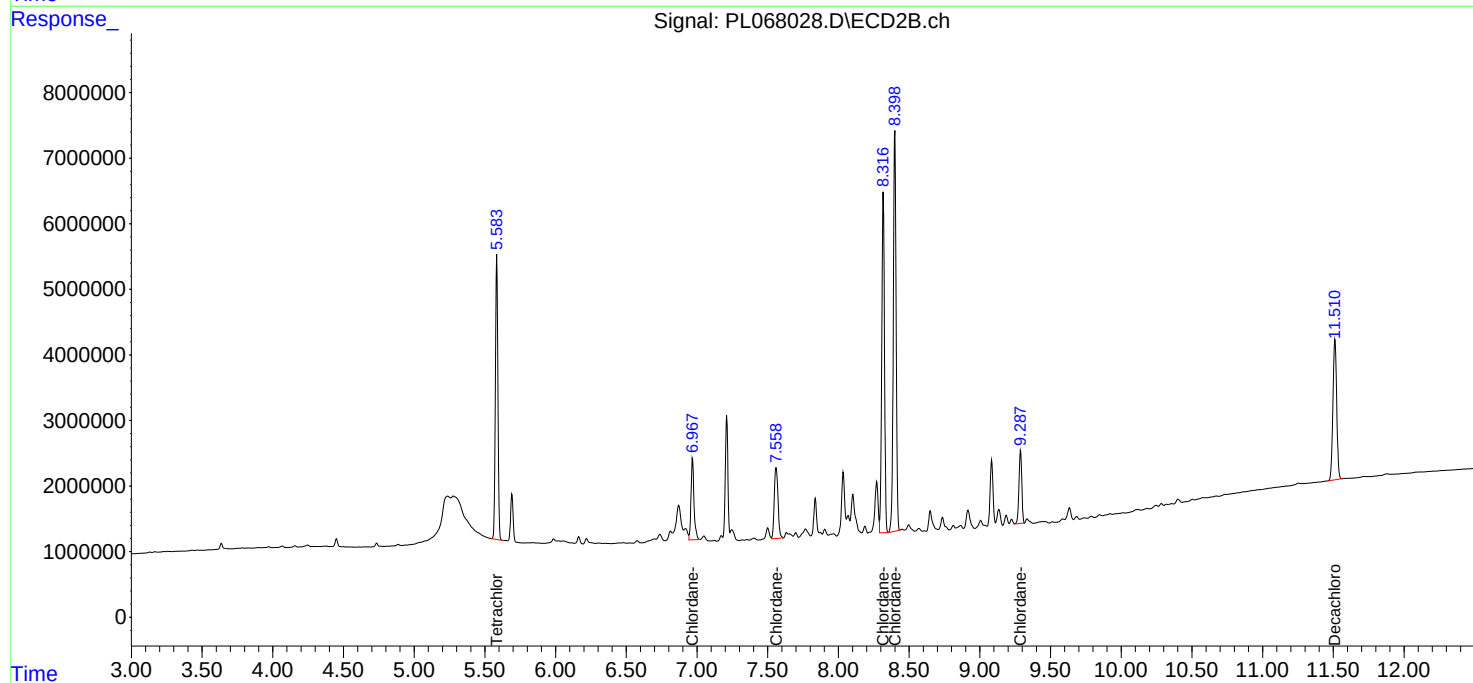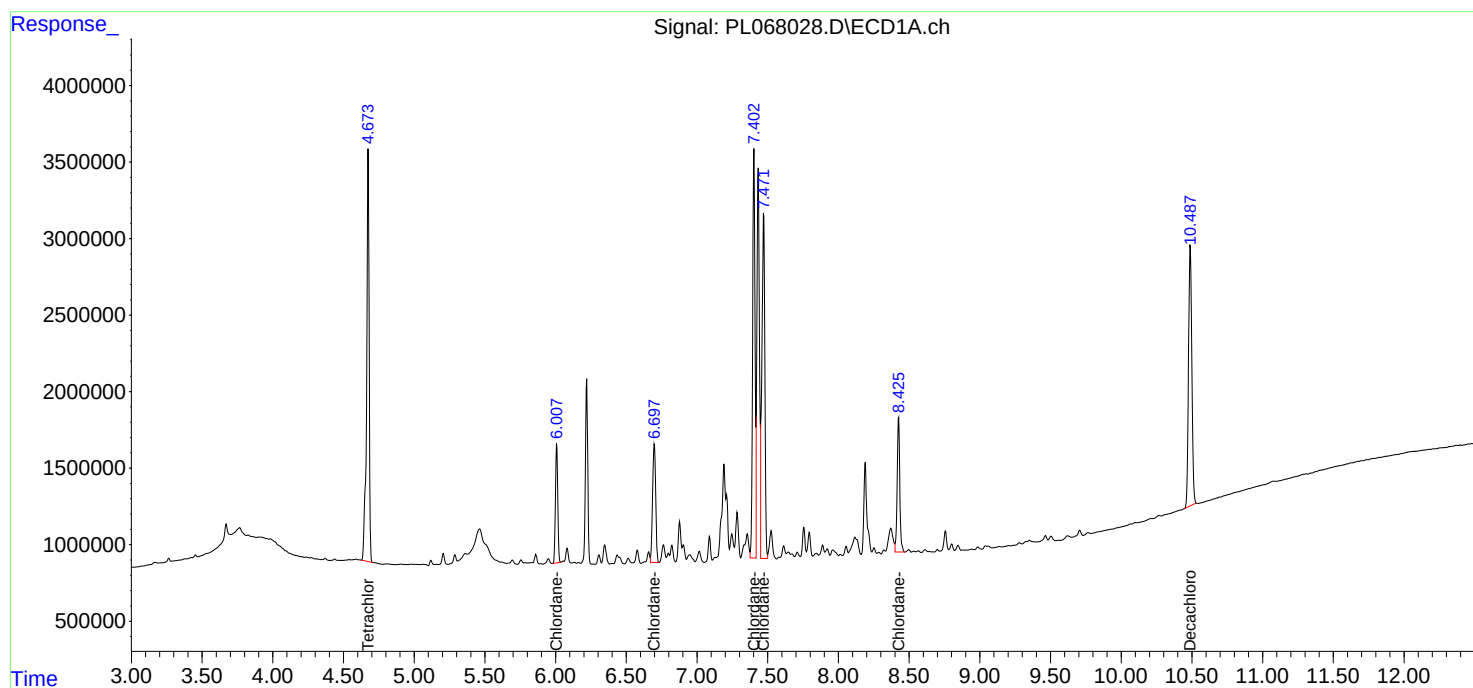


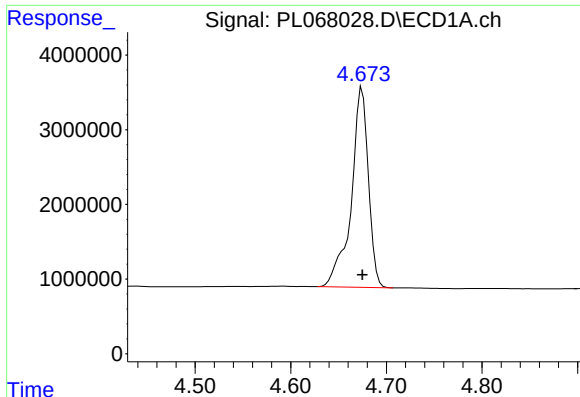

#1 Tetrachloro-m-xylene


R.T.: 4.675 min
Delta R.T.: 0.000 min
Response: 33446099
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

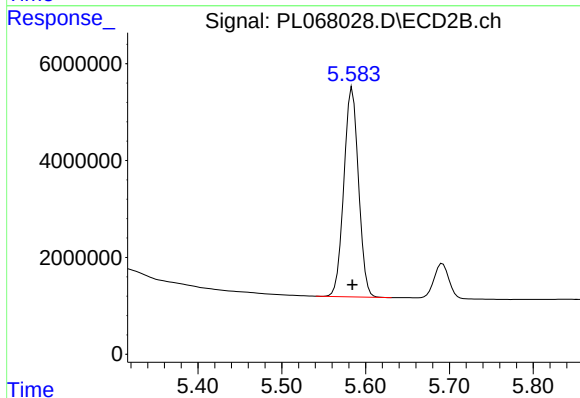


#1 Tetrachloro-m-xylene

R.T.: 5.584 min
Delta R.T.: 0.000 min
Response: 52526807
Conc: 50.00 ng/ml

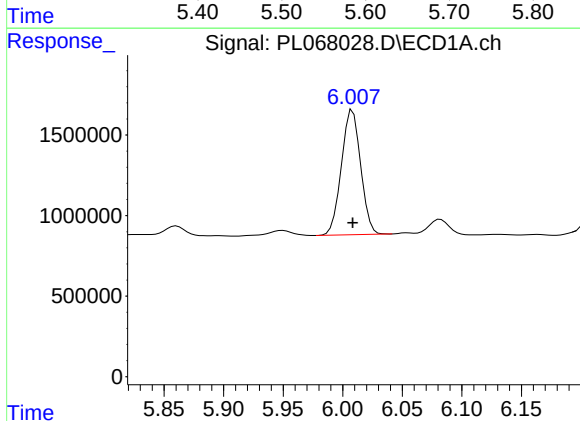


#23 Chlordane-1

R.T.: 6.008 min
Delta R.T.: 0.000 min
Response: 8708156
Conc: 500.00 ng/ml

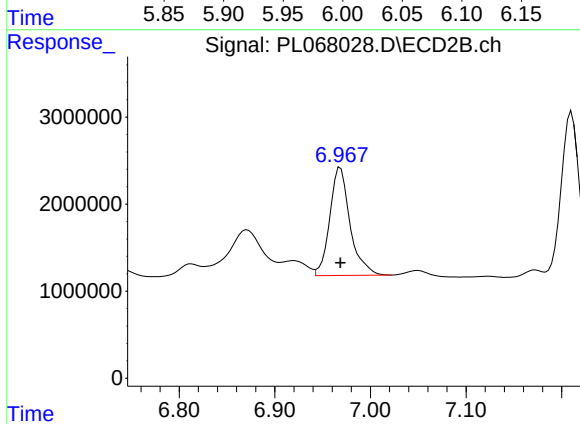

#23 Chlordane-1


R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 18272212
Conc: 500.00 ng/ml

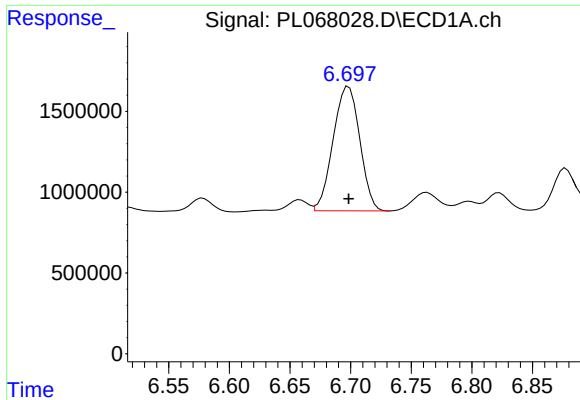

#24 Chlordane-2


R.T.: 6.698 min
Delta R.T.: 0.000 min
Response: 11773288
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

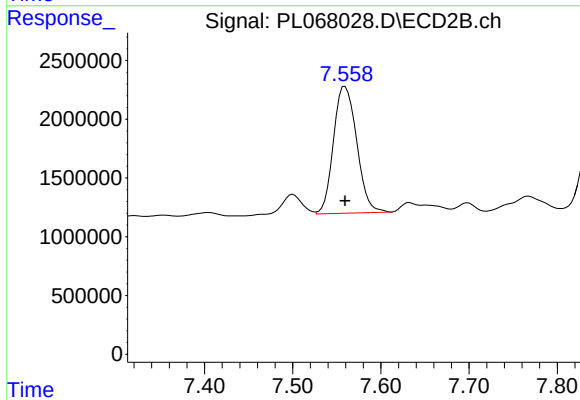


#24 Chlordane-2

R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 19814773
Conc: 500.00 ng/ml

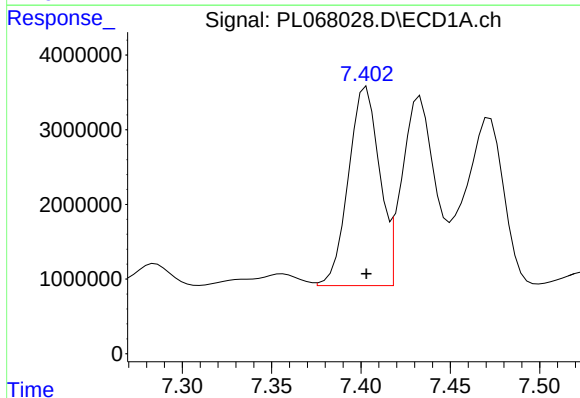


#25 Chlordane-3

R.T.: 7.403 min
Delta R.T.: 0.000 min
Response: 32077625
Conc: 500.00 ng/ml

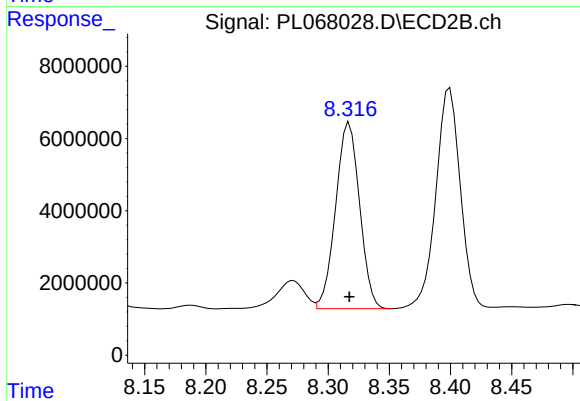

#25 Chlordane-3


R.T.: 8.317 min
Delta R.T.: 0.000 min
Response: 70195256
Conc: 500.00 ng/ml

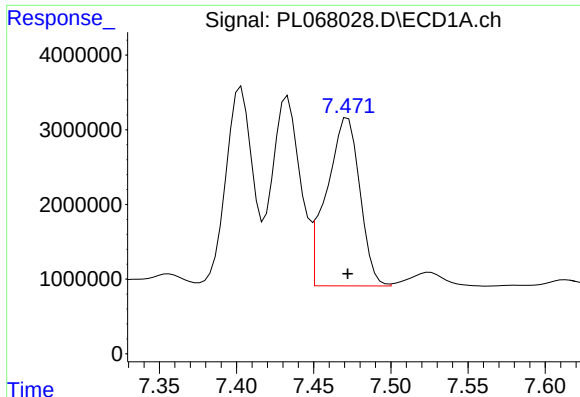

#26 Chlordane-4


R.T.: 7.472 min
Delta R.T.: 0.000 min
Response: 33671607
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

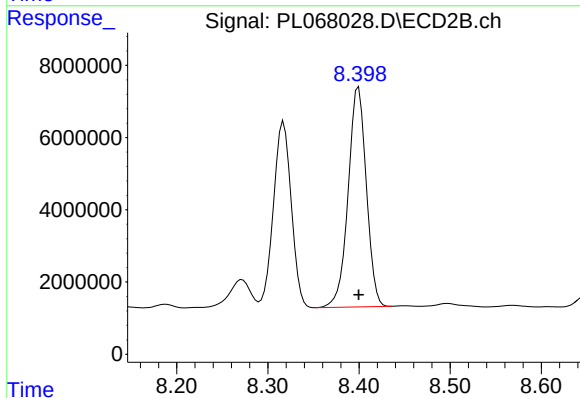


#26 Chlordane-4

R.T.: 8.400 min
Delta R.T.: 0.000 min
Response: 84353184
Conc: 500.00 ng/ml

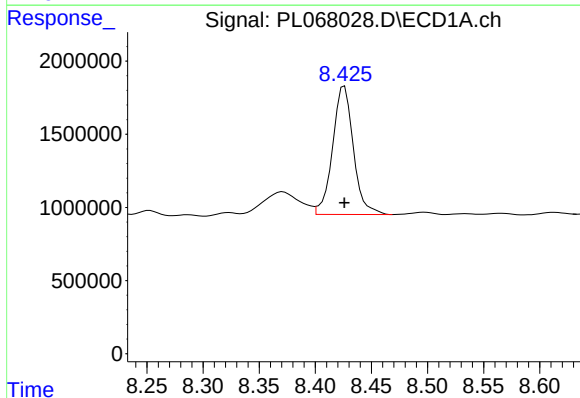


#27 Chlordane-5

R.T.: 8.426 min
Delta R.T.: 0.000 min
Response: 11316556
Conc: 500.00 ng/ml

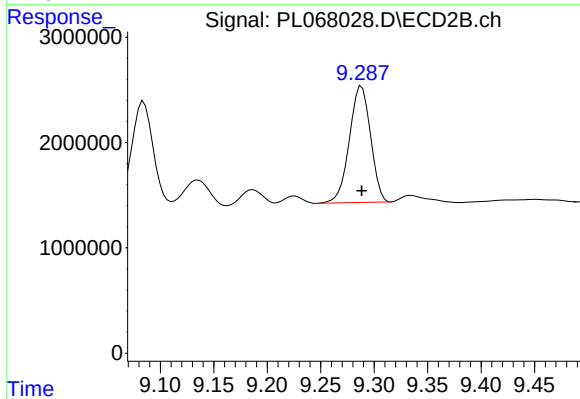

#27 Chlordane-5


R.T.: 9.288 min
Delta R.T.: 0.000 min
Response: 15255259
Conc: 500.00 ng/ml

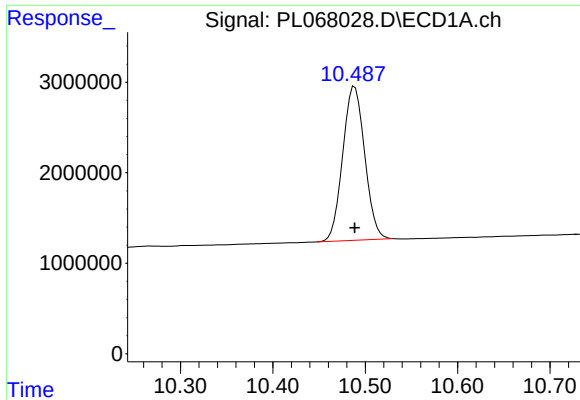

#28 Decachlorobiphenyl

R.T.: 10.489 min
Delta R.T.: 0.000 min
Response: 28190349
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

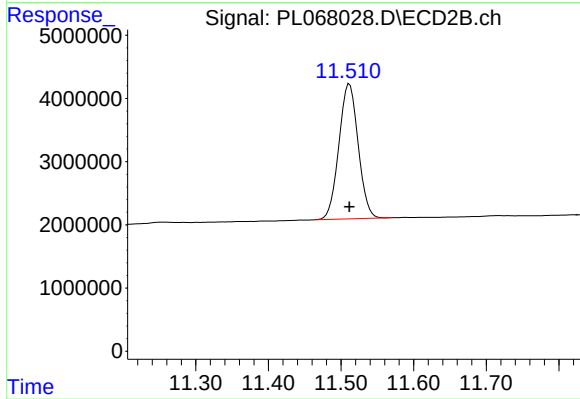

#28 Decachlorobiphenyl

R.T.: 11.512 min
Delta R.T.: 0.000 min
Response: 39434535
Conc: 50.00 ng/ml