

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
 Data File : PL068063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2021 23:16
 Operator : AR\AJ
 Sample : M2990-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 08:50:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 12 14:08:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.672	5.581	7556224	14644109	13.652	14.320
28)	SA Decachlor...	10.470	11.504	7632208	11592106	13.753	14.876
Target Compounds							
10)	B gamma-Chl...	7.397	8.312	255073	369613	0.387	0.361
11)	B alpha-Chl...	7.467	8.396	324088	873297	0.490	0.859 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
Data File : PL068063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2021 23:16
Operator : AR\AJ
Sample : M2990-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 08:50:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Mon Jul 12 14:08:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

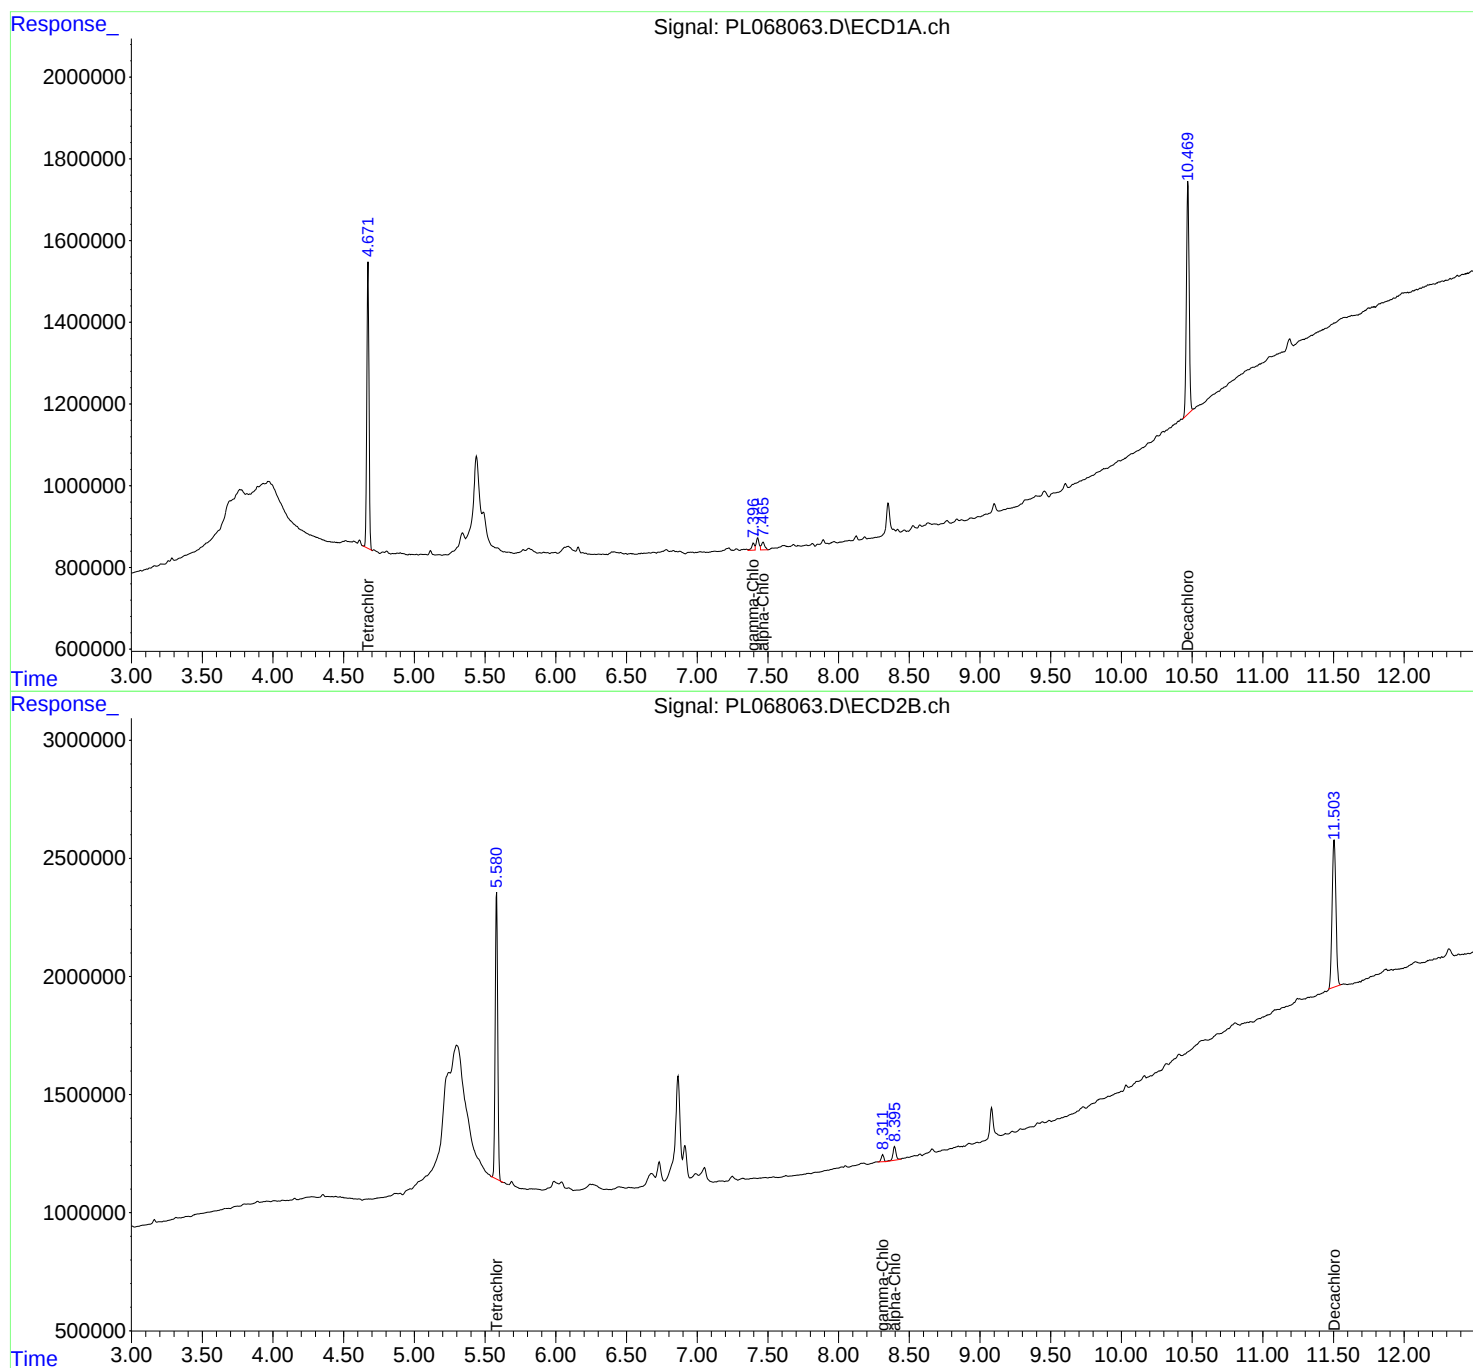


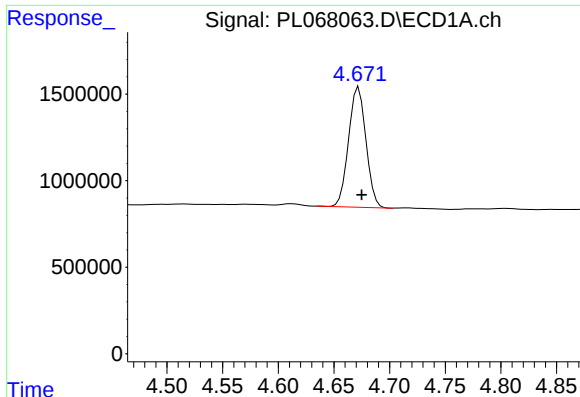

#1 Tetrachloro-m-xylene


R.T.: 4.672 min
Delta R.T.: -0.003 min
Response: 7556224
Conc: 13.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-E

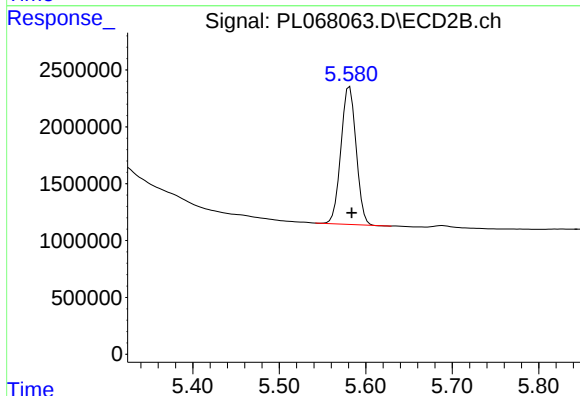


#1 Tetrachloro-m-xylene

R.T.: 5.581 min
Delta R.T.: -0.002 min
Response: 14644109
Conc: 14.32 ng/ml

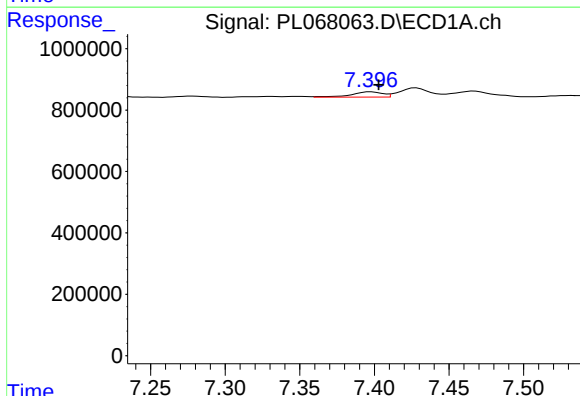


#10 gamma-Chlordane

R.T.: 7.397 min
Delta R.T.: -0.005 min
Response: 255073
Conc: 0.39 ng/ml

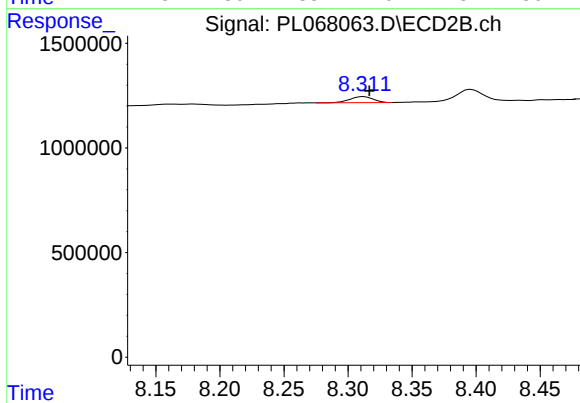

#10 gamma-Chlordane


R.T.: 8.312 min
Delta R.T.: -0.005 min
Response: 369613
Conc: 0.36 ng/ml

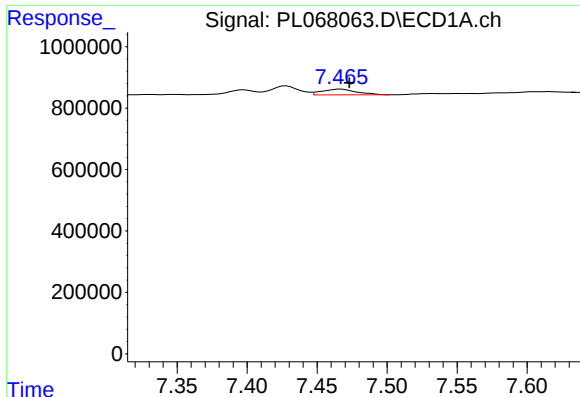

#11 alpha-Chlordane


R.T.: 7.467 min
Delta R.T.: -0.006 min
Response: 324088
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-E

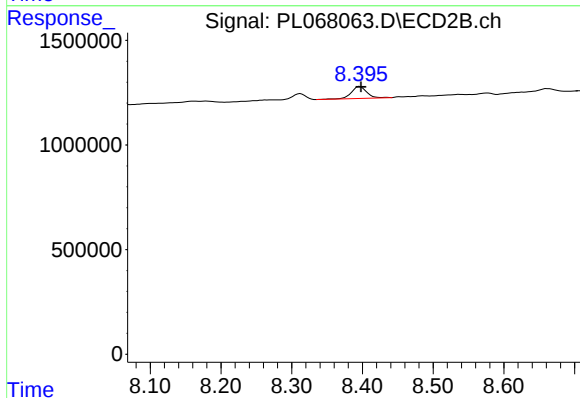


#11 alpha-Chlordane

R.T.: 8.396 min
Delta R.T.: -0.002 min
Response: 873297
Conc: 0.86 ng/ml

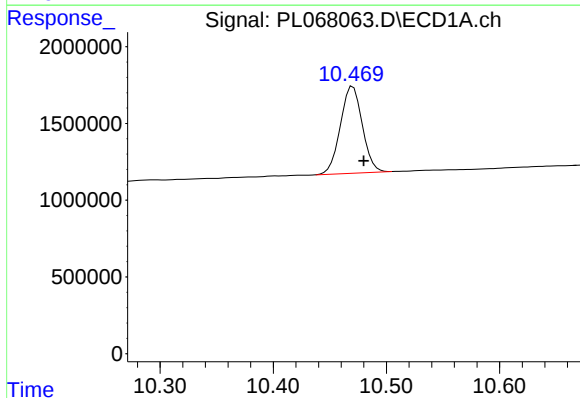

#28 Decachlorobiphenyl

R.T.: 10.470 min
Delta R.T.: -0.010 min
Response: 7632208
Conc: 13.75 ng/ml

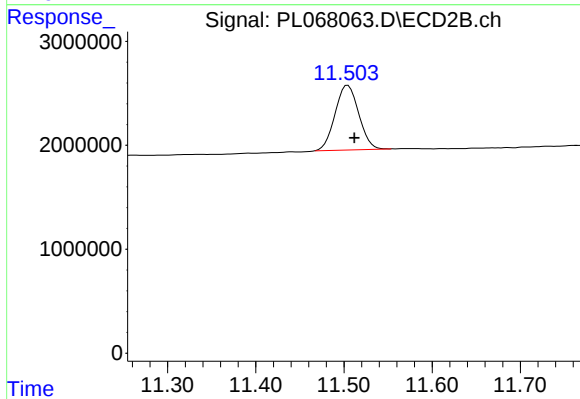

#28 Decachlorobiphenyl

R.T.: 11.504 min
Delta R.T.: -0.007 min
Response: 11592106
Conc: 14.88 ng/ml