

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
 Data File : PL068071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2021 01:30
 Operator : AR\AJ
 Sample : M3001-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N9994

Manual Integrations
 APPROVED

mohammad
 7/13/2021 9:07:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 05:51:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 12 14:08:44 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.674	5.582	5532853	10340914	9.997	10.112
28)	SA Decachlor...	10.473	11.505	7989510	11733699	14.396	15.058
Target Compounds							
11)	B alpha-Chl...	7.466	8.397	498748	1903918	0.754m	1.873 #
17)	MA 4,4'-DDT	8.530	9.437	677586	630103	1.255	0.758 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071221\
Data File : PL068071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2021 01:30
Operator : AR\AJ
Sample : M3001-03
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
N9994


Manual Integrations
APPROVED

mohammad
7/13/2021 9:07:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 05:51:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Mon Jul 12 14:08:44 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

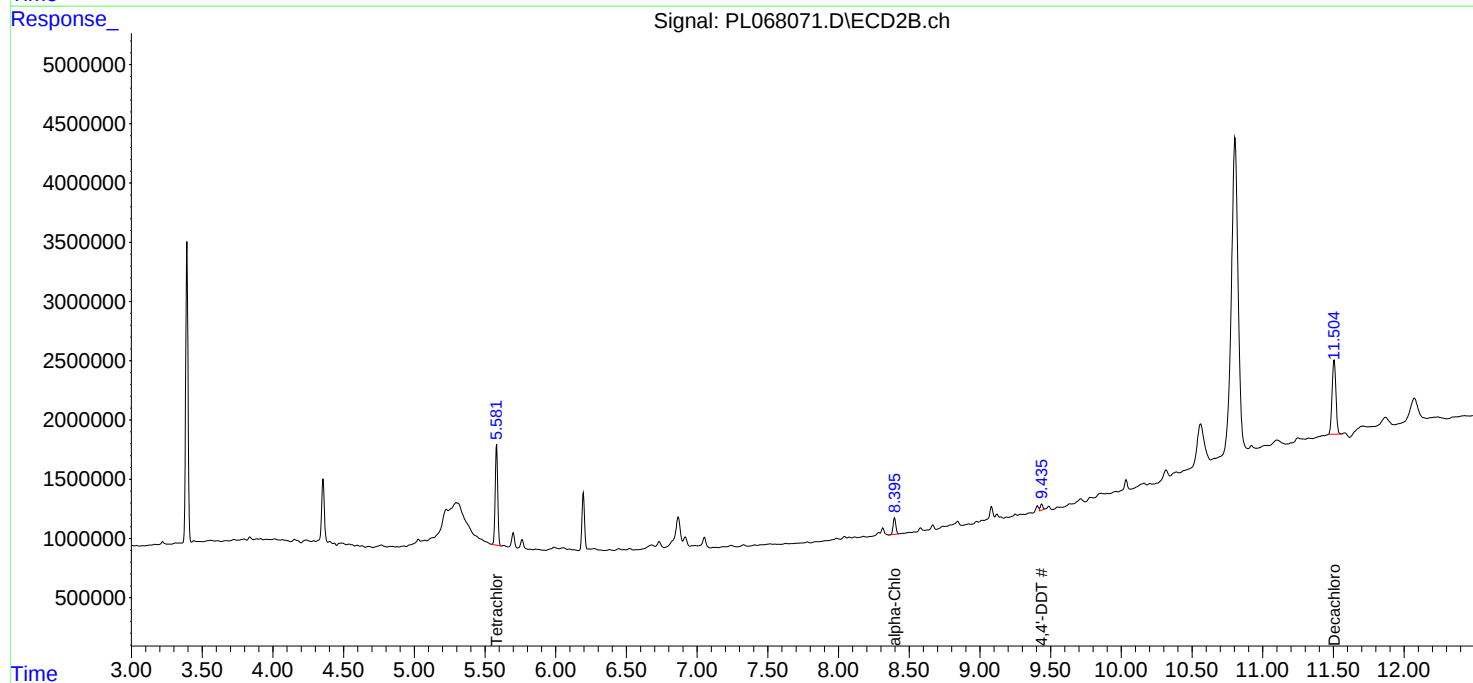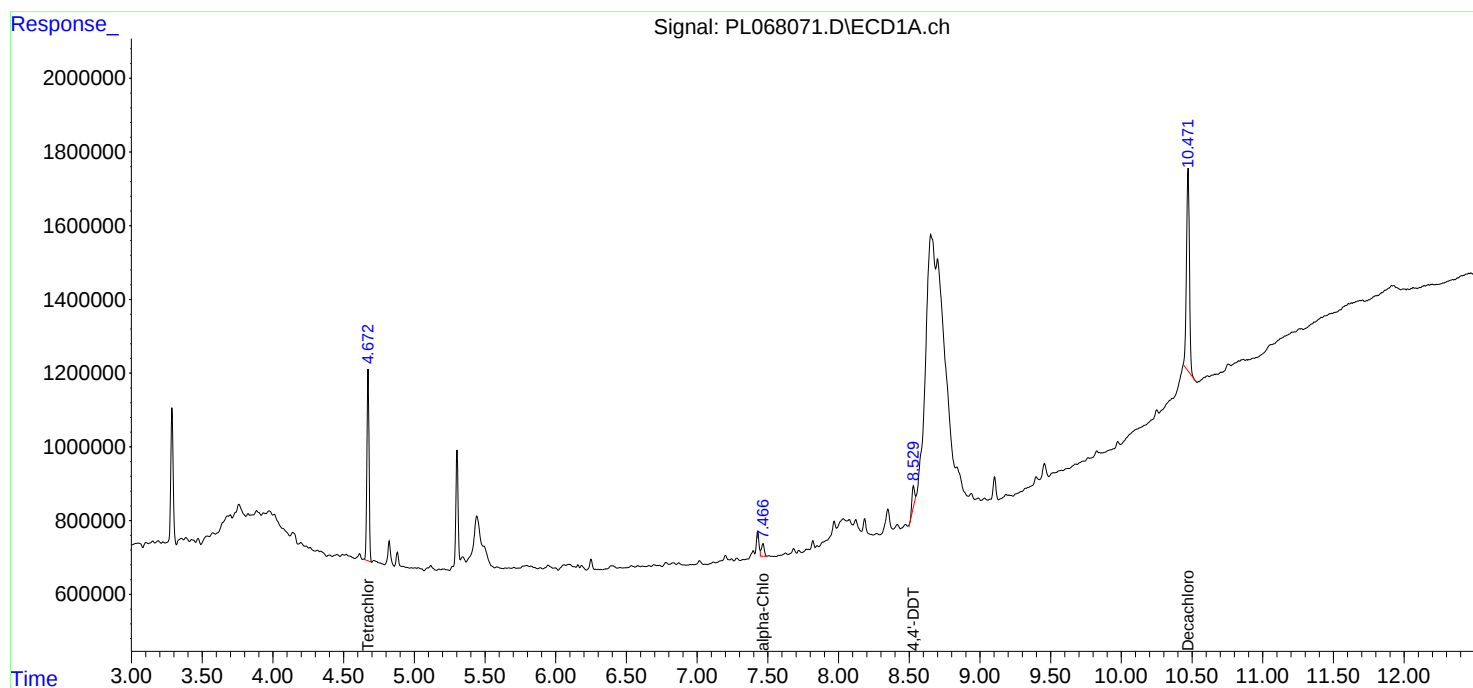

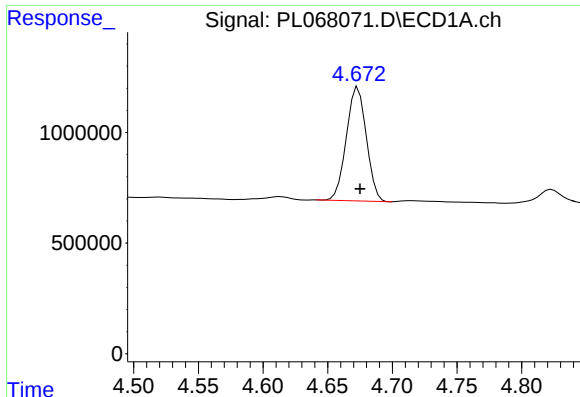


#1 Tetrachloro-m-xylene

R.T.: 4.674 min
Delta R.T.: -0.001 min
Response: 5532853
Conc: 10.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
N9994


Manual Integrations
APPROVED

mohammad
7/13/2021 9:07:45 AM

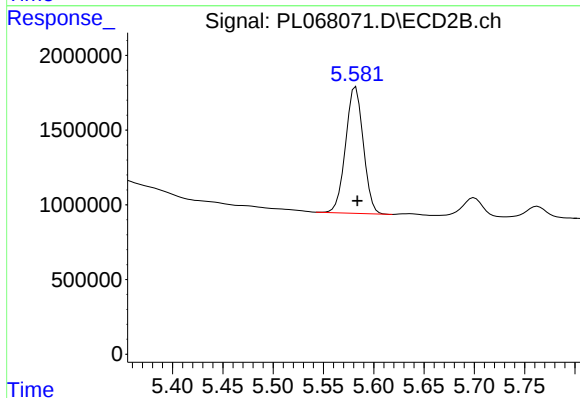


#1 Tetrachloro-m-xylene

R.T.: 5.582 min
Delta R.T.: -0.002 min
Response: 10340914
Conc: 10.11 ng/ml

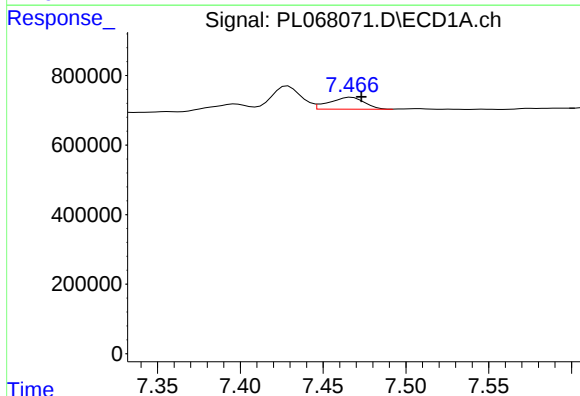


#11 alpha-Chlordane

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 498748
Conc: 0.75 ng/ml m

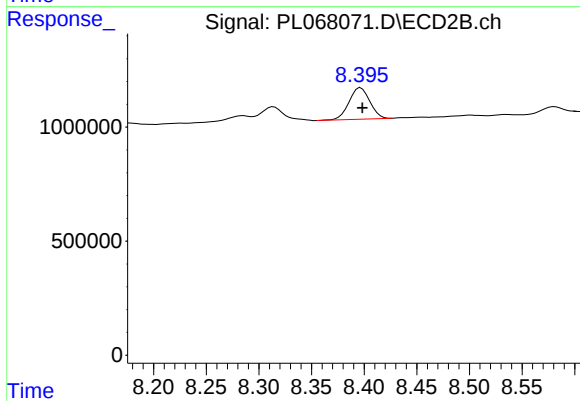

#11 alpha-Chlordane

R.T.: 8.397 min
Delta R.T.: -0.002 min
Response: 1903918
Conc: 1.87 ng/ml

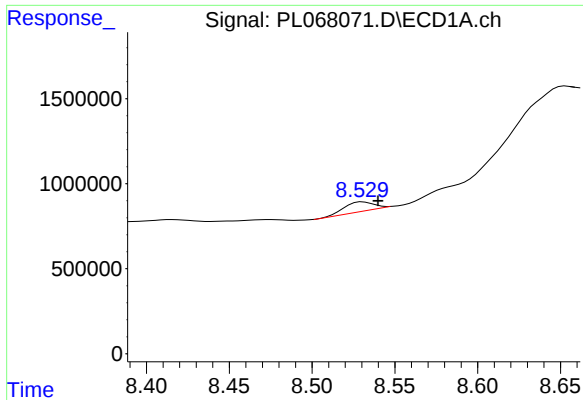


#17 4,4'-DDT

R.T.: 8.530 min
Delta R.T.: -0.010 min
Response: 677586
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
N9994


Manual Integrations
APPROVED

mohammad
7/13/2021 9:07:45 AM

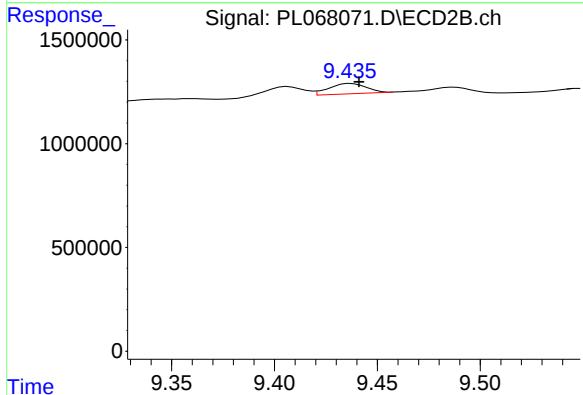


#17 4,4'-DDT

R.T.: 9.437 min
Delta R.T.: -0.004 min
Response: 630103
Conc: 0.76 ng/ml

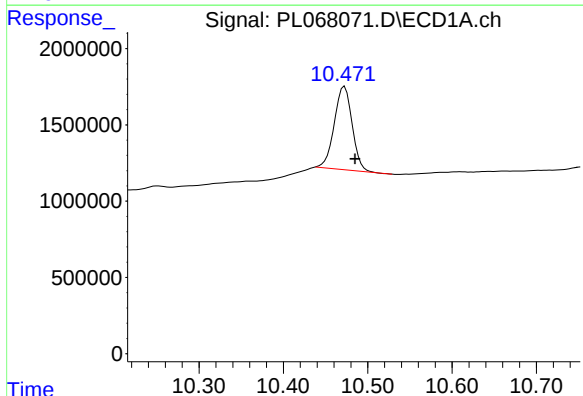

#28 Decachlorobiphenyl

R.T.: 10.473 min
Delta R.T.: -0.012 min
Response: 7989510
Conc: 14.40 ng/ml

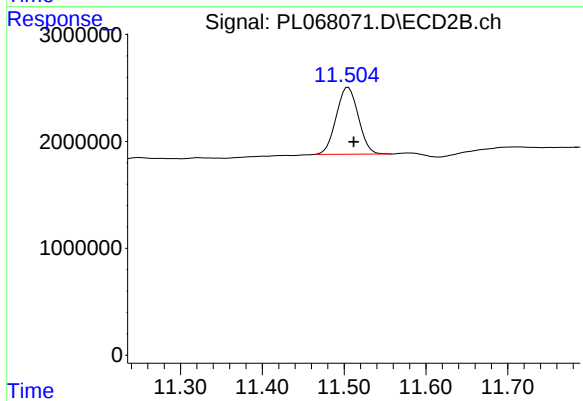

#28 Decachlorobiphenyl

R.T.: 11.505 min
Delta R.T.: -0.007 min
Response: 11733699
Conc: 15.06 ng/ml