

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071222\
 Data File : PL076376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2022 10:25
 Operator : AR\AJ
 Sample : L.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 14:11:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.627	15018707	38184916	20.848	18.886
28)	SA Decachlor...	11.633	10.367	8776599	29188301	14.877	17.395
Target Compounds							
7)	B delta-BHC	7.121f	6.392	550841	588181	0.823	0.246 #
10)	B gamma-Chl...	0.000	7.328	0	294517	N.D.	0.148 #
11)	B alpha-Chl...	0.000	7.394	0	153677	N.D.	0.076 #
15)	B Endosulfa...	9.302	0.000	737881	0	1.235	N.D. #
17)	MA 4,4'-DDT	0.000	8.452	0	120863	N.D.	0.077 #
21)	B Endrin ke...	10.185f	0.000	448705	0	0.664	N.D. #
22)	Mirex	10.668f	0.000	1078248	0	2.108	N.D. #
25)	Chlordane-3	0.000	7.328	0	294517	N.D.	1.739 #
26)	Chlordane-4	0.000	7.394	0	153677	N.D.	0.833 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071222\
Data File : PL076376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2022 10:25
Operator : AR\AJ
Sample : L.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 14:11:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

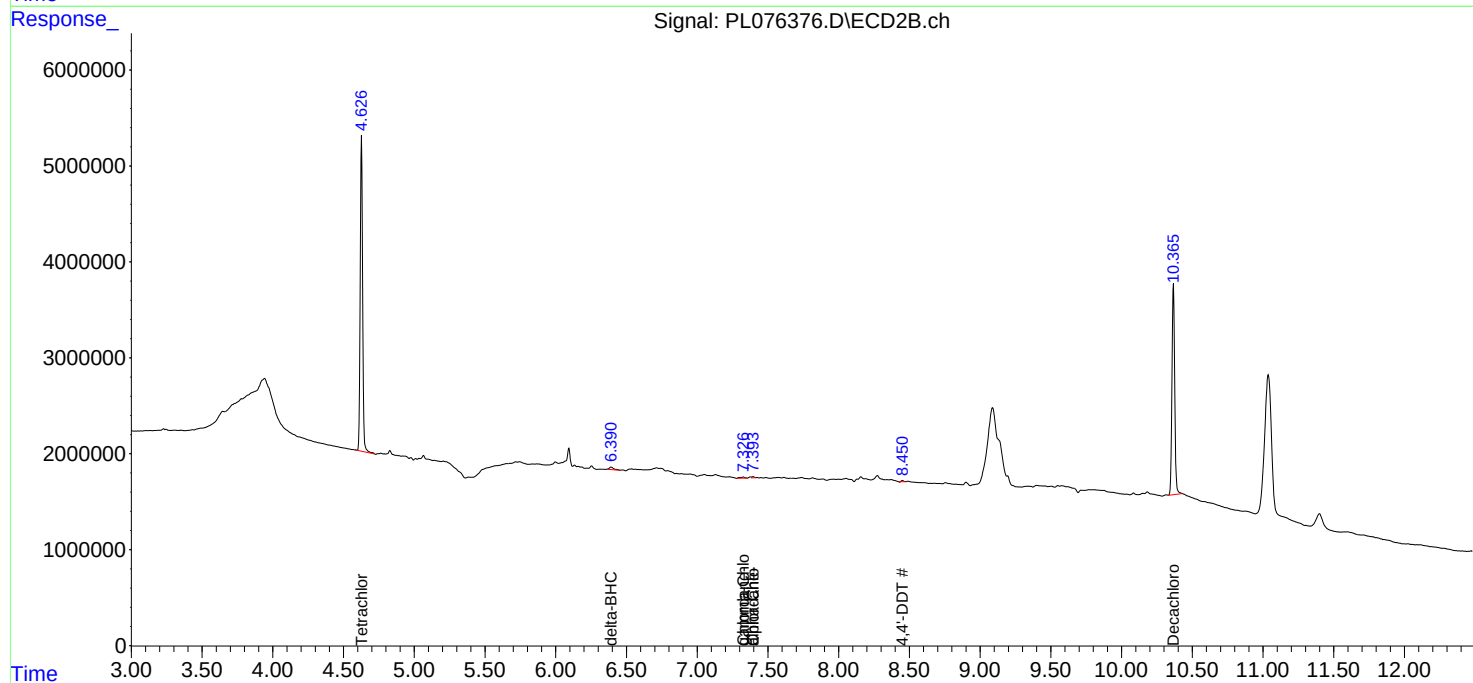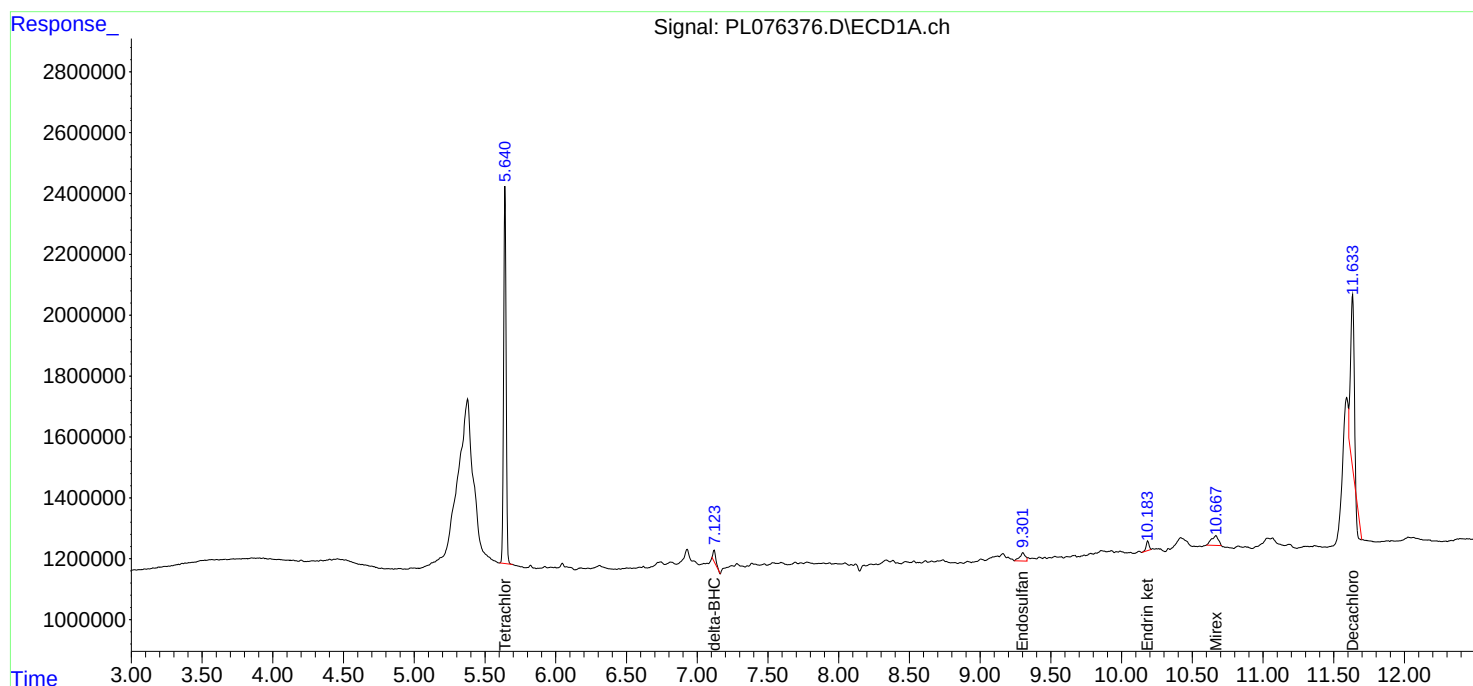


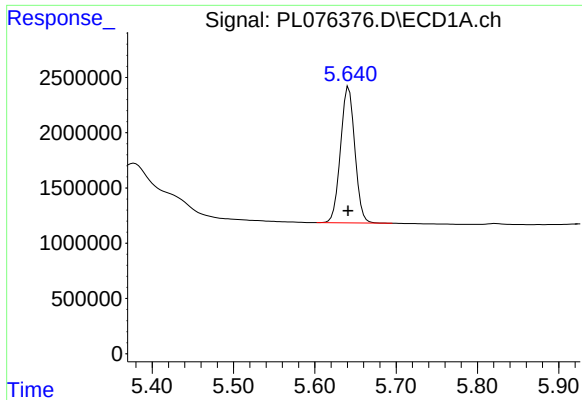

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.000 min
Response: 15018707
Conc: 20.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

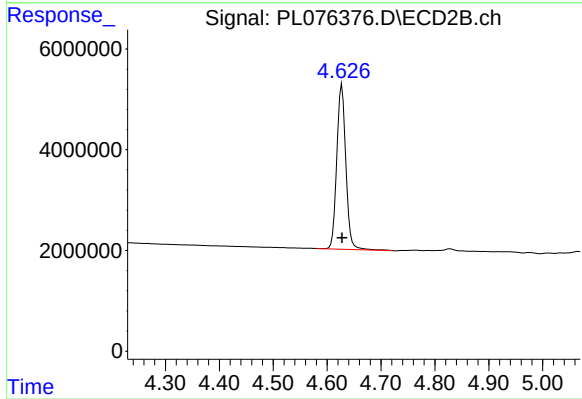


#1 Tetrachloro-m-xylene

R.T.: 4.627 min
Delta R.T.: 0.000 min
Response: 38184916
Conc: 18.89 ng/ml

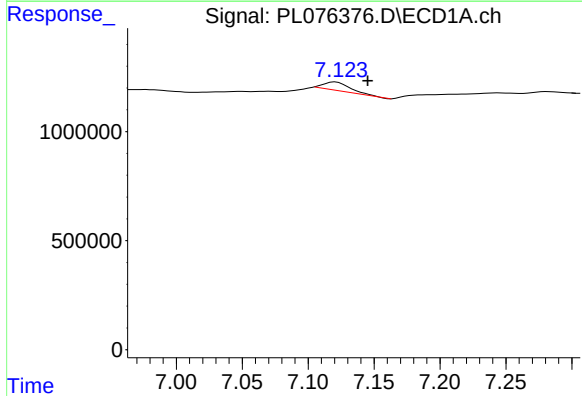


#7 delta-BHC

R.T.: 7.121 min
Delta R.T.: -0.024 min
Response: 550841
Conc: 0.82 ng/ml

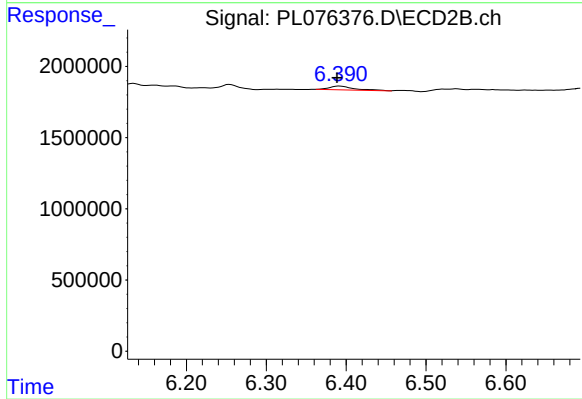

#7 delta-BHC


R.T.: 6.392 min
Delta R.T.: 0.003 min
Response: 588181
Conc: 0.25 ng/ml

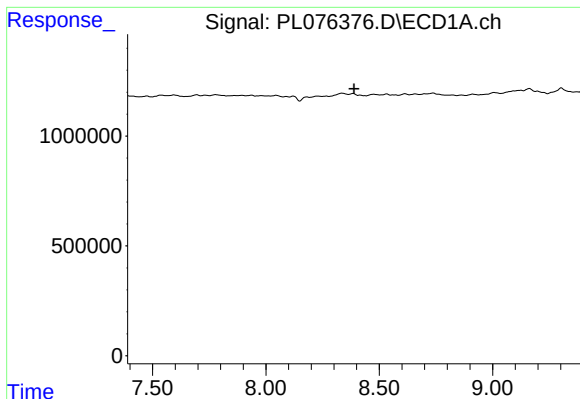

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

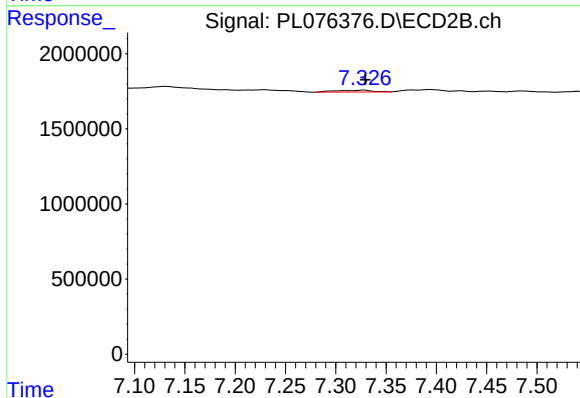


#10 gamma-Chlordane

R.T.: 7.328 min
Delta R.T.: -0.002 min
Response: 294517
Conc: 0.15 ng/ml

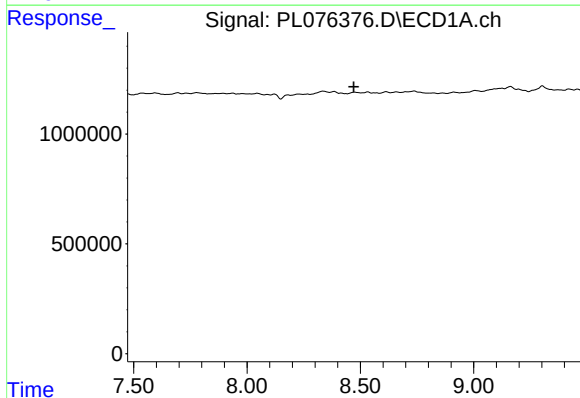


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 8.471 min
Response: 0
Conc: N.D.

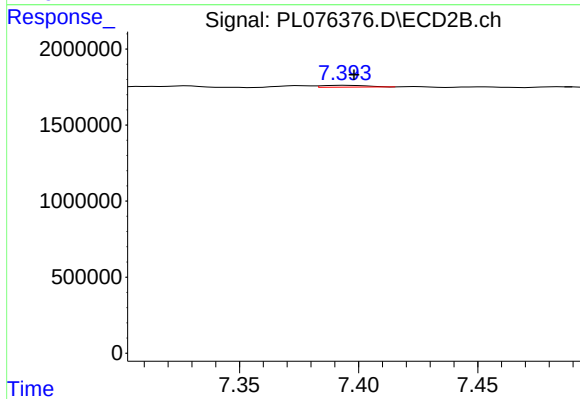

#11 alpha-Chlordane


R.T.: 7.394 min
Delta R.T.: -0.004 min
Response: 153677
Conc: 0.08 ng/ml

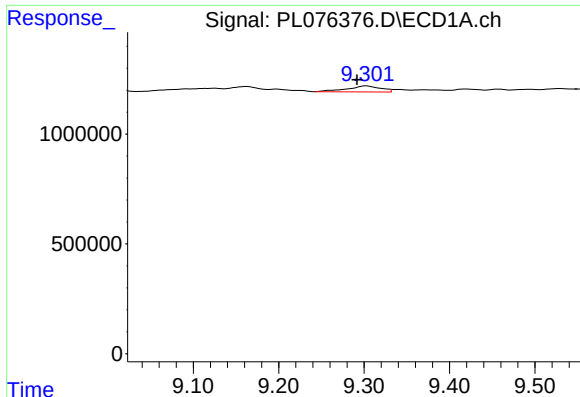

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.011 min
Response: 737881
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

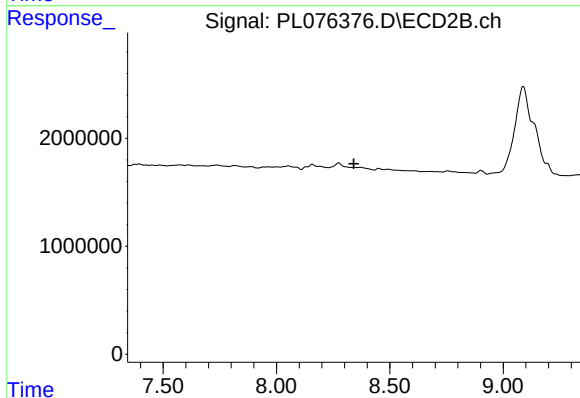


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.340 min
Response: 0
Conc: N.D.

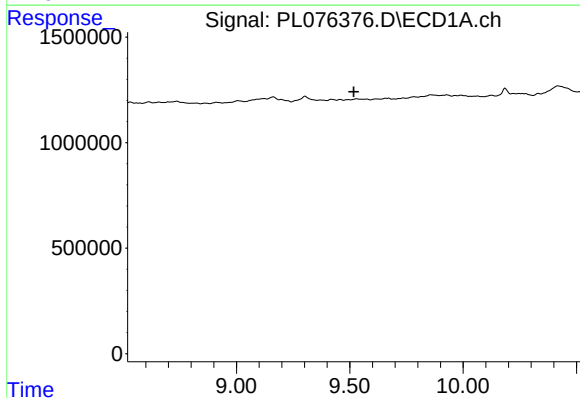


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.517 min
Response: 0
Conc: N.D.

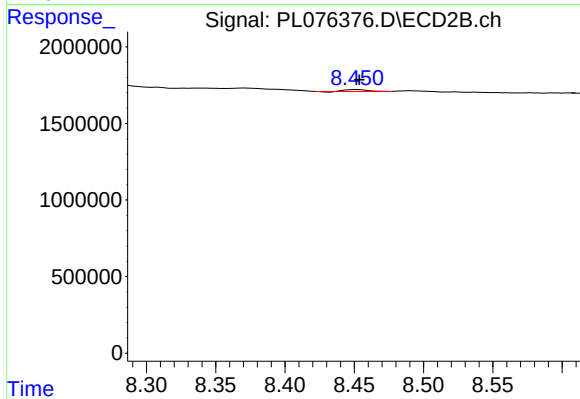

#17 4,4'-DDT


R.T.: 8.452 min
Delta R.T.: -0.002 min
Response: 120863
Conc: 0.08 ng/ml

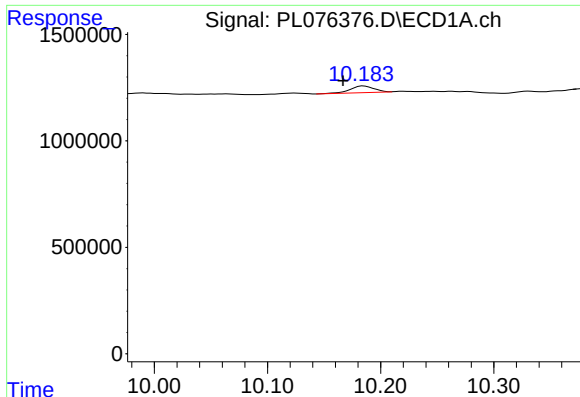

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.018 min
Response: 448705
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

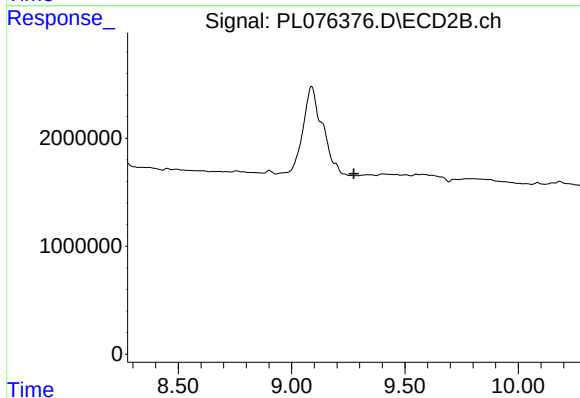


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.275 min
Response: 0
Conc: N.D.

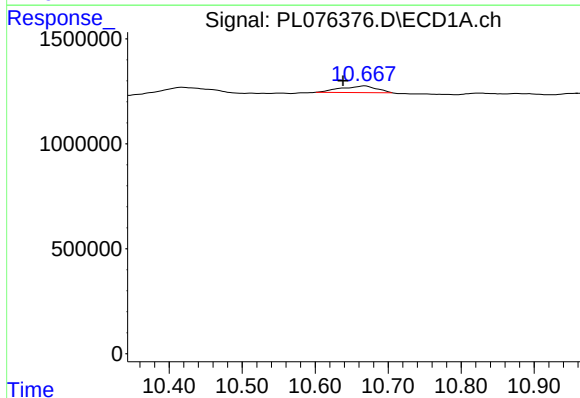


#22 Mirex

R.T.: 10.668 min
Delta R.T.: 0.030 min
Response: 1078248
Conc: 2.11 ng/ml

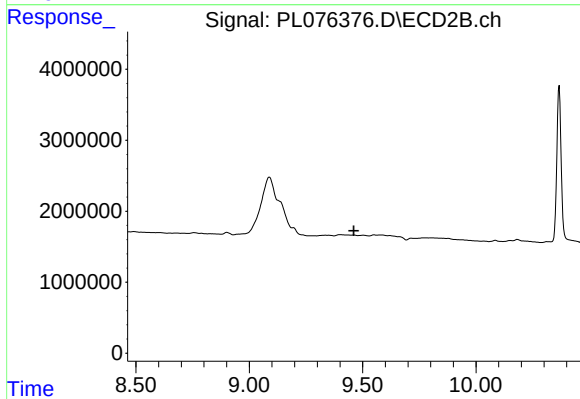

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.460 min
Response: 0
Conc: N.D.

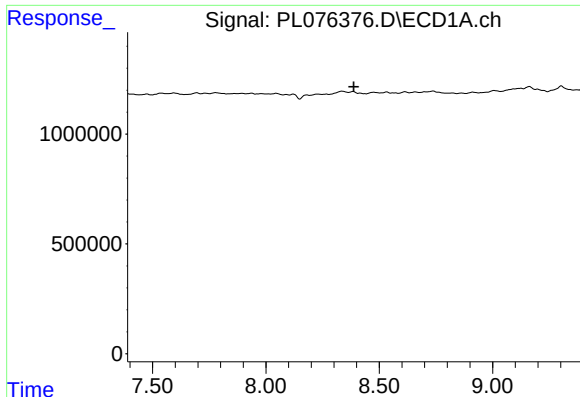

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 8.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

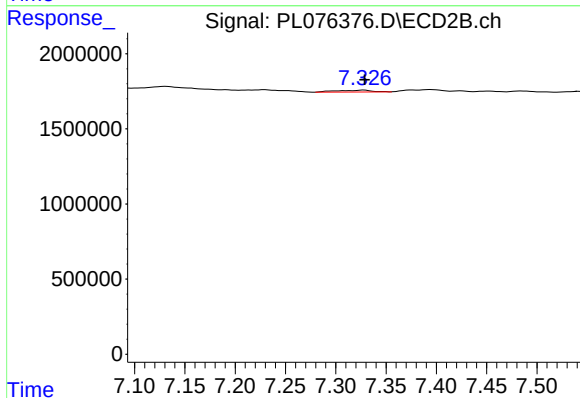


#25 Chlordane-3

R.T.: 7.328 min
Delta R.T.: 0.000 min
Response: 294517
Conc: 1.74 ng/ml

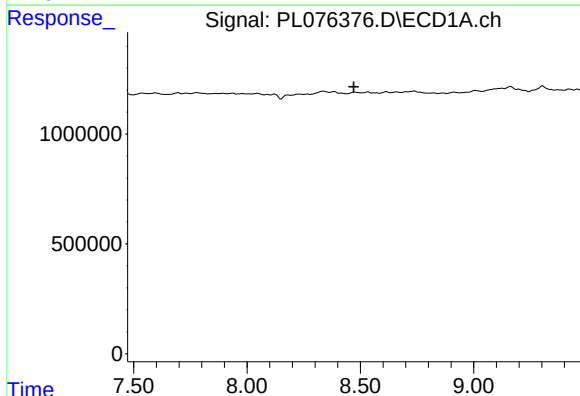


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

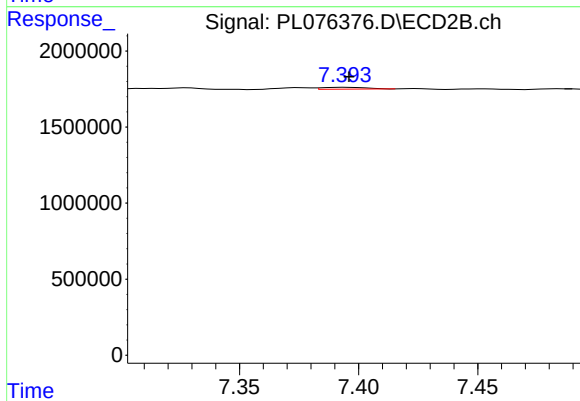

#26 Chlordane-4


R.T.: 7.394 min
Delta R.T.: -0.001 min
Response: 153677
Conc: 0.83 ng/ml

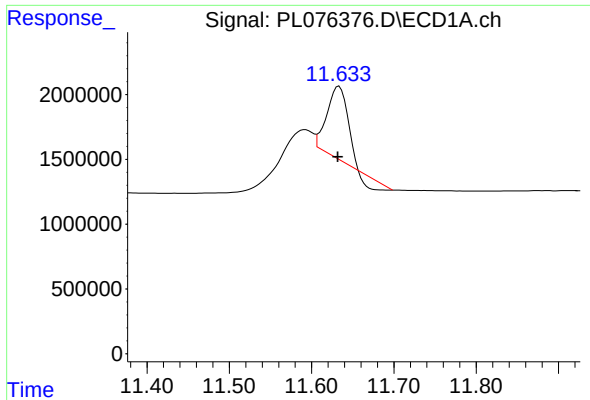

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.002 min
Response: 8776599
Conc: 14.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

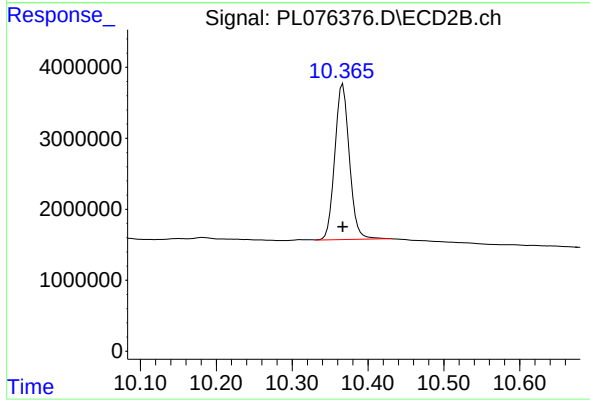

#28 Decachlorobiphenyl

R.T.: 10.367 min
Delta R.T.: 0.000 min
Response: 29188301
Conc: 17.40 ng/ml