

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
 Data File : PL083817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 11:18
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:00:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 13:00:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	2.683	195.8E6	336.7E6	104.466	103.860
28)	SA Decachlor...	9.018	7.871	112.1E6	117.7E6	96.886	100.098
Target Compounds							
23)	Chlordane-1	4.641	3.691	835.4E6	417.5E6	1064.407	1056.766
24)	Chlordane-2	5.174	4.271	772.2E6	410.5E6	1020.444	1006.530
25)	Chlordane-3	5.887	4.905	3655.9E6	1367.8E6	1055.757	993.849
26)	Chlordane-4	5.970	4.968	4193.7E6	1437.3E6	1050.802	996.817
27)	Chlordane-5	6.819	5.865	632.5E6	471.4E6	1068.308	1047.076



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
Data File : PL083817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 11:18
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:00:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 13:00:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

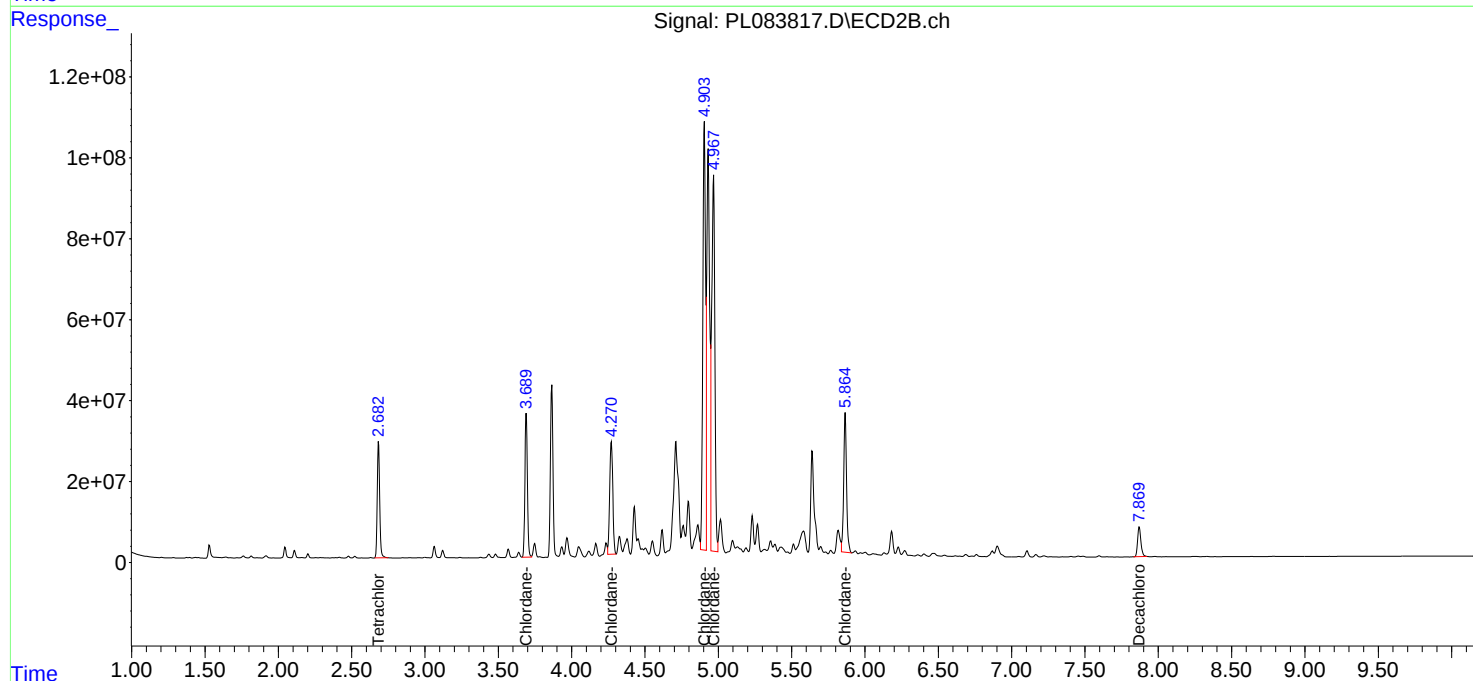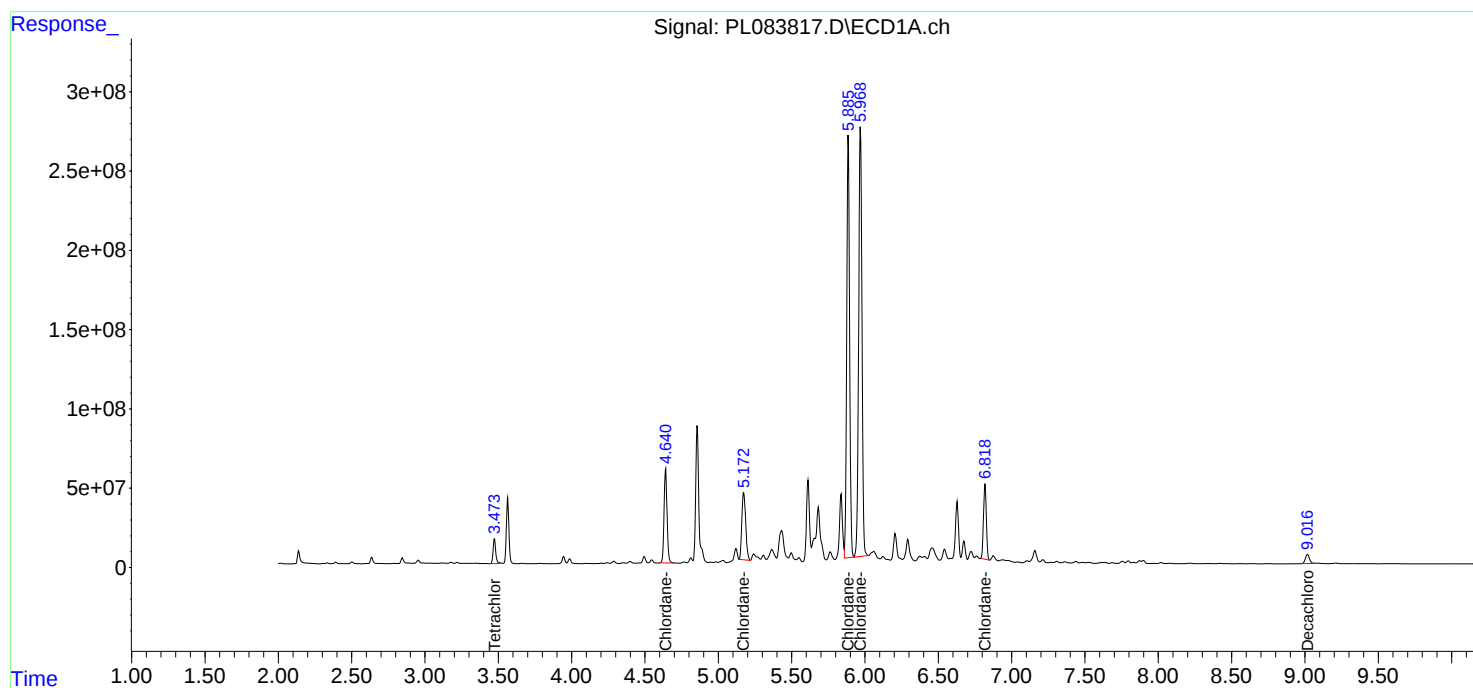


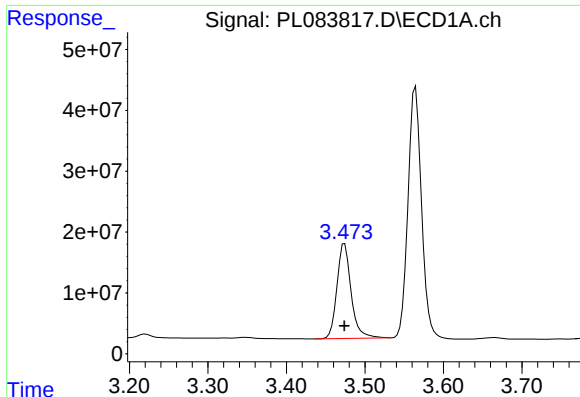

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 195778725
Conc: 104.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

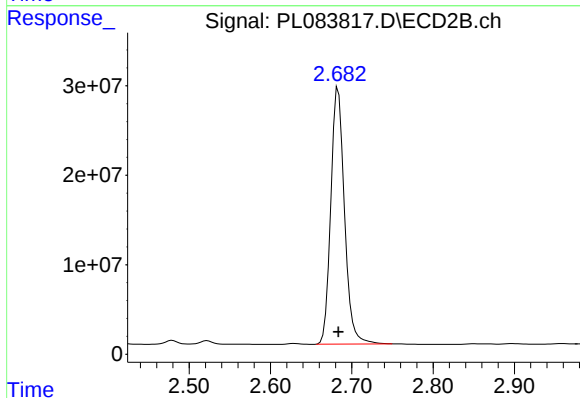


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 336660528
Conc: 103.86 ng/ml

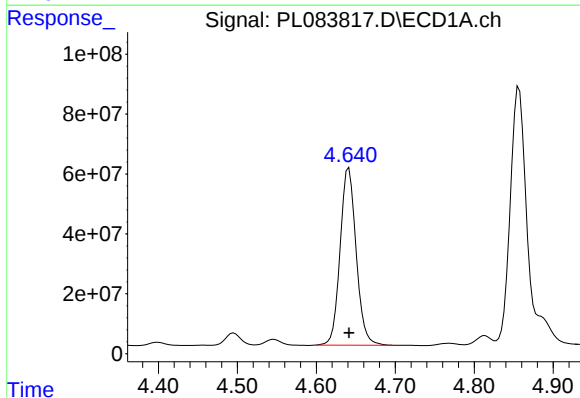


#23 Chlordane-1

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 835430279
Conc: 1064.41 ng/ml

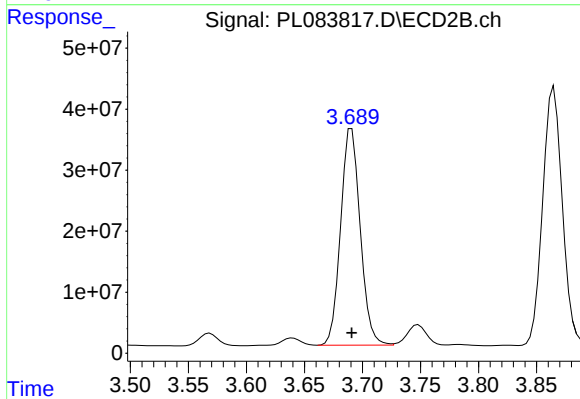

#23 Chlordane-1


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 417453636
Conc: 1056.77 ng/ml

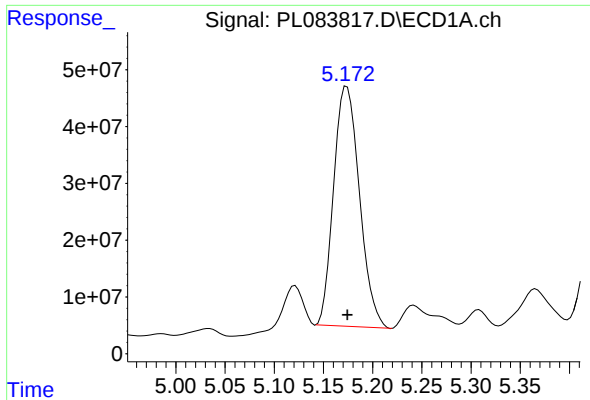

#24 Chlordane-2


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 772151399
Conc: 1020.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

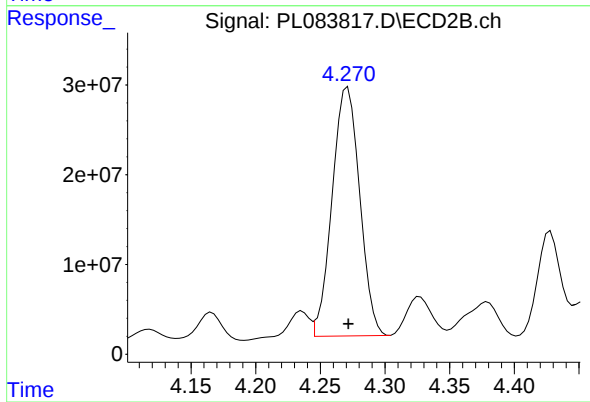


#24 Chlordane-2

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 410546344
Conc: 1006.53 ng/ml

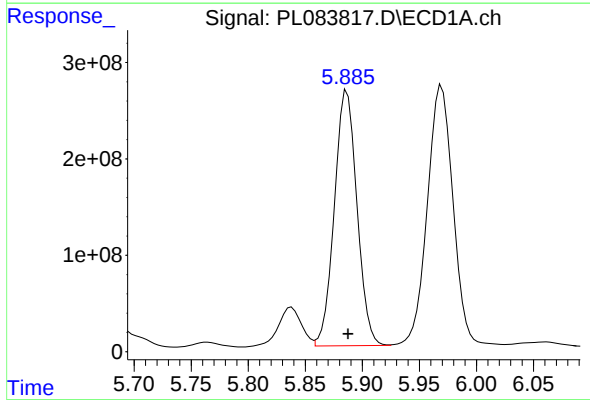


#25 Chlordane-3

R.T.: 5.887 min
Delta R.T.: 0.000 min
Response: 3655881676
Conc: 1055.76 ng/ml

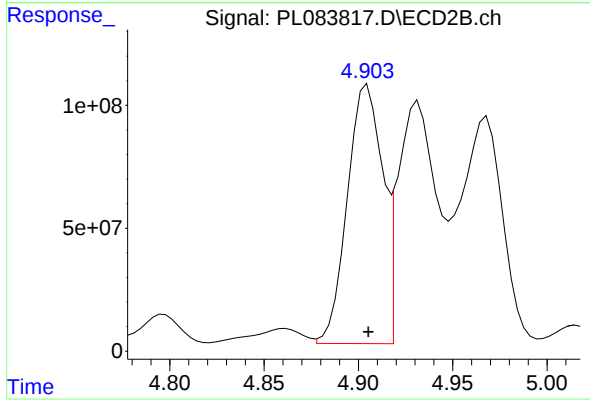

#25 Chlordane-3


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 1367793905
Conc: 993.85 ng/ml

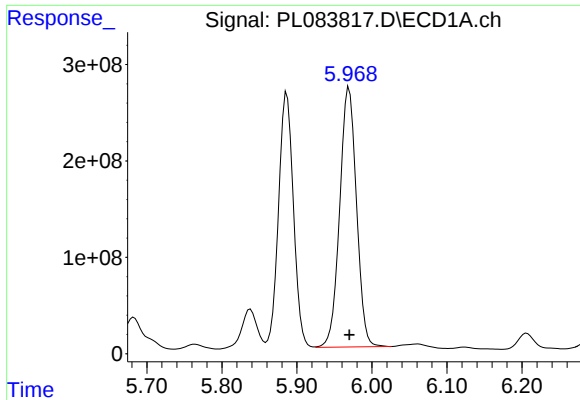

#26 Chlordane-4


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 4193696814
Conc: 1050.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

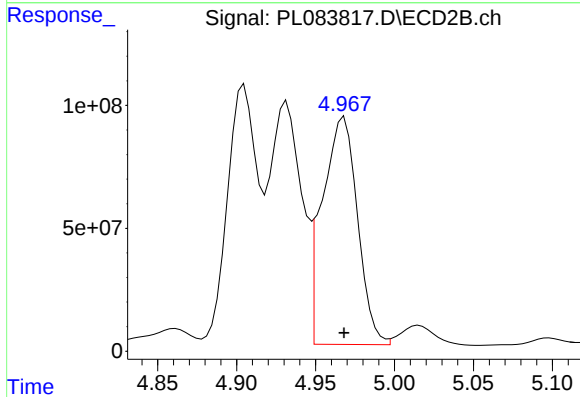


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 1437334809
Conc: 996.82 ng/ml

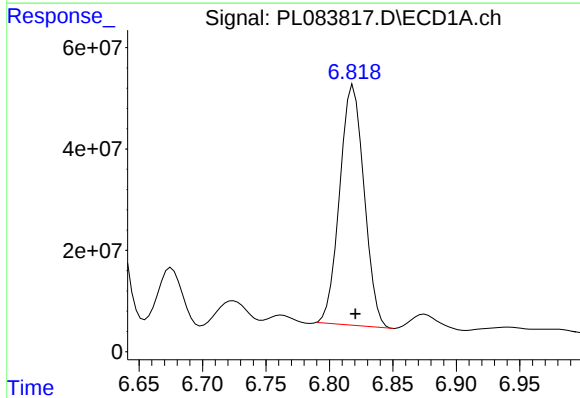


#27 Chlordane-5

R.T.: 6.819 min
Delta R.T.: -0.002 min
Response: 632461550
Conc: 1068.31 ng/ml

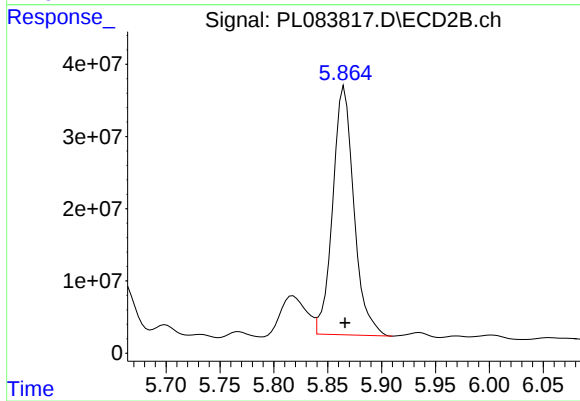

#27 Chlordane-5

R.T.: 5.865 min
Delta R.T.: 0.000 min
Response: 471428977
Conc: 1047.08 ng/ml

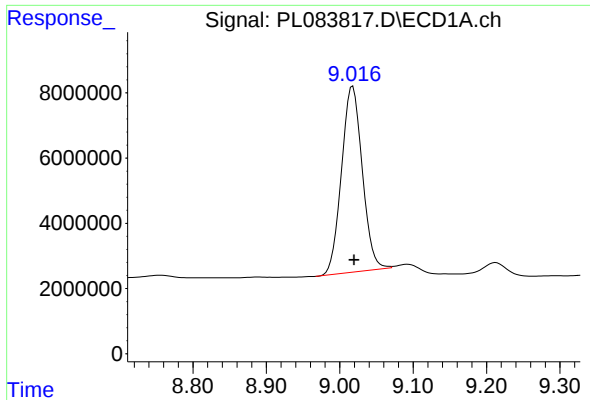

#28 Decachlorobiphenyl


R.T.: 9.018 min

Delta R.T.: -0.002 min

Response: 112089207

Conc: 96.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

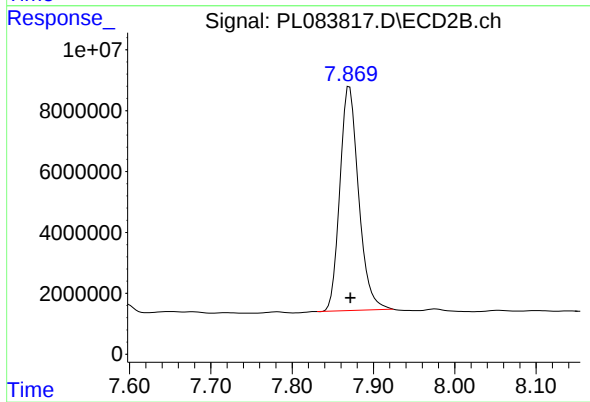

#28 Decachlorobiphenyl

R.T.: 7.871 min

Delta R.T.: 0.000 min

Response: 117659288

Conc: 100.10 ng/ml