

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
 Data File : PL083818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 11:32
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:00:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 13:00:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	2.683	141.4E6	244.9E6	75.447	75.541
28)	SA Decachlor...	9.019	7.871	82912656	86833313	71.667	73.873
Target Compounds							
23)	Chlordane-1	4.641	3.691	599.8E6	300.8E6	764.235	761.447
24)	Chlordane-2	5.175	4.271	563.9E6	302.2E6	745.234	740.919
25)	Chlordane-3	5.887	4.905	2643.5E6	1015.4E6	763.385	737.764
26)	Chlordane-4	5.970	4.968	3040.3E6	1066.4E6	761.801	739.540
27)	Chlordane-5	6.820	5.866	451.5E6	340.9E6	762.661	757.213



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
Data File : PL083818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 11:32
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:00:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 13:00:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

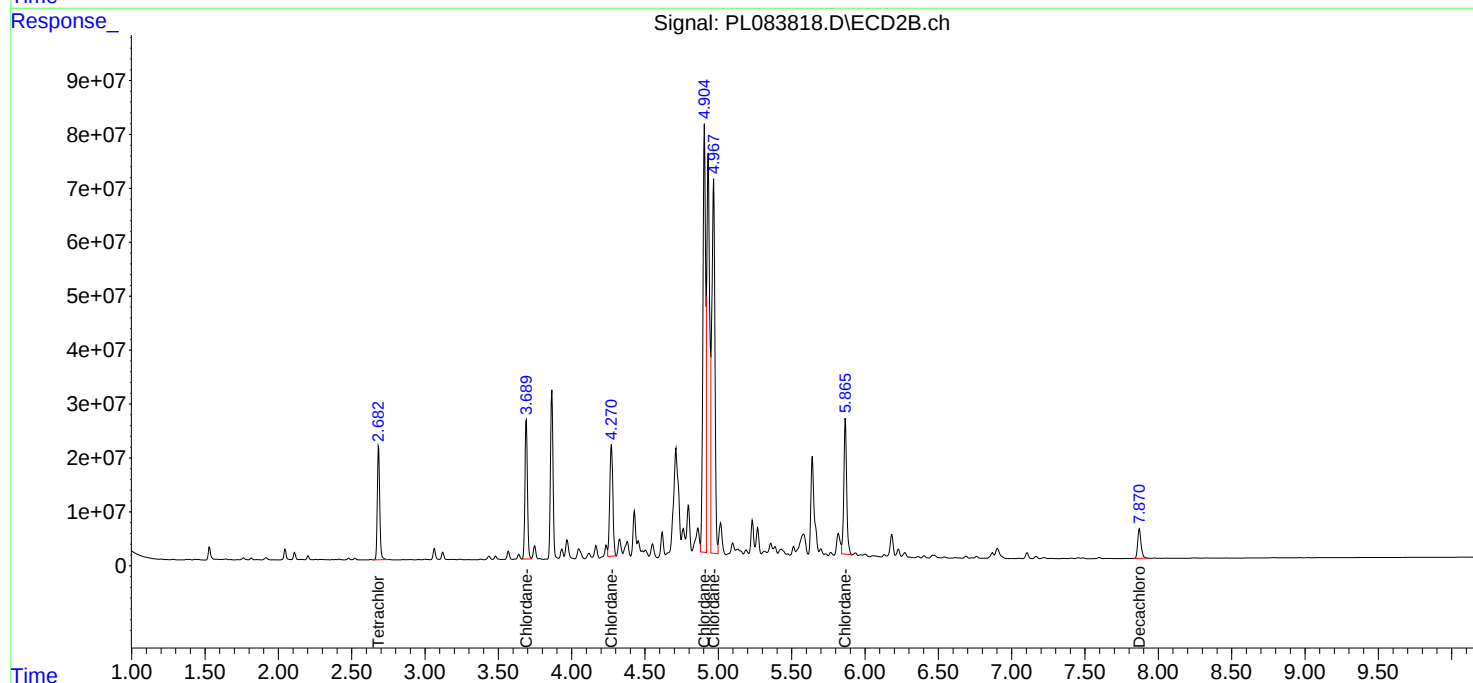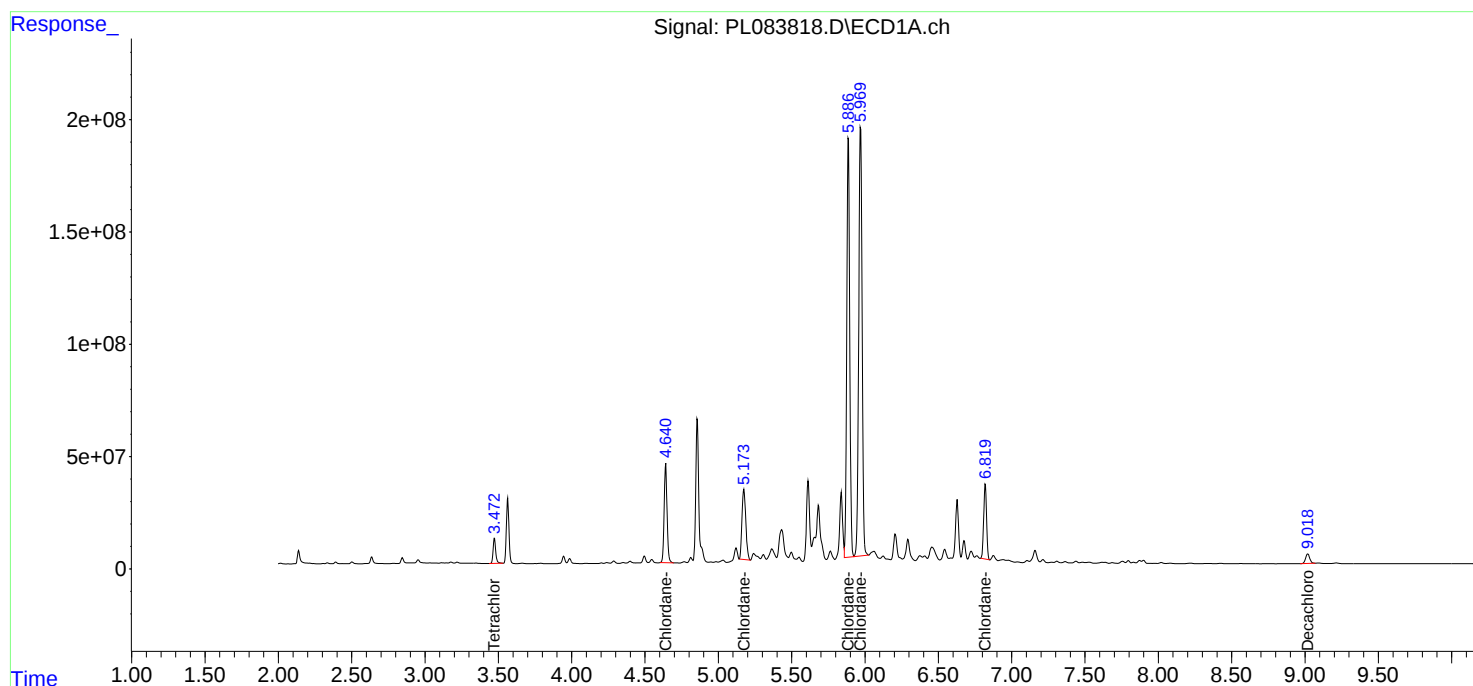


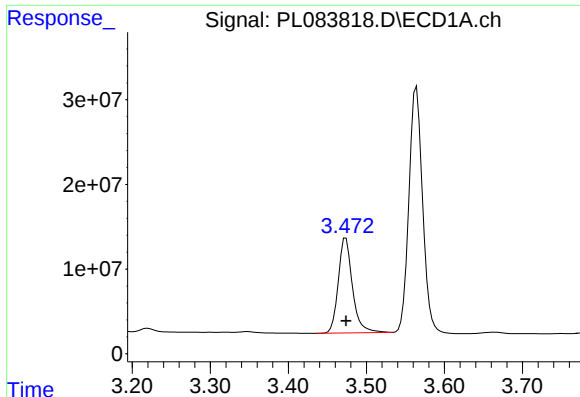

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 141395126
Conc: 75.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

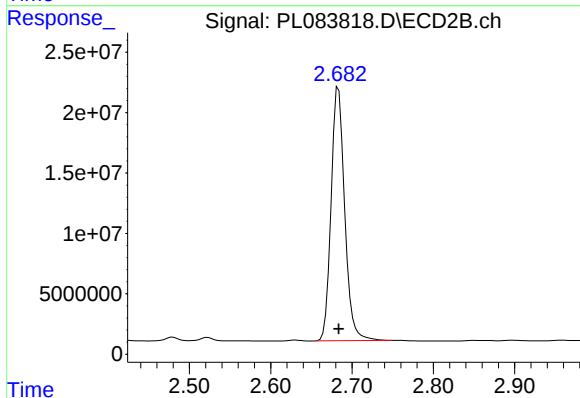


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 244864645
Conc: 75.54 ng/ml

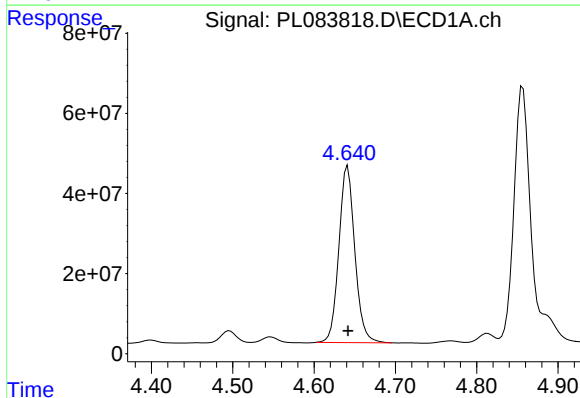


#23 Chlordane-1

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 599831640
Conc: 764.23 ng/ml

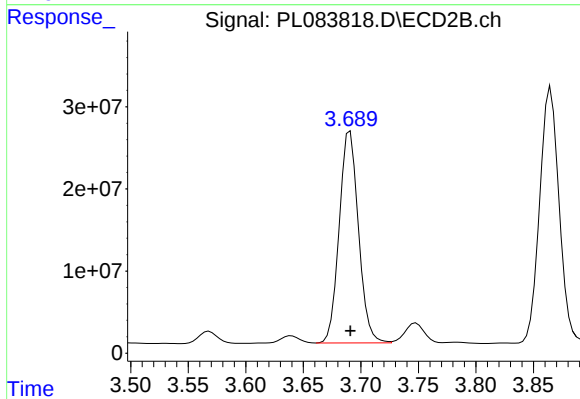

#23 Chlordane-1


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 300793777
Conc: 761.45 ng/ml

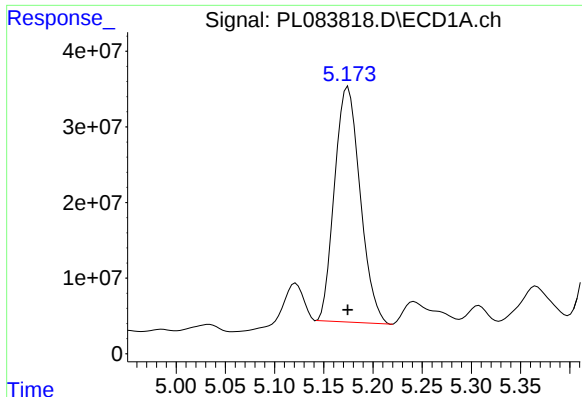

#24 Chlordane-2


R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 563904700
Conc: 745.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

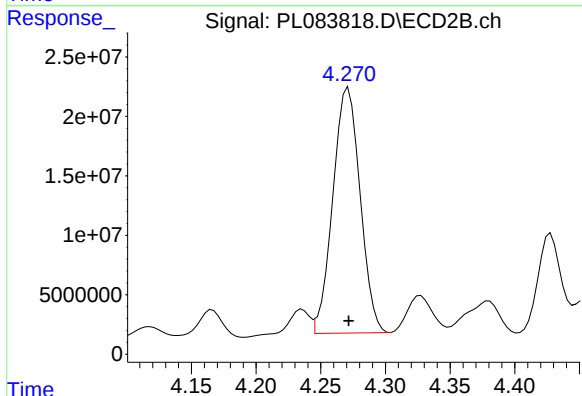


#24 Chlordane-2

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 302208457
Conc: 740.92 ng/ml

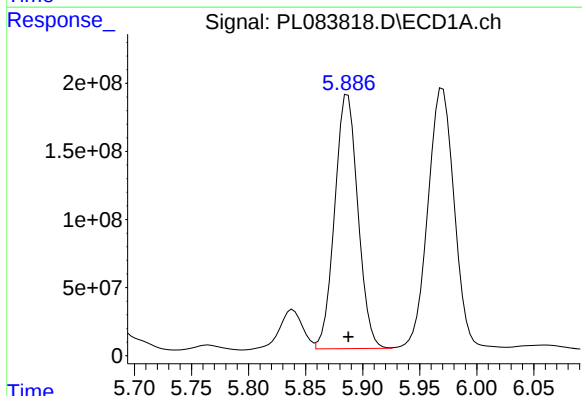


#25 Chlordane-3

R.T.: 5.887 min
Delta R.T.: 0.000 min
Response: 2643454333
Conc: 763.39 ng/ml

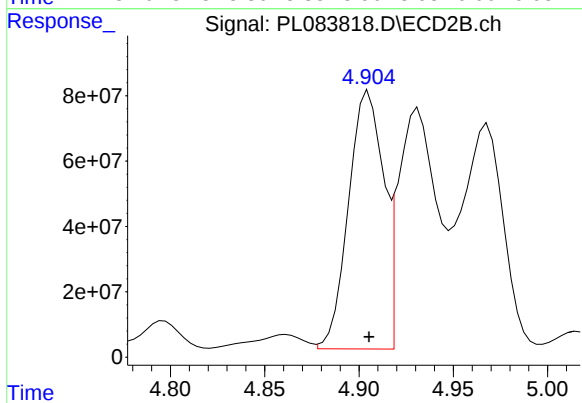

#25 Chlordane-3


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 1015354099
Conc: 737.76 ng/ml

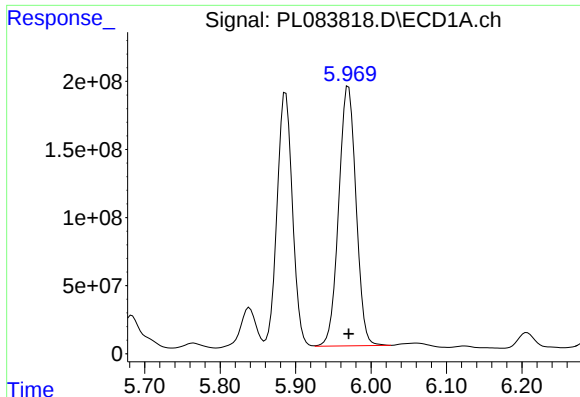

#26 Chlordane-4


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 3040308082
Conc: 761.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

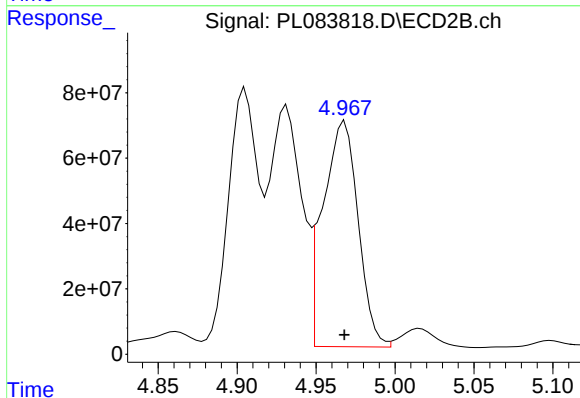


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 1066361278
Conc: 739.54 ng/ml

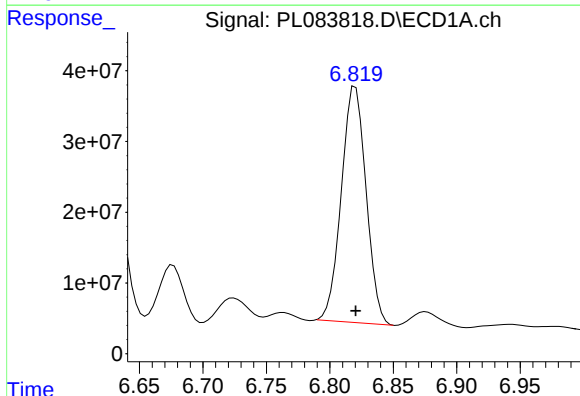


#27 Chlordane-5

R.T.: 6.820 min
Delta R.T.: 0.000 min
Response: 451511781
Conc: 762.66 ng/ml

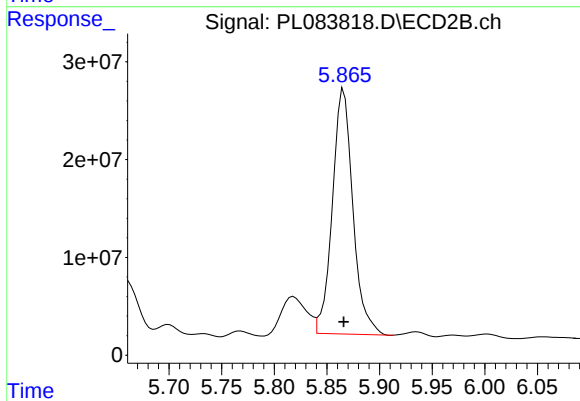

#27 Chlordane-5


R.T.: 5.866 min
Delta R.T.: 0.000 min
Response: 340923006
Conc: 757.21 ng/ml

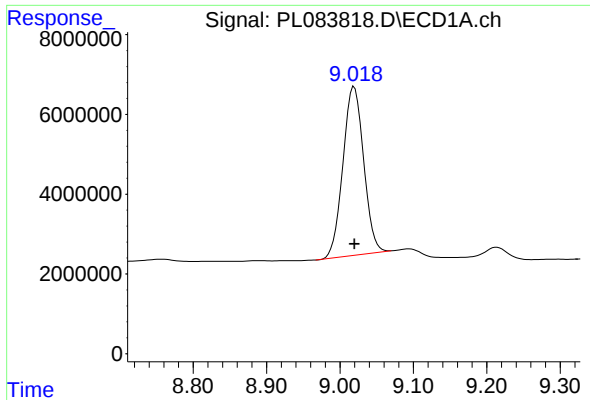

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 82912656
Conc: 71.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

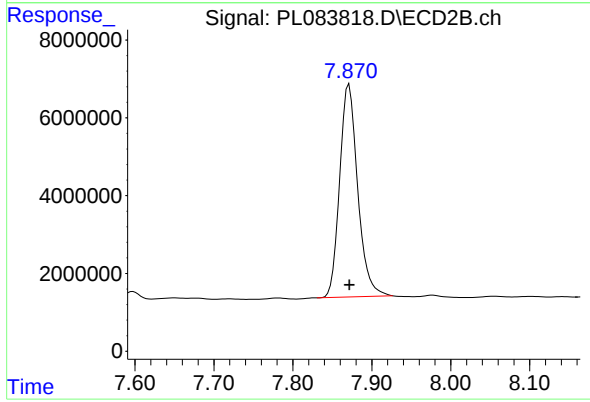

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: 0.000 min
Response: 86833313
Conc: 73.87 ng/ml