

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
 Data File : PL083819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 11:46
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:00:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 13:00:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	2.684	93704581	162.1E6	50.000	50.000
28)	SA Decachlor...	9.020	7.872	57846169	58771906	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.642	3.691	392.4E6	197.5E6	500.000	500.000
24)	Chlordane-2	5.174	4.272	378.3E6	203.9E6	500.000	500.000
25)	Chlordane-3	5.888	4.905	1731.4E6	688.1E6	500.000	500.000
26)	Chlordane-4	5.970	4.968	1995.5E6	721.0E6	500.000	500.000
27)	Chlordane-5	6.821	5.866	296.0E6	225.1E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
Data File : PL083819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 11:46
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:00:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 13:00:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

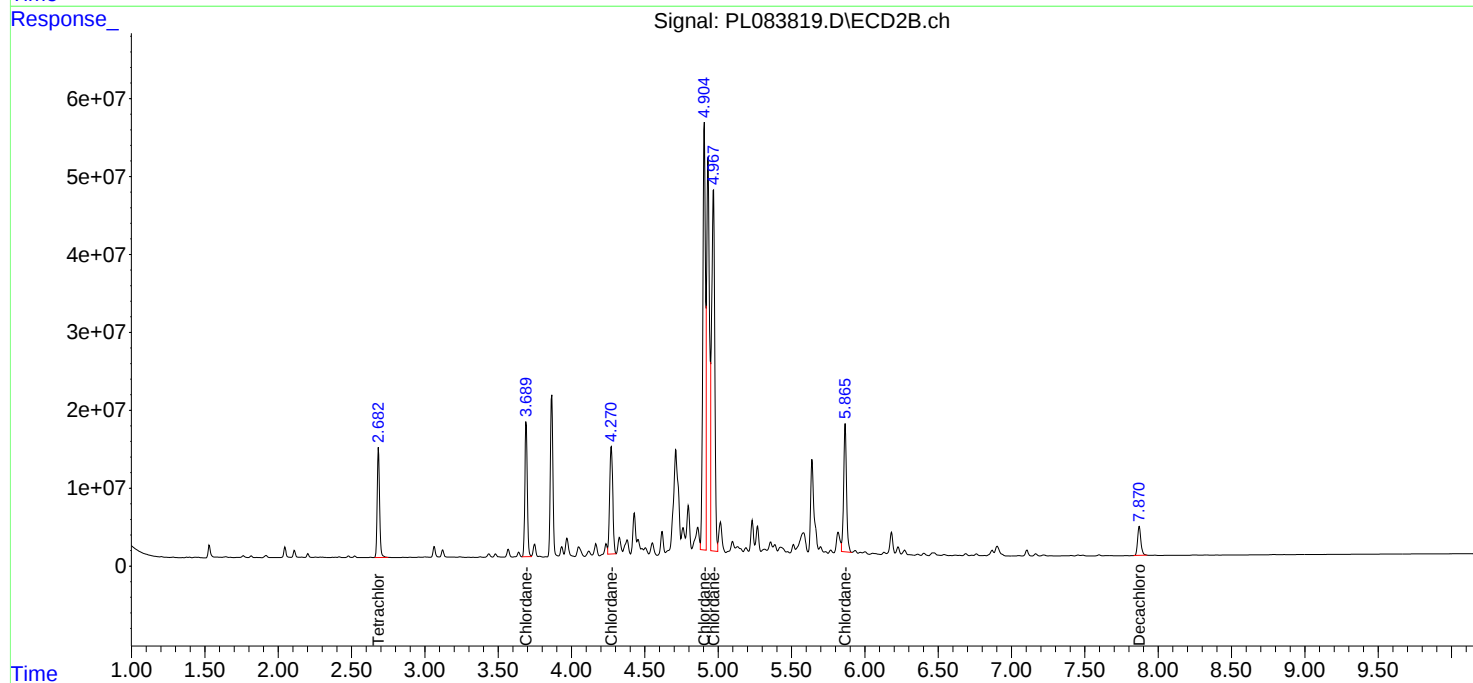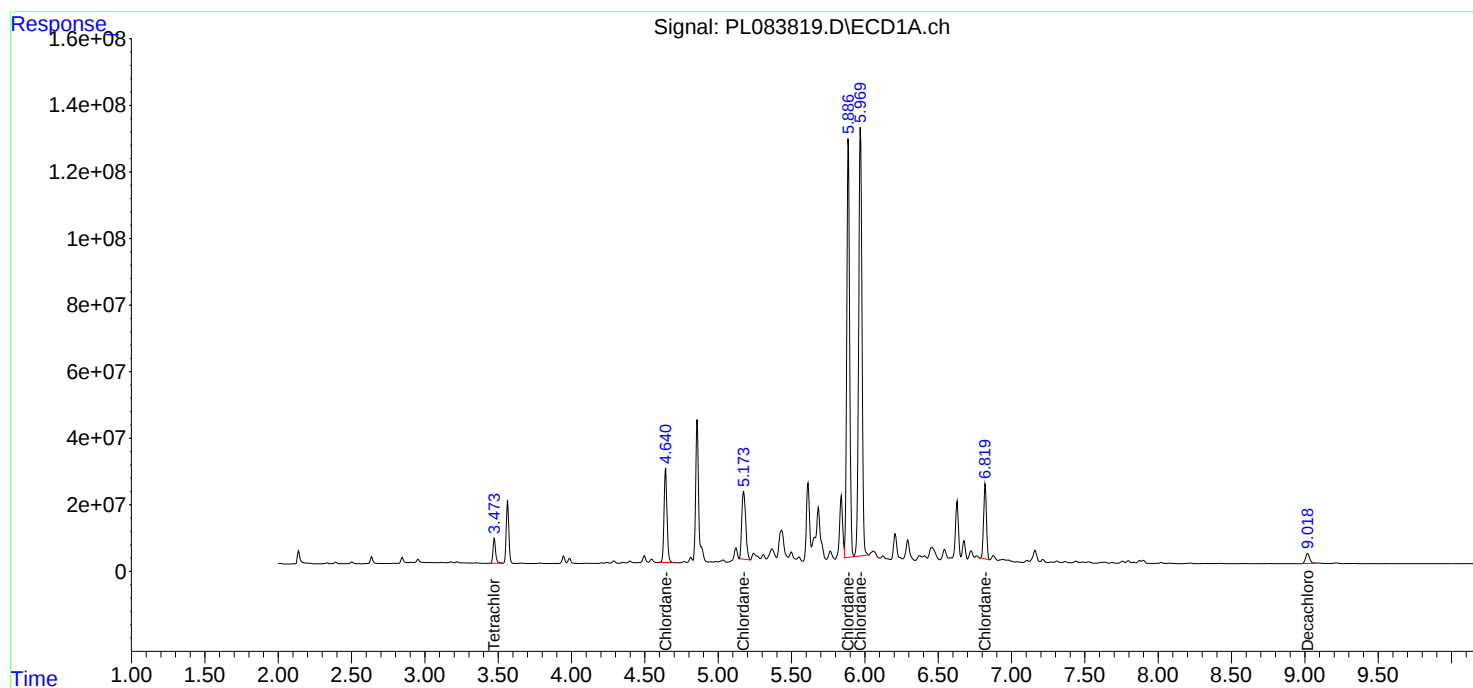


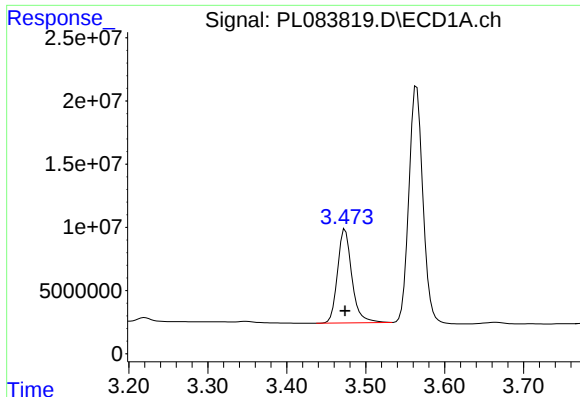

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 93704581
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

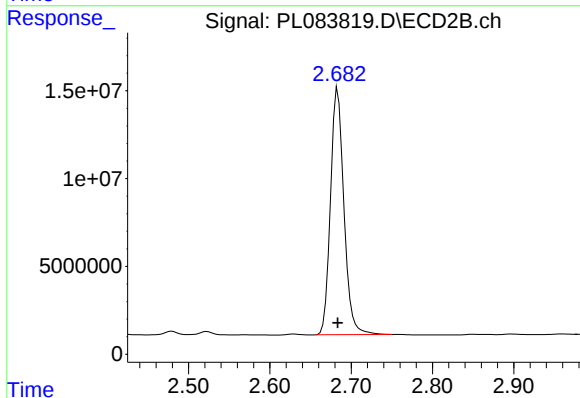


#1 Tetrachloro-m-xylene

R.T.: 2.684 min
Delta R.T.: 0.000 min
Response: 162074236
Conc: 50.00 ng/ml

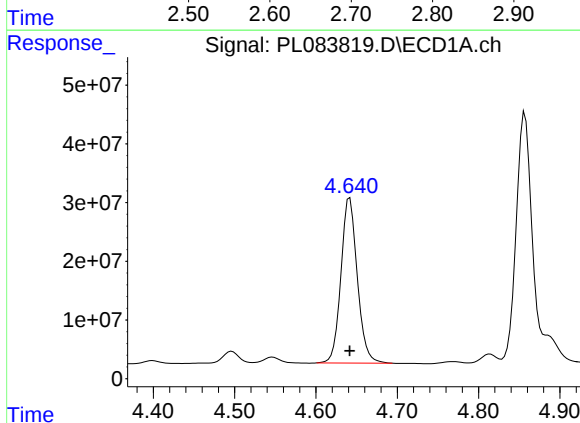


#23 Chlordane-1

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 392439301
Conc: 500.00 ng/ml

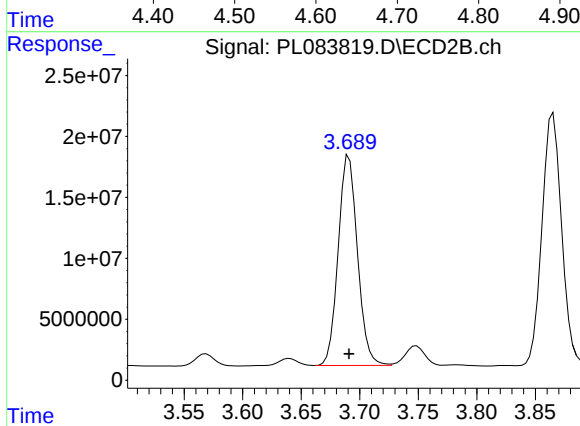

#23 Chlordane-1


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 197514683
Conc: 500.00 ng/ml

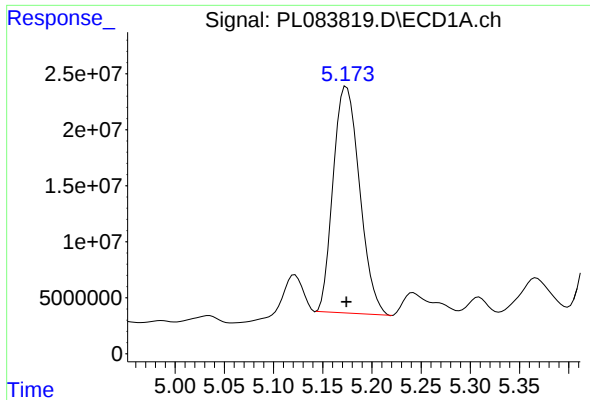

#24 Chlordane-2


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 378340865
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

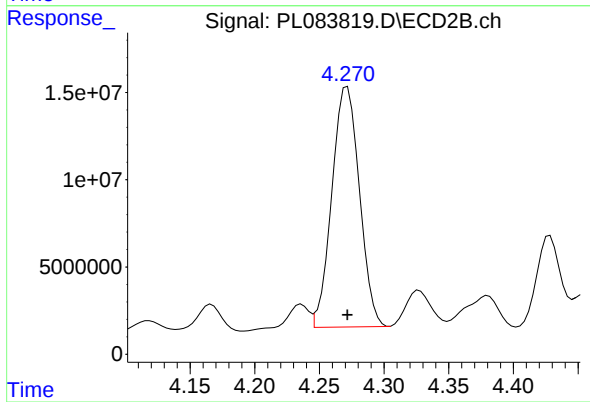


#24 Chlordane-2

R.T.: 4.272 min
Delta R.T.: 0.000 min
Response: 203941509
Conc: 500.00 ng/ml

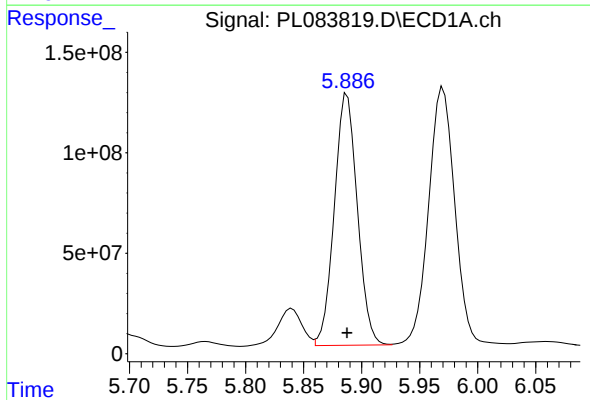


#25 Chlordane-3

R.T.: 5.888 min
Delta R.T.: 0.000 min
Response: 1731402634
Conc: 500.00 ng/ml

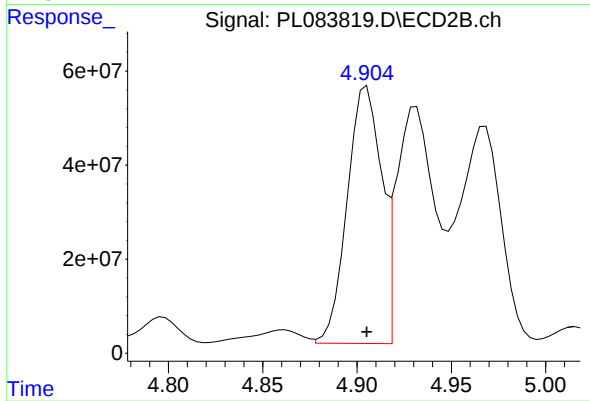

#25 Chlordane-3


R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 688129578
Conc: 500.00 ng/ml

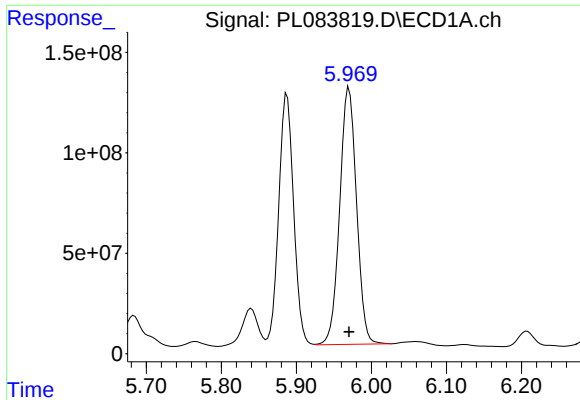

#26 Chlordane-4


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 1995474696
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

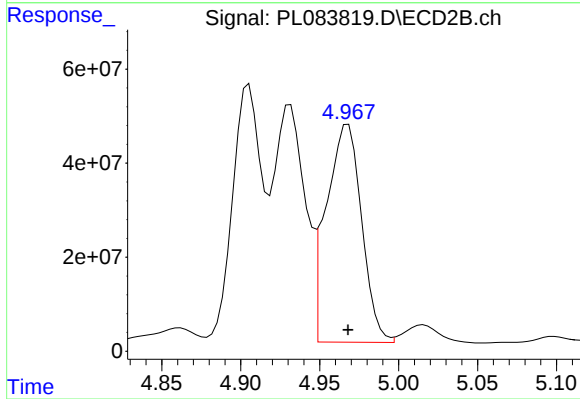


#26 Chlordane-4

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 720962082
Conc: 500.00 ng/ml

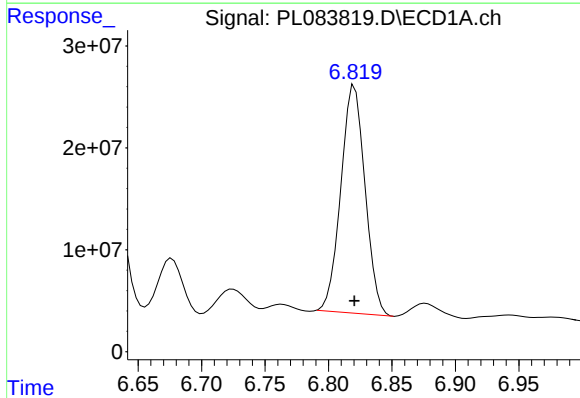


#27 Chlordane-5

R.T.: 6.821 min
Delta R.T.: 0.000 min
Response: 296010916
Conc: 500.00 ng/ml

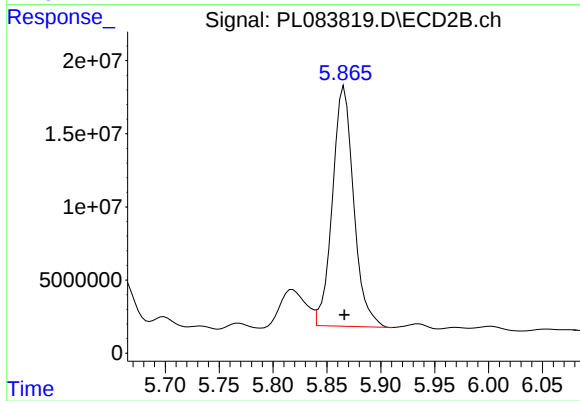

#27 Chlordane-5


R.T.: 5.866 min
Delta R.T.: 0.000 min
Response: 225116980
Conc: 500.00 ng/ml

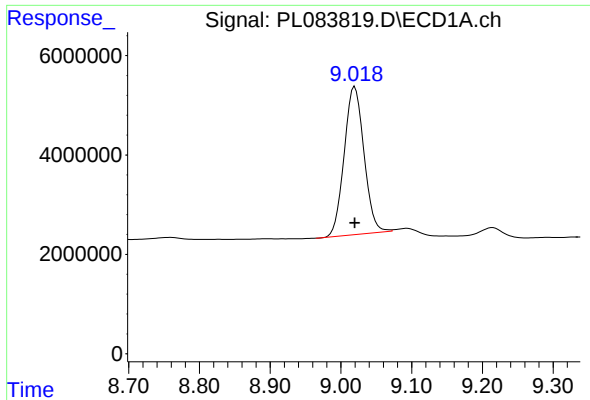

#28 Decachlorobiphenyl

R.T.: 9.020 min
Delta R.T.: 0.000 min
Response: 57846169
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

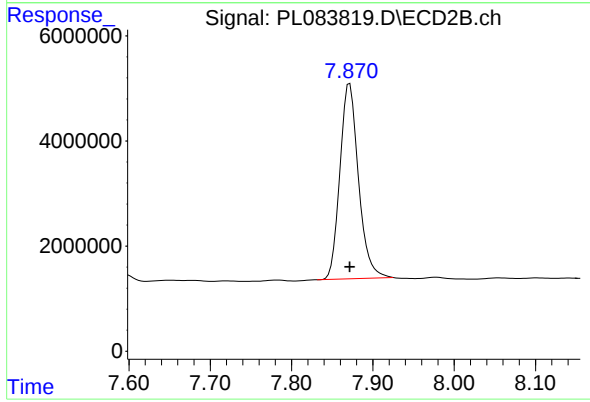

#28 Decachlorobiphenyl

R.T.: 7.872 min
Delta R.T.: 0.000 min
Response: 58771906
Conc: 50.00 ng/ml