

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
 Data File : PL083820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 12:00
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 13:01:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 13:00:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	2.683	49557621	82733230	26.444	25.523
28)	SA Decachlor...	9.020	7.872	31974322	31571059	27.637	26.859
Target Compounds							
23)	Chlordane-1	4.641	3.691	201.3E6	98239162	256.456	248.688
24)	Chlordane-2	5.175	4.272	202.4E6	107.7E6	267.528	264.006
25)	Chlordane-3	5.888	4.906	883.2E6	355.6E6	255.045	258.364
26)	Chlordane-4	5.971	4.969	1027.4E6	372.3E6	257.443	258.222
27)	Chlordane-5	6.820	5.867	149.7E6	114.7E6	252.881	254.833



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
Data File : PL083820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 12:00
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 13:01:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 13:00:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

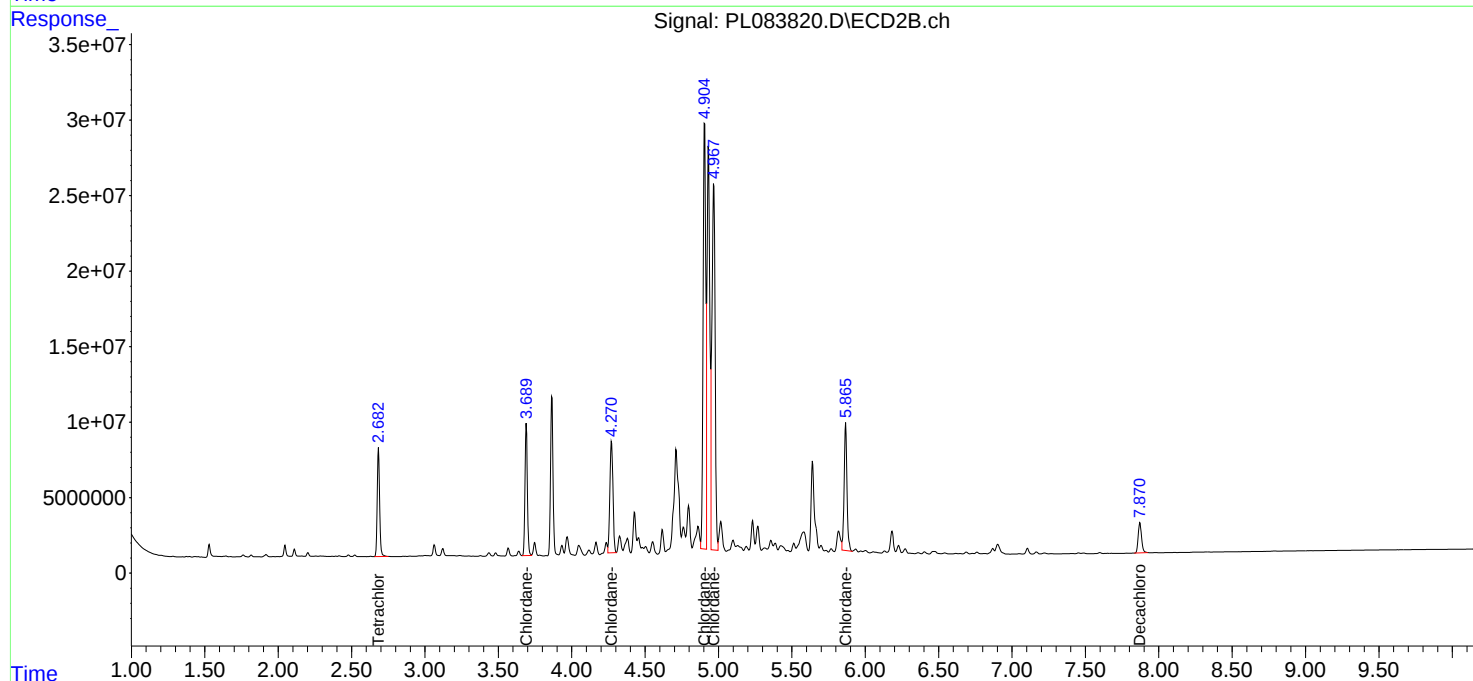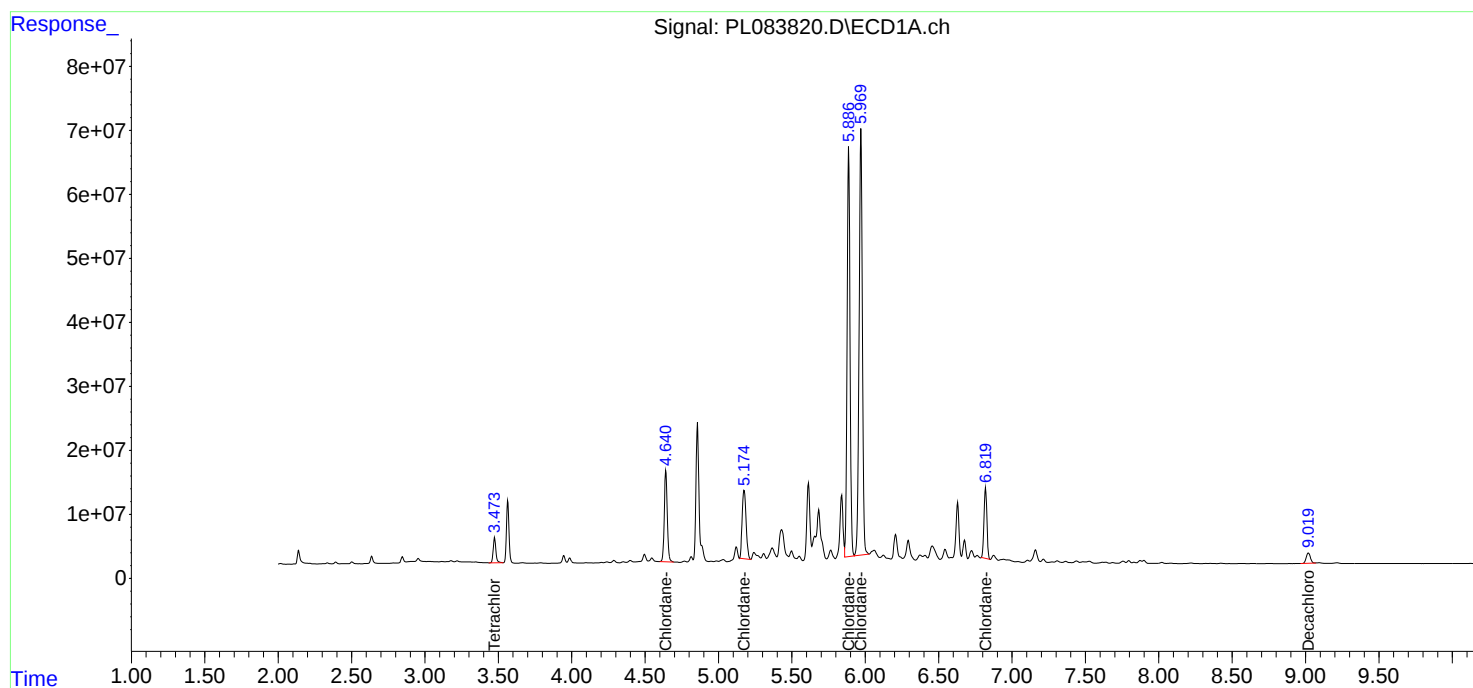


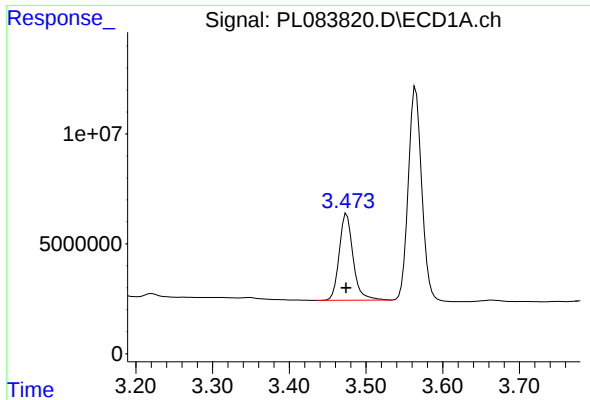

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: 0.000 min
Response: 49557621
Conc: 26.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

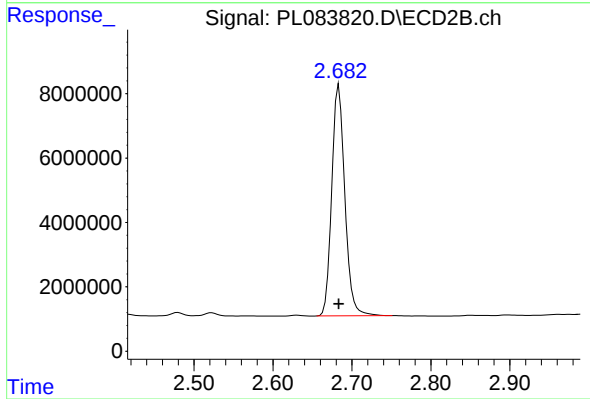


#1 Tetrachloro-m-xylene

R.T.: 2.683 min
Delta R.T.: 0.000 min
Response: 82733230
Conc: 25.52 ng/ml

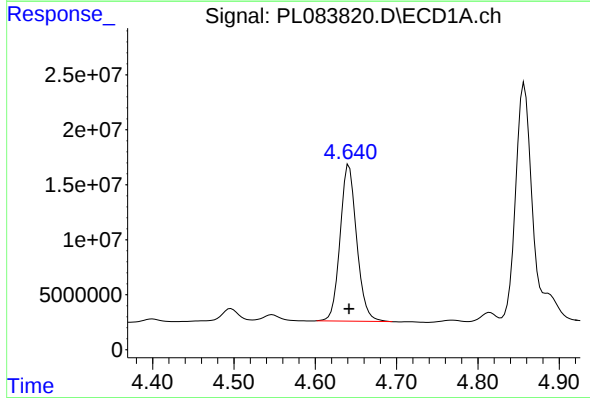


#23 Chlordane-1

R.T.: 4.641 min
Delta R.T.: 0.000 min
Response: 201286598
Conc: 256.46 ng/ml

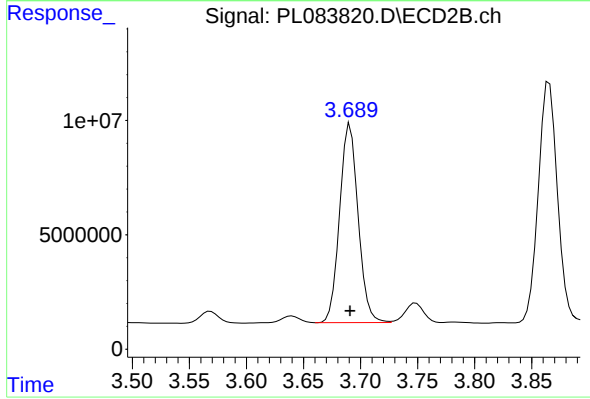

#23 Chlordane-1


R.T.: 3.691 min
Delta R.T.: 0.000 min
Response: 98239162
Conc: 248.69 ng/ml

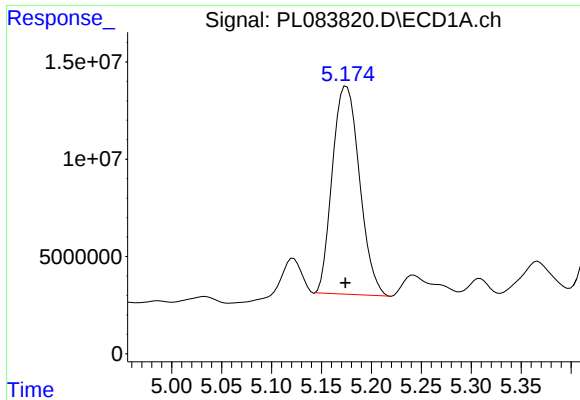

#24 Chlordane-2


R.T.: 5.175 min
Delta R.T.: 0.000 min
Response: 202433714
Conc: 267.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

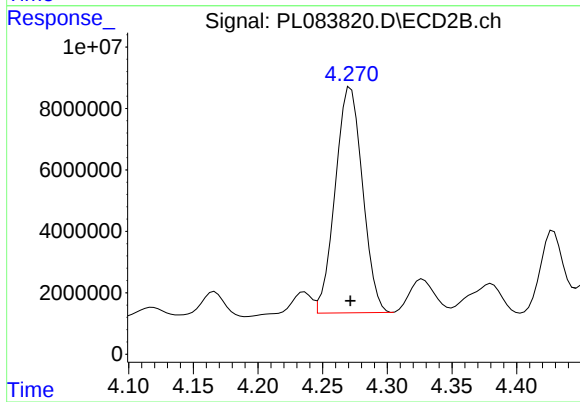


#24 Chlordane-2

R.T.: 4.272 min
Delta R.T.: 0.000 min
Response: 107683666
Conc: 264.01 ng/ml

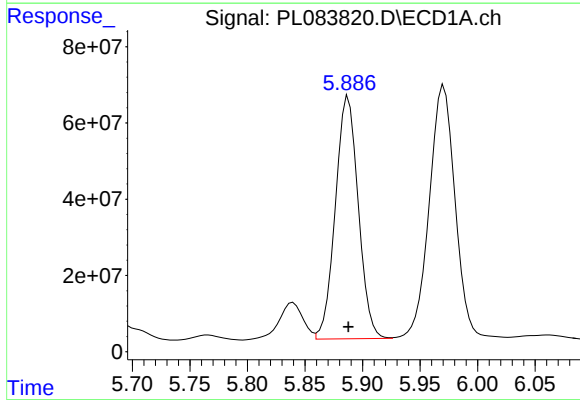


#25 Chlordane-3

R.T.: 5.888 min
Delta R.T.: 0.000 min
Response: 883169744
Conc: 255.04 ng/ml

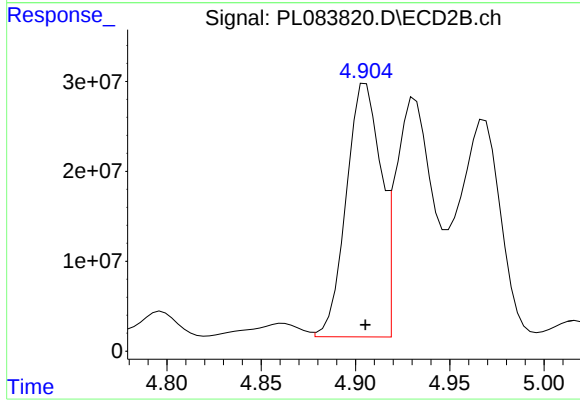

#25 Chlordane-3


R.T.: 4.906 min
Delta R.T.: 0.000 min
Response: 355575256
Conc: 258.36 ng/ml

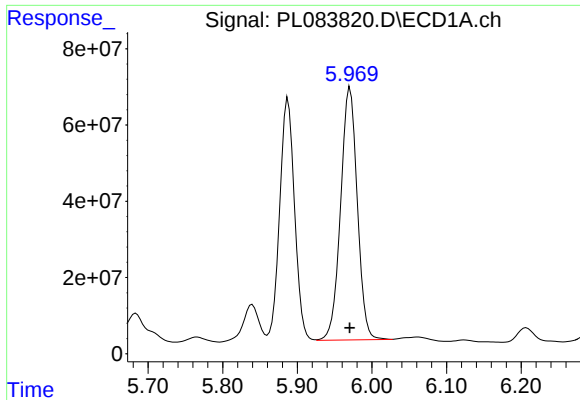

#26 Chlordane-4


R.T.: 5.971 min
Delta R.T.: 0.000 min
Response: 1027443133
Conc: 257.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

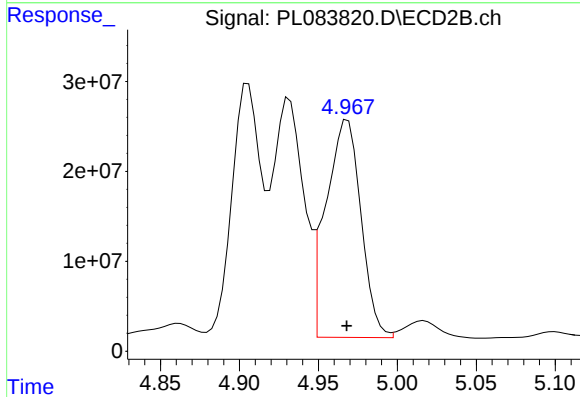


#26 Chlordane-4

R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 372336123
Conc: 258.22 ng/ml

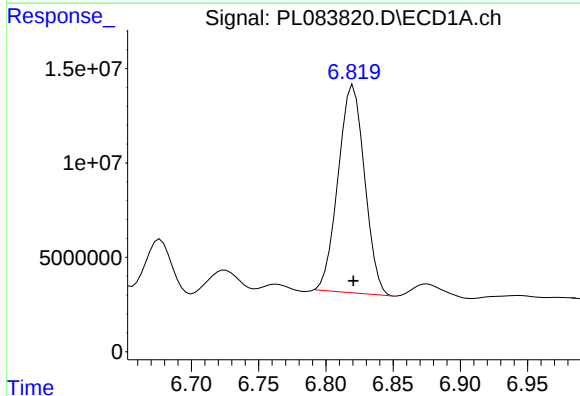


#27 Chlordane-5

R.T.: 6.820 min
Delta R.T.: 0.000 min
Response: 149710790
Conc: 252.88 ng/ml

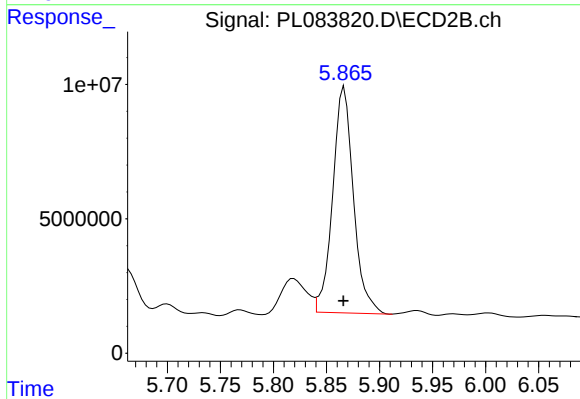

#27 Chlordane-5

R.T.: 5.867 min
Delta R.T.: 0.000 min
Response: 114734391
Conc: 254.83 ng/ml

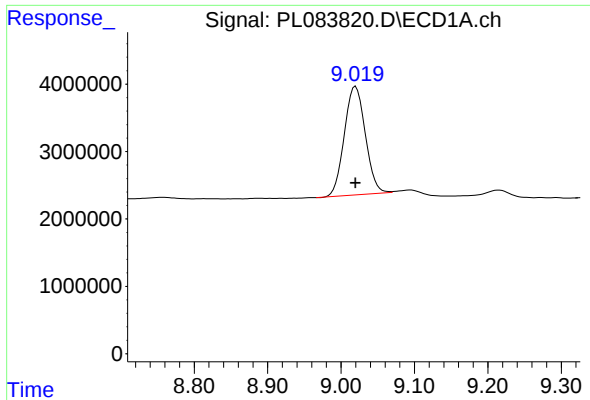

#28 Decachlorobiphenyl


R.T.: 9.020 min

Delta R.T.: 0.000 min

Response: 31974322

Conc: 27.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

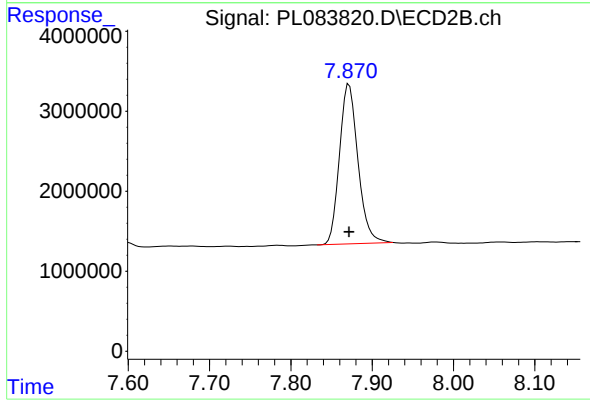

#28 Decachlorobiphenyl

R.T.: 7.872 min

Delta R.T.: 0.000 min

Response: 31571059

Conc: 26.86 ng/ml