

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
 Data File : PL083846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 19:31
 Operator : AR\AJ
 Sample : 03555-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-369

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/13/2023
 Supervised By :Ankita Jodhani 07/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 02:04:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 12 14:26:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.473	2.687	43121941	23222252	21.562m	20.910
28) SA Decachlor...	9.018	7.869	20574130	23022817	15.806	20.720 #
Target Compounds						
17) MA 4,4'-DDT	6.983	5.972	11043872	9528439	6.925	10.462 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
Data File : PL083846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 19:31
Operator : AR\AJ
Sample : 03555-05
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ETGI-369


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/13/2023
Supervised By : Ankita Jodhani 07/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 02:04:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Wed Jul 12 14:26:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

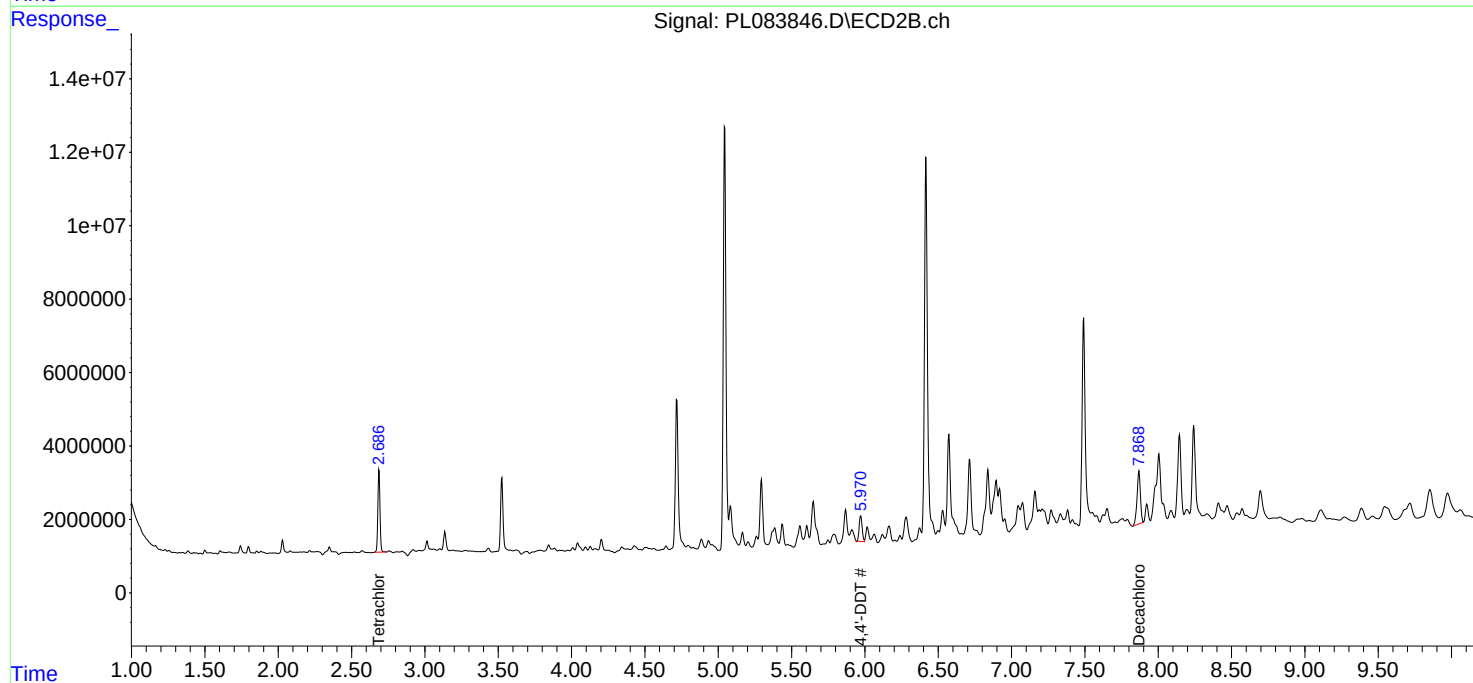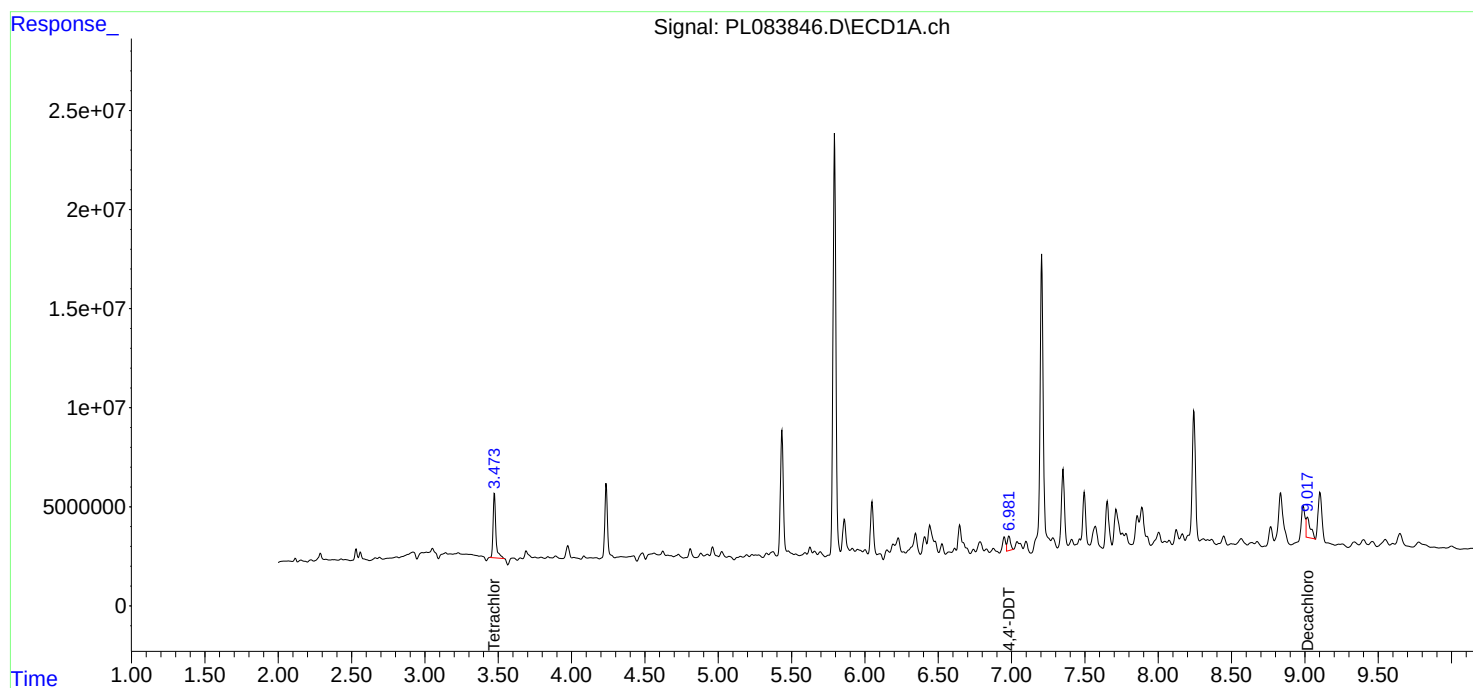

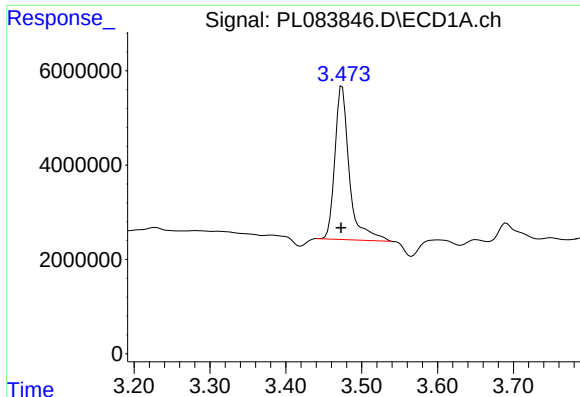


#1 Tetrachloro-m-xylene

R.T.: 3.473 min
Delta R.T.: 0.000 min
Response: 43121941
Conc: 21.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-369


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/13/2023
Supervised By :Ankita Jodhani 07/13/2023

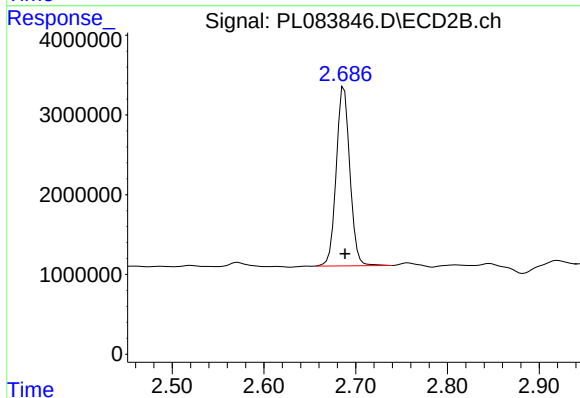


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 23222252
Conc: 20.91 ng/ml

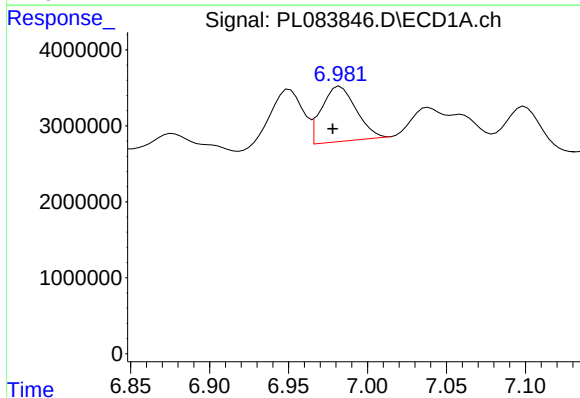


#17 4,4'-DDT

R.T.: 6.983 min
Delta R.T.: 0.005 min
Response: 11043872
Conc: 6.92 ng/ml

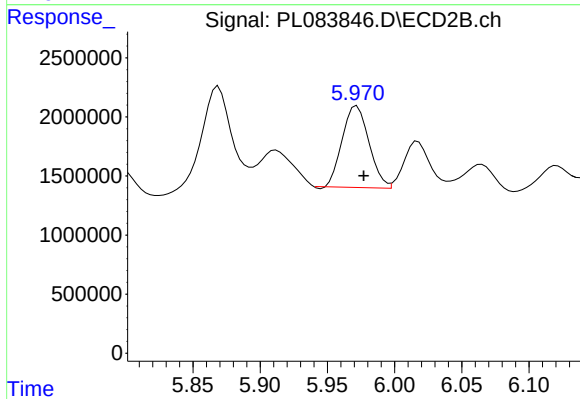

#17 4,4'-DDT

R.T.: 5.972 min
Delta R.T.: -0.005 min
Response: 9528439
Conc: 10.46 ng/ml

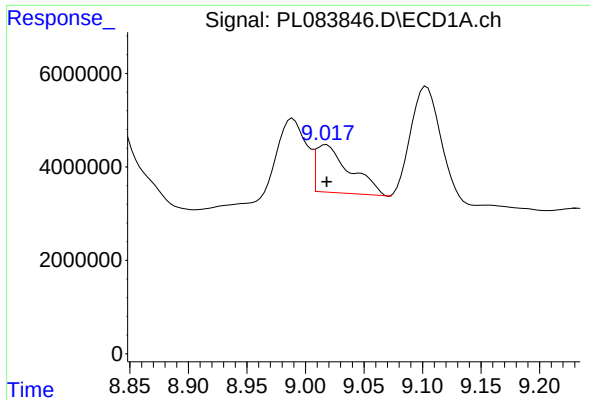


#28 Decachlorobiphenyl

R.T.: 9.018 min
Delta R.T.: 0.000 min
Response: 20574130
Conc: 15.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-369

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/13/2023
Supervised By :Ankita Jodhani 07/13/2023

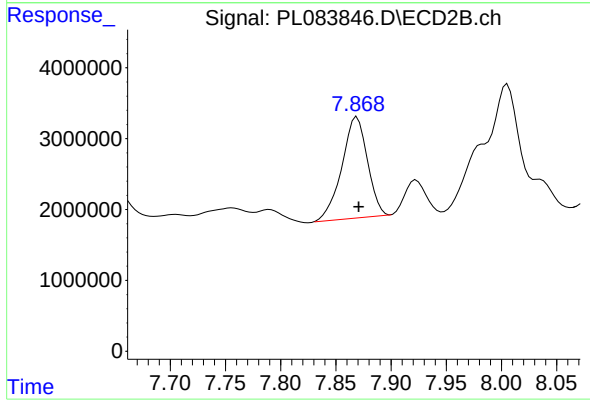

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.002 min
Response: 23022817
Conc: 20.72 ng/ml