

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
 Data File : PL037976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 19:12
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:05:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:05:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.930	593.7E6	202.8E6	73.499	74.384
28)	SA Decachlor...	8.004	8.938	557.8E6	174.2E6	72.656	71.085
Target Compounds							
23)	Chlordane-1	4.171	4.912	265.7E6	90239581	726.459	743.686
24)	Chlordane-2	4.664	5.375	277.2E6	90197152	736.821	730.602
25)	Chlordane-3	5.220	6.014	888.1E6	314.5E6	744.202	741.001
26)	Chlordane-4	5.275	6.090	800.3E6	373.8E6	740.792	738.462
27)	Chlordane-5	5.883	6.881	126.1E6	67221727	775.951	738.105



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
Data File : PL037976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 19:12
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:05:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:05:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

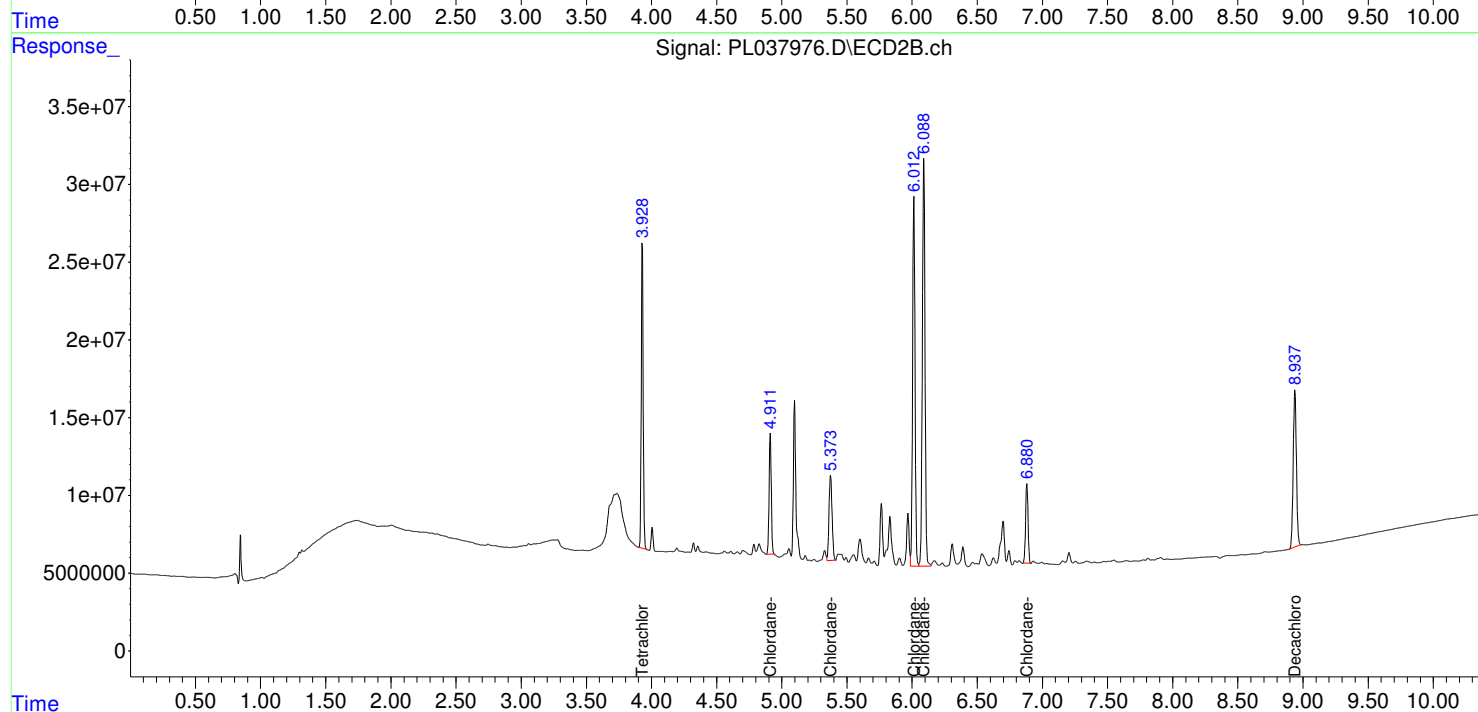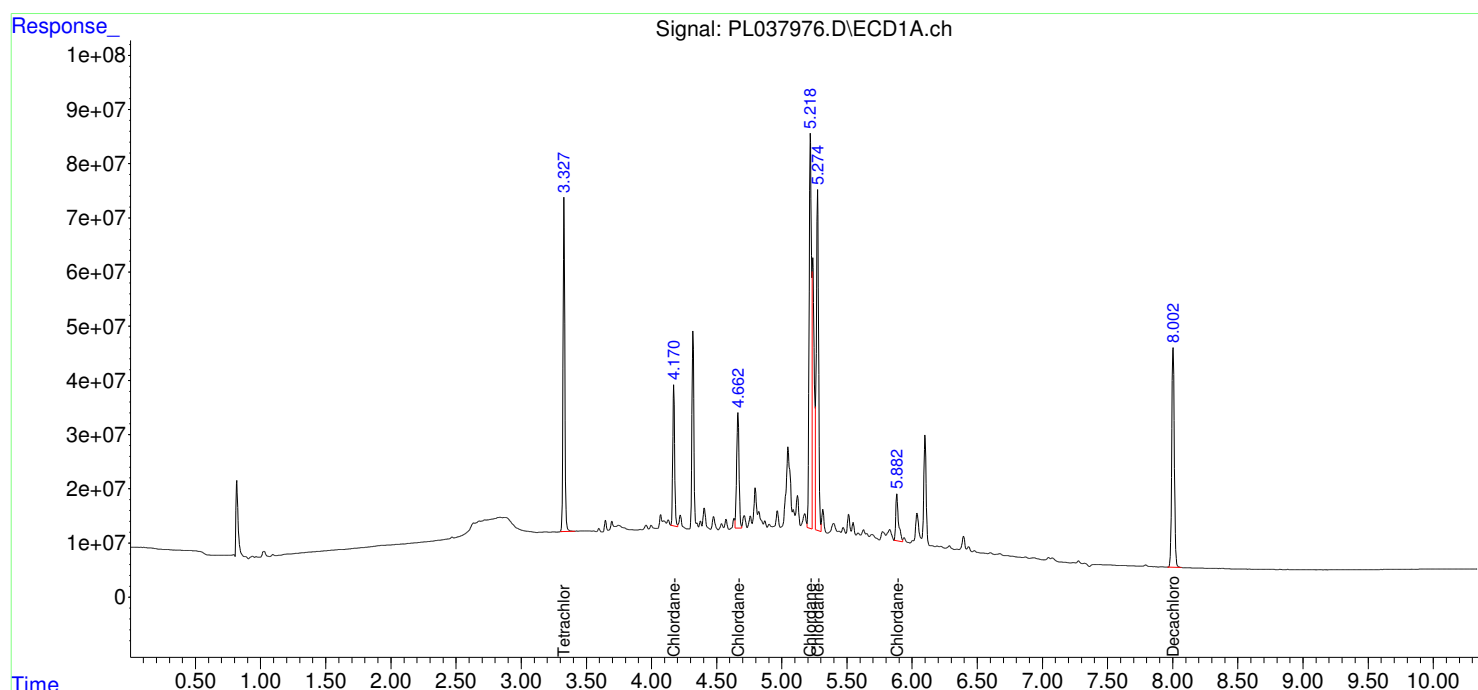


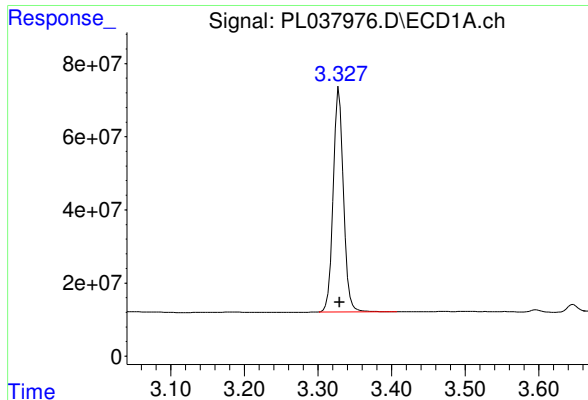

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 593665119
Conc: 73.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

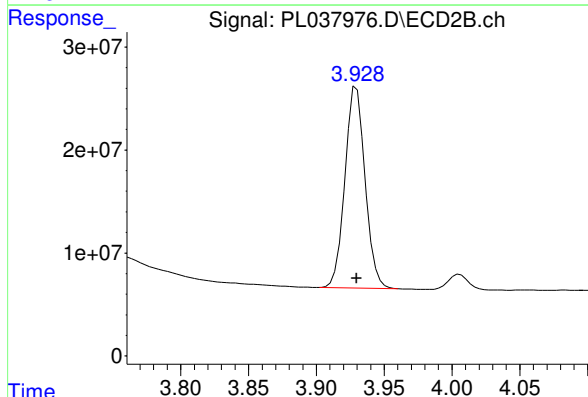


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 202848383
Conc: 74.38 ng/ml

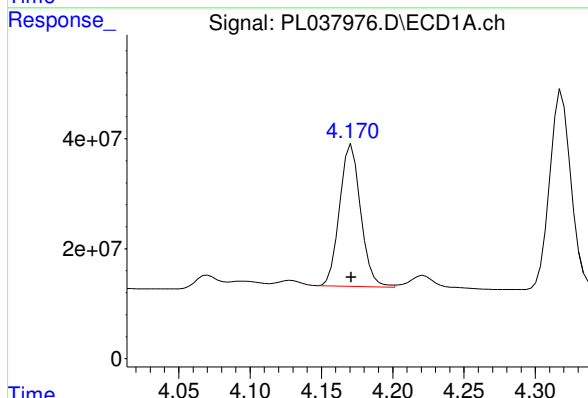


#23 Chlordane-1

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 265674251
Conc: 726.46 ng/ml

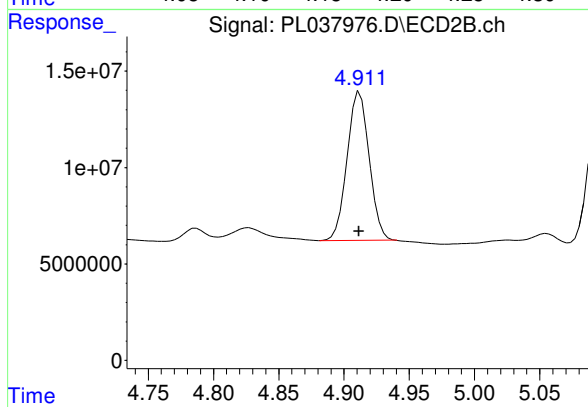

#23 Chlordane-1


R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 90239581
Conc: 743.69 ng/ml

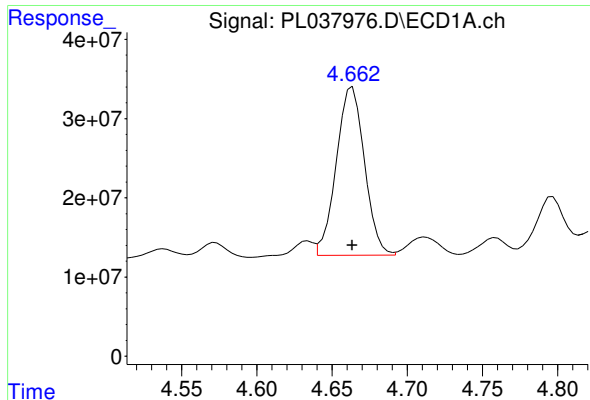

#24 Chlordane-2


R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 277214892
Conc: 736.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

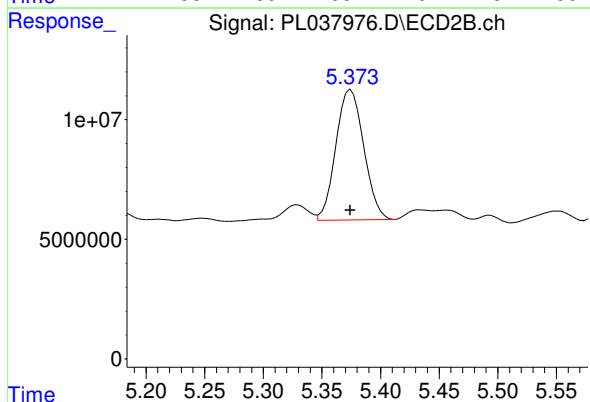


#24 Chlordane-2

R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 90197152
Conc: 730.60 ng/ml

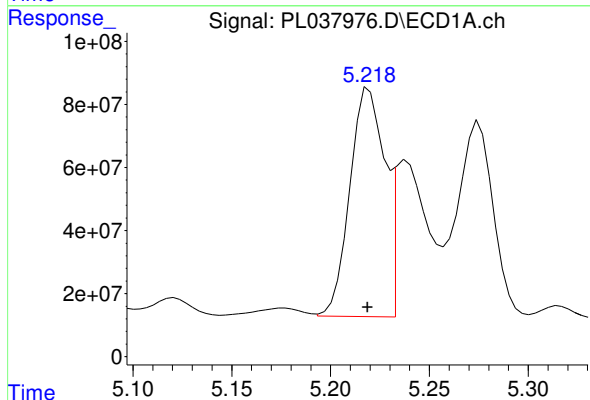


#25 Chlordane-3

R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 888146220
Conc: 744.20 ng/ml

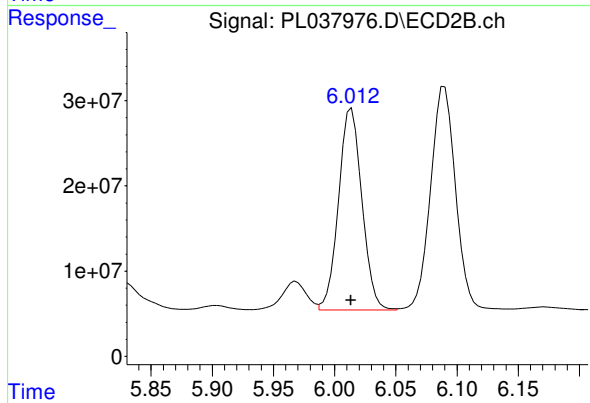

#25 Chlordane-3


R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 314459840
Conc: 741.00 ng/ml

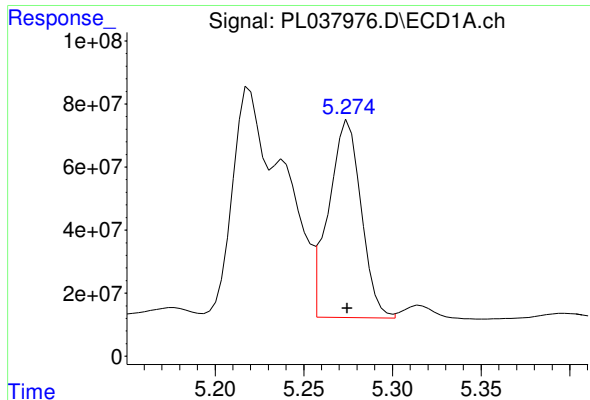

#26 Chlordane-4


R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 800308499
Conc: 740.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

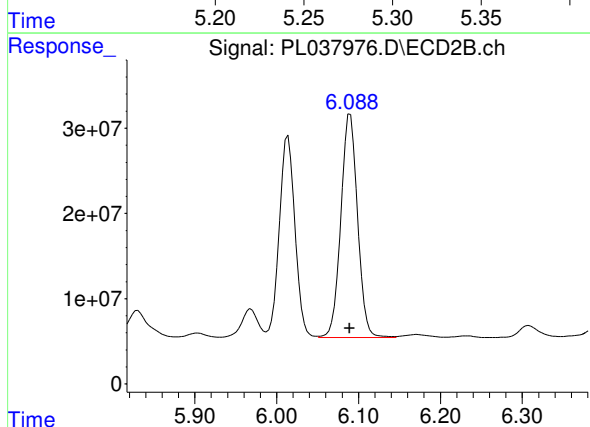


#26 Chlordane-4

R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 373814234
Conc: 738.46 ng/ml

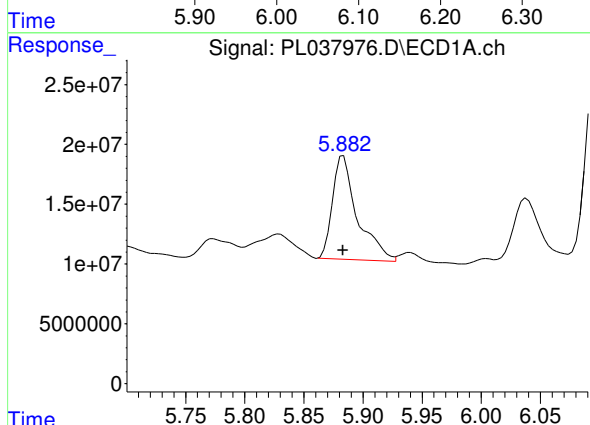


#27 Chlordane-5

R.T.: 5.883 min
Delta R.T.: 0.000 min
Response: 126118572
Conc: 775.95 ng/ml

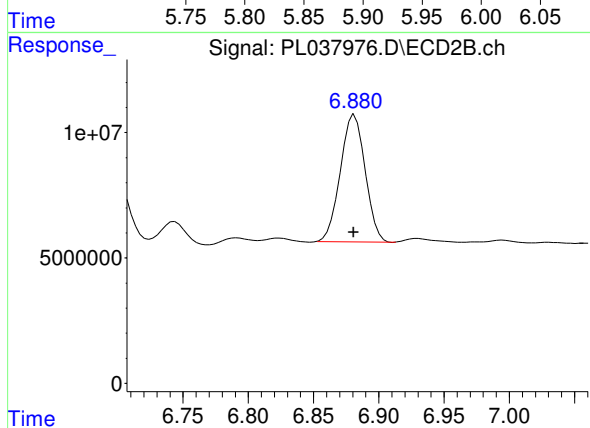

#27 Chlordane-5


R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 67221727
Conc: 738.10 ng/ml

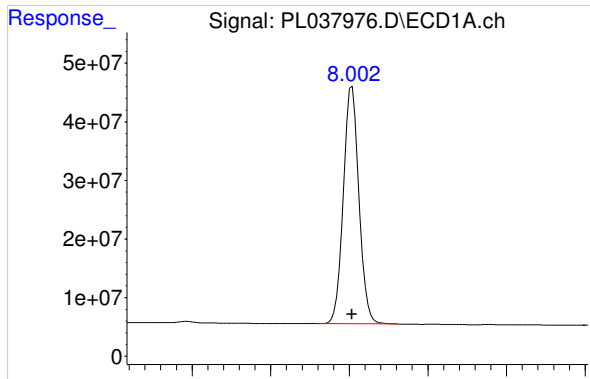

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 557822701
Conc: 72.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

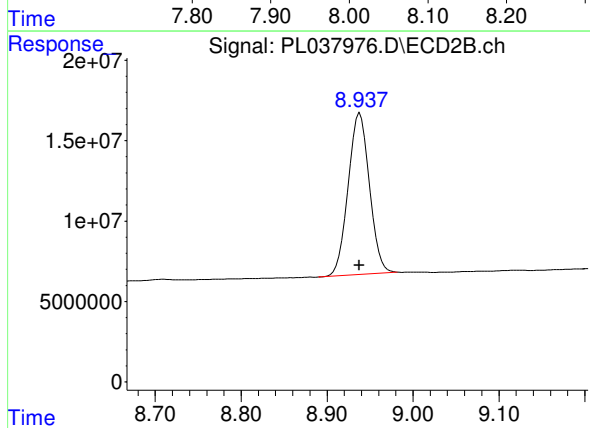

#28 Decachlorobiphenyl

R.T.: 8.938 min
Delta R.T.: 0.000 min
Response: 174247578
Conc: 71.08 ng/ml