

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
 Data File : PL037978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 19:40
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:06:07 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:05:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.328	3.930	200.0E6	66326102	24.756	24.322
28) SA Decachlor...	8.004	8.937	195.6E6	61129929	25.476	24.938
Target Compounds						
23) Chlordane-1	4.171	4.912	94971720	28732006	259.690	236.787
24) Chlordane-2	4.664	5.375	94527897	30279562	251.250	245.266
25) Chlordane-3	5.220	6.014	296.4E6	101.5E6	248.381	239.086
26) Chlordane-4	5.275	6.089	266.6E6	121.8E6	246.746	240.582
27) Chlordane-5	5.883	6.881	39479570	22016799	242.900	241.748



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
Data File : PL037978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 19:40
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:06:07 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:05:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

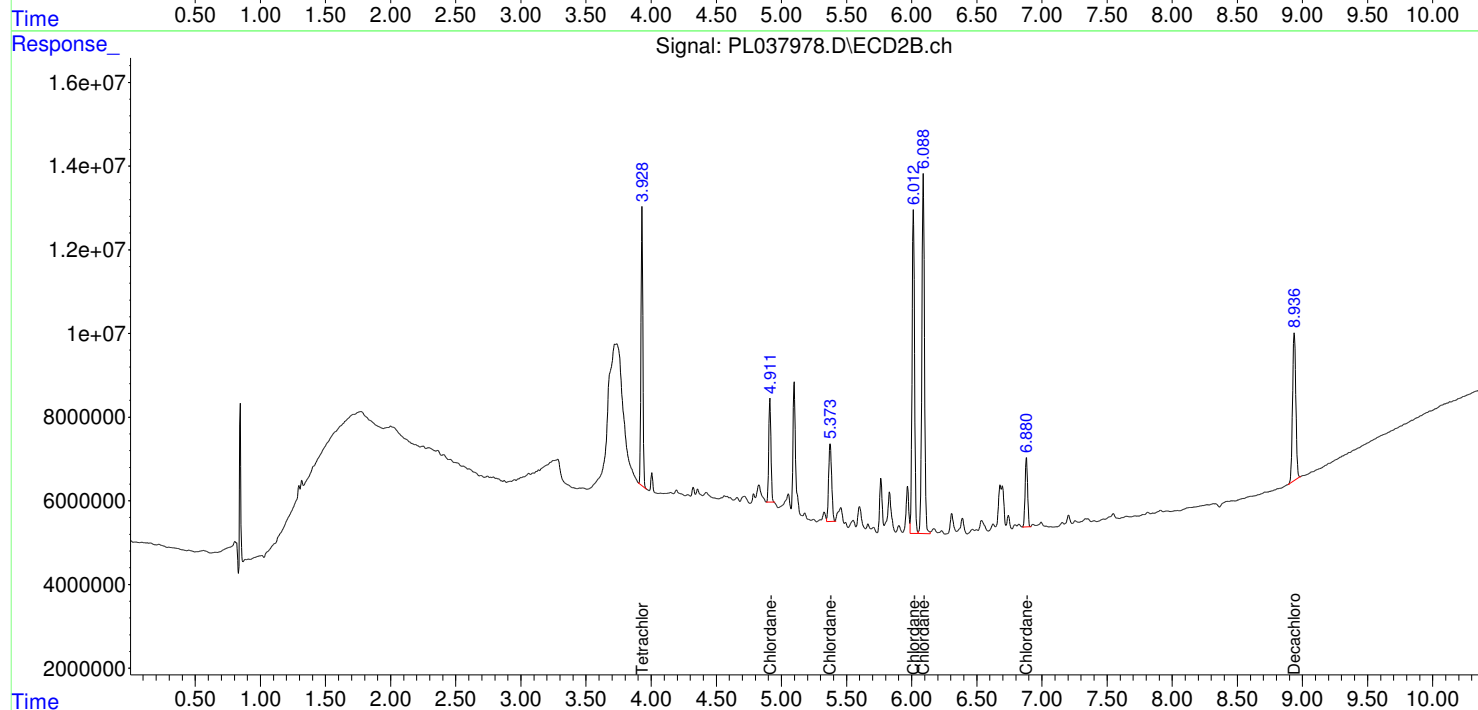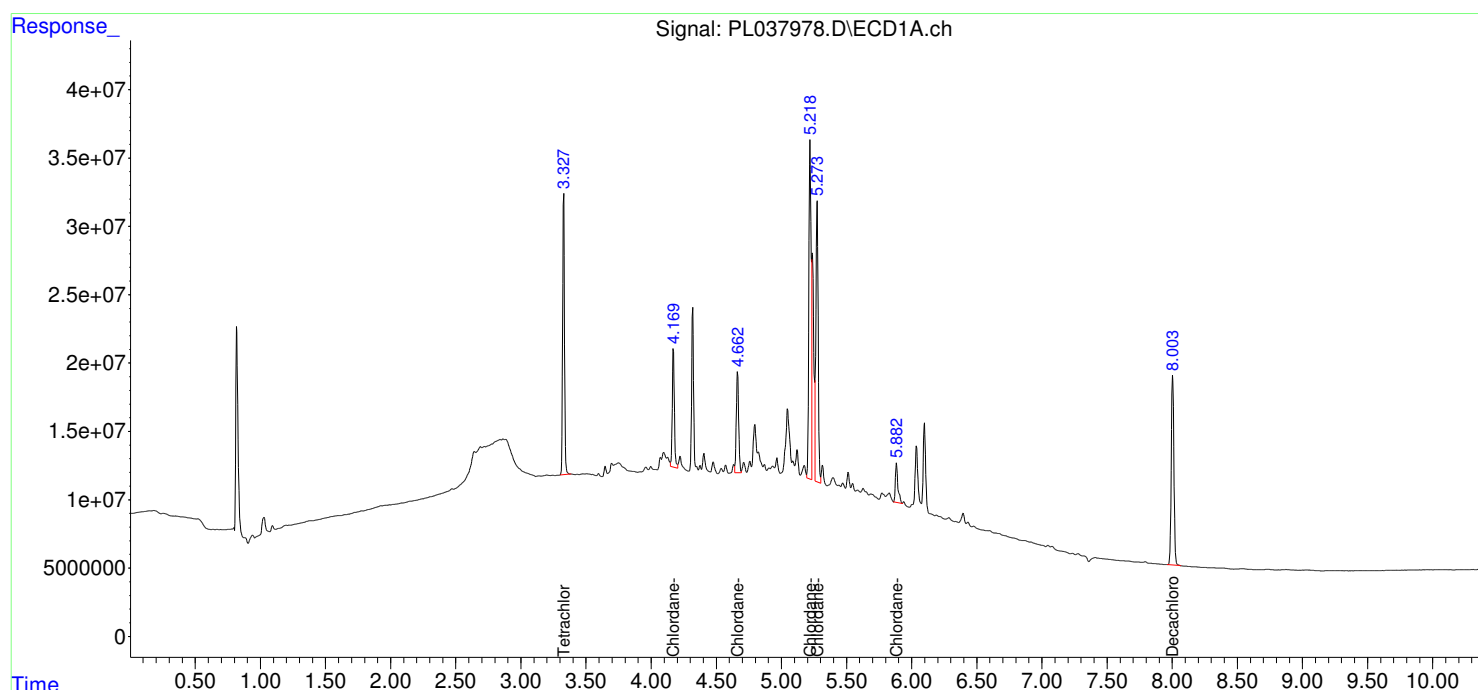


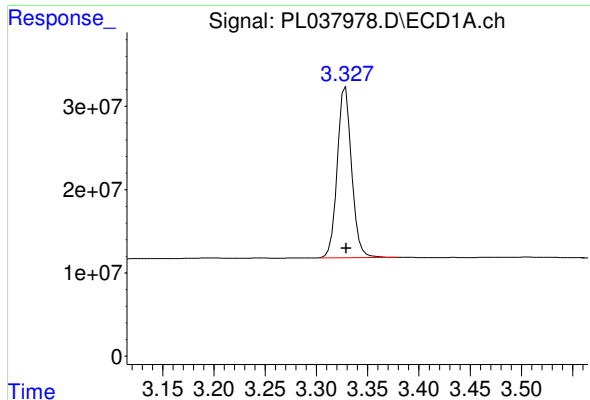

#1 Tetrachloro-m-xylene


R.T.: 3.328 min
Delta R.T.: 0.000 min
Response: 199955777
Conc: 24.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

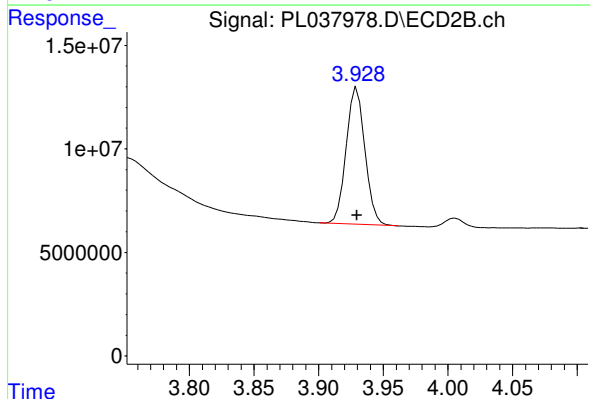


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 66326102
Conc: 24.32 ng/ml

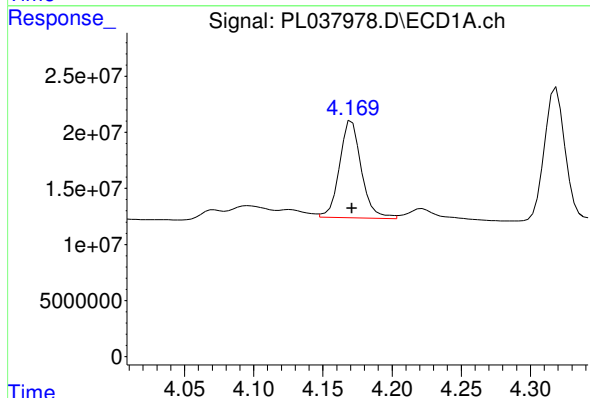


#23 Chlordane-1

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 94971720
Conc: 259.69 ng/ml

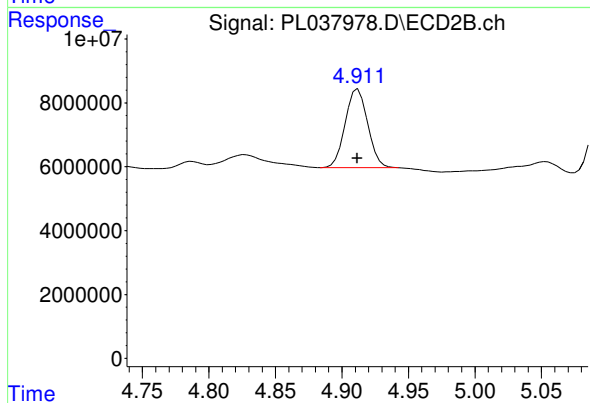

#23 Chlordane-1


R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 28732006
Conc: 236.79 ng/ml

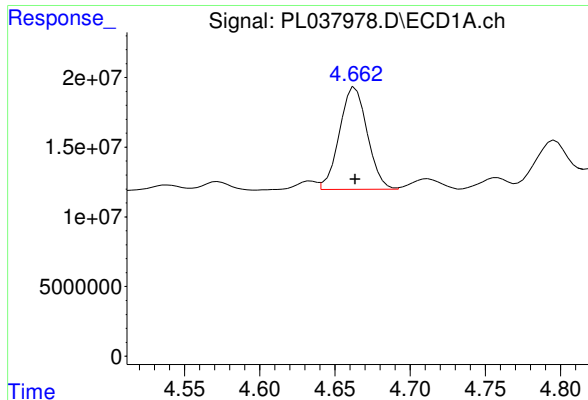

#24 Chlordane-2


R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 94527897
Conc: 251.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

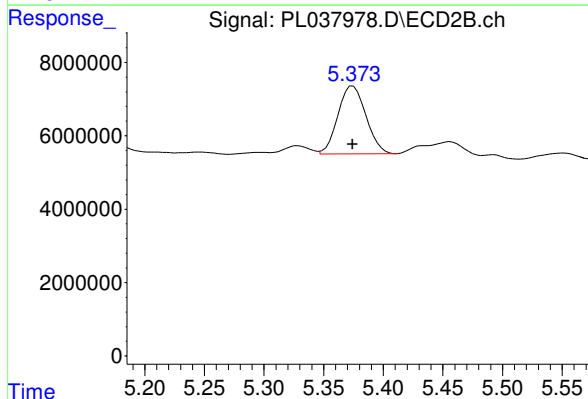


#24 Chlordane-2

R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 30279562
Conc: 245.27 ng/ml

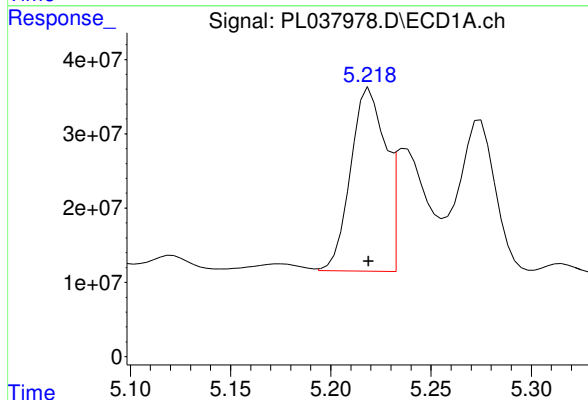


#25 Chlordane-3

R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 296423747
Conc: 248.38 ng/ml

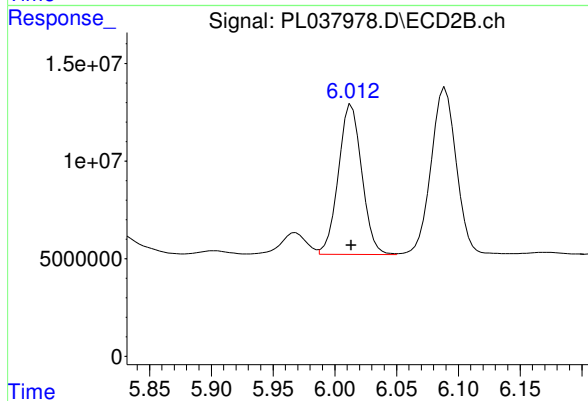

#25 Chlordane-3


R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 101461490
Conc: 239.09 ng/ml

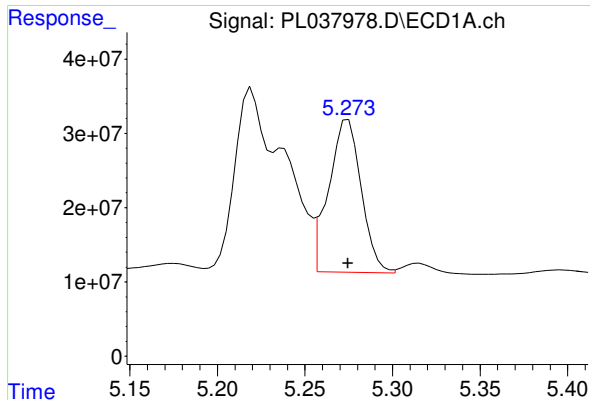

#26 Chlordane-4


R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 266570476
Conc: 246.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

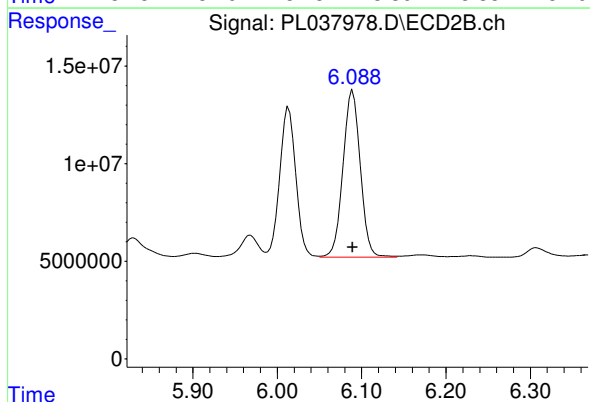


#26 Chlordane-4

R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 121783992
Conc: 240.58 ng/ml

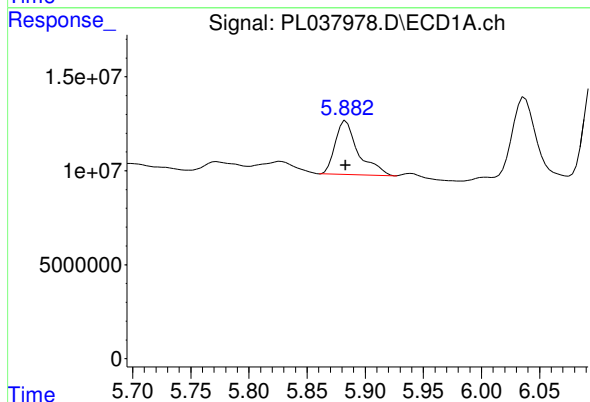


#27 Chlordane-5

R.T.: 5.883 min
Delta R.T.: 0.000 min
Response: 39479570
Conc: 242.90 ng/ml

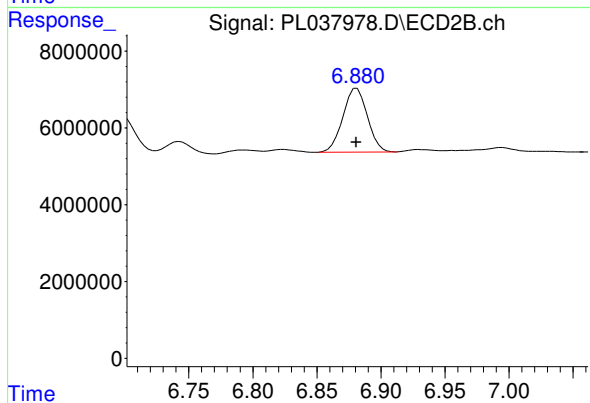

#27 Chlordane-5


R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 22016799
Conc: 241.75 ng/ml

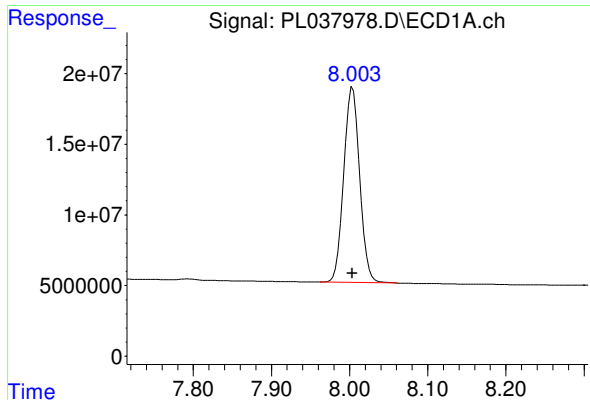

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 195592025
Conc: 25.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

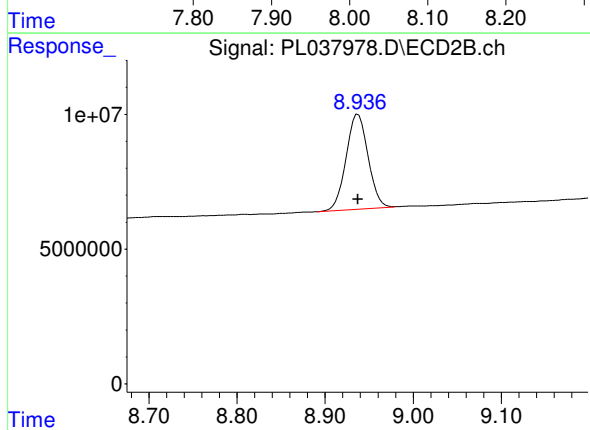

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 61129929
Conc: 24.94 ng/ml