

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
 Data File : PL037979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 19:54
 Operator : AJ\SJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:06:11 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:05:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.329	3.930	38327851	12188019	4.745	4.469
28) SA Decachlor...	8.004	8.938	41084639	12563200	5.351	5.125
Target Compounds						
23) Chlordane-1	4.171	4.912	29002904	5081851	79.305	41.881 #
24) Chlordane-2	4.663	5.375	18152241	5709969	48.248	46.251
25) Chlordane-3	5.219	6.014	54672148	21854585	45.811	51.499
26) Chlordane-4	5.275	6.090	48881891	26297252	45.247	51.950
27) Chlordane-5	5.883	6.882	7810527	4410833	48.055	48.432



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
Data File : PL037979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 19:54
Operator : AJ\SJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:06:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:05:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

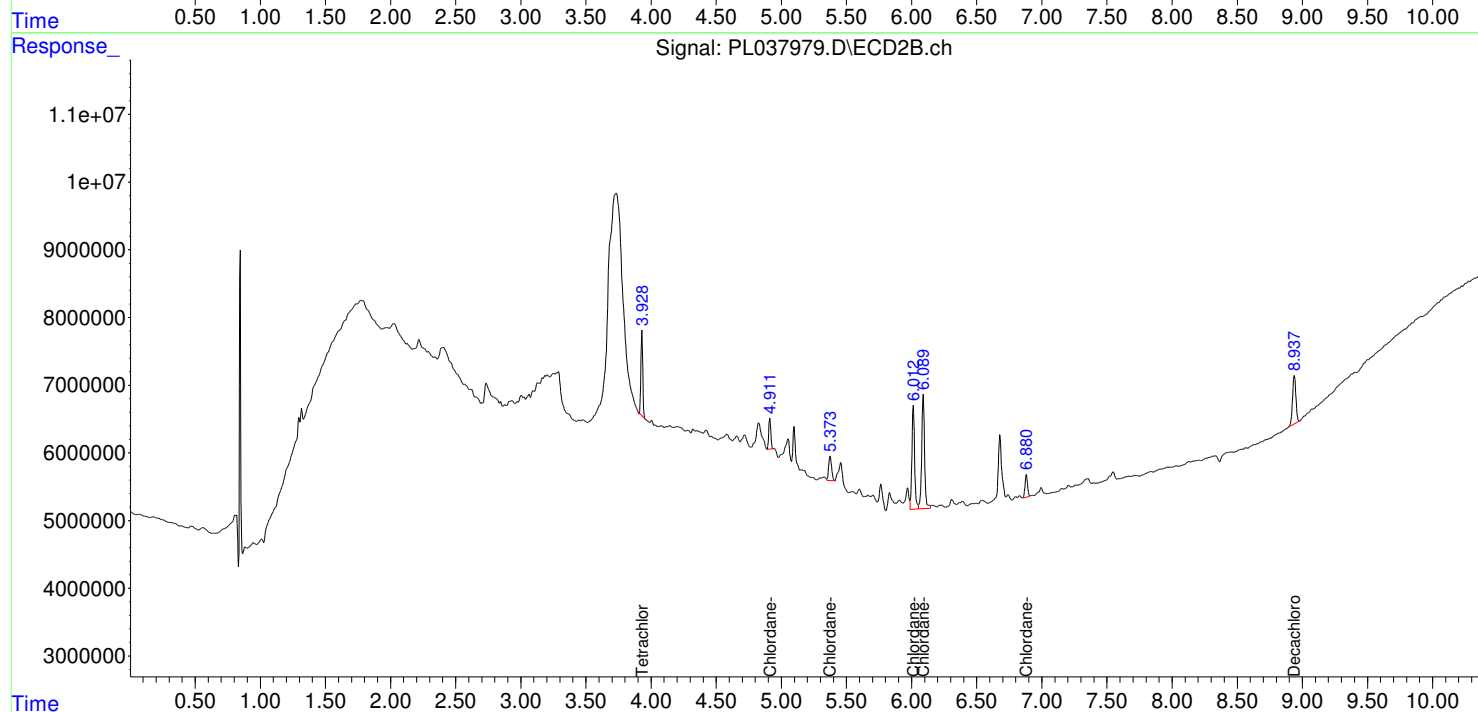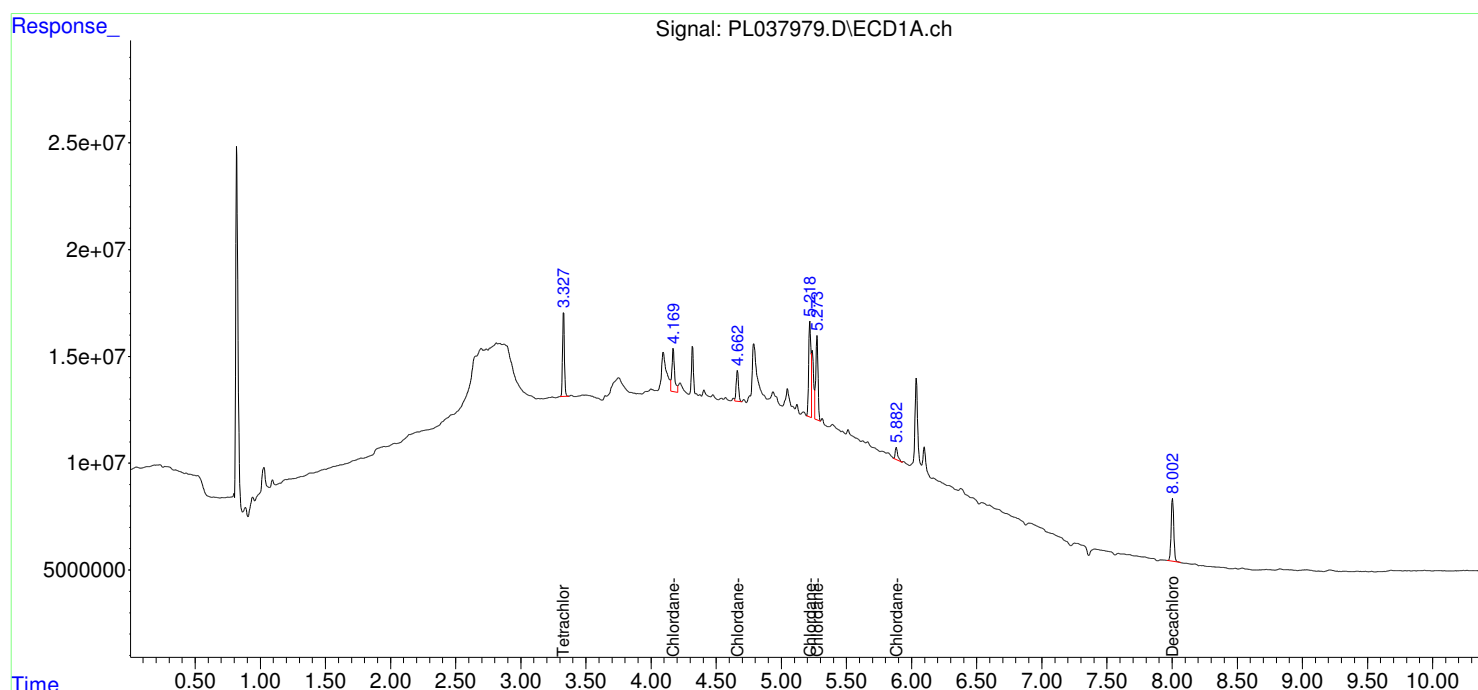


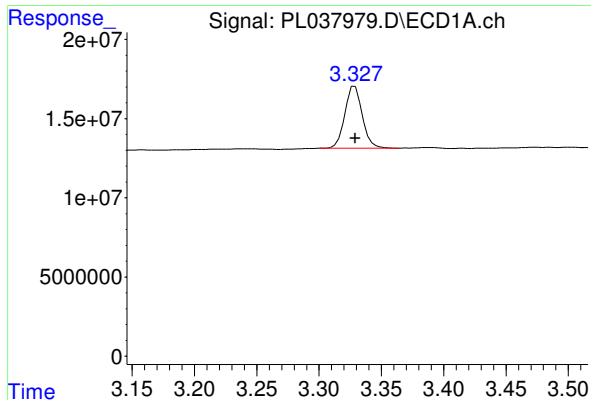

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 38327851
Conc: 4.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

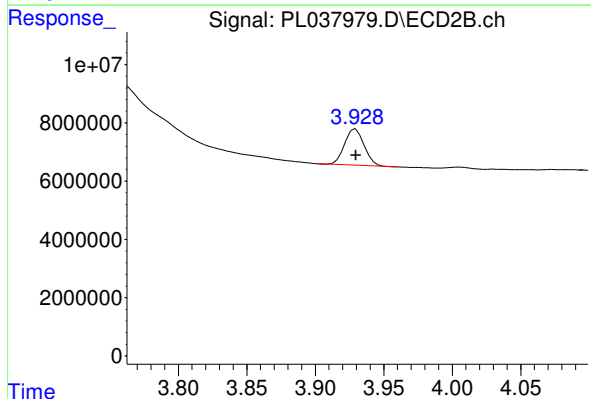


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 12188019
Conc: 4.47 ng/ml

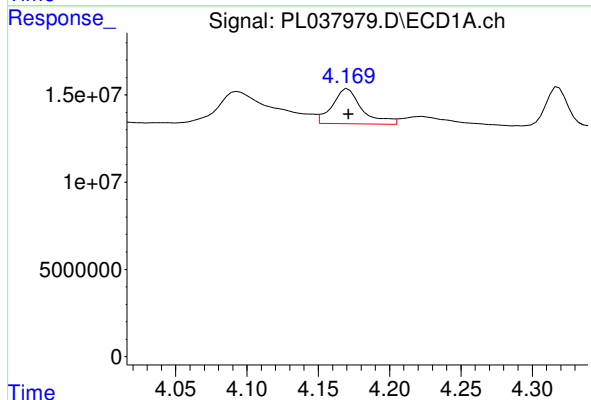


#23 Chlordane-1

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 29002904
Conc: 79.31 ng/ml

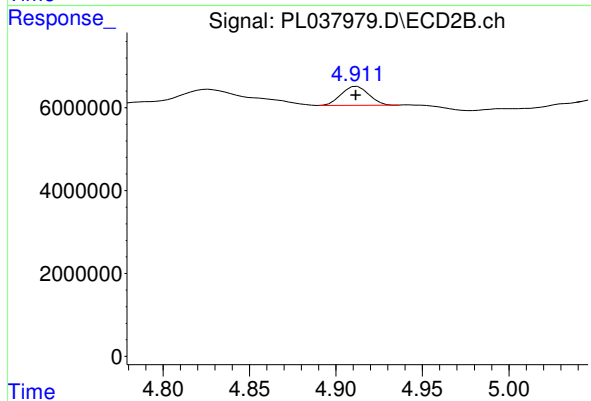

#23 Chlordane-1


R.T.: 4.912 min
Delta R.T.: 0.000 min
Response: 5081851
Conc: 41.88 ng/ml

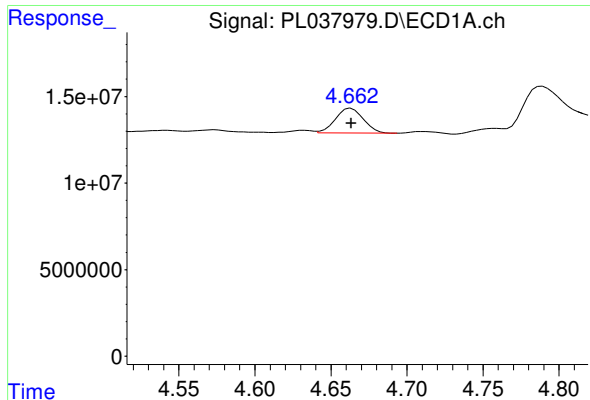

#24 Chlordane-2


R.T.: 4.663 min
Delta R.T.: 0.000 min
Response: 18152241
Conc: 48.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

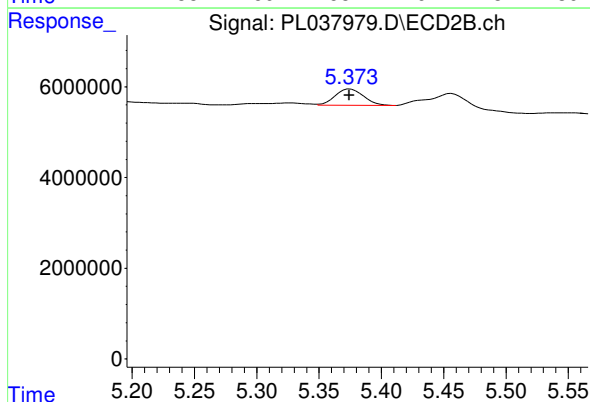


#24 Chlordane-2

R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 5709969
Conc: 46.25 ng/ml

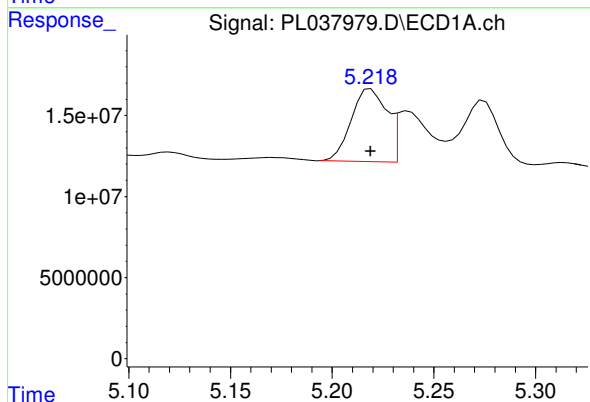


#25 Chlordane-3

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 54672148
Conc: 45.81 ng/ml

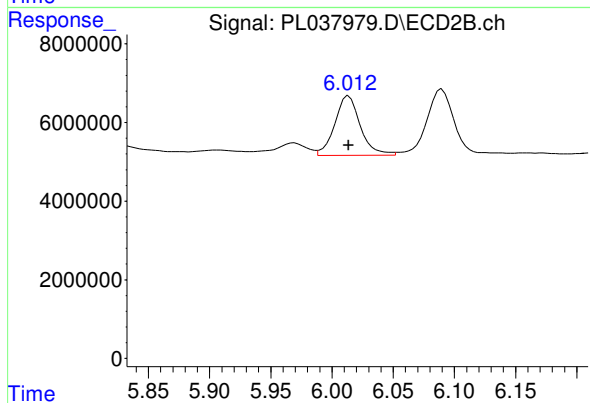

#25 Chlordane-3


R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 21854585
Conc: 51.50 ng/ml

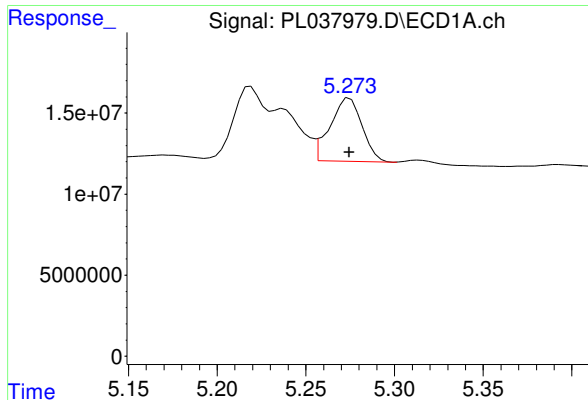

#26 Chlordane-4


R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 48881891
Conc: 45.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

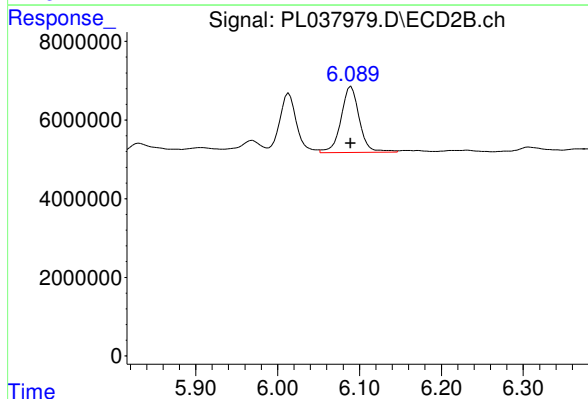


#26 Chlordane-4

R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 26297252
Conc: 51.95 ng/ml

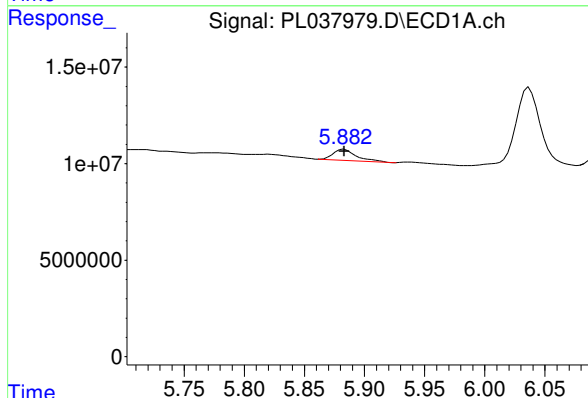


#27 Chlordane-5

R.T.: 5.883 min
Delta R.T.: 0.000 min
Response: 7810527
Conc: 48.05 ng/ml

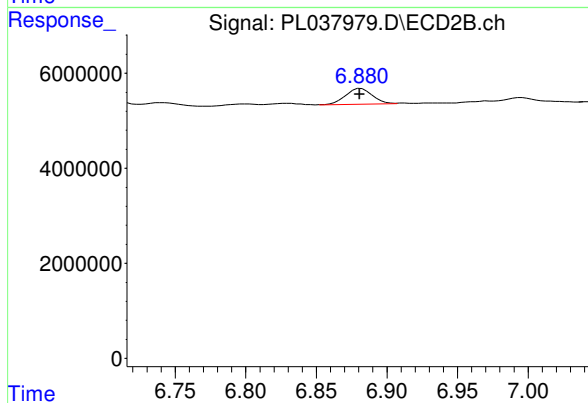

#27 Chlordane-5


R.T.: 6.882 min
Delta R.T.: 0.000 min
Response: 4410833
Conc: 48.43 ng/ml

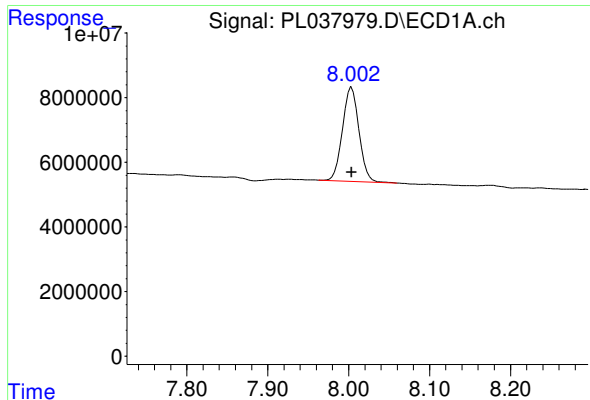

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 41084639
Conc: 5.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

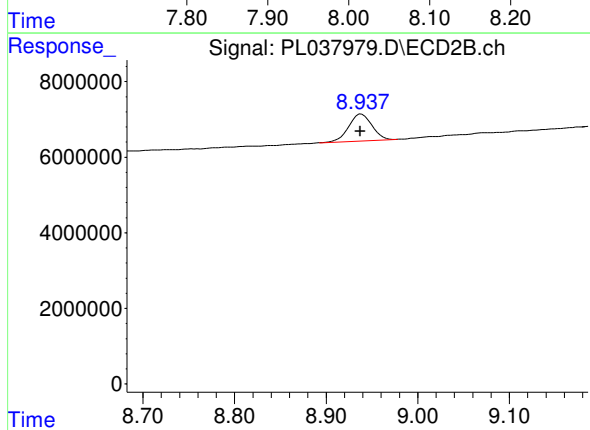

#28 Decachlorobiphenyl

R.T.: 8.938 min
Delta R.T.: 0.001 min
Response: 12563200
Conc: 5.13 ng/ml