

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
 Data File : PL037977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2018 19:26
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:06:01 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:05:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.929	403.9E6	136.4E6	50.000	50.000
28)	SA Decachlor...	8.003	8.937	383.9E6	122.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.171	4.911	182.9E6	60670510	500.000	500.000
24)	Chlordane-2	4.663	5.374	188.1E6	61727994	500.000	500.000
25)	Chlordane-3	5.219	6.013	596.7E6	212.2E6	500.000	500.000
26)	Chlordane-4	5.274	6.089	540.2E6	253.1E6	500.000	500.000
27)	Chlordane-5	5.883	6.881	81267107	45536714	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071318\
Data File : PL037977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2018 19:26
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:06:01 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:05:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

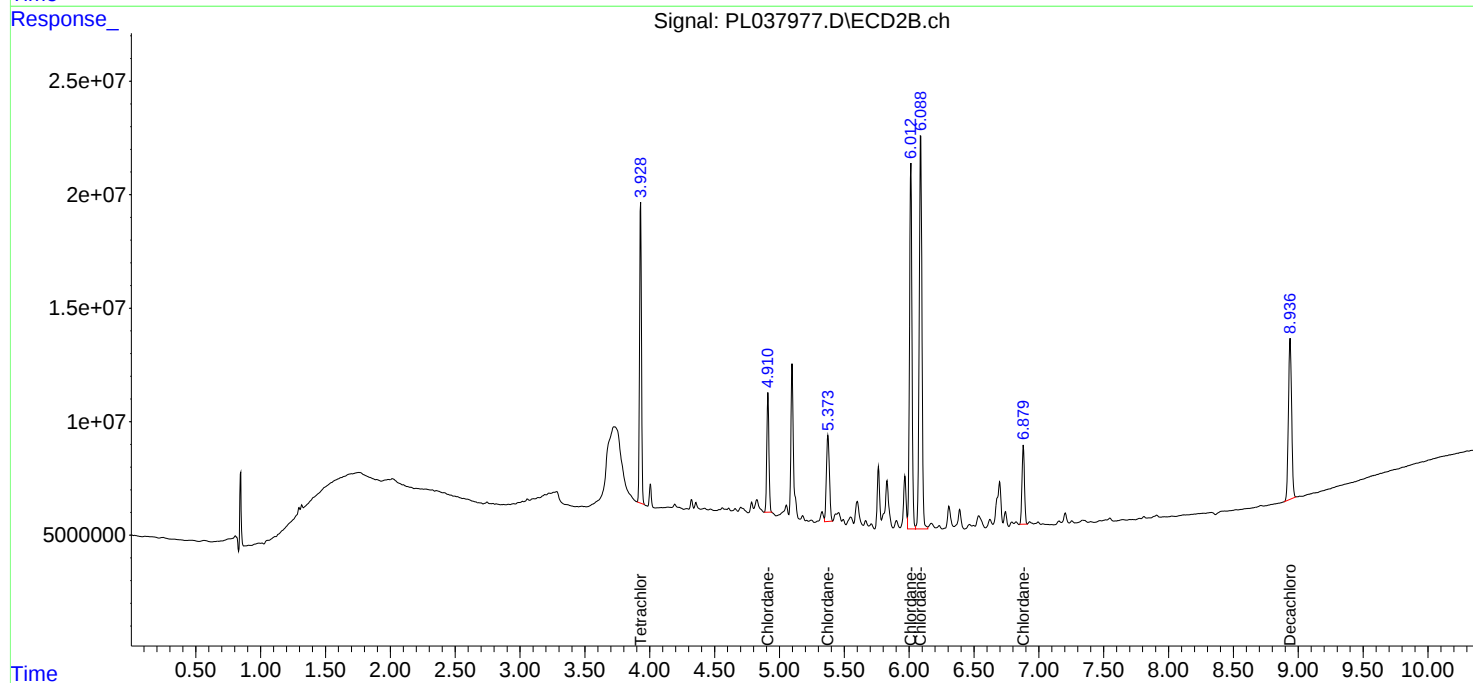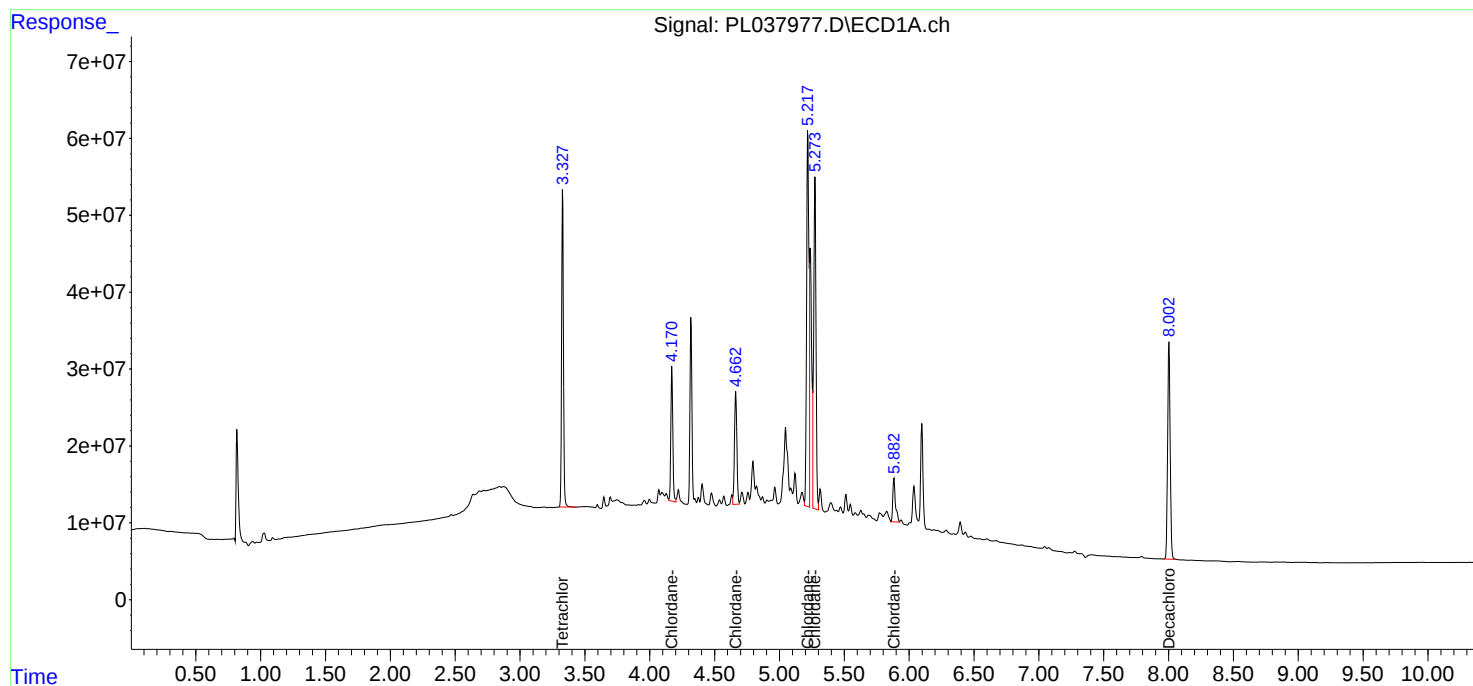


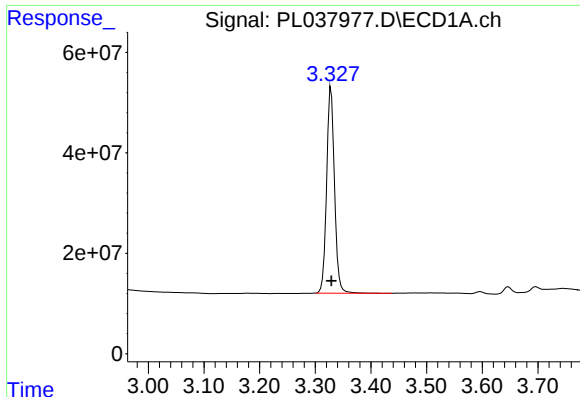

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 403859754
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

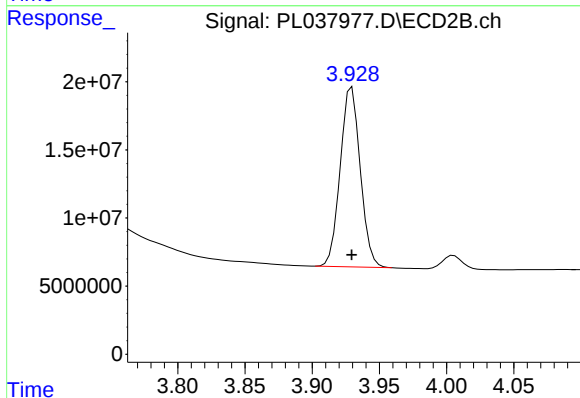


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: 0.000 min
Response: 136352372
Conc: 50.00 ng/ml

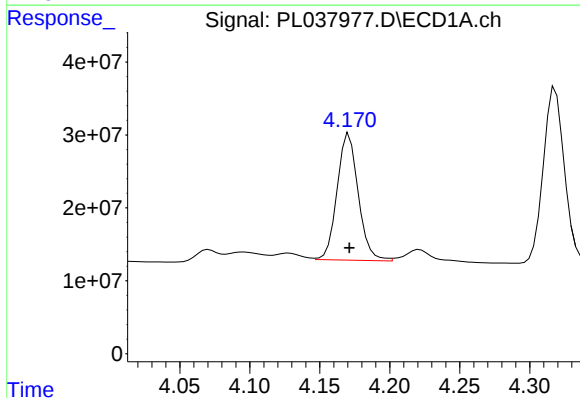


#23 Chlordane-1

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 182855633
Conc: 500.00 ng/ml

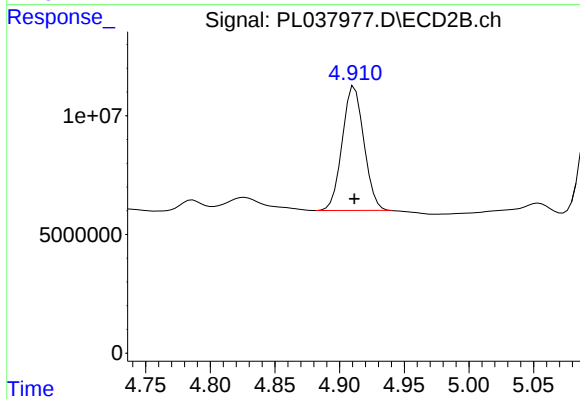

#23 Chlordane-1


R.T.: 4.911 min
Delta R.T.: 0.000 min
Response: 60670510
Conc: 500.00 ng/ml

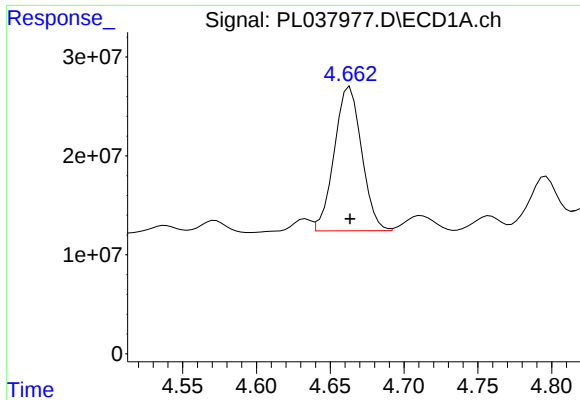

#24 Chlordane-2


R.T.: 4.663 min
Delta R.T.: 0.000 min
Response: 188115583
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

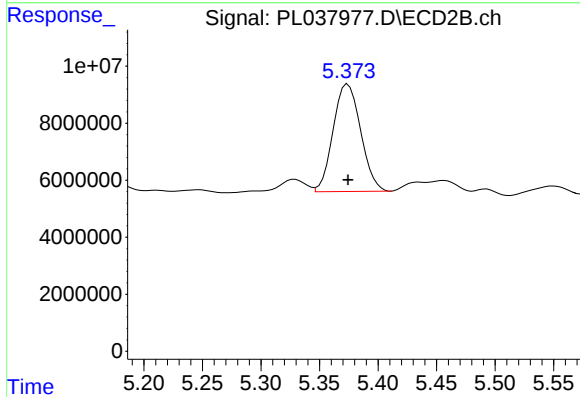


#24 Chlordane-2

R.T.: 5.374 min
Delta R.T.: 0.000 min
Response: 61727994
Conc: 500.00 ng/ml

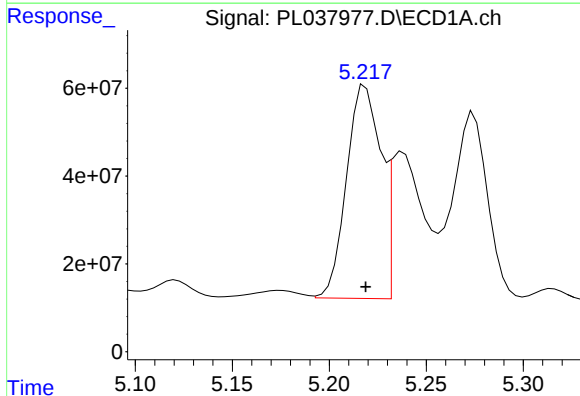


#25 Chlordane-3

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 596710649
Conc: 500.00 ng/ml

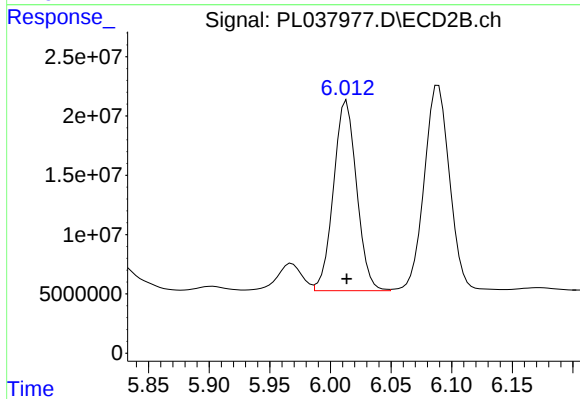

#25 Chlordane-3


R.T.: 6.013 min
Delta R.T.: 0.000 min
Response: 212185855
Conc: 500.00 ng/ml

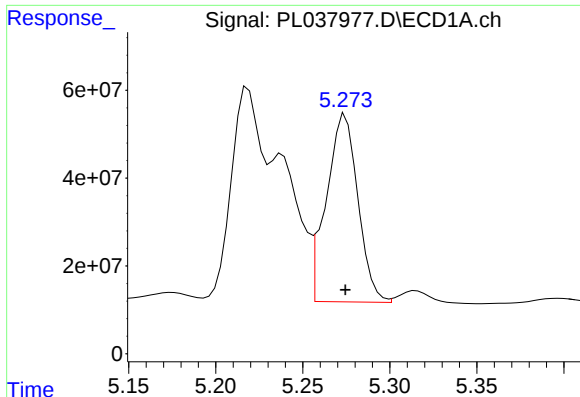

#26 Chlordane-4


R.T.: 5.274 min
Delta R.T.: 0.000 min
Response: 540171004
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

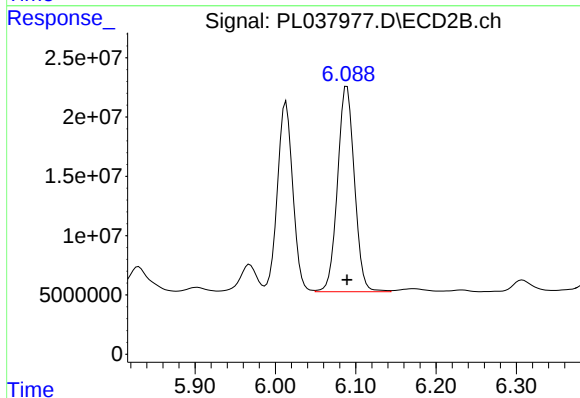


#26 Chlordane-4

R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 253103236
Conc: 500.00 ng/ml

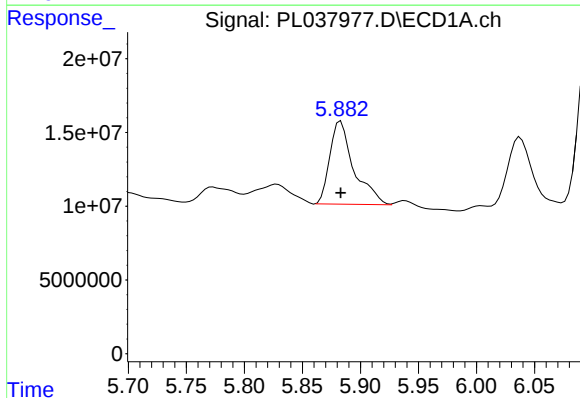


#27 Chlordane-5

R.T.: 5.883 min
Delta R.T.: 0.000 min
Response: 81267107
Conc: 500.00 ng/ml

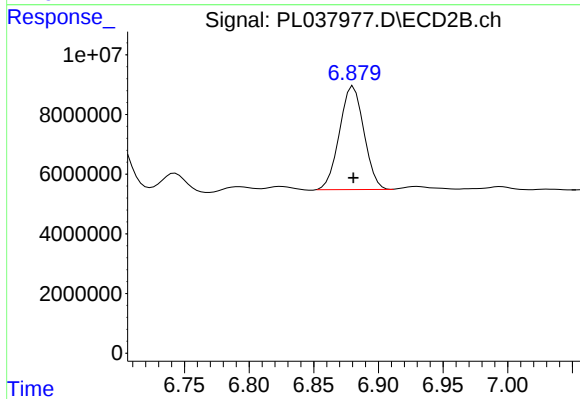

#27 Chlordane-5


R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 45536714
Conc: 500.00 ng/ml

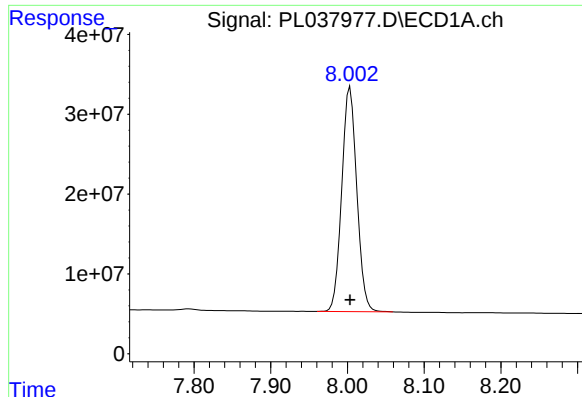

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 383879571
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

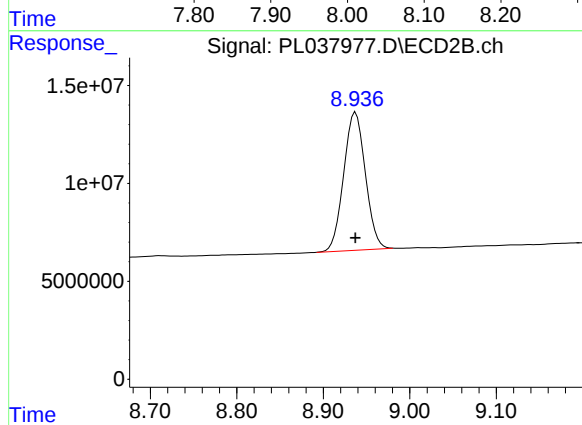

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 122563023
Conc: 50.00 ng/ml