

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071320\
 Data File : PL059847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2020 13:07
 Operator : DD\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 14:03:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.012	111.0E6	133.3E6	57.400	50.306
28)	SA Decachlor...	8.230	9.104	84817309	100.3E6	51.558	47.947
Target Compounds							
23)	Chlordane-1	4.338	5.009	28707741	46916628	468.571	483.137
24)	Chlordane-2	4.840	5.479	29870653	54425314	471.776	475.018
25)	Chlordane-3	5.411	6.128	81022584	187.8E6	479.096	485.383
26)	Chlordane-4	5.469	6.203	66729624	225.2E6	478.282	486.466
27)	Chlordane-5	6.305	7.009	26952525	39421513	475.014	507.583



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071320\
Data File : PL059847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2020 13:07
Operator : DD\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:03:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

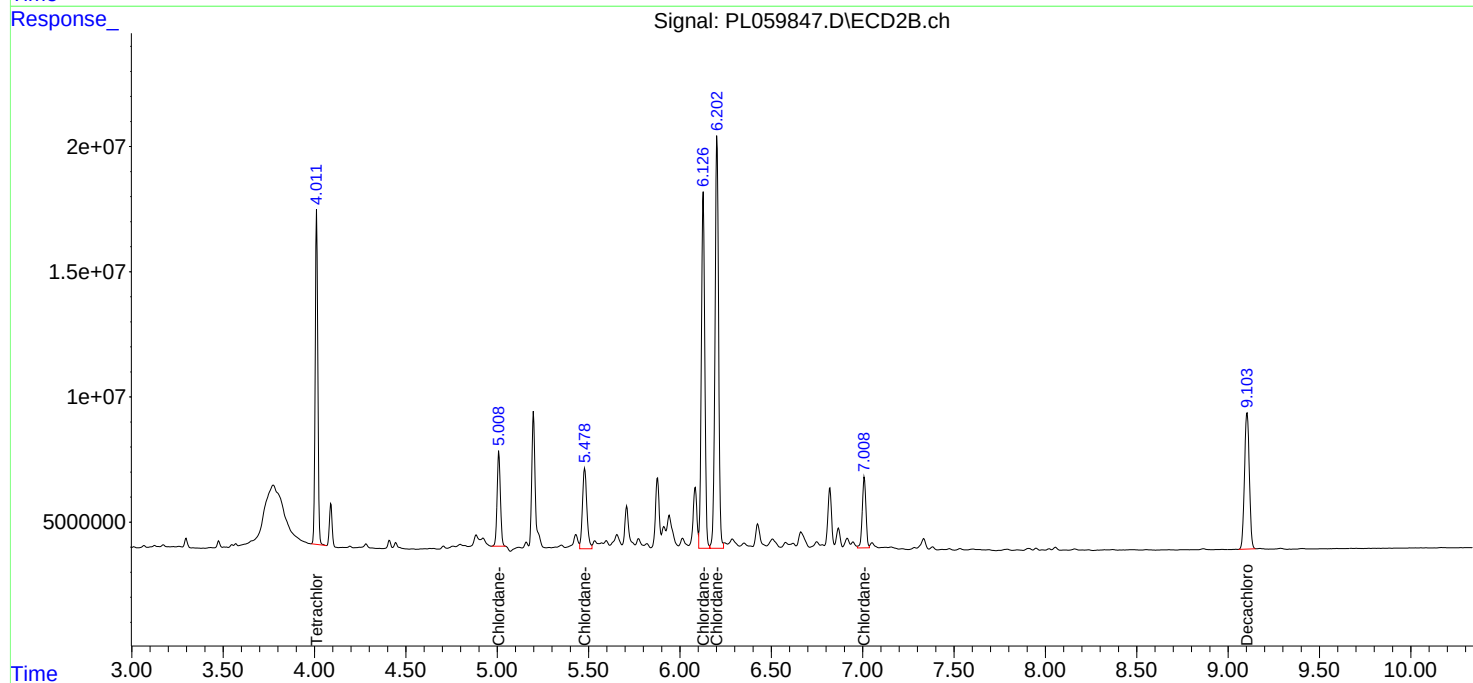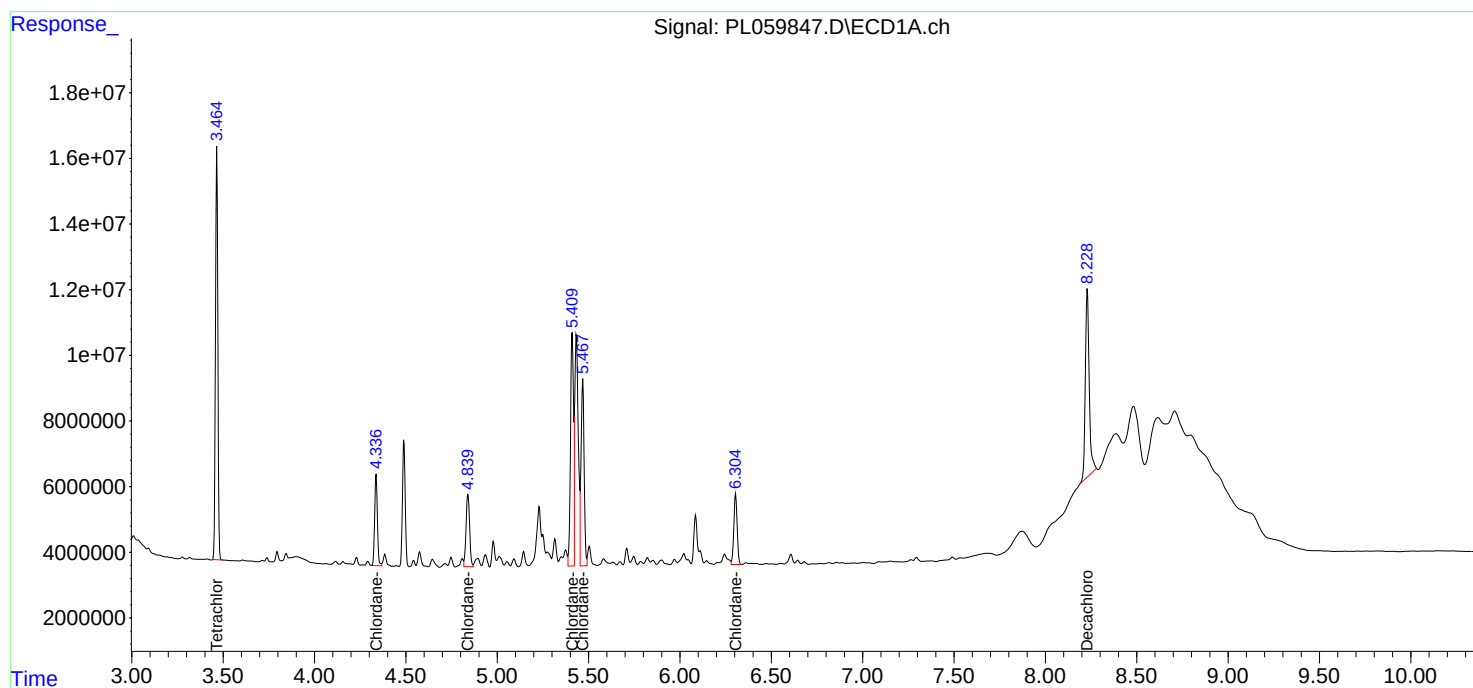


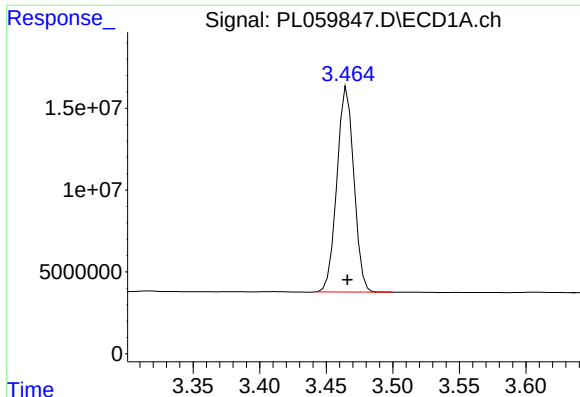

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 111023962
Conc: 57.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

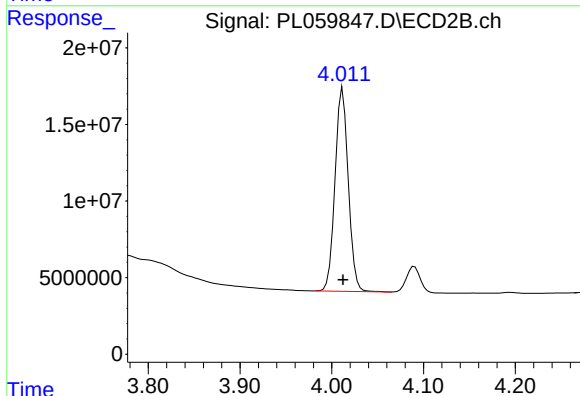


#1 Tetrachloro-m-xylene

R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 133320130
Conc: 50.31 ng/ml

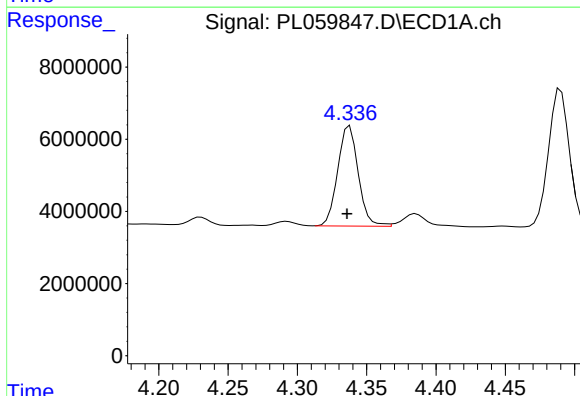


#23 Chlordane-1

R.T.: 4.338 min
Delta R.T.: 0.002 min
Response: 28707741
Conc: 468.57 ng/ml

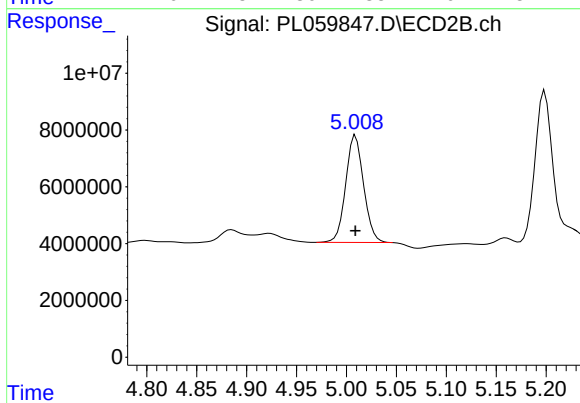

#23 Chlordane-1


R.T.: 5.009 min
Delta R.T.: 0.000 min
Response: 46916628
Conc: 483.14 ng/ml

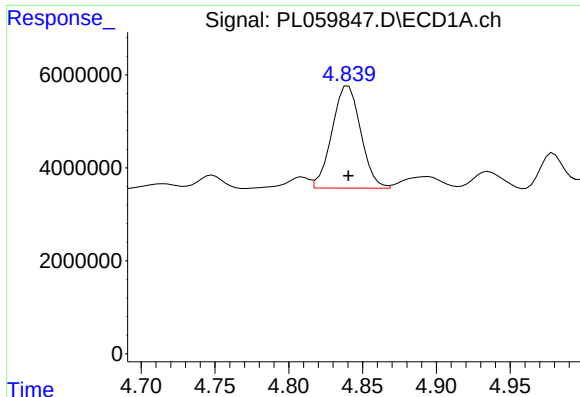

#24 Chlordane-2


R.T.: 4.840 min
Delta R.T.: 0.000 min
Response: 29870653
Conc: 471.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

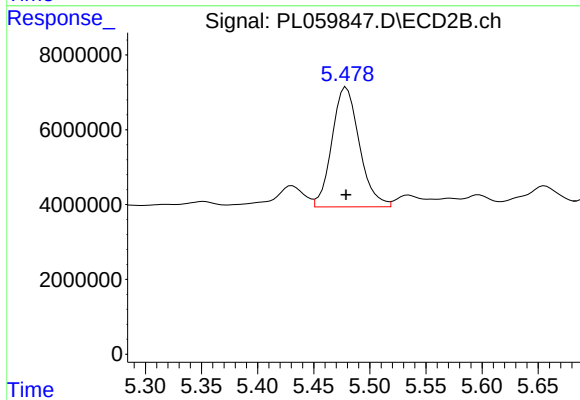


#24 Chlordane-2

R.T.: 5.479 min
Delta R.T.: 0.000 min
Response: 54425314
Conc: 475.02 ng/ml

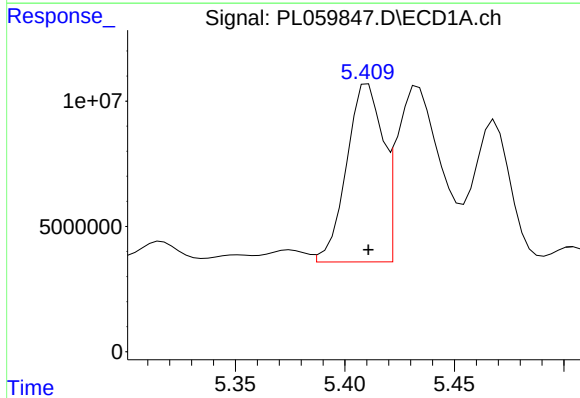


#25 Chlordane-3

R.T.: 5.411 min
Delta R.T.: 0.000 min
Response: 81022584
Conc: 479.10 ng/ml

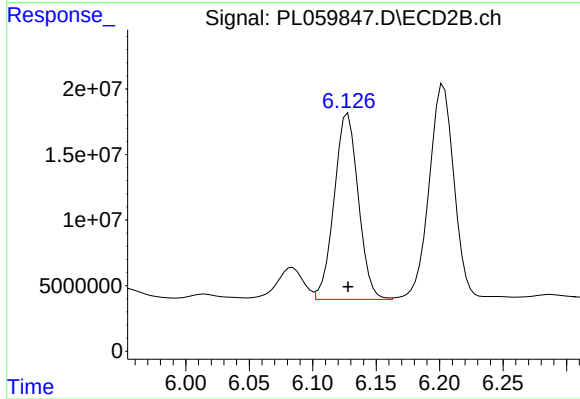

#25 Chlordane-3


R.T.: 6.128 min
Delta R.T.: 0.000 min
Response: 187803322
Conc: 485.38 ng/ml

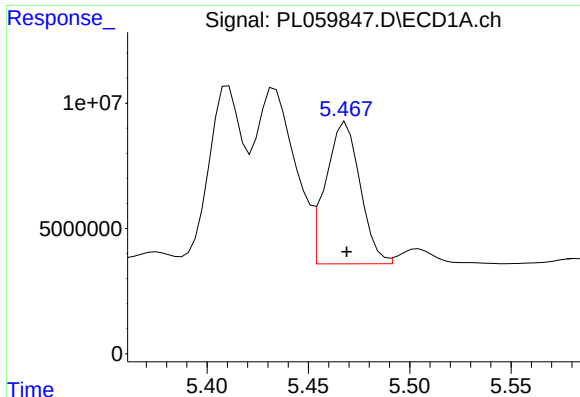

#26 Chlordane-4


R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 66729624
Conc: 478.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

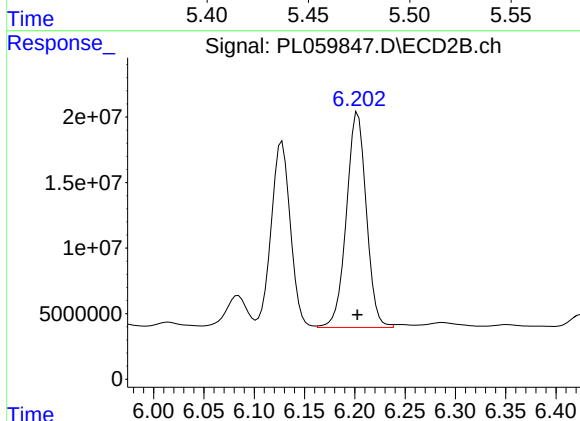


#26 Chlordane-4

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 225184549
Conc: 486.47 ng/ml

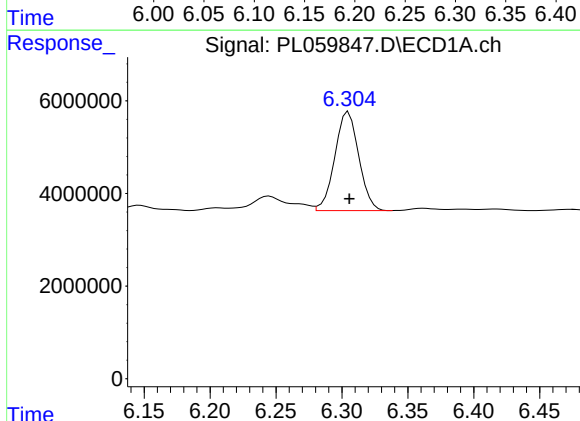


#27 Chlordane-5

R.T.: 6.305 min
Delta R.T.: 0.000 min
Response: 26952525
Conc: 475.01 ng/ml

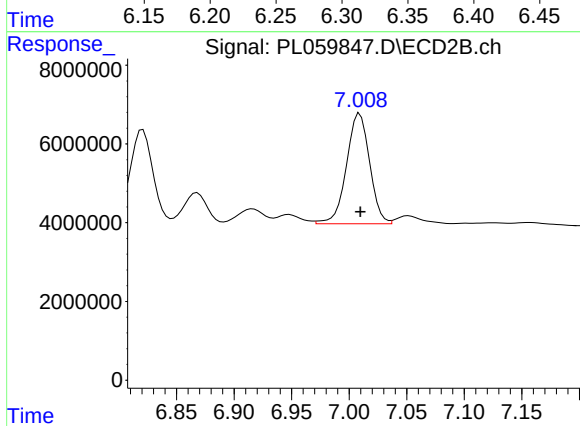

#27 Chlordane-5

R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 39421513
Conc: 507.58 ng/ml

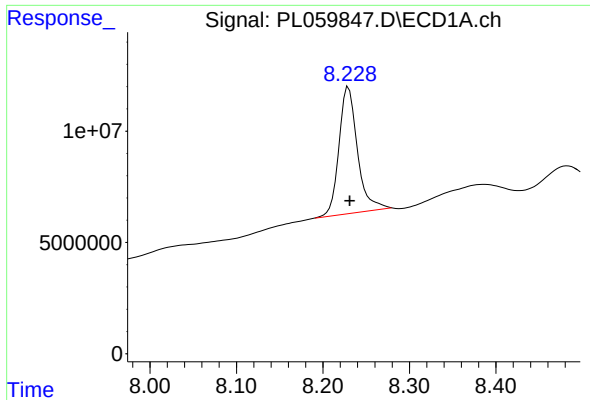

#28 Decachlorobiphenyl


R.T.: 8.230 min

Delta R.T.: -0.001 min

Response: 84817309

Conc: 51.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

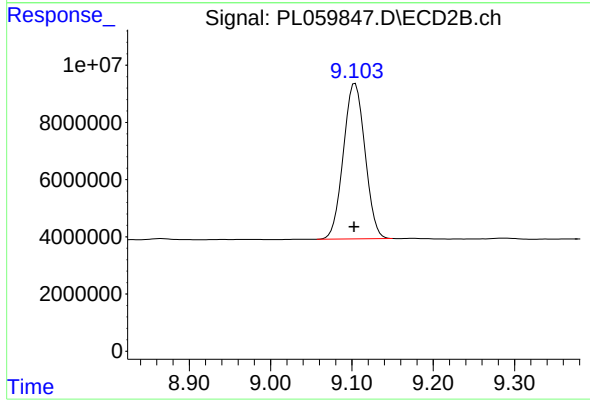

#28 Decachlorobiphenyl

R.T.: 9.104 min

Delta R.T.: 0.001 min

Response: 100276503

Conc: 47.95 ng/ml