

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071320\
 Data File : PL059863.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2020 17:58
 Operator : DD\AJ
 Sample : L3277-04RE
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TI-633RE

Manual Integrations
 APPROVED

Ankita
 7/14/2020 11:09:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 06:29:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	4.011	108.9E6	55457634	56.282	20.926m#
28)	SA Decachlor...	8.229	9.103	29265490	36593087	17.790	17.497

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071320\
Data File : PL059863.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2020 17:58
Operator : DD\AJ
Sample : L3277-04RE
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TI-633RE


Manual Integrations
APPROVED

Ankita
7/14/2020 11:09:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 06:29:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

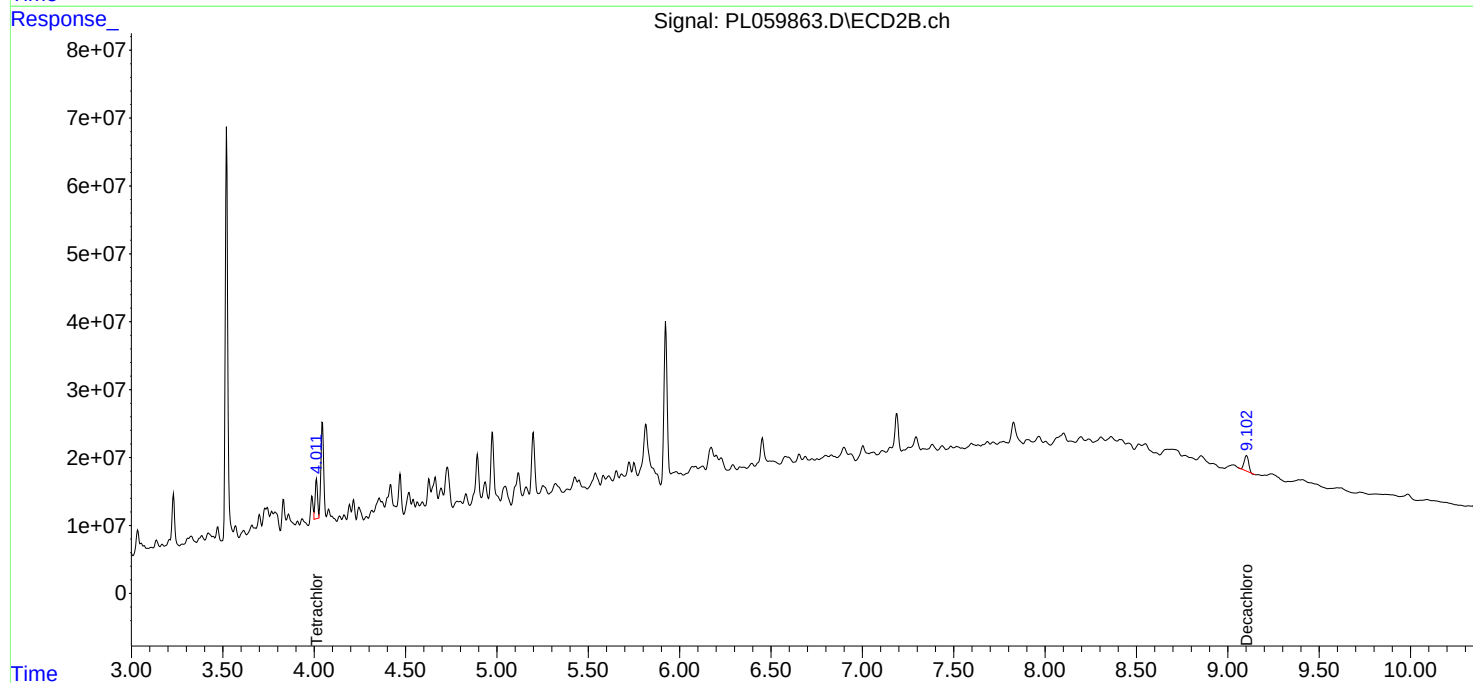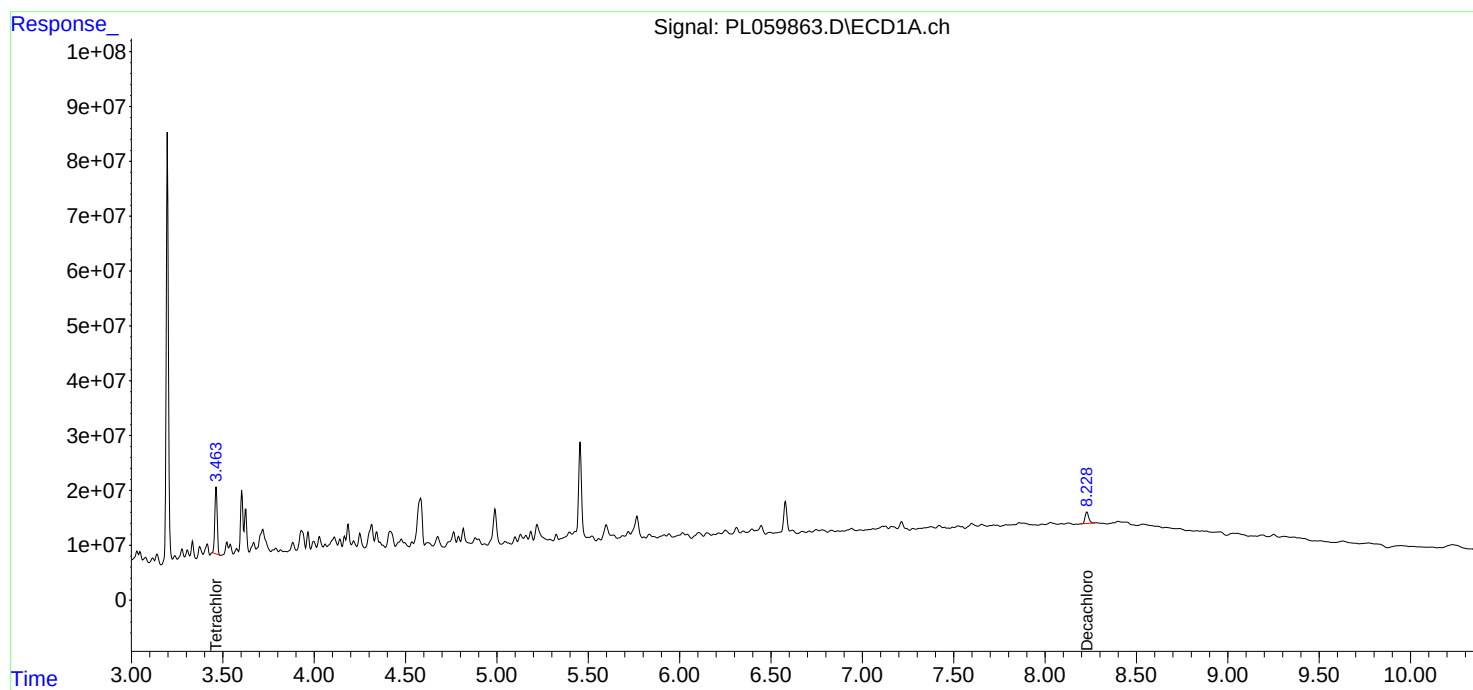

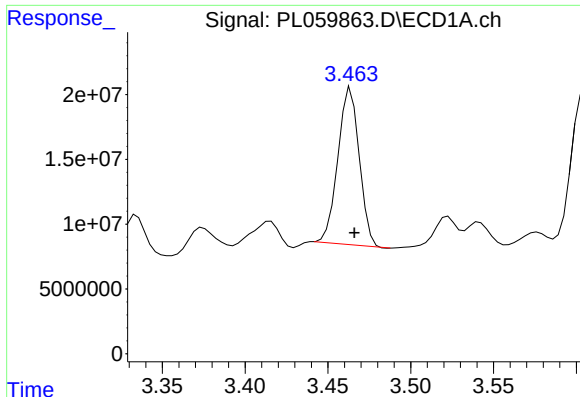


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.002 min
Response: 108861876
Conc: 56.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TI-633RE


Manual Integrations
APPROVED

Ankita
7/14/2020 11:09:58 AM

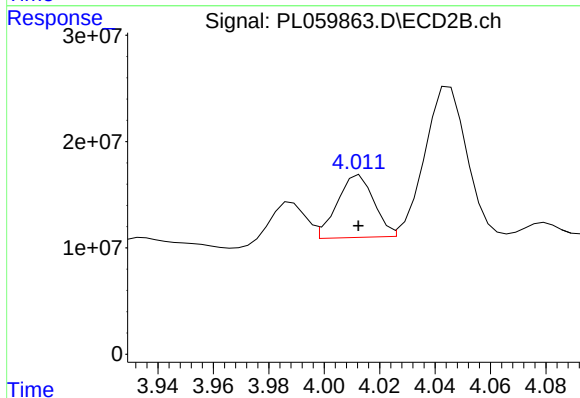


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 55457634
Conc: 20.93 ng/ml m

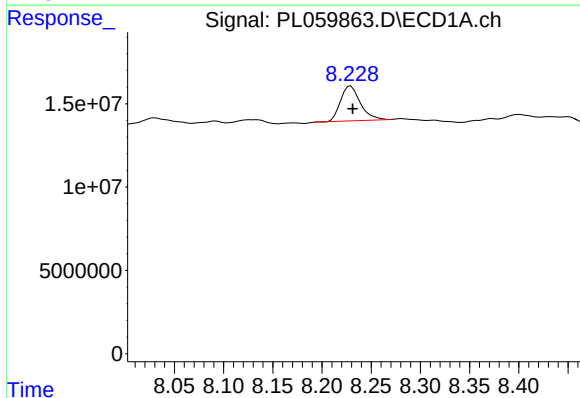

#28 Decachlorobiphenyl

R.T.: 8.229 min
Delta R.T.: -0.002 min
Response: 29265490
Conc: 17.79 ng/ml

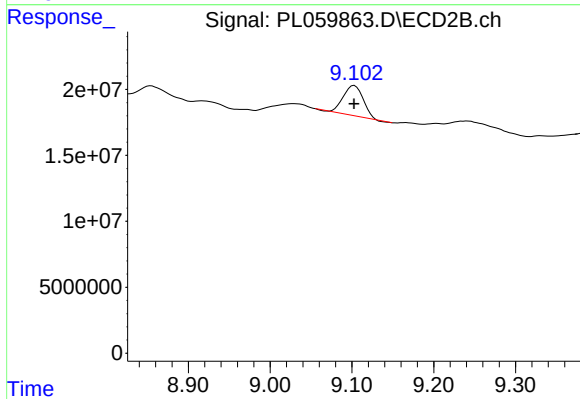

#28 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: 0.000 min
Response: 36593087
Conc: 17.50 ng/ml