

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071321\
 Data File : PL068096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2021 14:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 05:06:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 04:57:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.673	5.583	10490396	20336389	18.954	19.886
28)	SA Decachlor...	10.480	11.510	10873654	16501817	19.593	21.176
Target Compounds							
4)	MA Heptachlor	6.193f	0.000	362176	0	0.495	N.D. #
6)	B beta-BHC	6.193	0.000	362176	0	1.008	N.D. #
24)	Chlordane-2	6.691	0.000	147812	0	6.277	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071321\
Data File : PL068096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2021 14:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 05:06:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 04:57:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

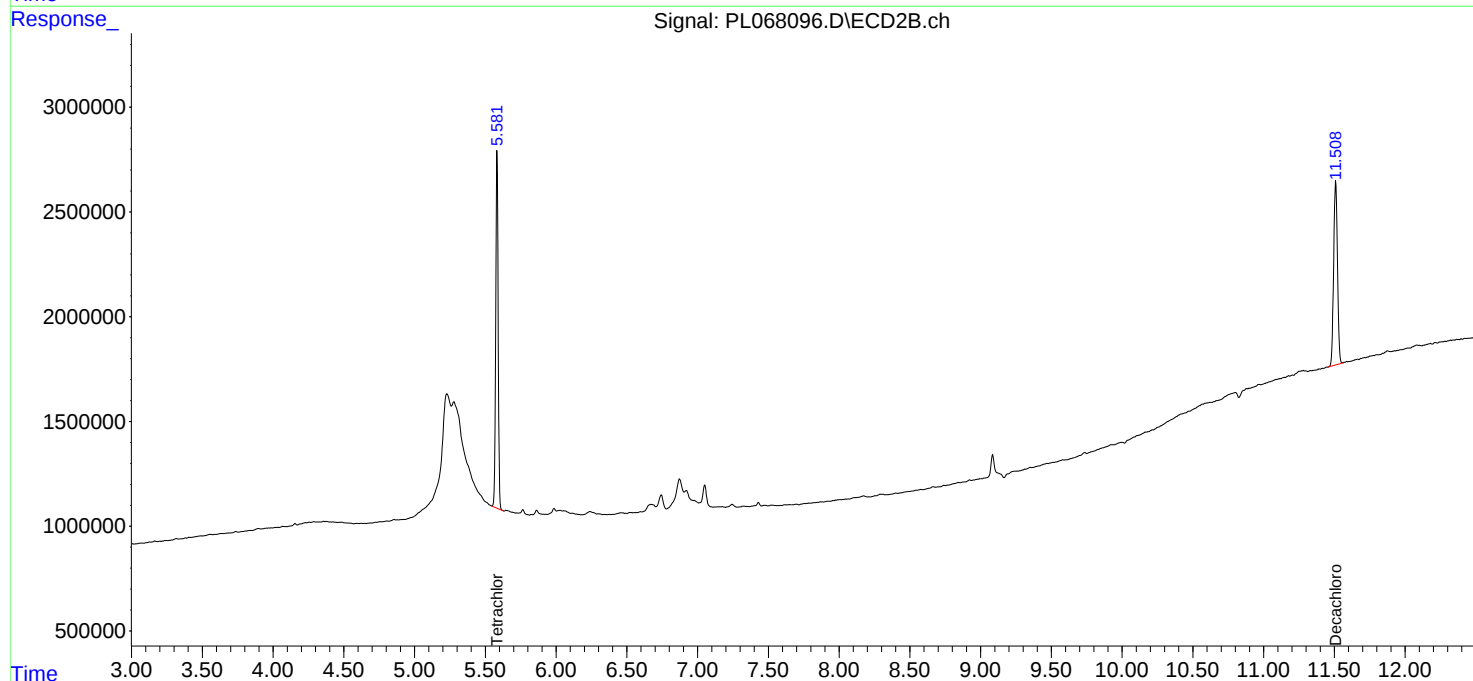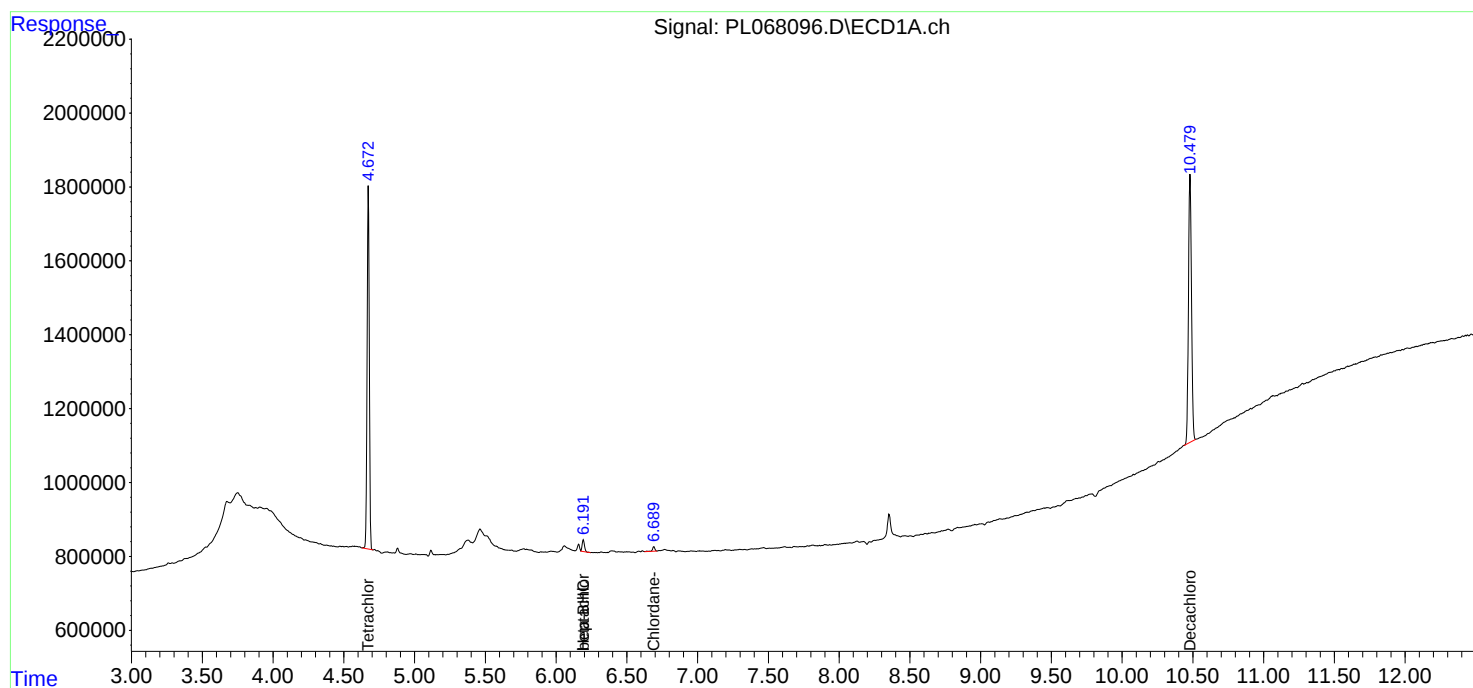


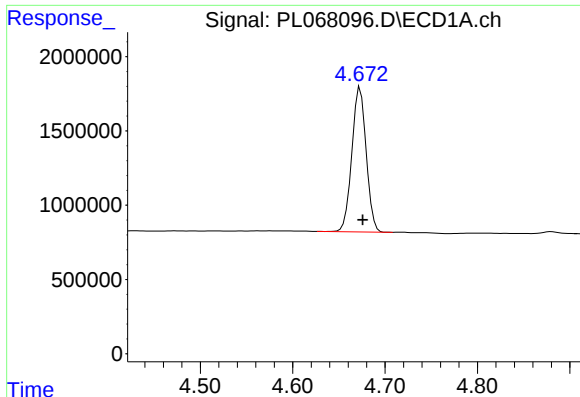

#1 Tetrachloro-m-xylene


R.T.: 4.673 min
Delta R.T.: -0.003 min
Response: 10490396
Conc: 18.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

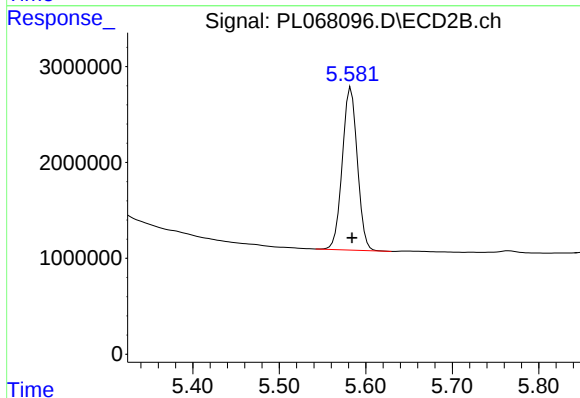


#1 Tetrachloro-m-xylene

R.T.: 5.583 min
Delta R.T.: -0.001 min
Response: 20336389
Conc: 19.89 ng/ml

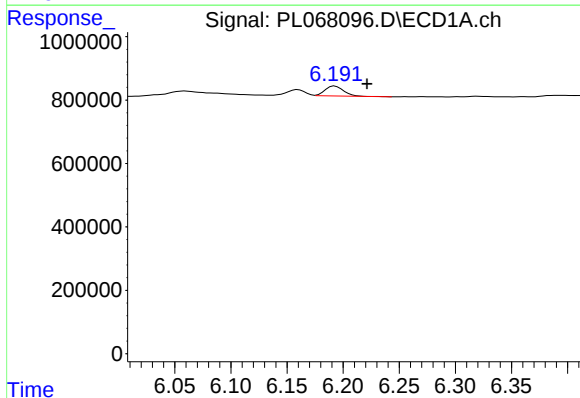


#4 Heptachlor

R.T.: 6.193 min
Delta R.T.: -0.028 min
Response: 362176
Conc: 0.49 ng/ml

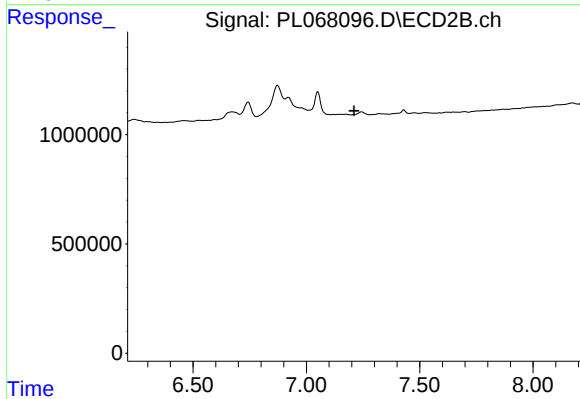

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.210 min
Response: 0
Conc: N.D.

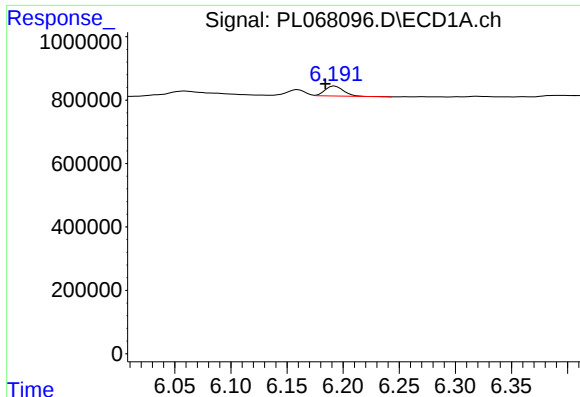

#6 beta-BHC


R.T.: 6.193 min
Delta R.T.: 0.008 min
Response: 362176
Conc: 1.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

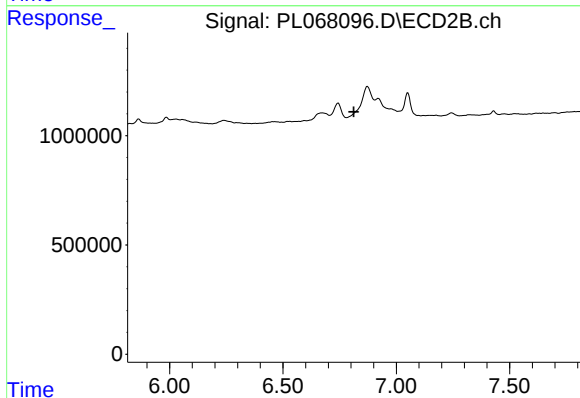


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.812 min
Response: 0
Conc: N.D.

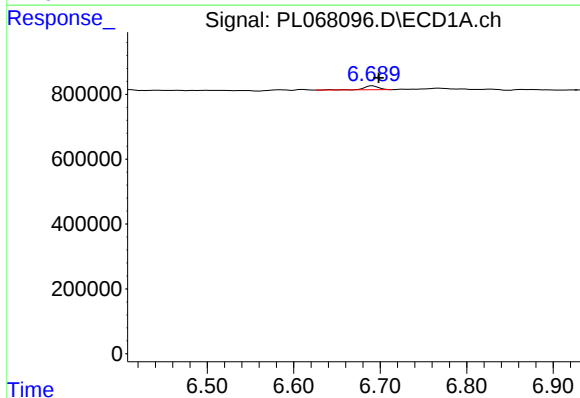


#24 Chlordane-2

R.T.: 6.691 min
Delta R.T.: -0.008 min
Response: 147812
Conc: 6.28 ng/ml

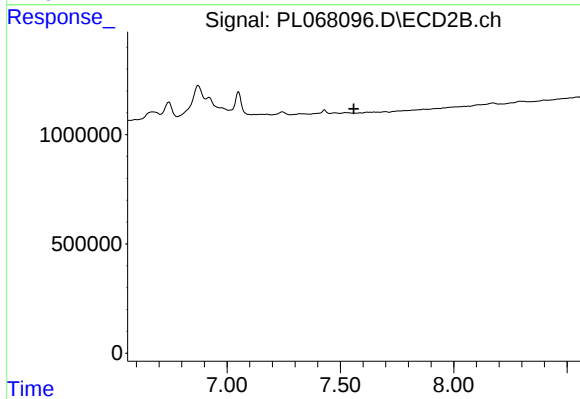

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 7.559 min
Response: 0
Conc: N.D.

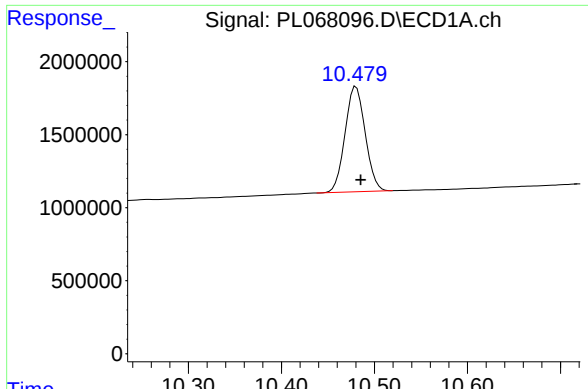

#28 Decachlorobiphenyl

R.T.: 10.480 min
Delta R.T.: -0.005 min
Response: 10873654
Conc: 19.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

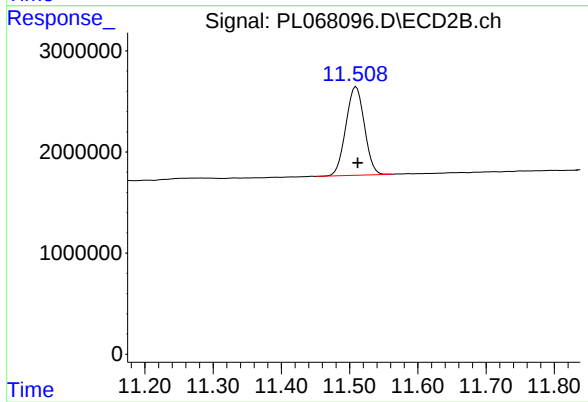

#28 Decachlorobiphenyl

R.T.: 11.510 min
Delta R.T.: -0.002 min
Response: 16501817
Conc: 21.18 ng/ml