

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071321\
 Data File : PL068104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2021 17:09
 Operator : AR\AJ
 Sample : M3014-01 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 05:08:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 14 04:57:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.671	5.581	1719297	3092411	3.106	3.024
28)	SA Decachlor...	10.473	11.504	1602143	2588275	2.887	3.321
Target Compounds							
6)	B beta-BHC	6.191	0.000	293496	0	0.817	N.D. #
15)	B Endosulfa...	8.392f	0.000	120998	0	0.230	N.D. #
17)	MA 4,4'-DDT	0.000	9.441	0	214218	N.D.	0.258 #
19)	B Endosulfa...	0.000	9.582	0	311410	N.D.	0.388 #
24)	Chlordane-2	6.700	0.000	2299384	0	97.653	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071321\
Data File : PL068104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2021 17:09
Operator : AR\AJ
Sample : M3014-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 05:08:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071221.M
Quant Title : GC Extractables
QLast Update : Wed Jul 14 04:57:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

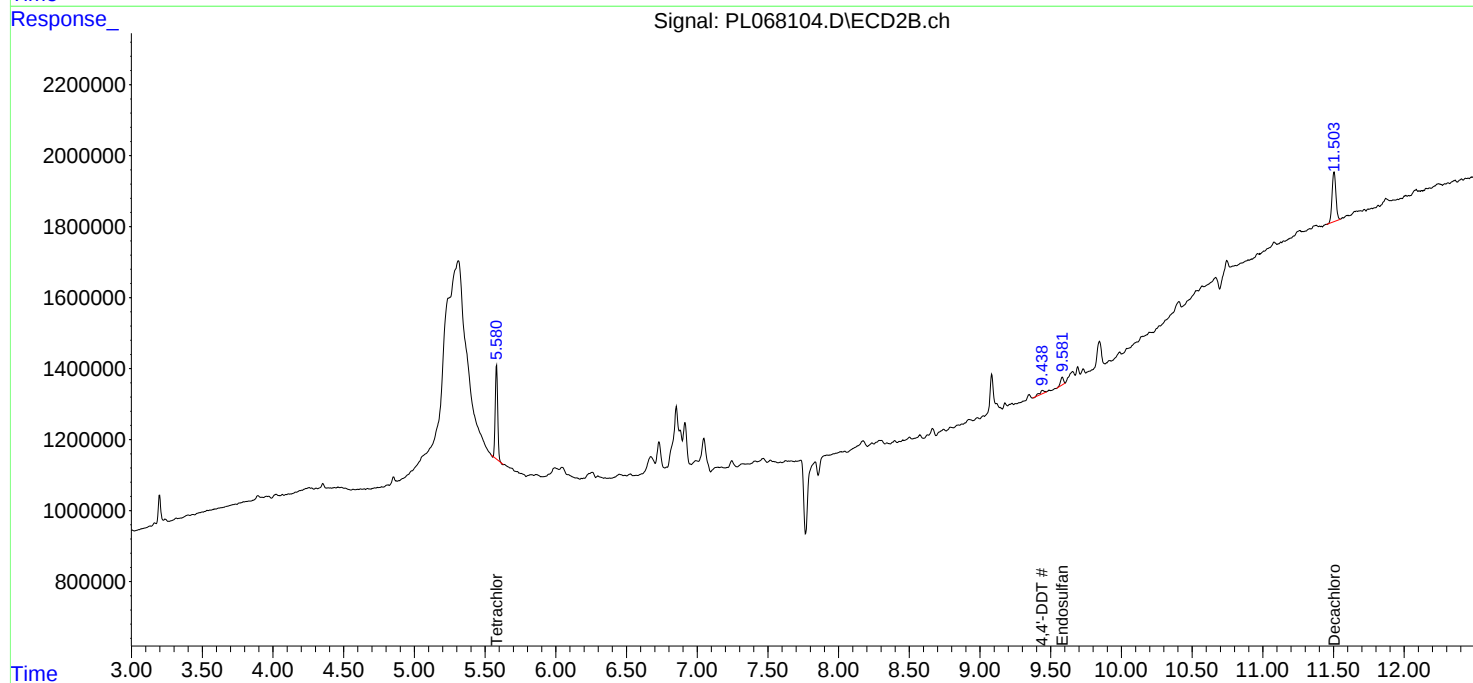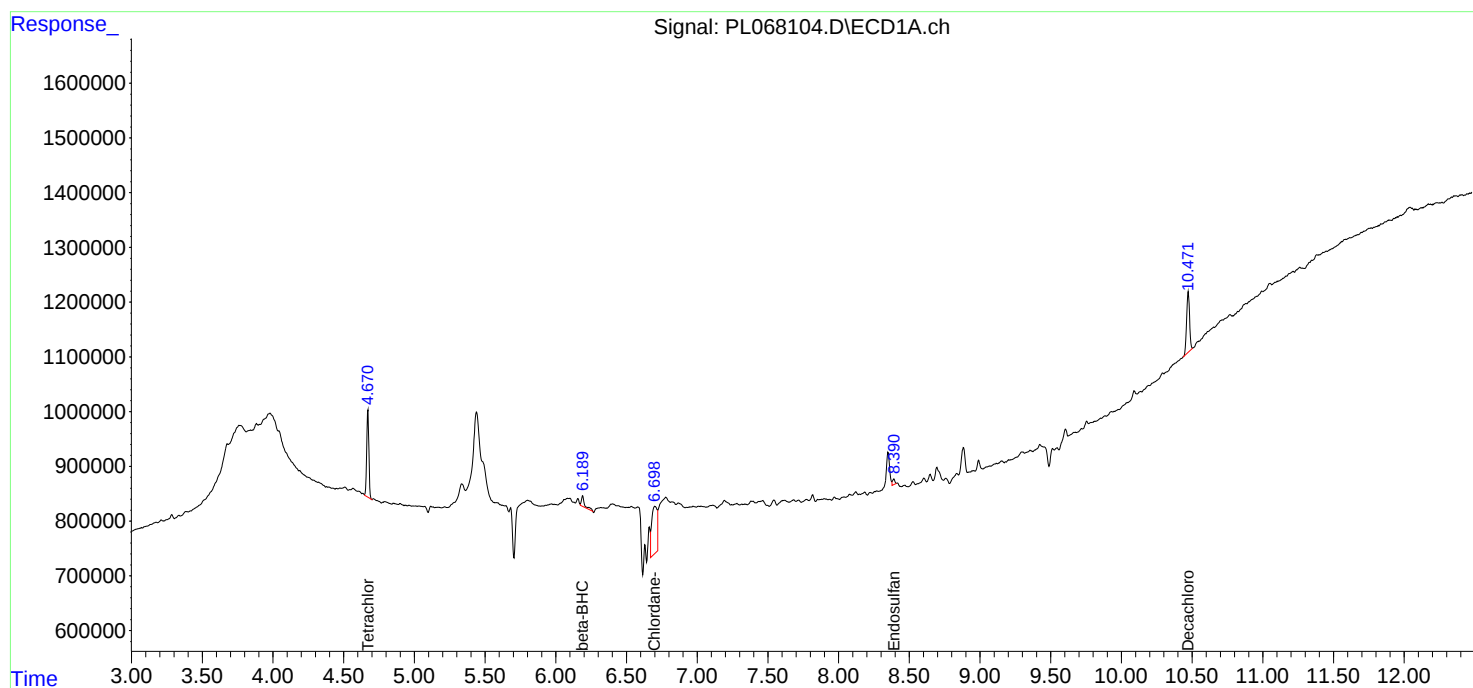


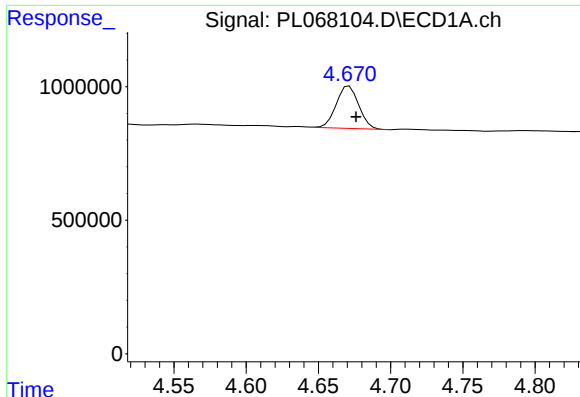

#1 Tetrachloro-m-xylene


R.T.: 4.671 min
Delta R.T.: -0.005 min
Response: 1719297
Conc: 3.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

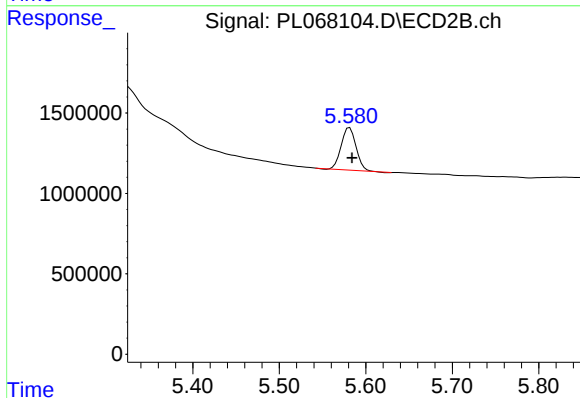


#1 Tetrachloro-m-xylene

R.T.: 5.581 min
Delta R.T.: -0.003 min
Response: 3092411
Conc: 3.02 ng/ml

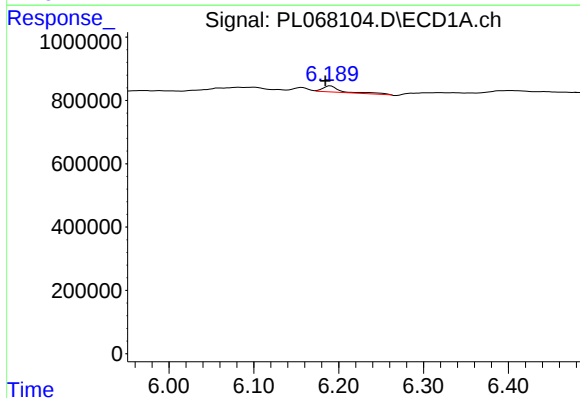


#6 beta-BHC

R.T.: 6.191 min
Delta R.T.: 0.006 min
Response: 293496
Conc: 0.82 ng/ml

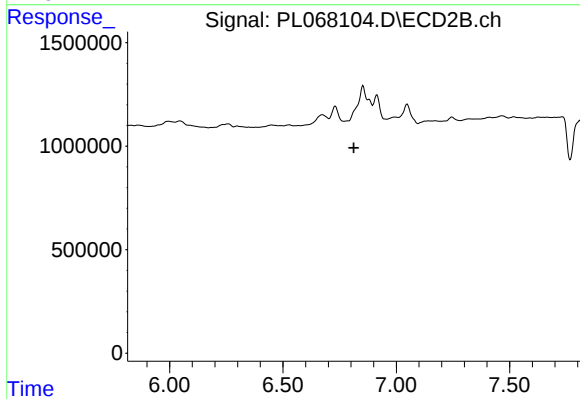

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.812 min
Response: 0
Conc: N.D.

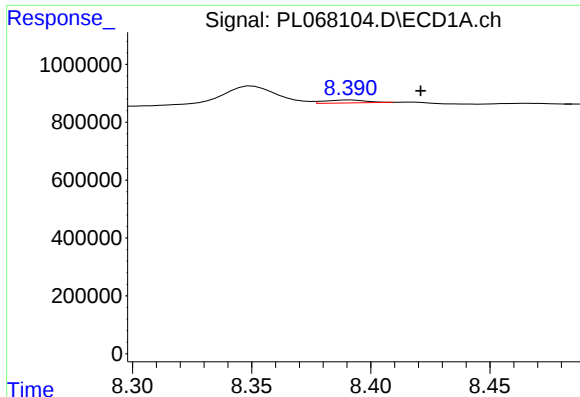

#15 Endosulfan II


R.T.: 8.392 min
Delta R.T.: -0.029 min
Response: 120998
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

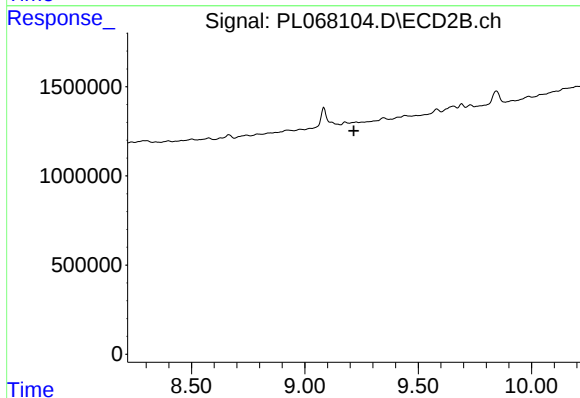


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.216 min
Response: 0
Conc: N.D.

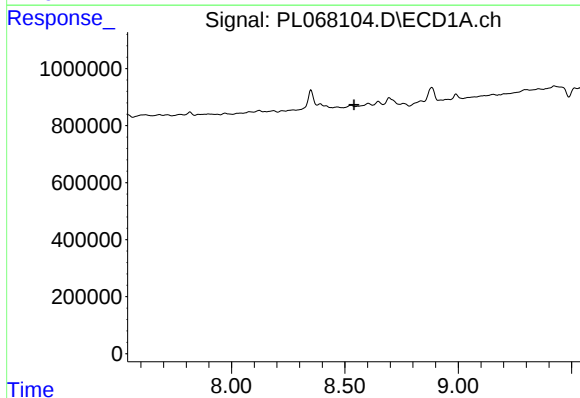


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

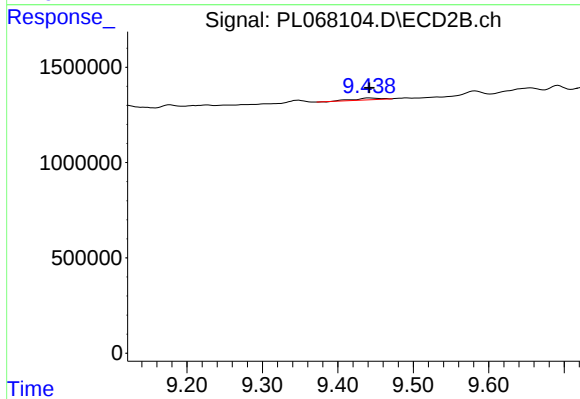

#17 4,4'-DDT


R.T.: 9.441 min
Delta R.T.: 0.000 min
Response: 214218
Conc: 0.26 ng/ml

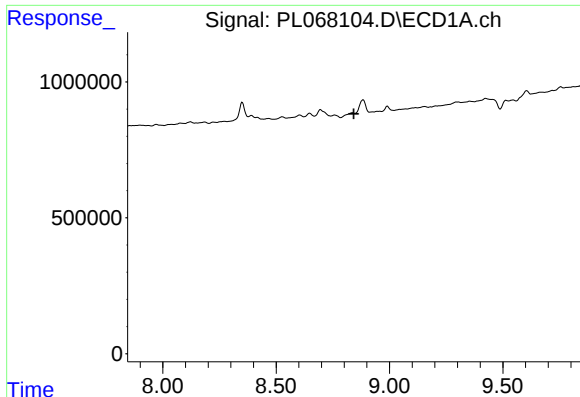

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.842 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

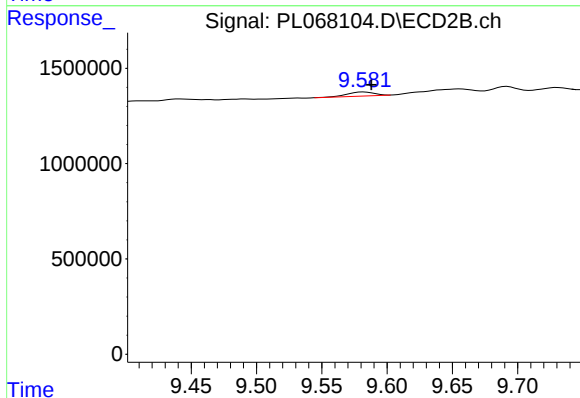


#19 Endosulfan Sulfate

R.T.: 9.582 min
Delta R.T.: -0.006 min
Response: 311410
Conc: 0.39 ng/ml

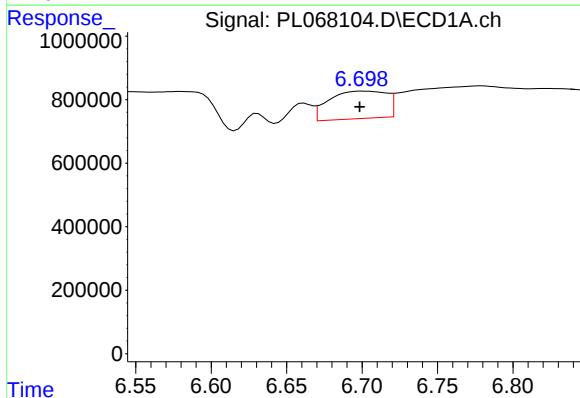


#24 Chlordane-2

R.T.: 6.700 min
Delta R.T.: 0.002 min
Response: 2299384
Conc: 97.65 ng/ml

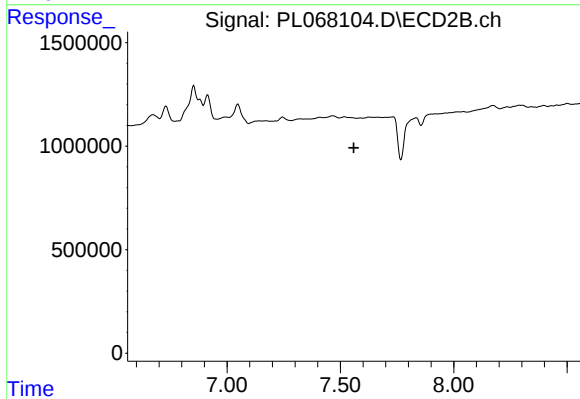

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.559 min
Response: 0
Conc: N.D.

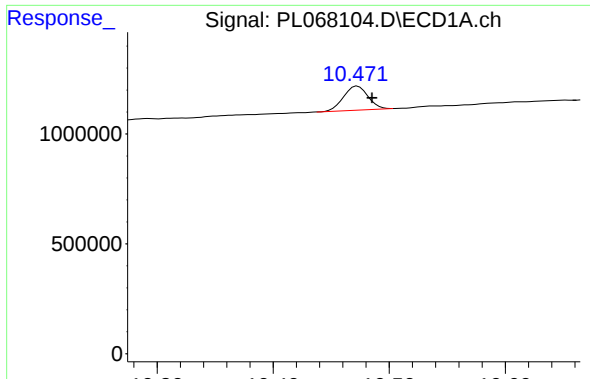

#28 Decachlorobiphenyl

R.T.: 10.473 min
Delta R.T.: -0.012 min
Response: 1602143
Conc: 2.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

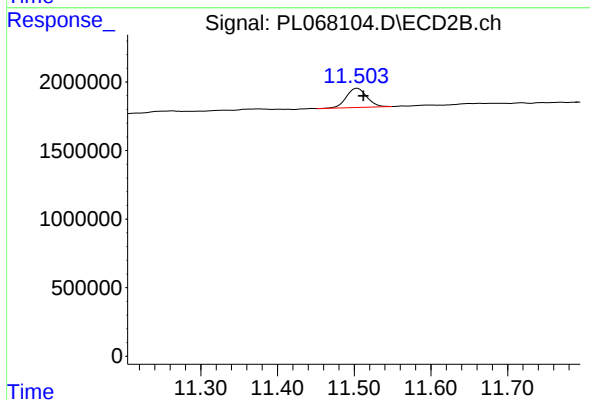

#28 Decachlorobiphenyl

R.T.: 11.504 min
Delta R.T.: -0.008 min
Response: 2588275
Conc: 3.32 ng/ml