

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071322\
 Data File : PL076408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 09:12
 Operator : AR\AJ
 Sample : L.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:08:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.640	4.626	14088416	36860155	19.556	18.231
28)	SA Decachlor...	11.628	10.362	10721764	31485156	18.174	18.764
Target Compounds							
7)	B delta-BHC	7.118f	6.391	326234	605238	0.487	0.253 #
11)	B alpha-Chl...	0.000	7.376f	0	411323	N.D.	0.205 #
13)	MA Dieldrin	0.000	7.736	0	213933	N.D.	0.113 #
15)	B Endosulfa...	9.299	0.000	236486	0	0.396	N.D. #
17)	MA 4,4'-DDT	0.000	8.448	0	332465	N.D.	0.213 #
21)	B Endrin ke...	10.182	0.000	364045	0	0.538	N.D. #
22)	Mirex	10.668f	0.000	564362	0	1.103	N.D. #
26)	Chlordane-4	0.000	7.376f	0	411323	N.D.	2.230 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071322\
Data File : PL076408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 09:12
Operator : AR\AJ
Sample : L.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:08:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

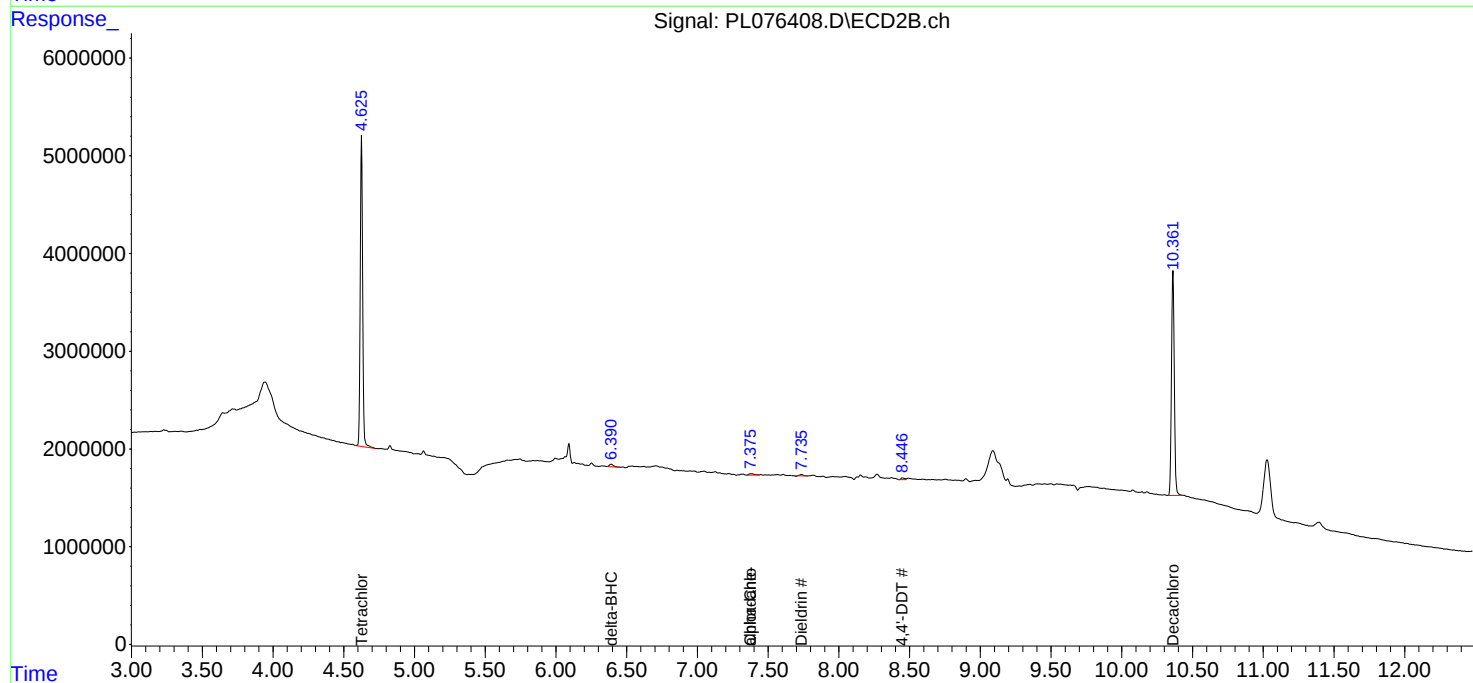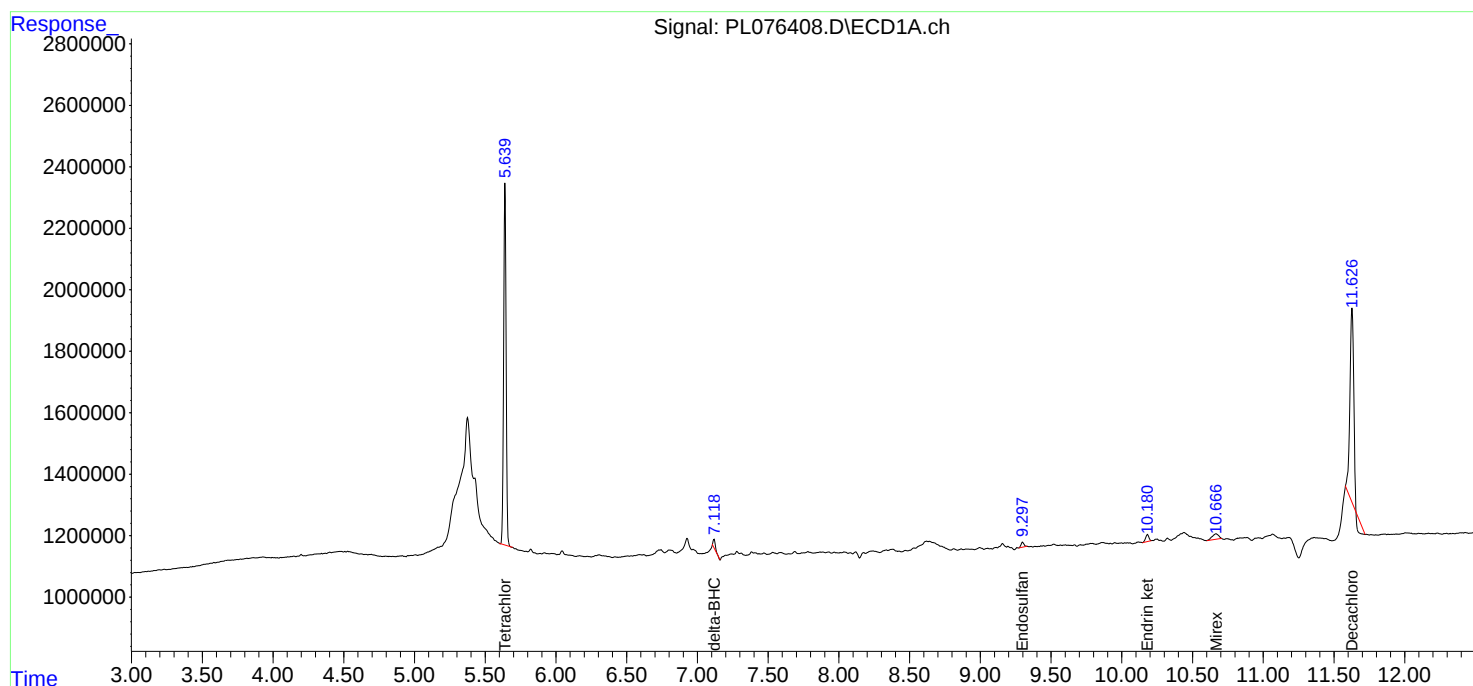


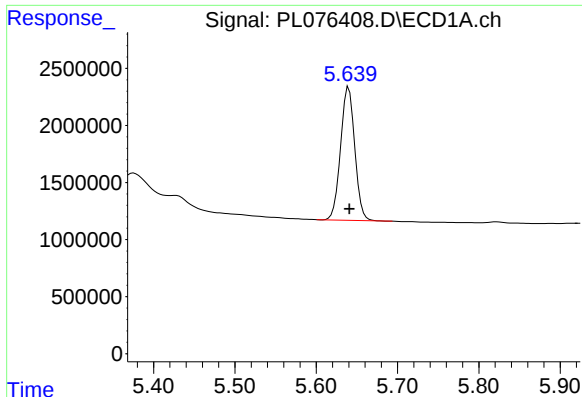

#1 Tetrachloro-m-xylene


R.T.: 5.640 min
Delta R.T.: -0.001 min
Response: 14088416
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

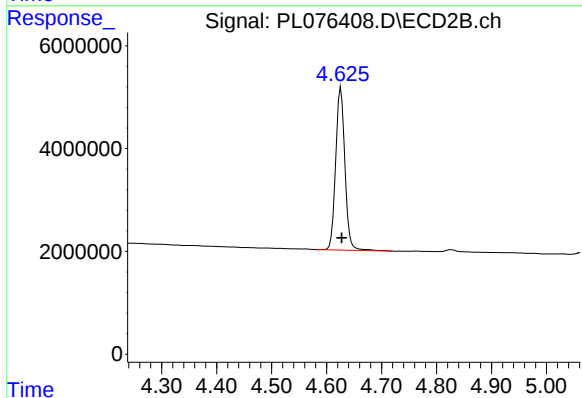


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: -0.002 min
Response: 36860155
Conc: 18.23 ng/ml

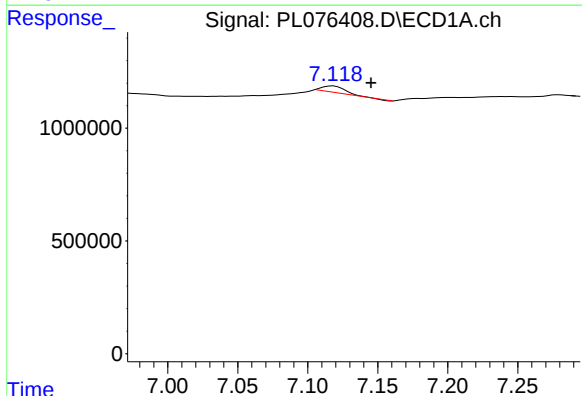


#7 delta-BHC

R.T.: 7.118 min
Delta R.T.: -0.027 min
Response: 326234
Conc: 0.49 ng/ml

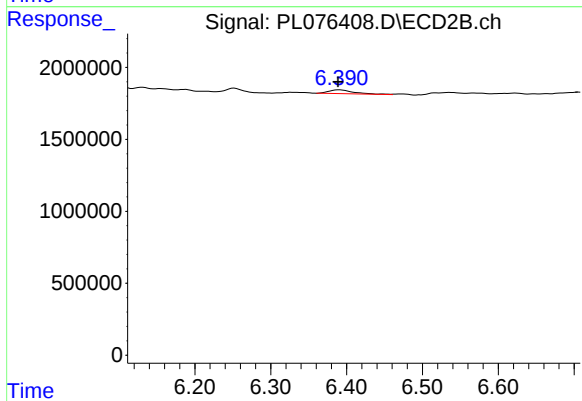

#7 delta-BHC


R.T.: 6.391 min
Delta R.T.: 0.002 min
Response: 605238
Conc: 0.25 ng/ml

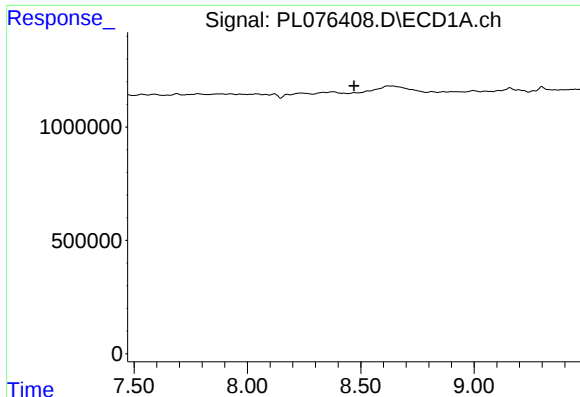

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

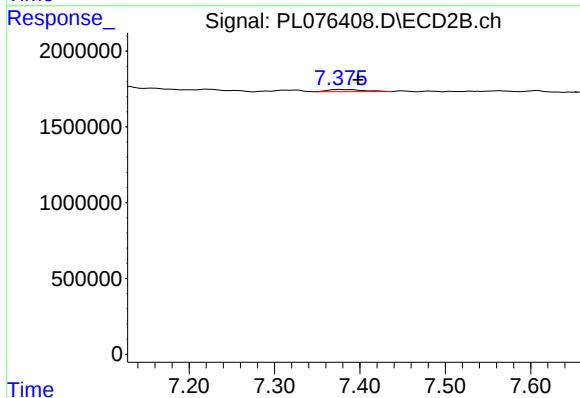


#11 alpha-Chlordane

R.T.: 7.376 min
Delta R.T.: -0.022 min
Response: 411323
Conc: 0.20 ng/ml

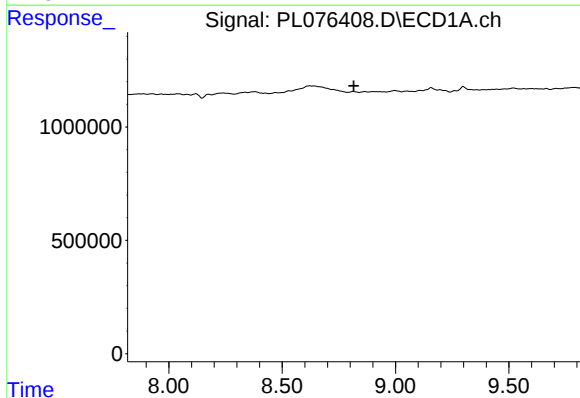


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

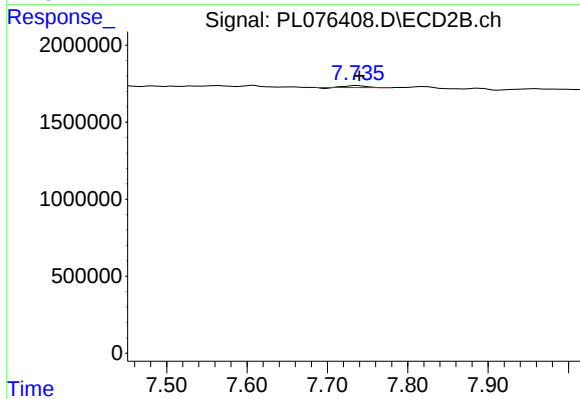

#13 Dieldrin


R.T.: 7.736 min
Delta R.T.: -0.004 min
Response: 213933
Conc: 0.11 ng/ml

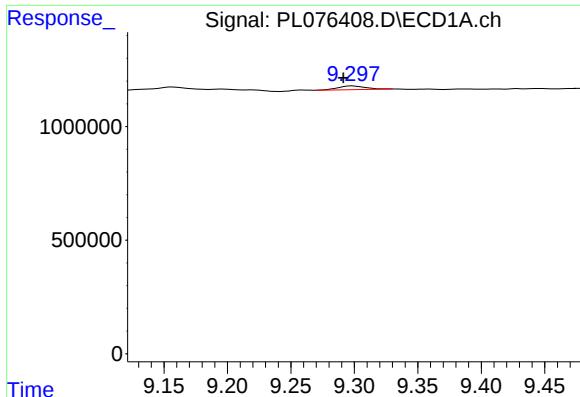

#15 Endosulfan II


R.T.: 9.299 min
Delta R.T.: 0.007 min
Response: 236486
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

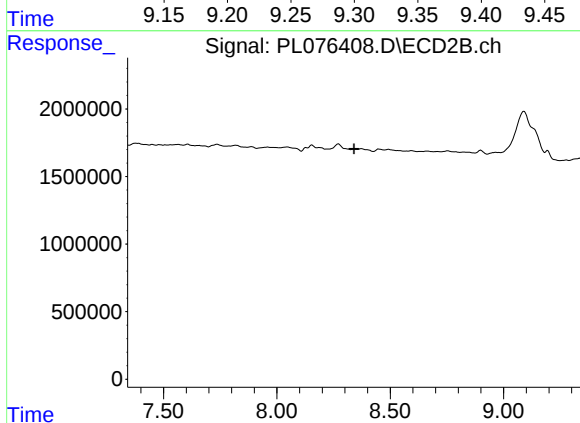


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.340 min
Response: 0
Conc: N.D.

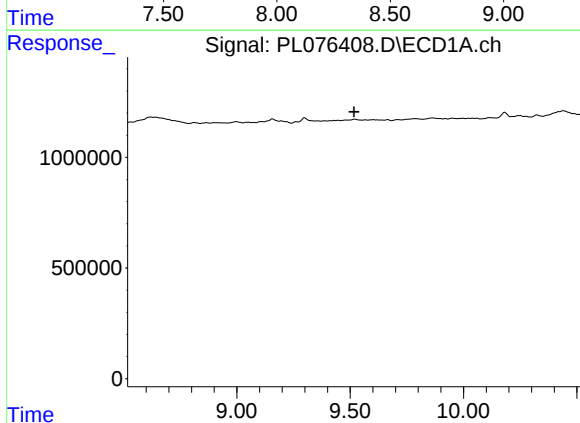


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.517 min
Response: 0
Conc: N.D.

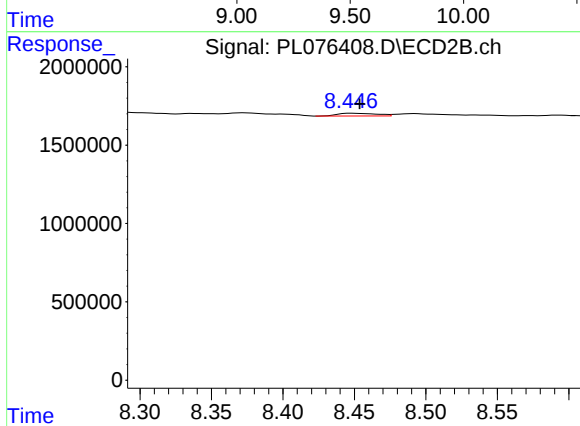

#17 4,4'-DDT


R.T.: 8.448 min
Delta R.T.: -0.006 min
Response: 332465
Conc: 0.21 ng/ml

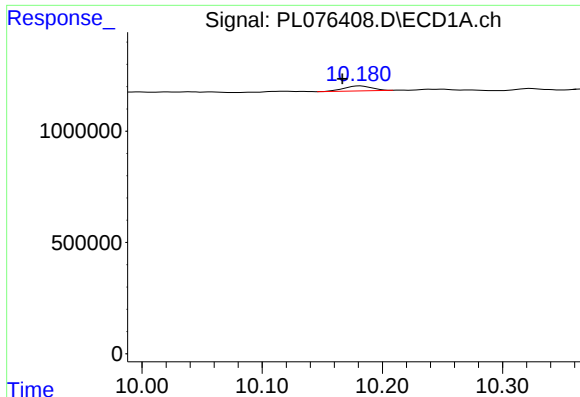

#21 Endrin ketone


R.T.: 10.182 min
Delta R.T.: 0.015 min
Response: 364045
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

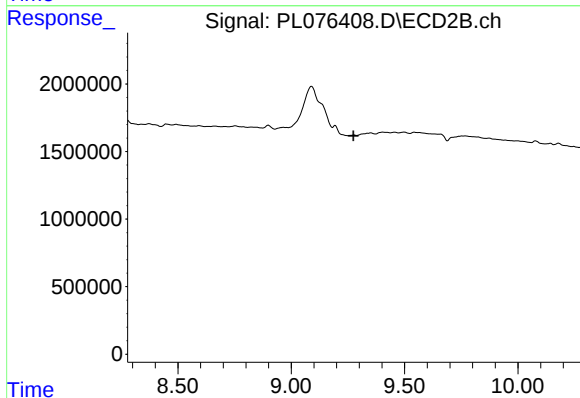


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.275 min
Response: 0
Conc: N.D.

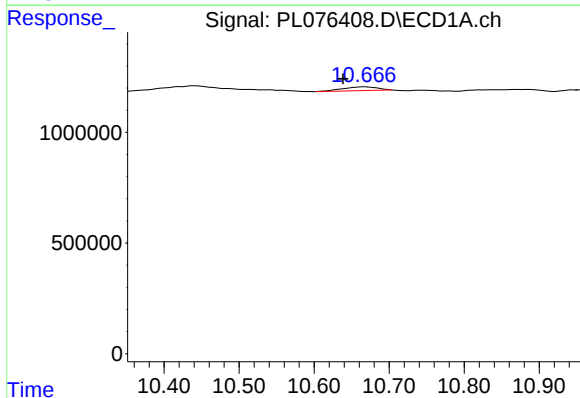


#22 Mirex

R.T.: 10.668 min
Delta R.T.: 0.029 min
Response: 564362
Conc: 1.10 ng/ml

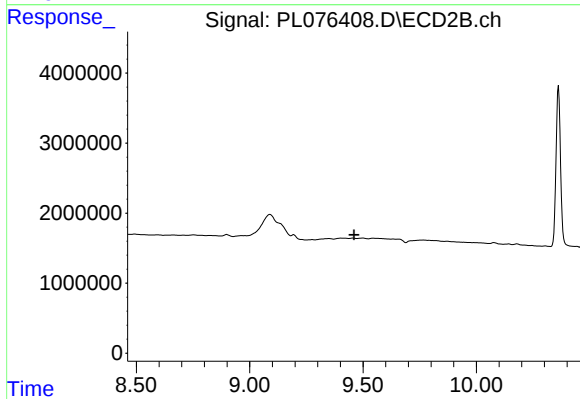

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.460 min
Response: 0
Conc: N.D.

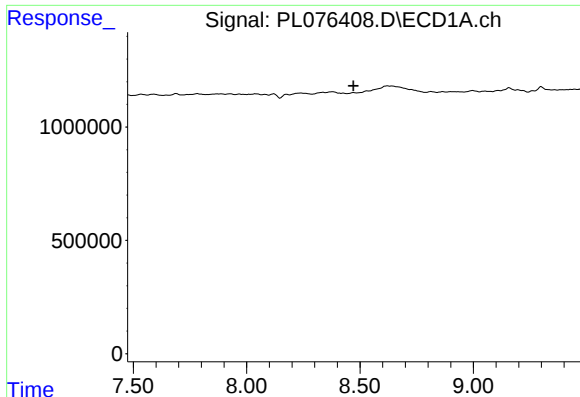

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

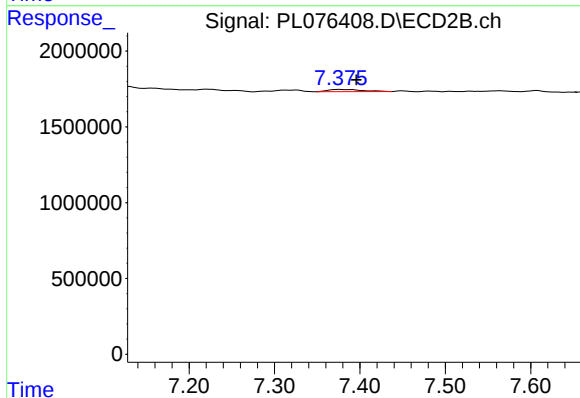


#26 Chlordane-4

R.T.: 7.376 min
Delta R.T.: -0.020 min
Response: 411323
Conc: 2.23 ng/ml

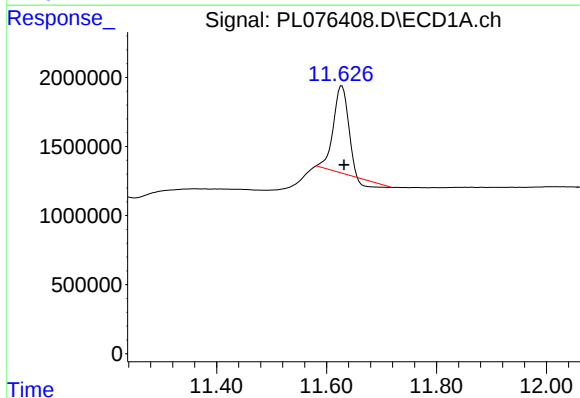

#28 Decachlorobiphenyl

R.T.: 11.628 min
Delta R.T.: -0.004 min
Response: 10721764
Conc: 18.17 ng/ml

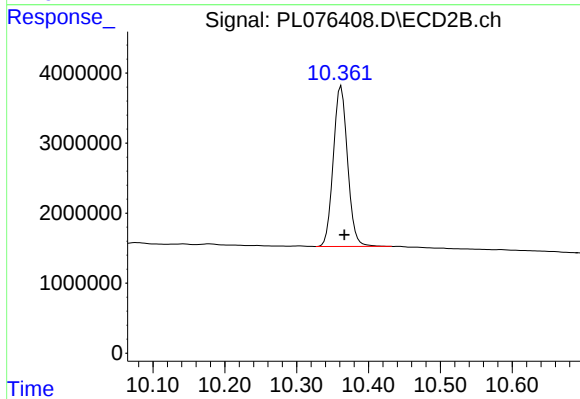

#28 Decachlorobiphenyl

R.T.: 10.362 min
Delta R.T.: -0.005 min
Response: 31485156
Conc: 18.76 ng/ml