

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071322\
 Data File : PL076412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 11:35
 Operator : AR\AJ
 Sample : PB146156BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:11:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 08 16:50:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.625	12168916	32302144	16.892	15.976
28)	SA Decachlor...	11.633	10.363	11284960	28873694	19.128	17.208
Target Compounds							
4)	MA Heptachlor	7.298f	0.000	632975	0	0.730	N.D. #
8)	B Heptachlo...	8.124	0.000	979924	0	1.259	N.D. #
11)	B alpha-Chl...	0.000	7.370f	0	1064930	N.D.	0.530 #
14)	MA Endrin	0.000	8.051f	0	751187	N.D.	0.520 #
15)	B Endosulfa...	9.302	0.000	367130	0	0.615	N.D. #
21)	B Endrin ke...	10.183f	0.000	658234	0	0.974	N.D. #
23)	Chlordane-1	0.000	5.960	0	1641696	N.D.	29.174 #
24)	Chlordane-2	0.000	6.643	0	2229552	N.D.	34.365 #
26)	Chlordane-4	0.000	7.370f	0	1064930	N.D.	5.774 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071322\
Data File : PL076412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 11:35
Operator : AR\AJ
Sample : PB146156BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:11:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070822.M
Quant Title : GC Extractables
QLast Update : Fri Jul 08 16:50:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

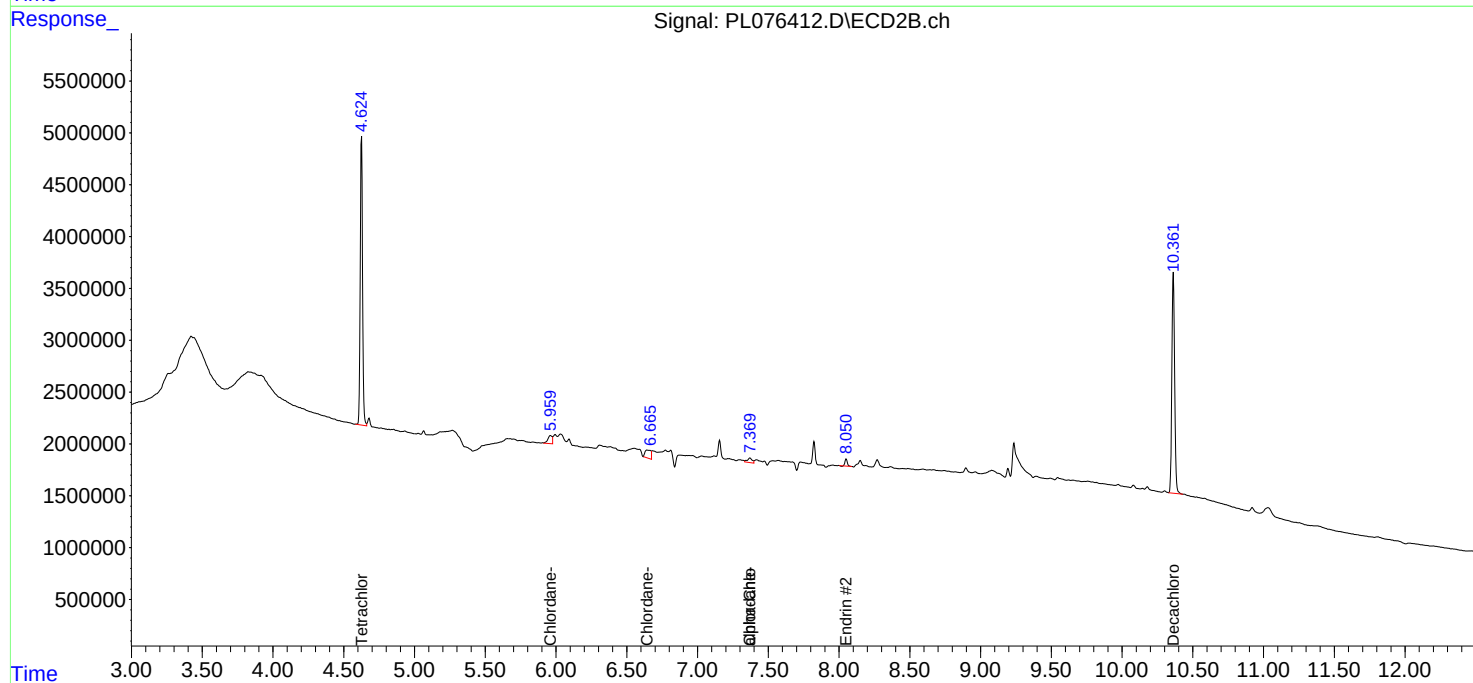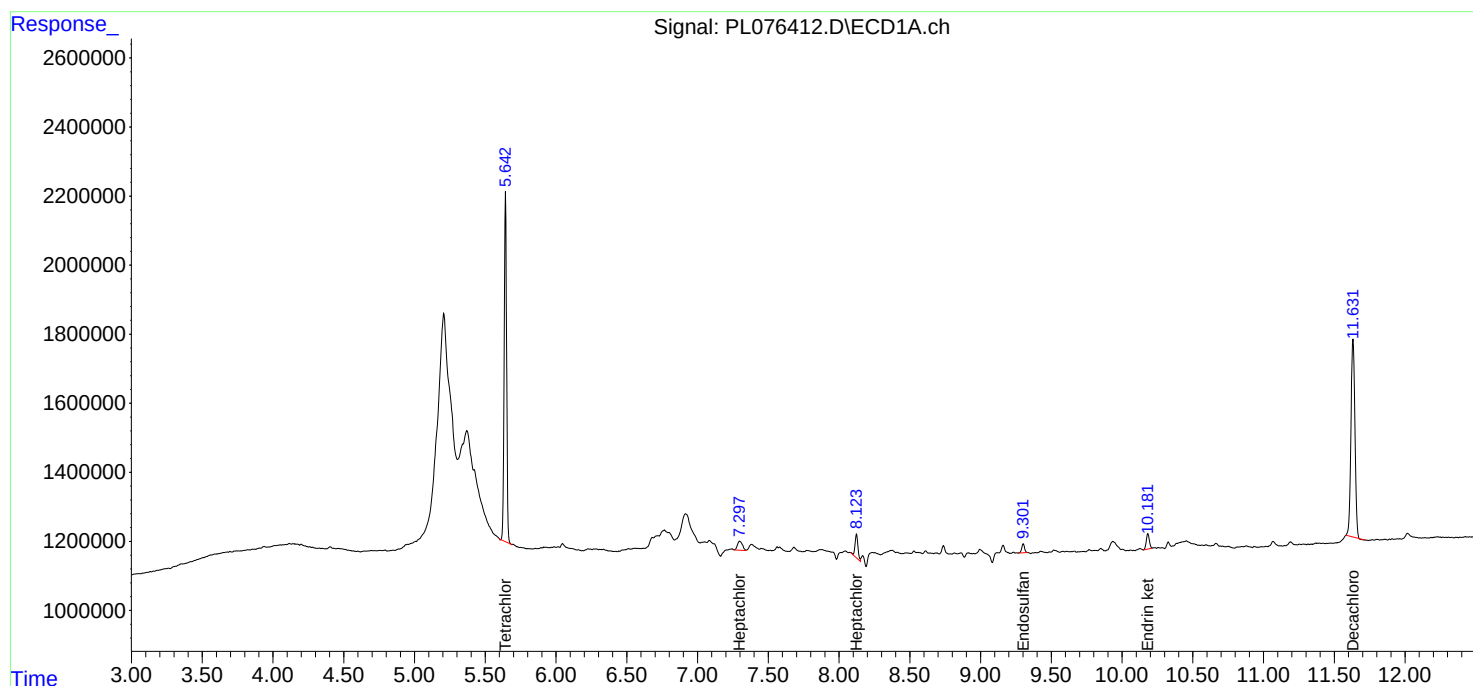


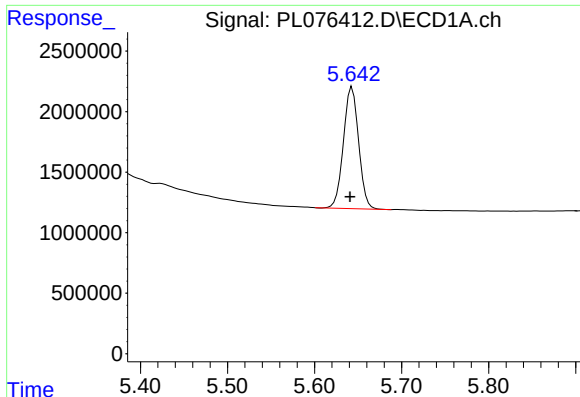

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 12168916
Conc: 16.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

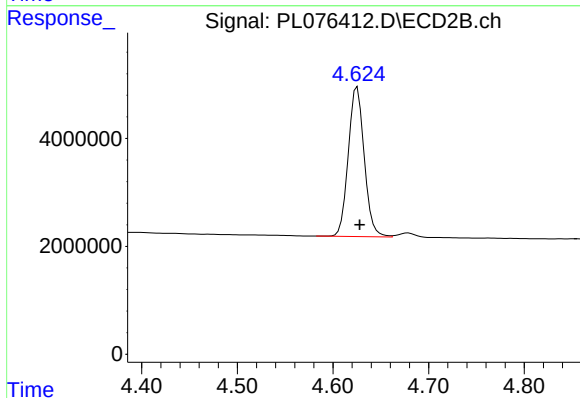


#1 Tetrachloro-m-xylene

R.T.: 4.625 min
Delta R.T.: -0.002 min
Response: 32302144
Conc: 15.98 ng/ml

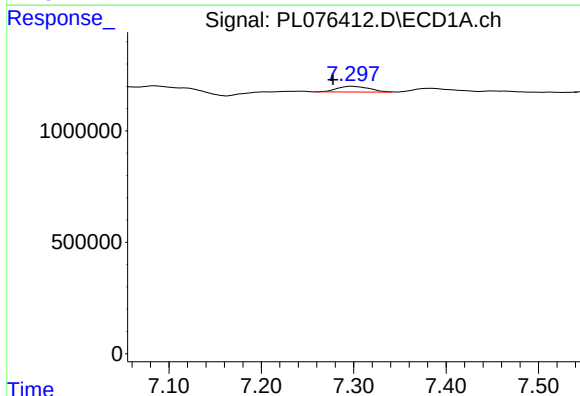


#4 Heptachlor

R.T.: 7.298 min
Delta R.T.: 0.020 min
Response: 632975
Conc: 0.73 ng/ml

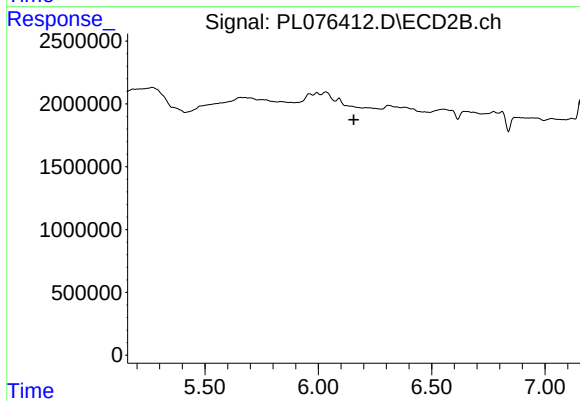

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 6.156 min
Response: 0
Conc: N.D.

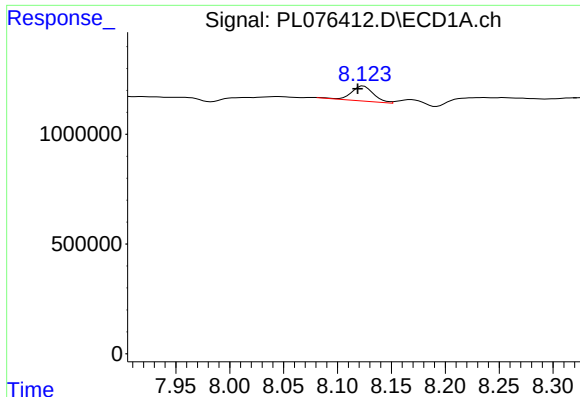

#8 Heptachlor epoxide


R.T.: 8.124 min
Delta R.T.: 0.005 min
Response: 979924
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

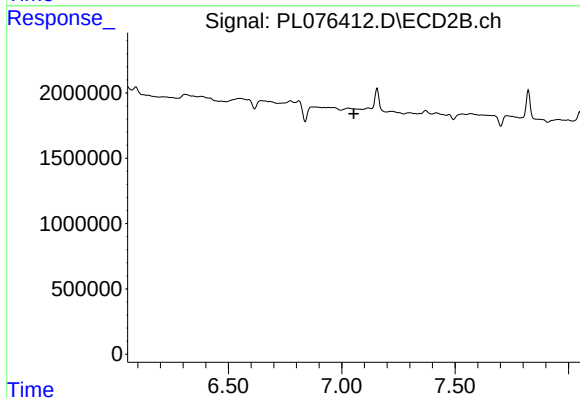


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.053 min
Response: 0
Conc: N.D.

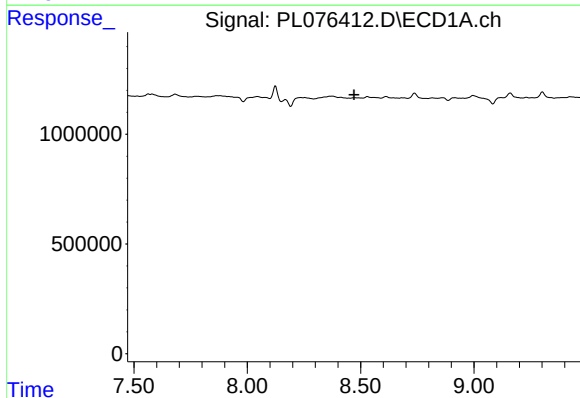


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.471 min
Response: 0
Conc: N.D.

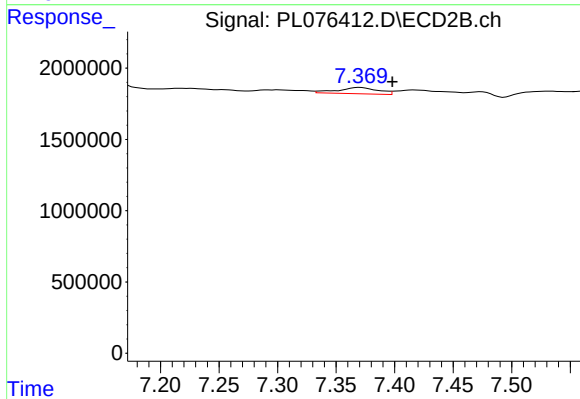

#11 alpha-Chlordane


R.T.: 7.370 min
Delta R.T.: -0.028 min
Response: 1064930
Conc: 0.53 ng/ml

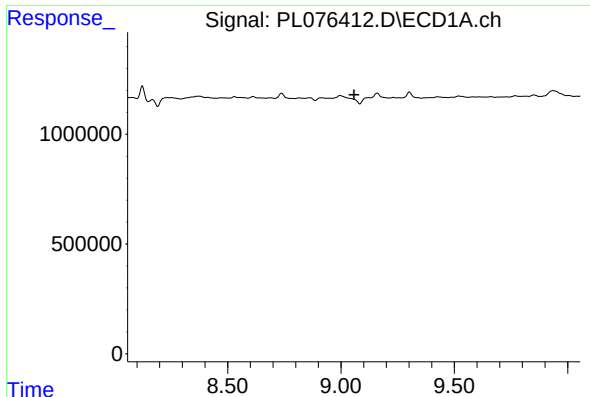

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

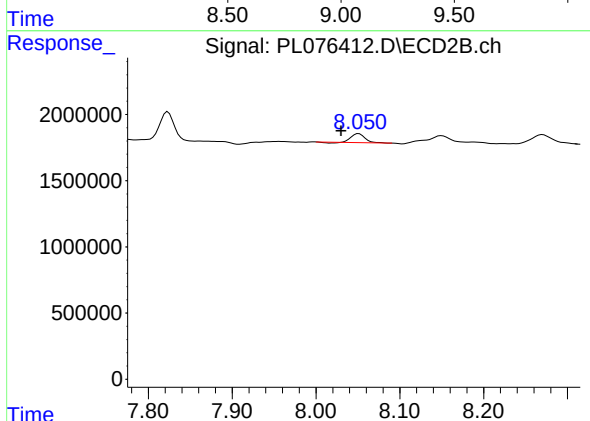


#14 Endrin

R.T.: 8.051 min
Delta R.T.: 0.021 min
Response: 751187
Conc: 0.52 ng/ml

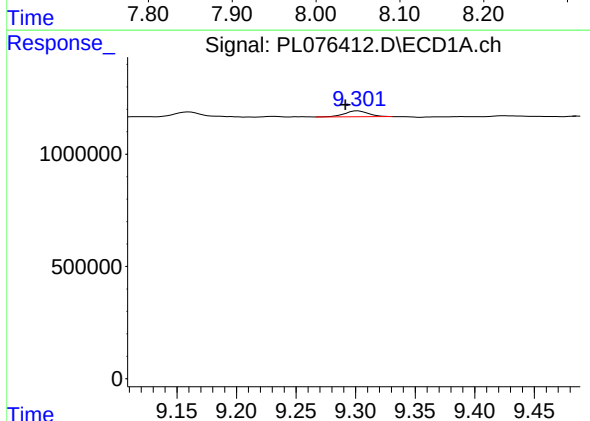


#15 Endosulfan II

R.T.: 9.302 min
Delta R.T.: 0.011 min
Response: 367130
Conc: 0.61 ng/ml

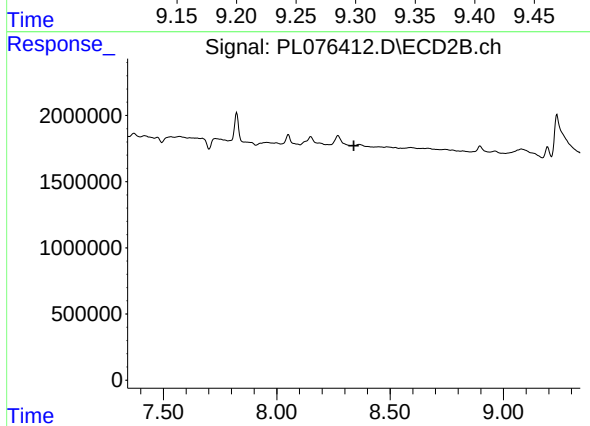

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.340 min
Response: 0
Conc: N.D.

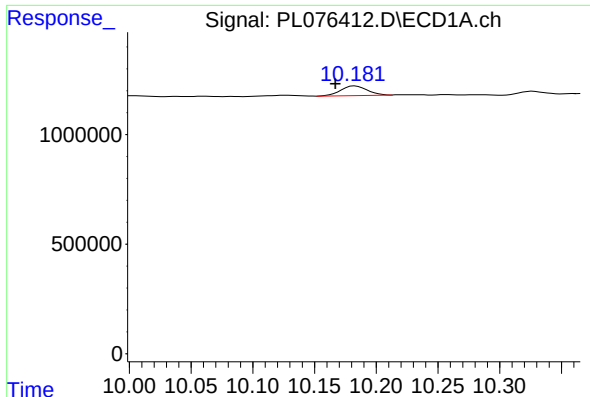

#21 Endrin ketone


R.T.: 10.183 min
Delta R.T.: 0.016 min
Response: 658234
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

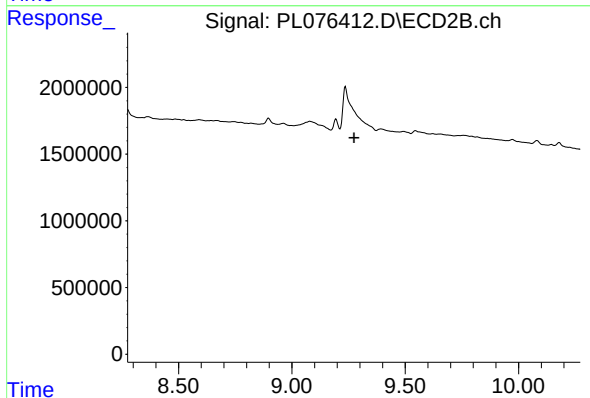


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.275 min
Response: 0
Conc: N.D.

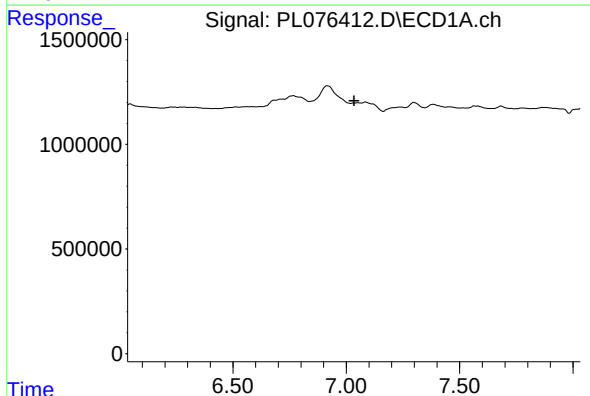


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 7.034 min
Response: 0
Conc: N.D.

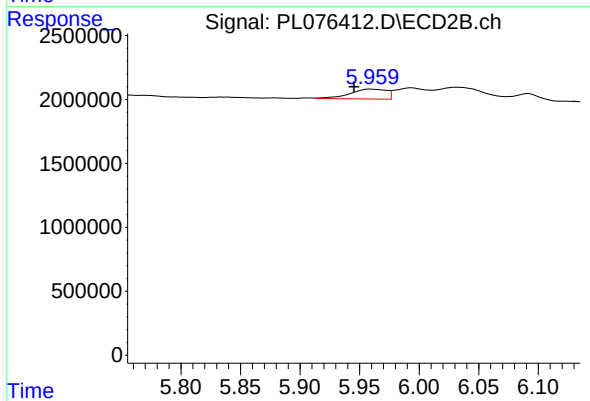

#23 Chlordane-1


R.T.: 5.960 min
Delta R.T.: 0.014 min
Response: 1641696
Conc: 29.17 ng/ml

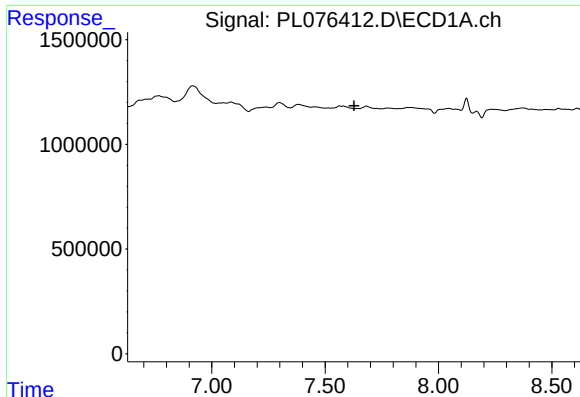

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.627 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

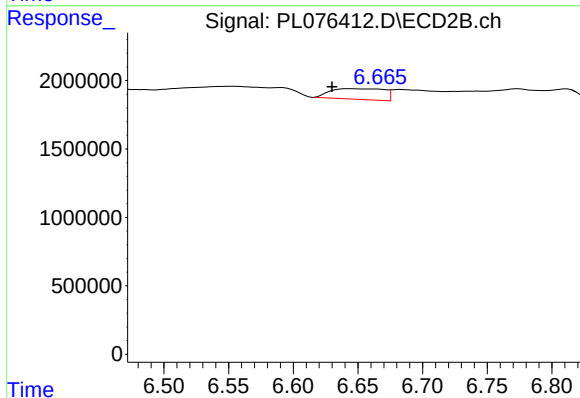


#24 Chlordane-2

R.T.: 6.643 min
Delta R.T.: 0.013 min
Response: 2229552
Conc: 34.36 ng/ml

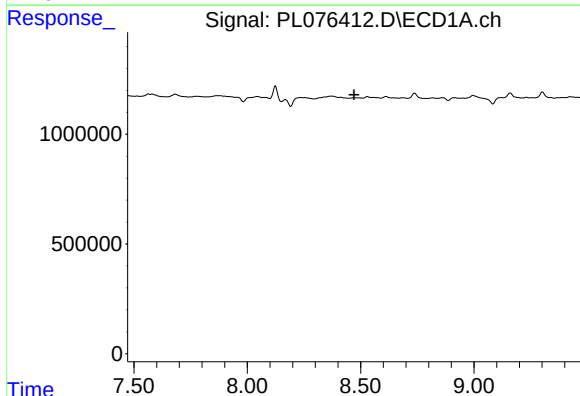


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

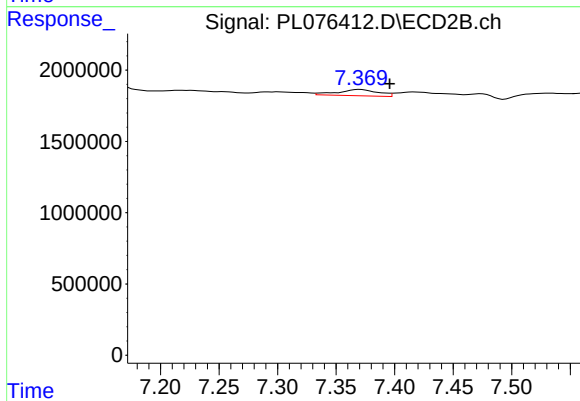

#26 Chlordane-4


R.T.: 7.370 min
Delta R.T.: -0.026 min
Response: 1064930
Conc: 5.77 ng/ml

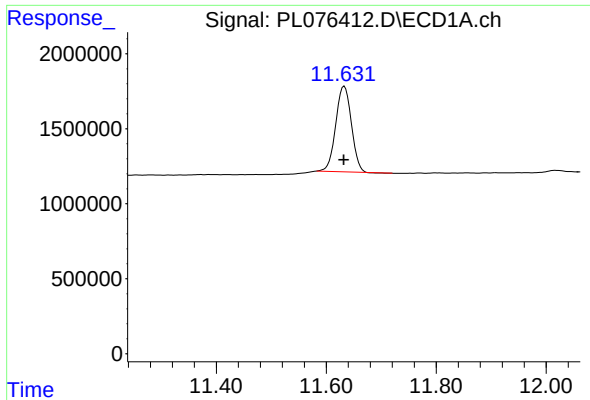

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.001 min
Response: 11284960
Conc: 19.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

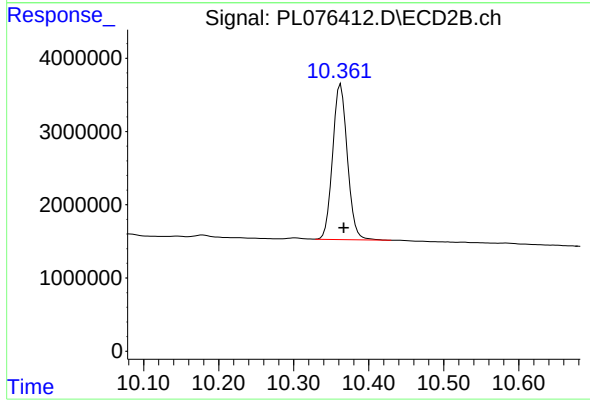

#28 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: -0.004 min
Response: 28873694
Conc: 17.21 ng/ml