

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071323\
 Data File : PL083879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2023 14:13
 Operator : AR\AJ
 Sample : 03560-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 QUARTERLY-OUTFALL-002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:09:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	2.689	31646524	18644190	15.824	16.788
28)	SA Decachlor...	9.031	7.874	51699693	28889395	39.718	26.000 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071323\
Data File : PL083879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2023 14:13
Operator : AR\AJ
Sample : 03560-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:09:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

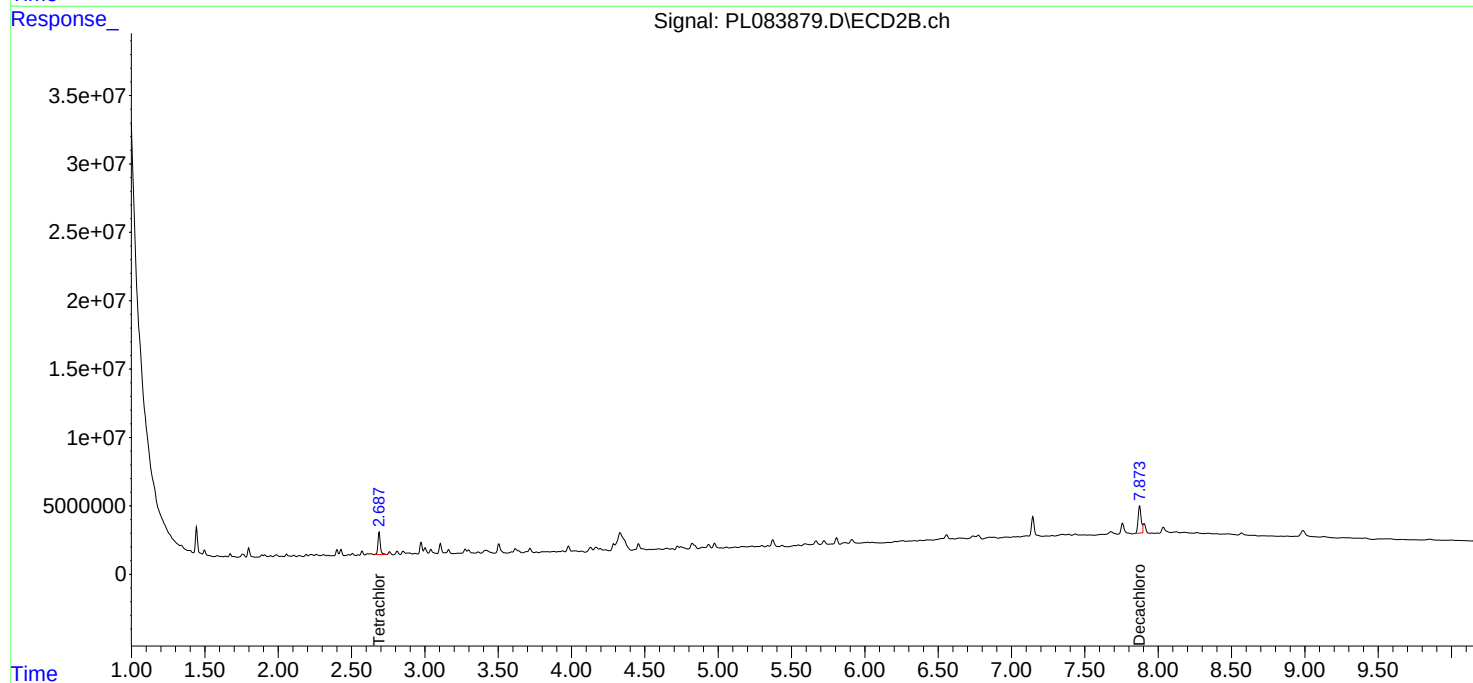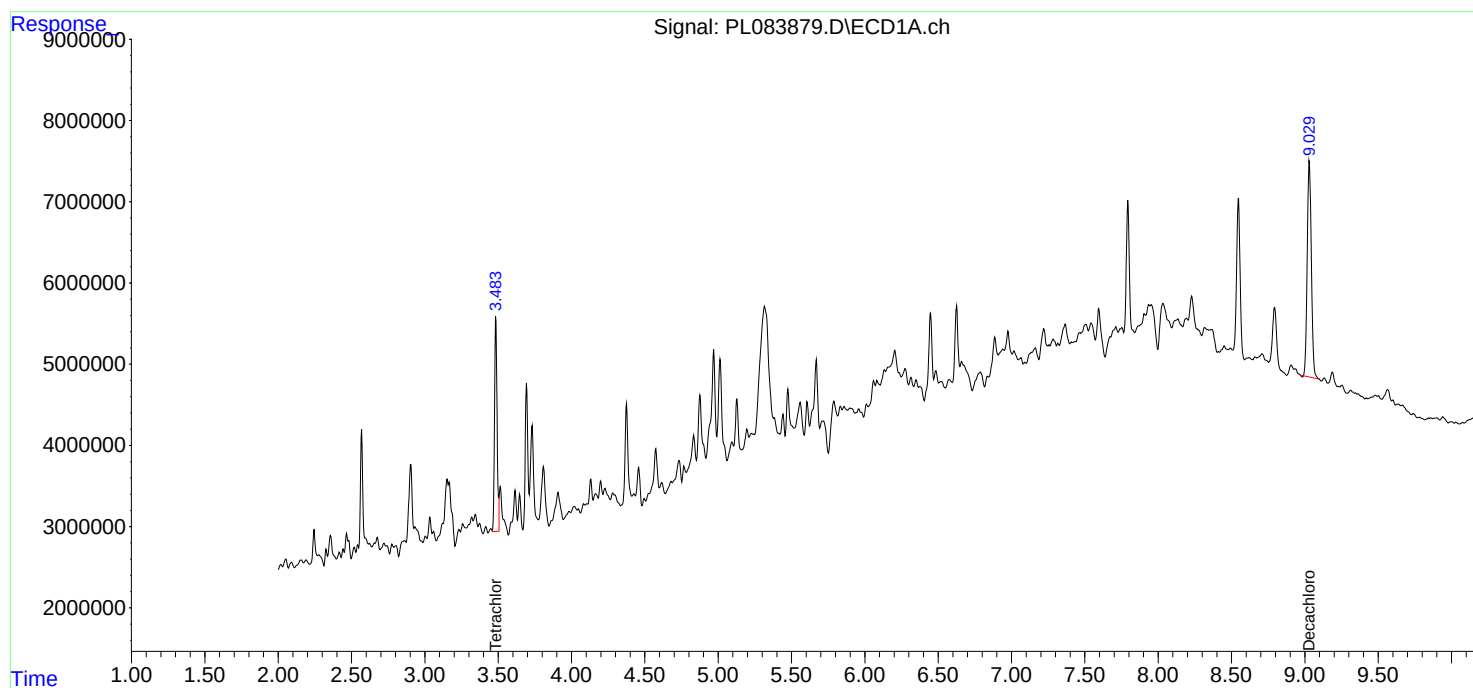


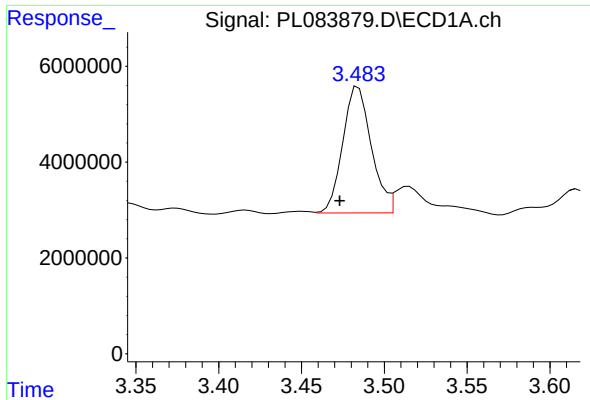

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.011 min
Response: 31646524
Conc: 15.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002

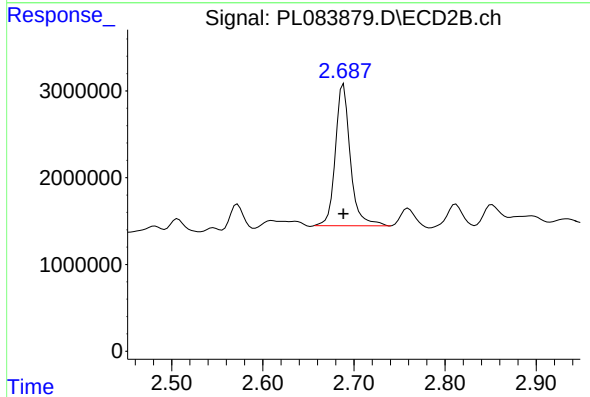


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 18644190
Conc: 16.79 ng/ml

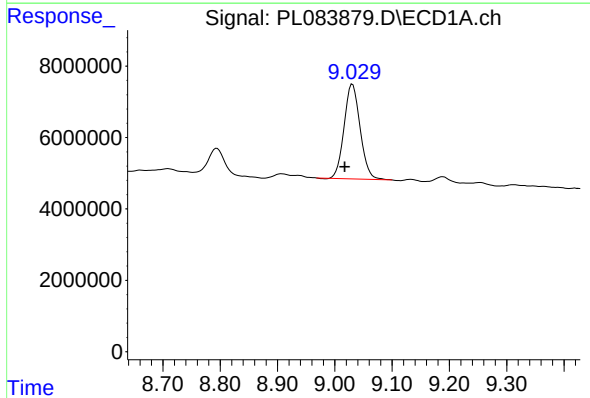

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: 0.013 min
Response: 51699693
Conc: 39.72 ng/ml

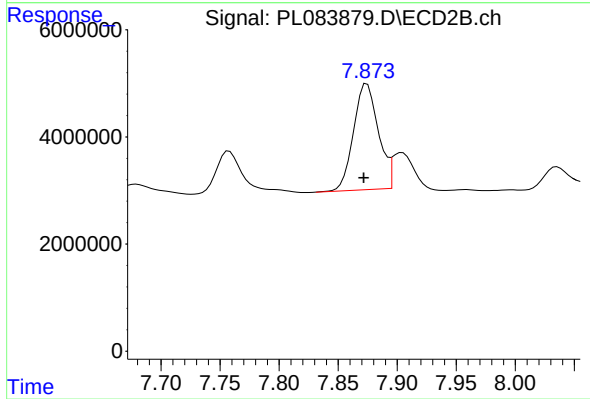

#28 Decachlorobiphenyl

R.T.: 7.874 min
Delta R.T.: 0.003 min
Response: 28889395
Conc: 26.00 ng/ml