

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071323\
 Data File : PL083897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2023 19:40
 Operator : AR\AJ
 Sample : 03600-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-3-071223

Manual Integrations APPROVED

Reviewed By :Abdul
 Mirza

07/14/2023
 Supervised By :Ankita
 Jodhani

07/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 00:16:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.474	2.687	18131671	12149465	9.066m	10.940
28) SA Decachlor...	9.021	7.871	12347653	12419796	9.486m	11.178

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071223\
Data File : PL083897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2023 19:40
Operator : AR\AJ
Sample : 03600-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SU-3-071223

Manual Integrations
APPROVED



Reviewed By : Abdul
Mirza


07/14/2023
Supervised By : Ankita
Jodhani

07/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 00:16:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

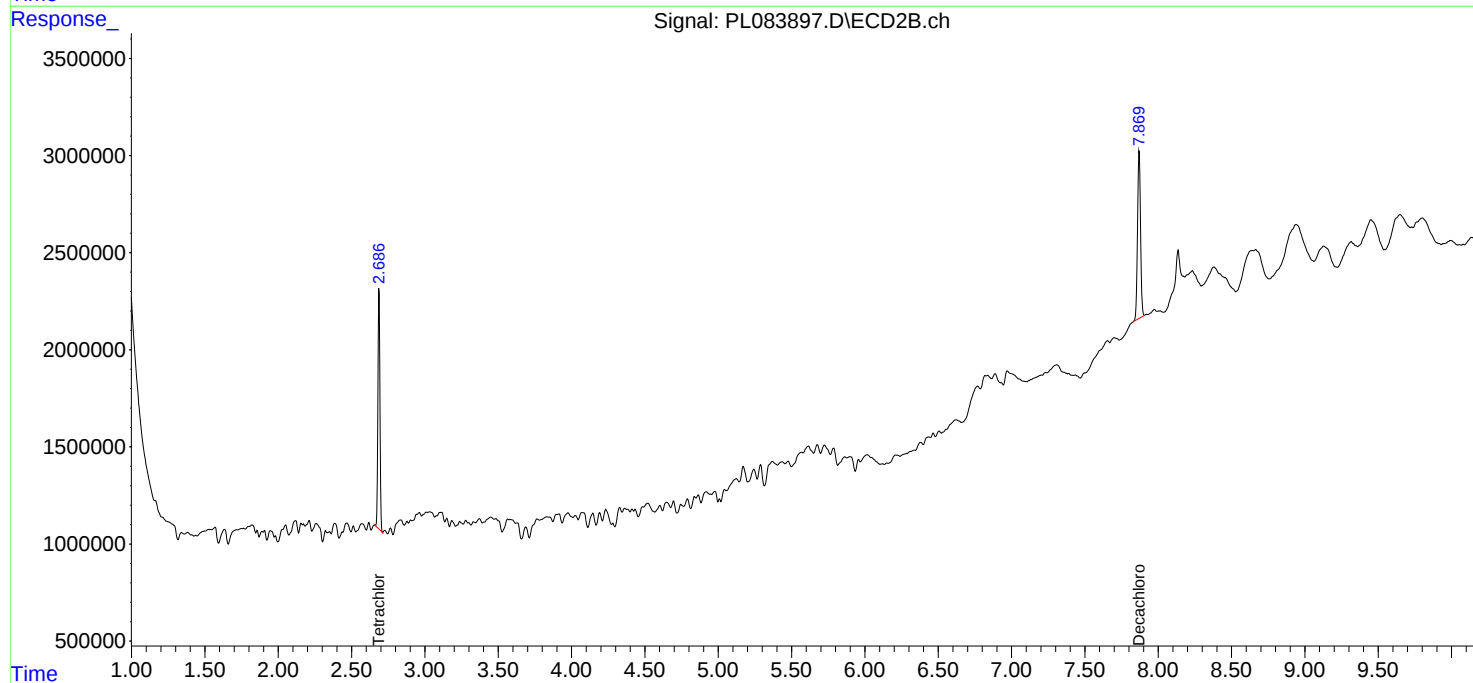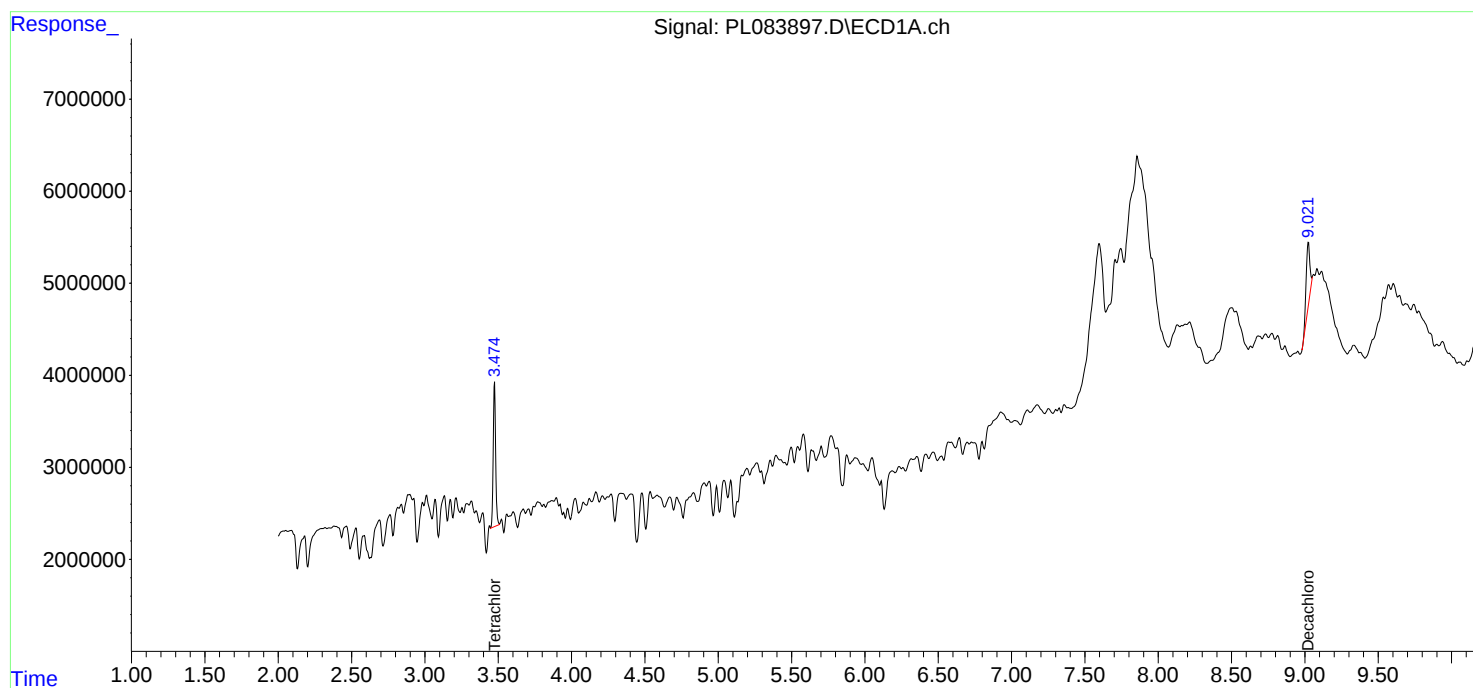

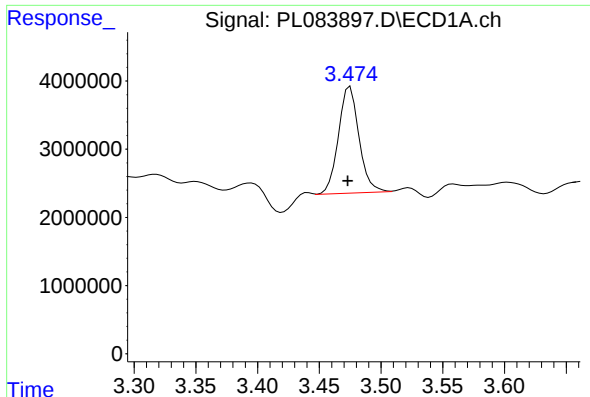

#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 18131671
Conc: 9.07 ng/ml


Instrument :
ECD_L
ClientSampleId :
SU-3-071223

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza


07/14/2023
Supervised By :Ankita
Jodhani

07/14/2023

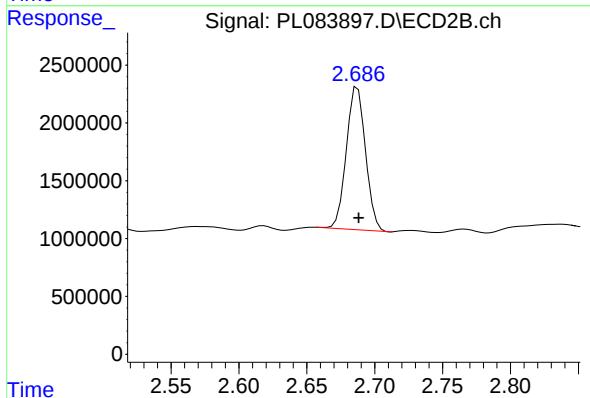


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: 0.000 min
Response: 12149465
Conc: 10.94 ng/ml

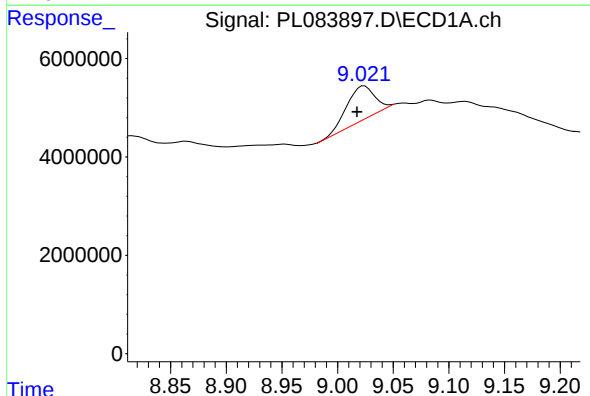

#28 Decachlorobiphenyl

R.T.: 9.021 min
Delta R.T.: 0.004 min
Response: 12347653
Conc: 9.49 ng/ml m

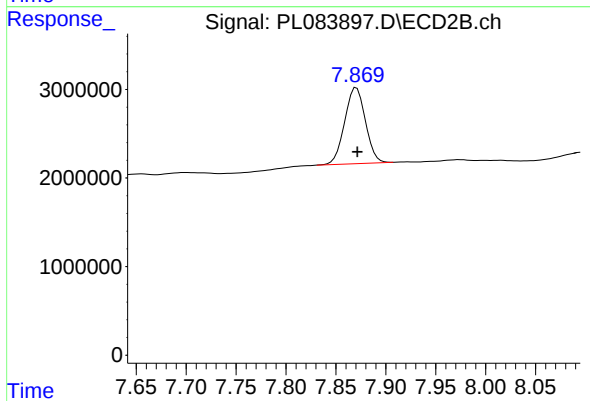

#28 Decachlorobiphenyl

R.T.: 7.871 min
Delta R.T.: 0.000 min
Response: 12419796
Conc: 11.18 ng/ml