

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071420\
 Data File : PL059889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2020 14:11
 Operator : DD\AJ
 Sample : L3181-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-070920

Manual Integrations
 APPROVED

Ankita
 7/15/2020 11:13:32 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 16:16:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.464	4.011	29624133	35548795	15.316	13.414
28) SA Decachlor...	8.228	9.099	23304848	32095894	14.166	15.347m
Target Compounds						
10) B gamma-Chl...	5.409	6.125	3937618	3860711	2.171m	1.348m#
11) B alpha-Chl...	5.466	6.199	3815512	9835915	2.116m	3.440m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071420\
Data File : PL059889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2020 14:11
Operator : DD\AJ
Sample : L3181-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CL-02-070920


Manual Integrations
APPROVED

Ankita
7/15/2020 11:13:32 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 16:16:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

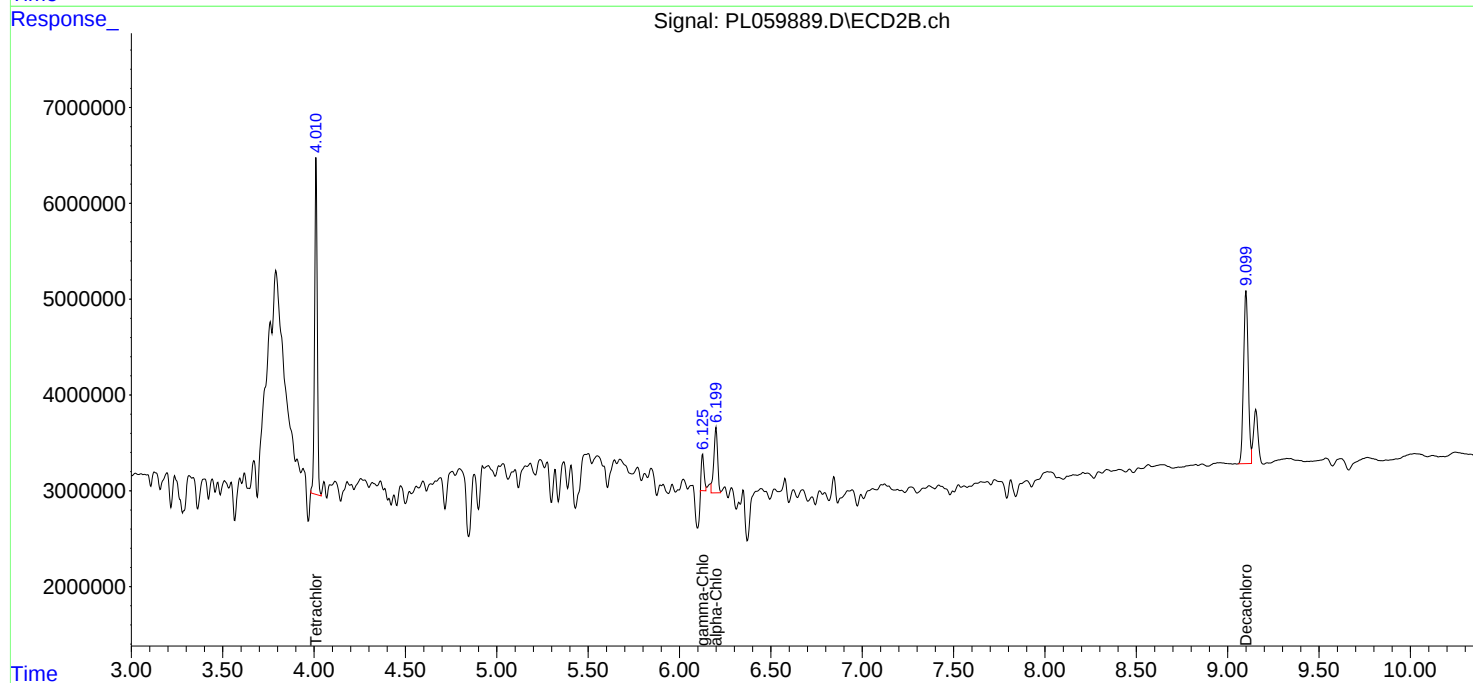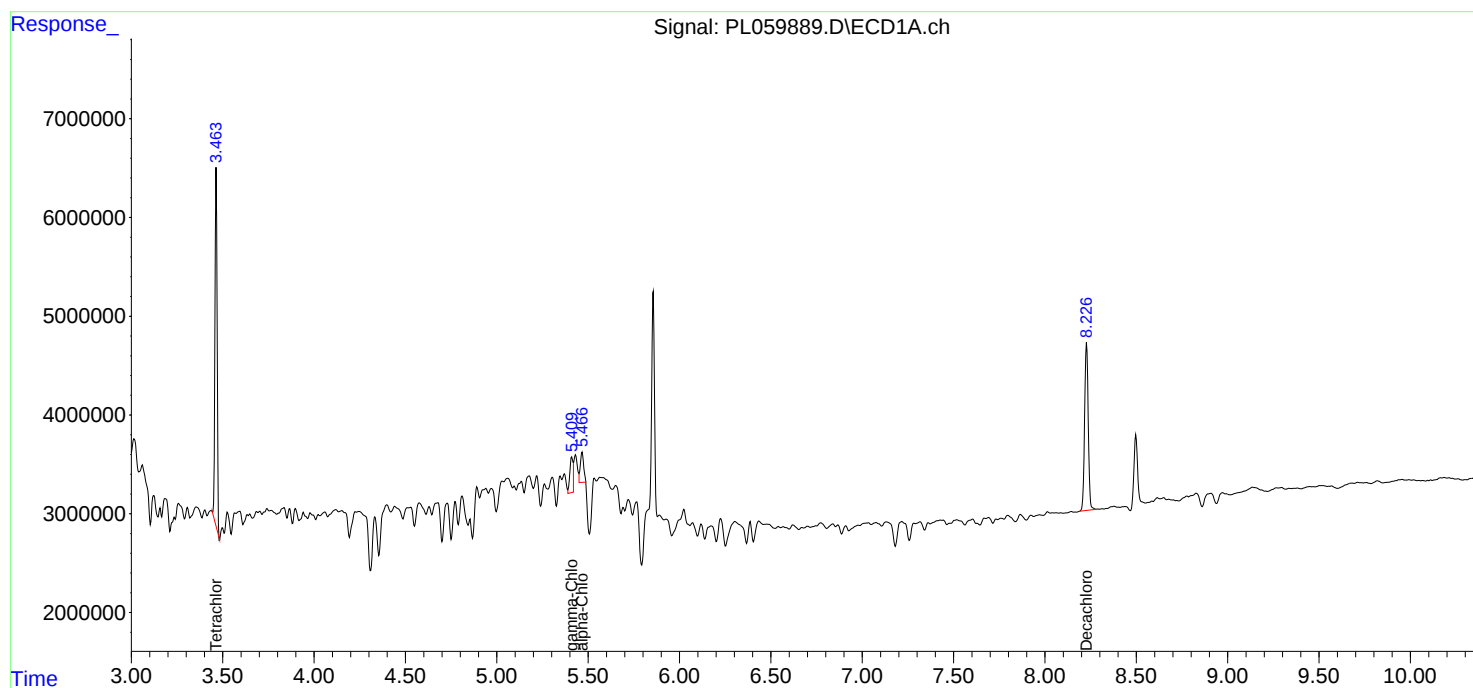

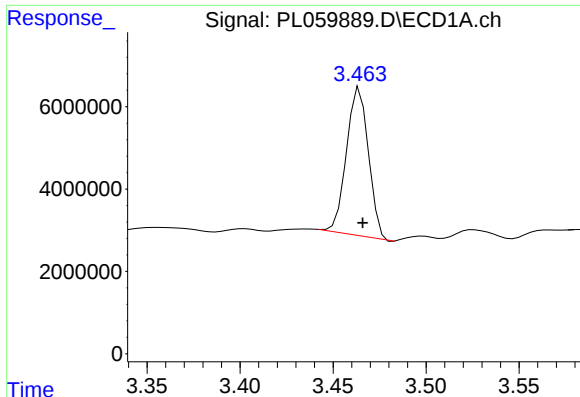


#1 Tetrachloro-m-xylene

R.T.: 3.464 min
Delta R.T.: -0.002 min
Response: 29624133
Conc: 15.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-070920


Manual Integrations
APPROVED

Ankita
7/15/2020 11:13:32 AM

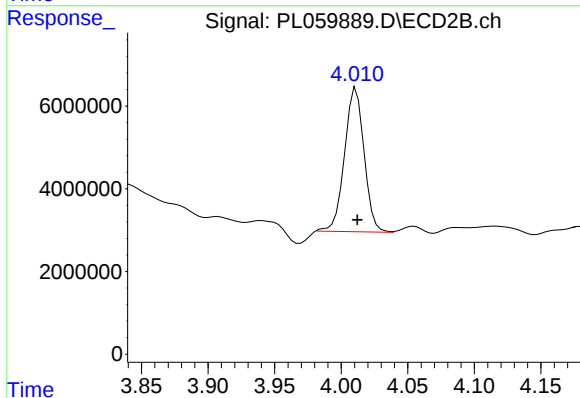


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.001 min
Response: 35548795
Conc: 13.41 ng/ml

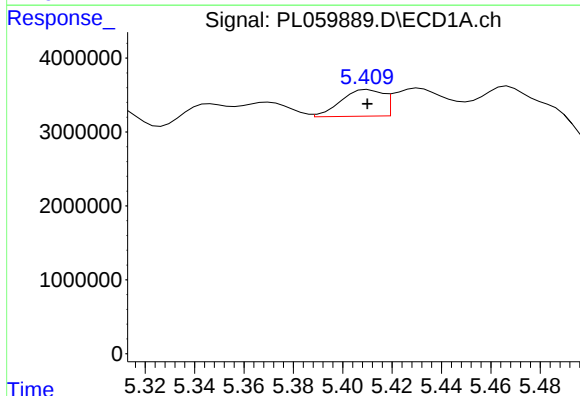


#10 gamma-Chlordane

R.T.: 5.409 min
Delta R.T.: -0.001 min
Response: 3937618
Conc: 2.17 ng/ml m

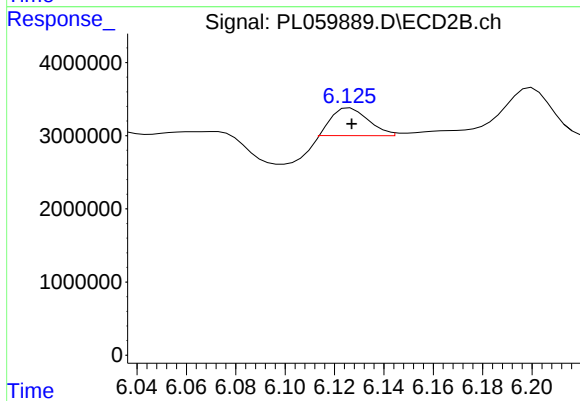

#10 gamma-Chlordane

R.T.: 6.125 min
Delta R.T.: -0.002 min
Response: 3860711
Conc: 1.35 ng/ml m

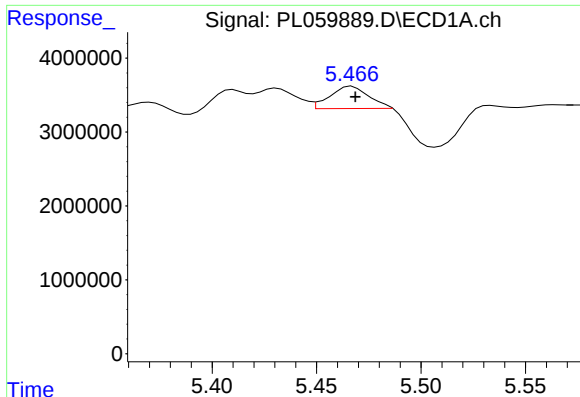


#11 alpha-Chlordane

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 3815512
Conc: 2.12 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-070920


Manual Integrations
APPROVED

Ankita
7/15/2020 11:13:32 AM

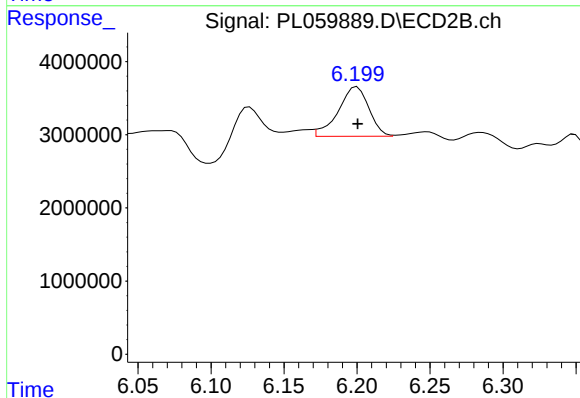


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: -0.002 min
Response: 9835915
Conc: 3.44 ng/ml m

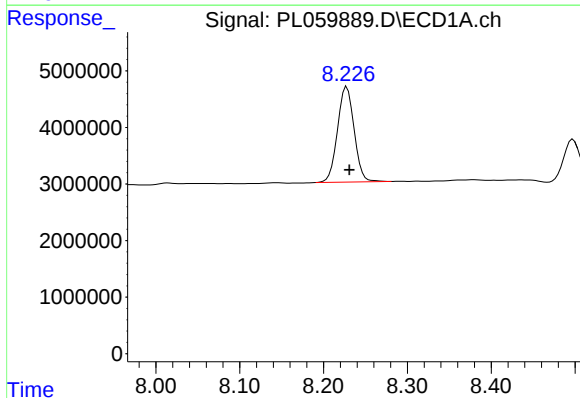

#28 Decachlorobiphenyl

R.T.: 8.228 min
Delta R.T.: -0.003 min
Response: 23304848
Conc: 14.17 ng/ml

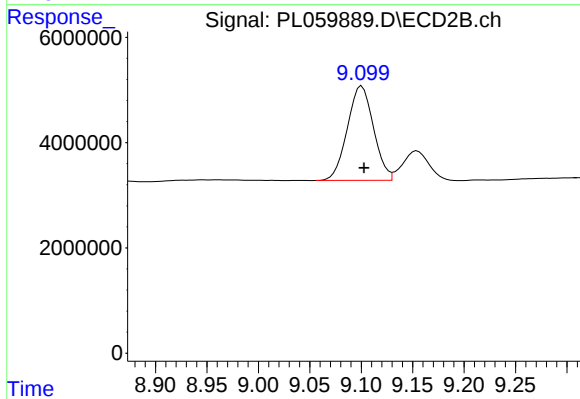

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.004 min
Response: 32095894
Conc: 15.35 ng/ml m