

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071423\
 Data File : PL083905.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 11:48
 Operator : AR\AJ
 Sample : 03563-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HOUSE-BASEMENTRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 15:42:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.685	10682627	19071852	5.342m	17.173 #
28)	SA Decachlor...	9.024	7.870	8067353	5480415	6.198	4.932
Target Compounds							
10)	B gamma-Chl...	5.890	4.905	16986429	6527321	6.579m	4.900 #
11)	B alpha-Chl...	5.971	4.969	21920631	10756777	8.623	7.985
16)	A 4,4'-DDD	6.666	5.724	8083689	5793273	5.505m	6.039m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071423\
Data File : PL083905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 11:48
Operator : AR\AJ
Sample : 03563-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HOUSE-BASEMENTRE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/17/2023
Supervised By : Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 15:42:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

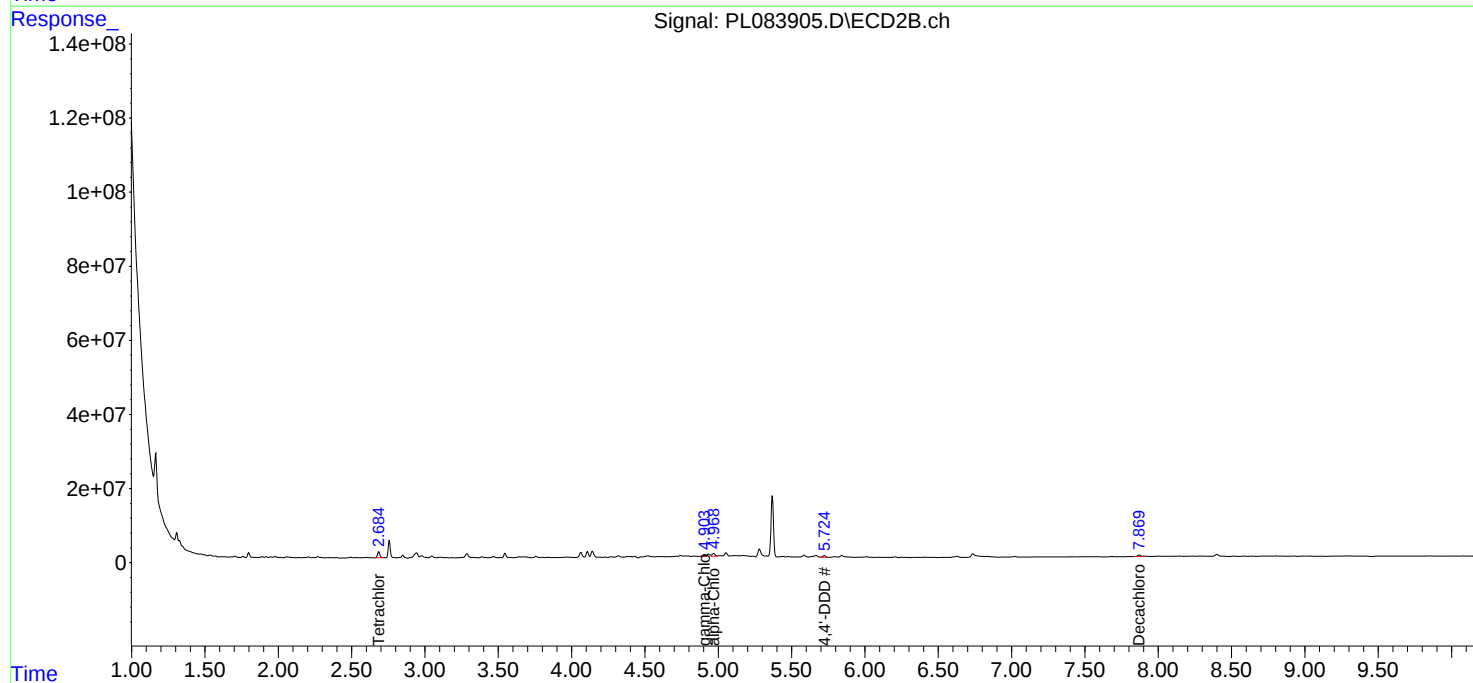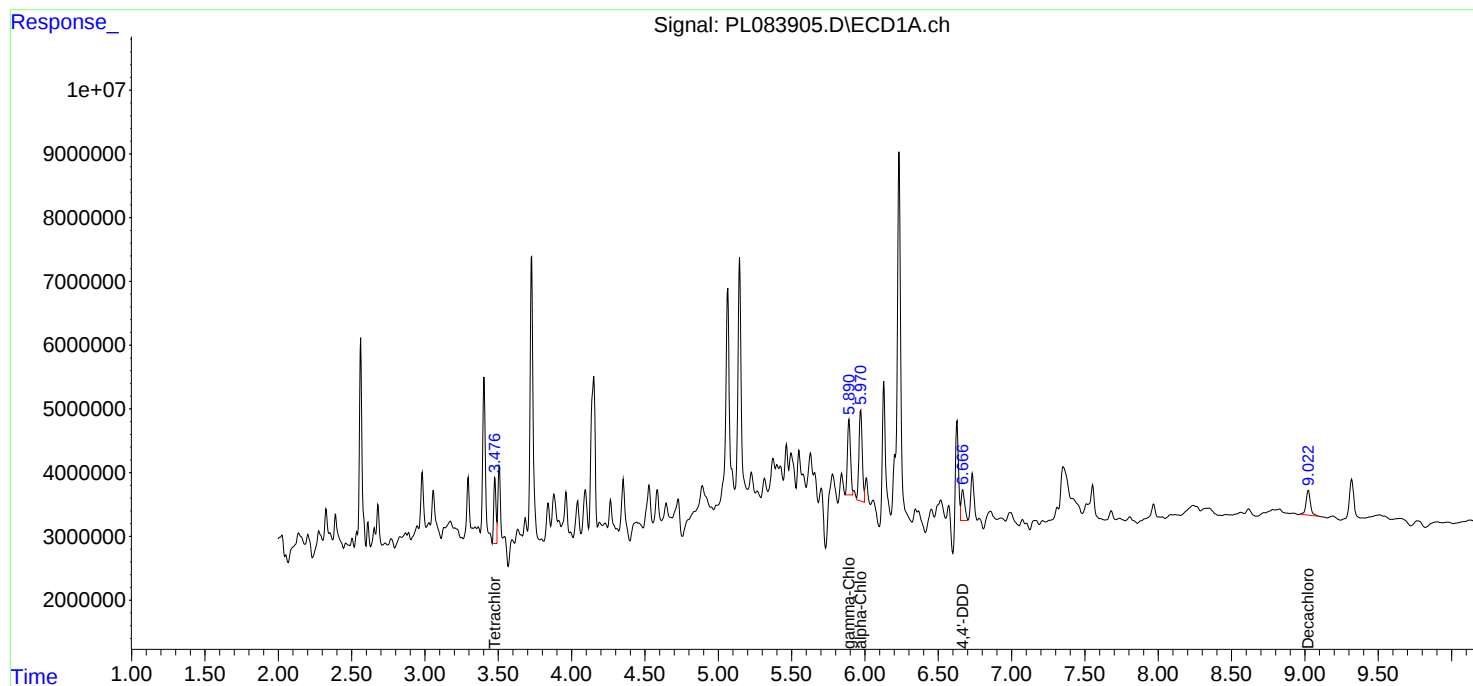

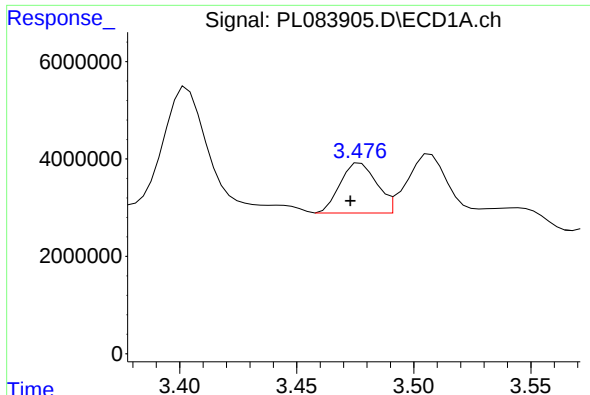


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 10682627
Conc: 5.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
HOUSE-BASEMENTRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

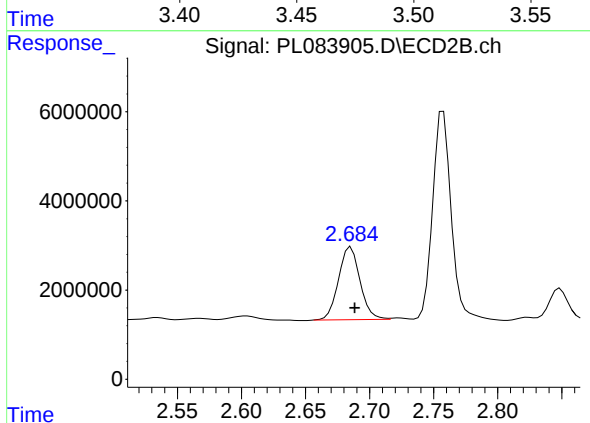


#1 Tetrachloro-m-xylene

R.T.: 2.685 min
Delta R.T.: -0.003 min
Response: 19071852
Conc: 17.17 ng/ml

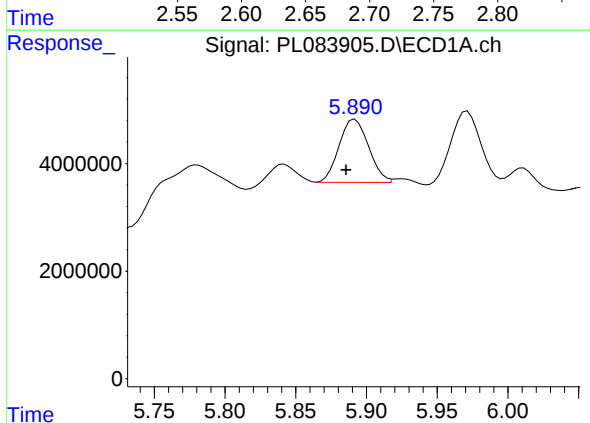


#10 gamma-Chlordane

R.T.: 5.890 min
Delta R.T.: 0.005 min
Response: 16986429
Conc: 6.58 ng/ml m

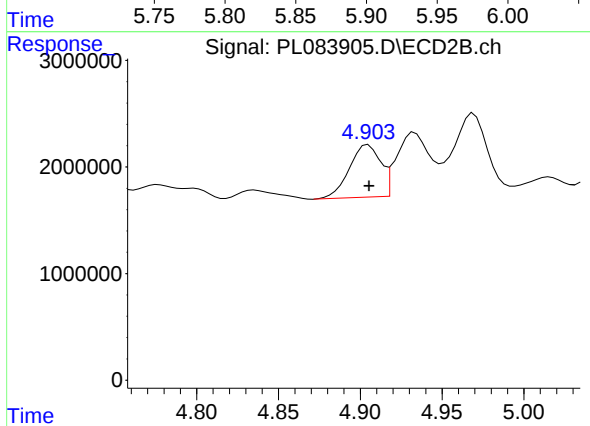

#10 gamma-Chlordane

R.T.: 4.905 min
Delta R.T.: 0.000 min
Response: 6527321
Conc: 4.90 ng/ml

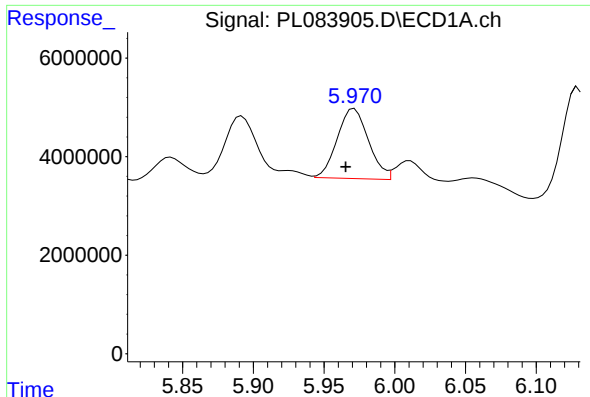


#11 alpha-Chlordane

R.T.: 5.971 min
Delta R.T.: 0.006 min
Response: 21920631
Conc: 8.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
HOUSE-BASEMENTRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

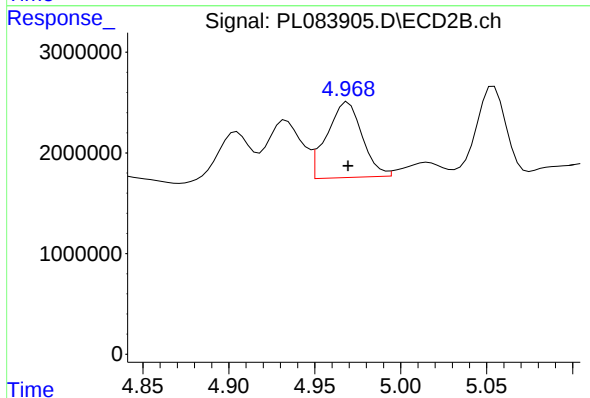


#11 alpha-Chlordane

R.T.: 4.969 min
Delta R.T.: 0.000 min
Response: 10756777
Conc: 7.98 ng/ml

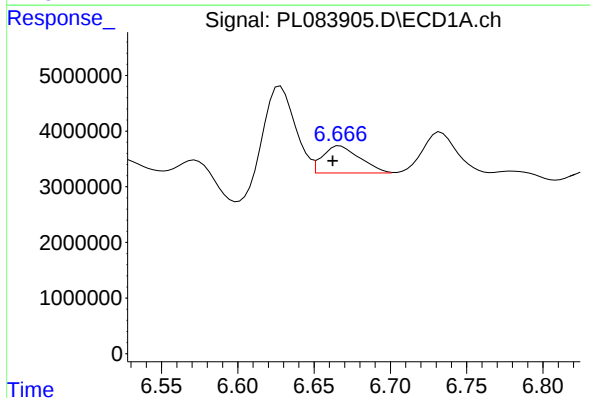


#16 4,4'-DDD

R.T.: 6.666 min
Delta R.T.: 0.003 min
Response: 8083689
Conc: 5.50 ng/ml m

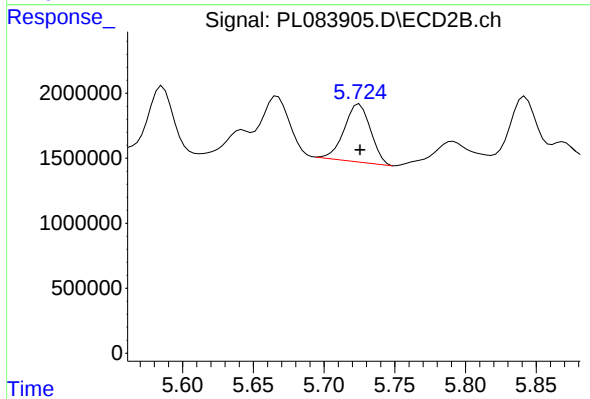

#16 4,4'-DDD

R.T.: 5.724 min
Delta R.T.: -0.002 min
Response: 5793273
Conc: 6.04 ng/ml m

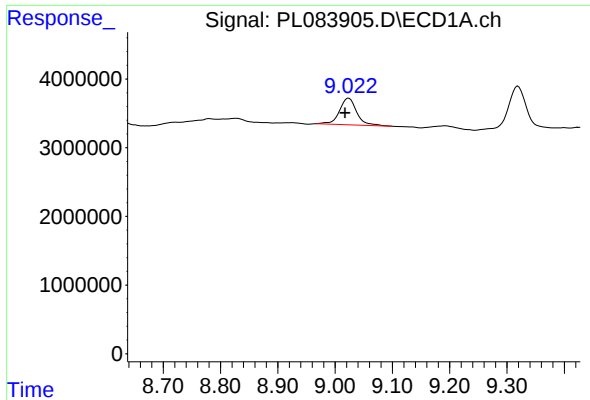


#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.006 min
Response: 8067353
Conc: 6.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
HOUSE-BASEMENTRE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

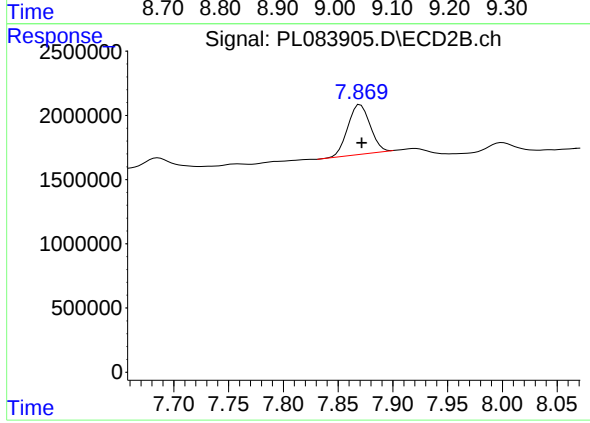

#28 Decachlorobiphenyl

R.T.: 7.870 min
Delta R.T.: -0.001 min
Response: 5480415
Conc: 4.93 ng/ml