

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071425\
 Data File : PL096356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2025 16:07
 Operator : AR\AJ
 Sample : Q2589-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-06-071125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 02:20:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 07 15:22:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.826	27308739	38241490	7.484	6.626
28)	SA Decachlor...	9.019	7.993	29908668	32185298	10.632	6.454 #
Target Compounds							
10)	B gamma-Chl...	5.917	0.000	7321821	0	1.655	N.D. #
11)	B alpha-Chl...	6.001	0.000	7714995	0	1.762	N.D. #
25)	Chlordane-3	5.917	0.000	7321821	0	9.938	N.D. #
26)	Chlordane-4	6.001	0.000	7714995	0	8.599	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071425\
Data File : PL096356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2025 16:07
Operator : AR\AJ
Sample : Q2589-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-06-071125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 02:20:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL070725.M
Quant Title : GC Extractables
QLast Update : Mon Jul 07 15:22:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

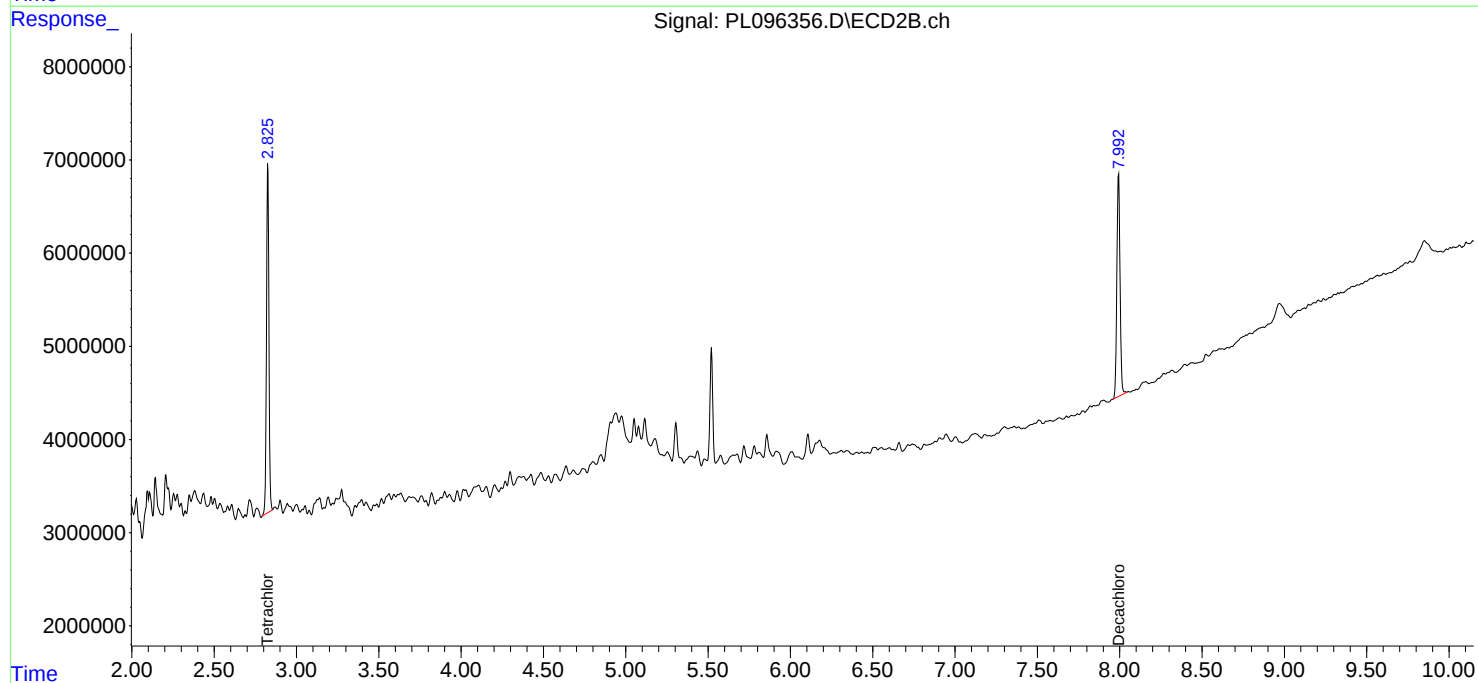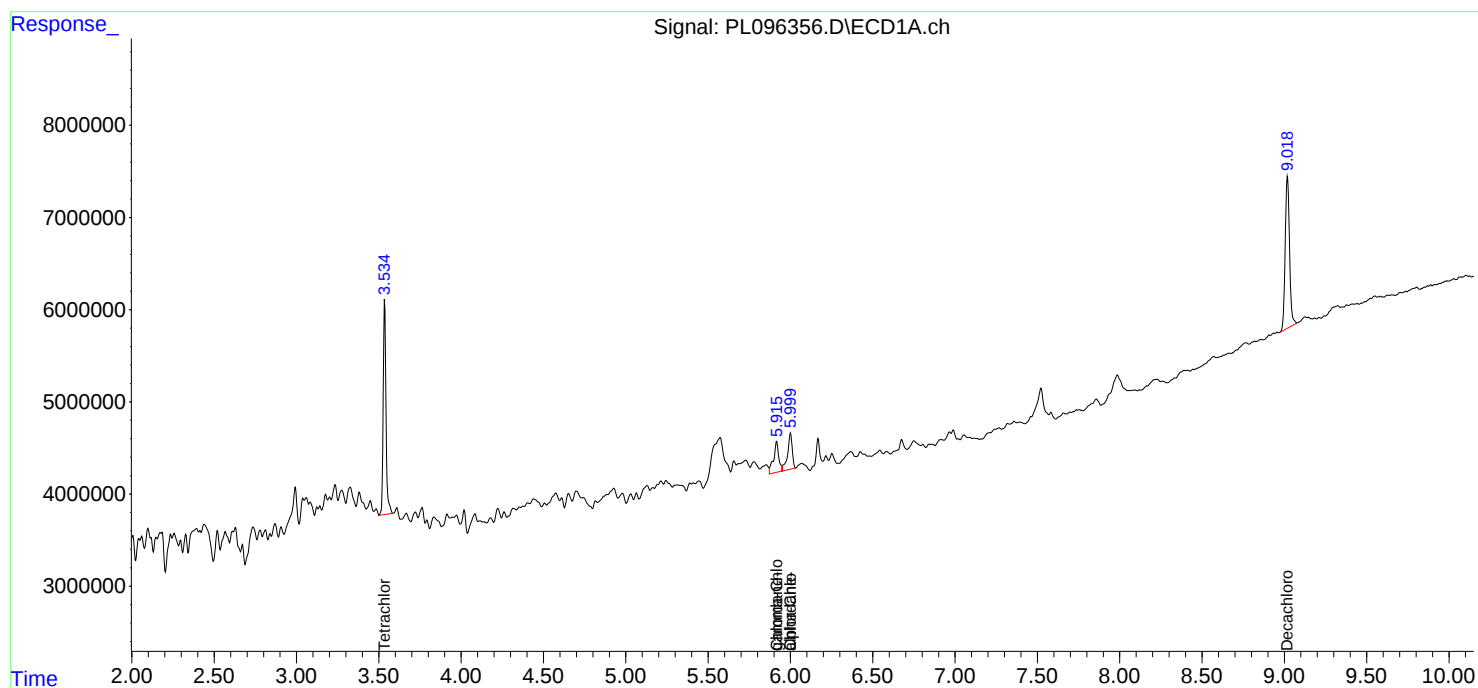


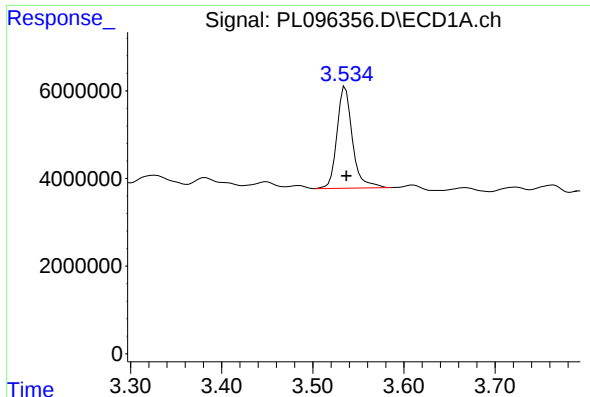

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.001 min
Response: 27308739
Conc: 7.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-071125

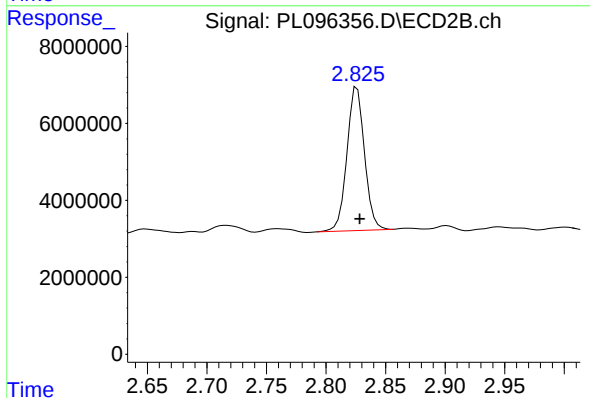


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: -0.002 min
Response: 38241490
Conc: 6.63 ng/ml

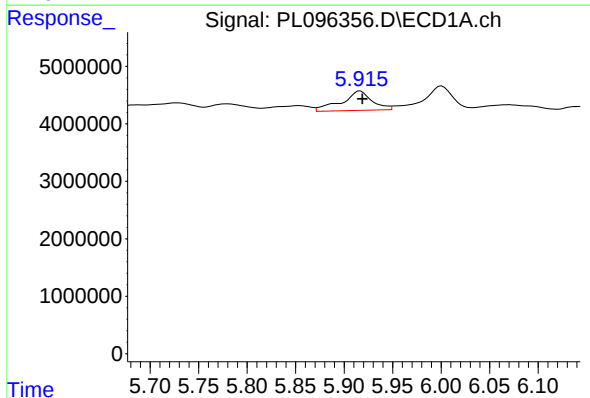


#10 gamma-Chlordane

R.T.: 5.917 min
Delta R.T.: -0.002 min
Response: 7321821
Conc: 1.65 ng/ml

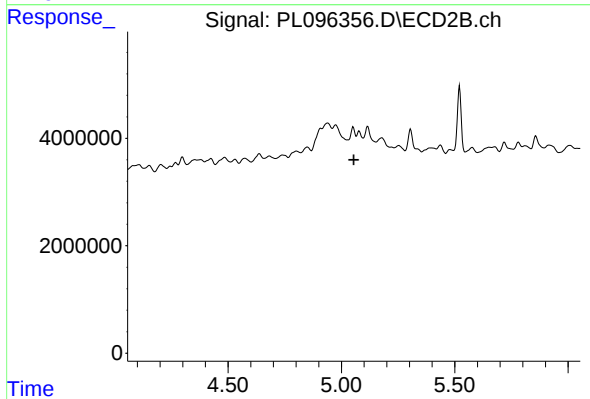

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.054 min
Response: 0
Conc: N.D.

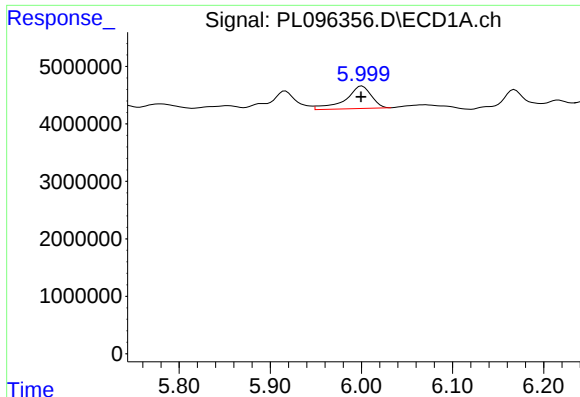

#11 alpha-Chlordane


R.T.: 6.001 min
Delta R.T.: 0.001 min
Response: 7714995
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-071125

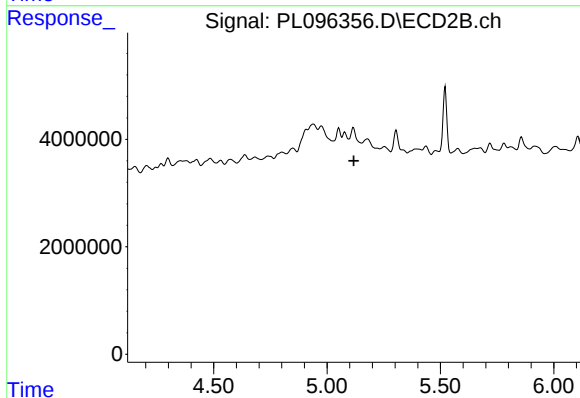


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

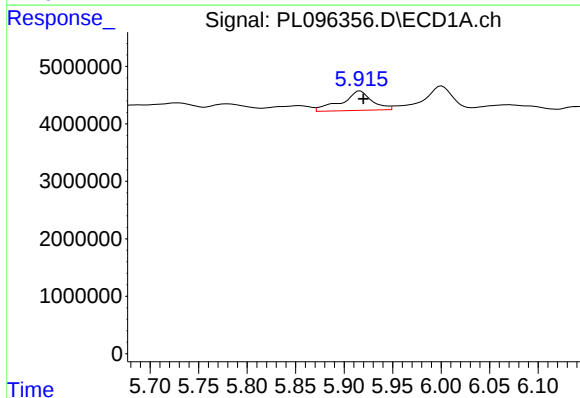


#25 Chlordane-3

R.T.: 5.917 min
Delta R.T.: -0.003 min
Response: 7321821
Conc: 9.94 ng/ml

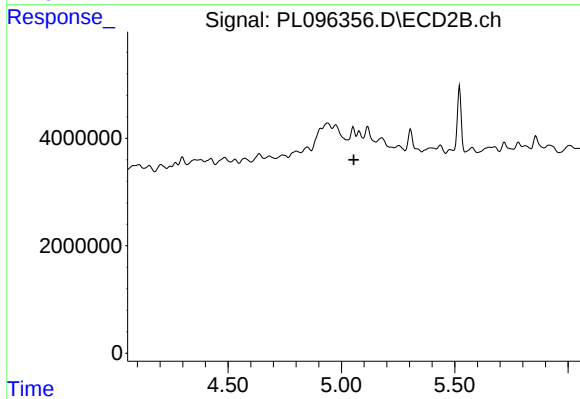

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.055 min
Response: 0
Conc: N.D.

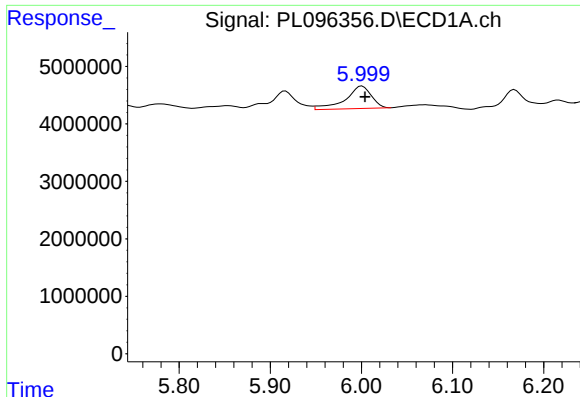

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: -0.003 min
Response: 7714995
Conc: 8.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-071125

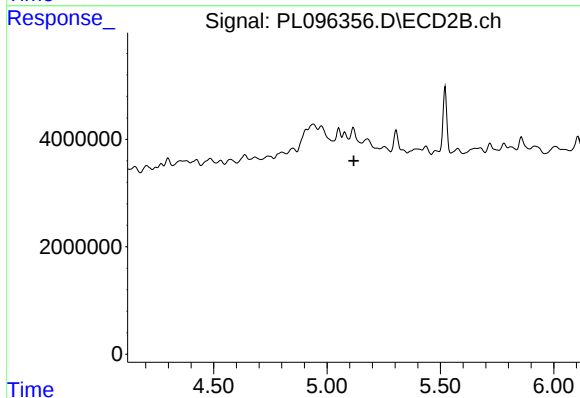


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.118 min
Response: 0
Conc: N.D.

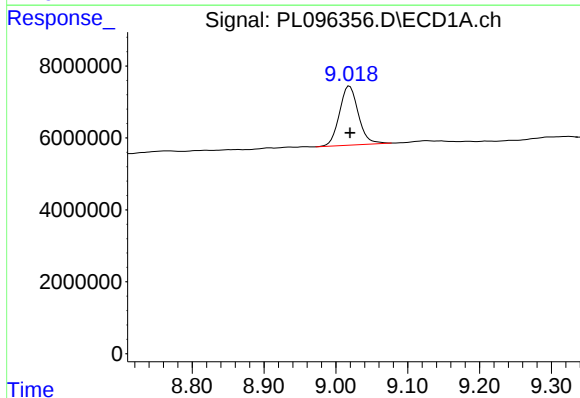

#28 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: 0.000 min
Response: 29908668
Conc: 10.63 ng/ml

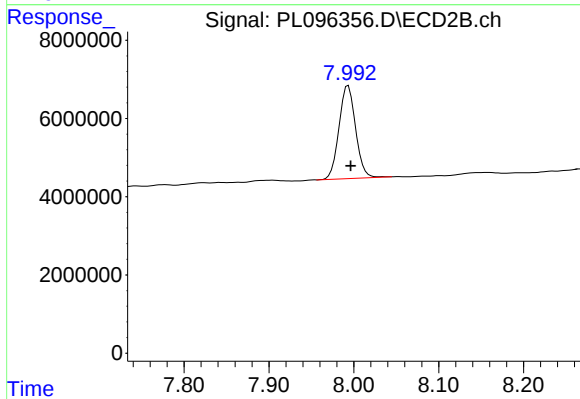

#28 Decachlorobiphenyl

R.T.: 7.993 min
Delta R.T.: -0.003 min
Response: 32185298
Conc: 6.45 ng/ml