

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071518\
 Data File : PL038051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2018 23:33
 Operator : AJ\SJ
 Sample : J3934-01
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TS-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 7/16/2018 1:40:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 04:32:11 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.930	81643286	27204485	10.964	10.364
28)	SA Decachlor...	8.003	8.940	50189396	20807010	6.616m	8.512 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071518\
Data File : PL038051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2018 23:33
Operator : AJ\SJ
Sample : J3934-01
Misc :
ALS Vial : 69 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
7/16/2018 1:40:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 04:32:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

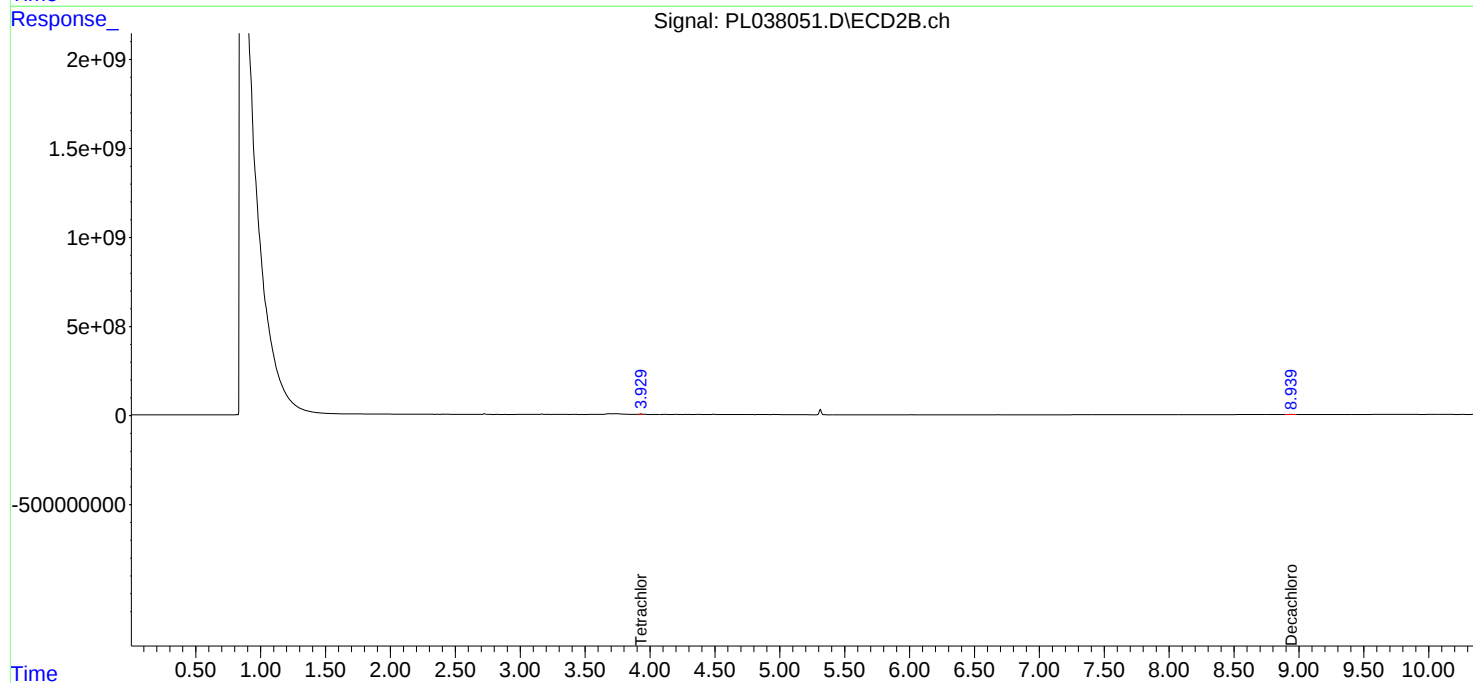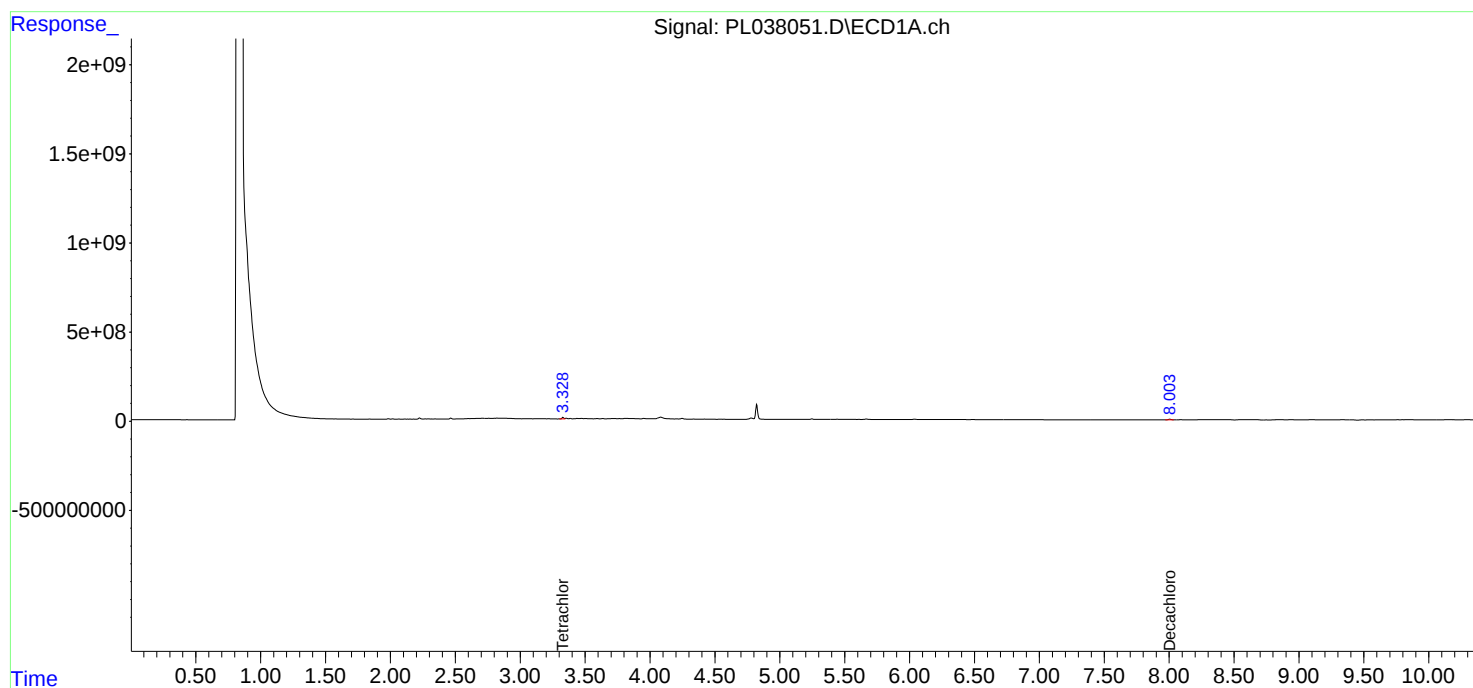

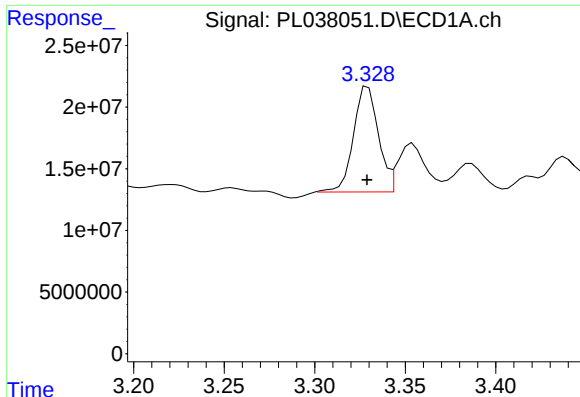


#1 Tetrachloro-m-xylene

R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 81643286
Conc: 10.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
TS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
7/16/2018 1:40:28 PM

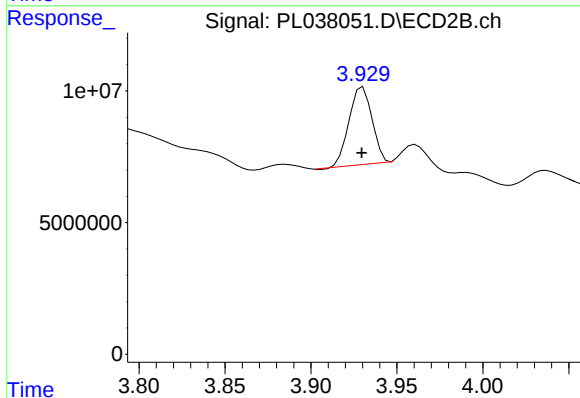


#1 Tetrachloro-m-xylene

R.T.: 3.930 min
Delta R.T.: 0.000 min
Response: 27204485
Conc: 10.36 ng/ml

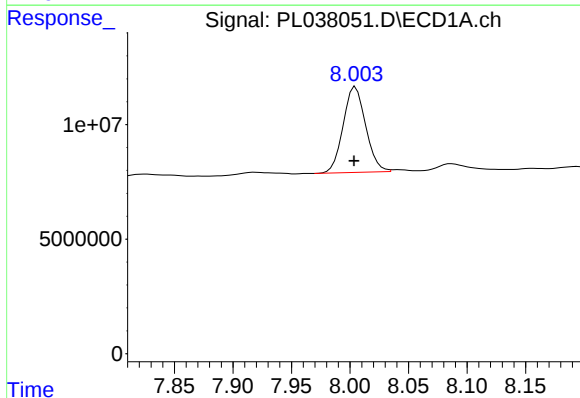

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 50189396
Conc: 6.62 ng/ml m

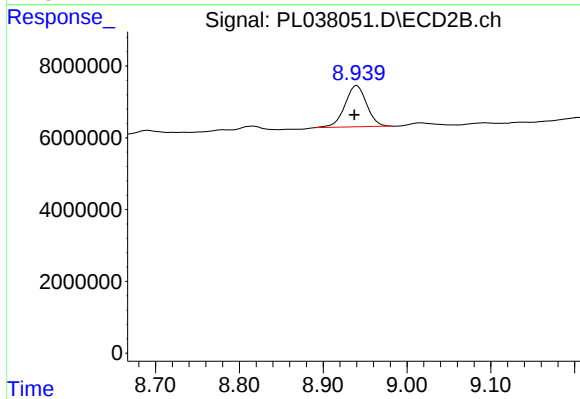

#28 Decachlorobiphenyl

R.T.: 8.940 min
Delta R.T.: 0.003 min
Response: 20807010
Conc: 8.51 ng/ml