

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068120.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2021 17:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 04:46:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	7430824	20131682	18.434	19.521
28)	SA Decachlor...	10.432	11.509	7559930	18445832	18.320	20.502
Target Compounds							
4)	MA Heptachlor	6.175f	0.000	300904	0	0.545	N.D. #
5)	MB Aldrin	0.000	7.569	0	1362721	N.D.	1.130 #
6)	B beta-BHC	6.175	0.000	300904	0	1.157	N.D. #
8)	B Heptachlo...	7.107	0.000	39015	0	0.082	N.D. #
15)	B Endosulfa...	0.000	9.228	0	531965	N.D.	0.601 #
24)	Chlordane-2	6.671	7.569	31513	1362721	1.617	29.731 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068120.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 17:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 04:46:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

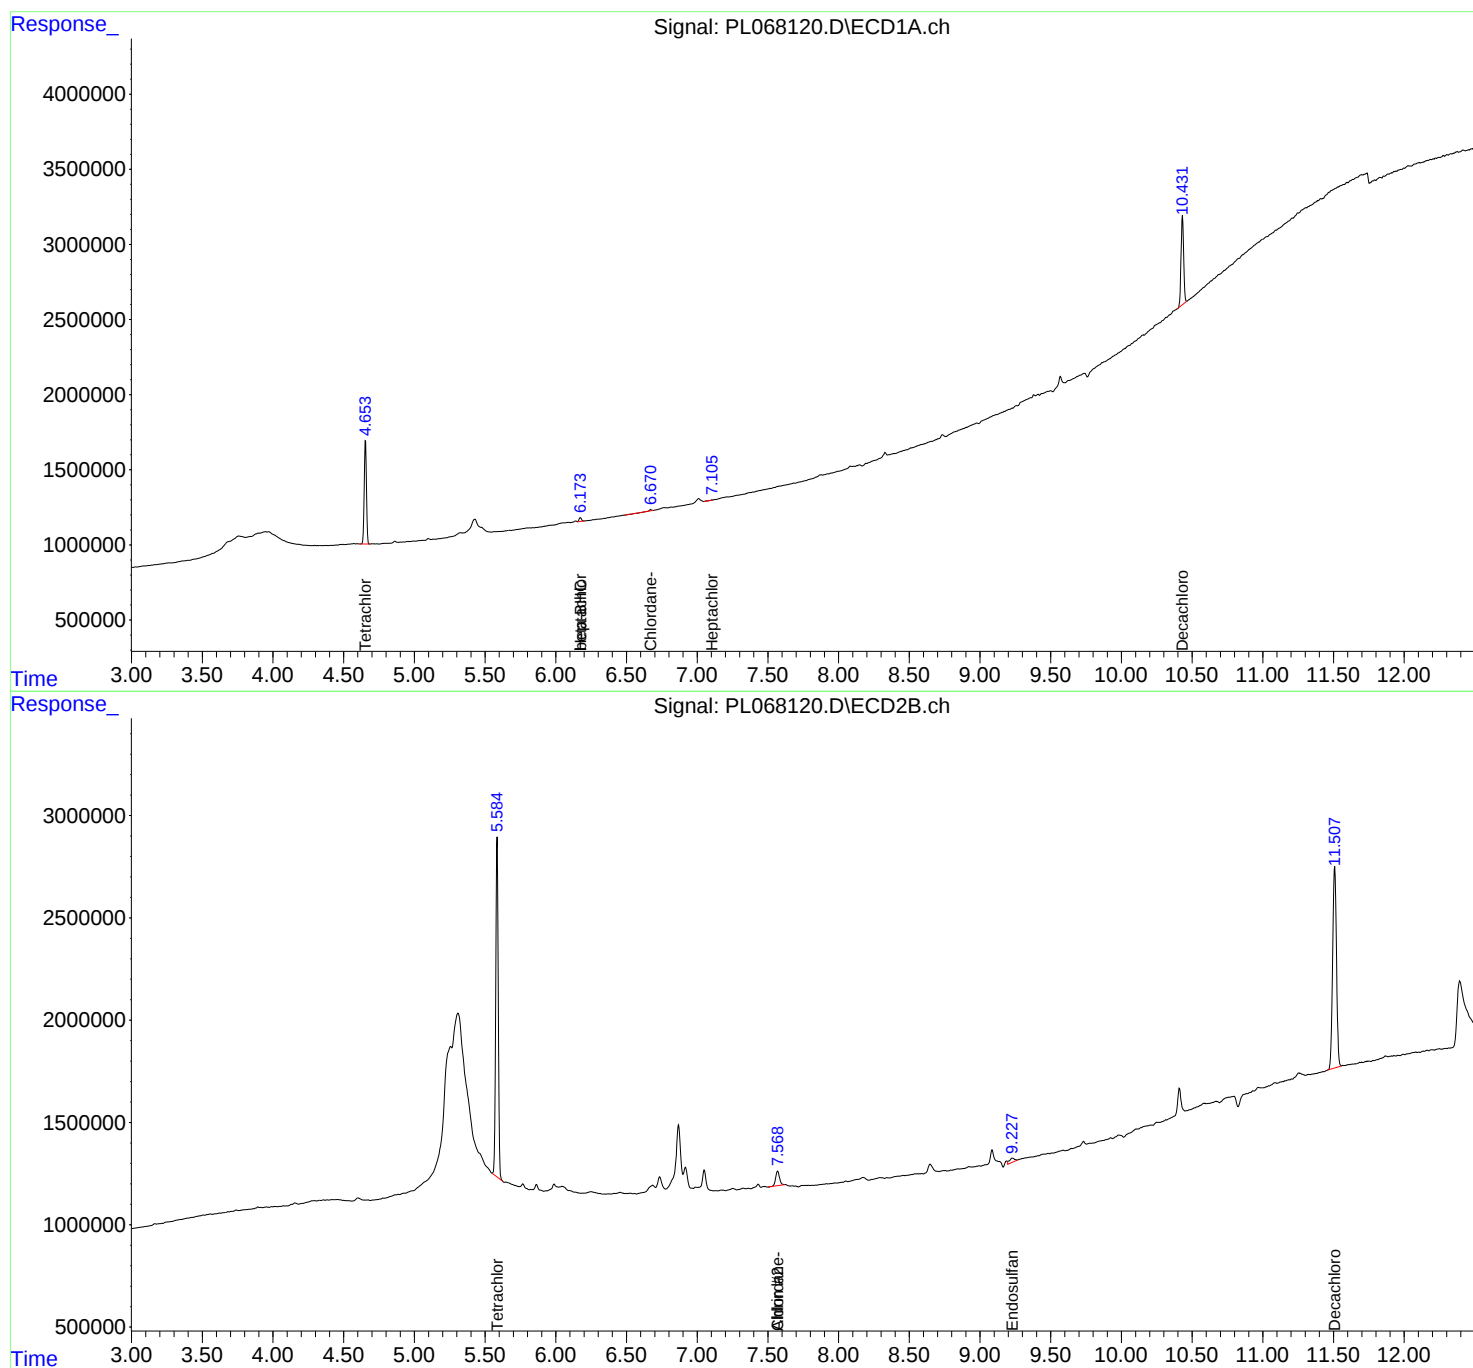

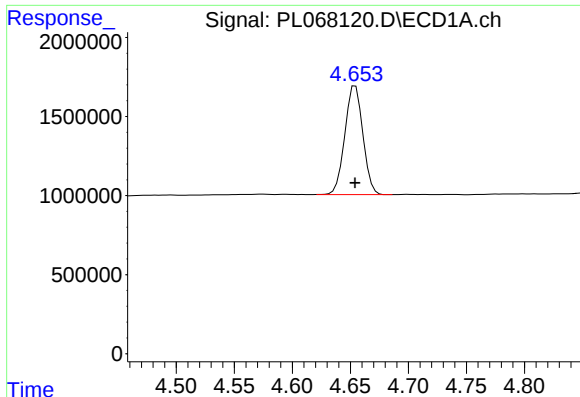


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 7430824
Conc: 18.43 ng/ml

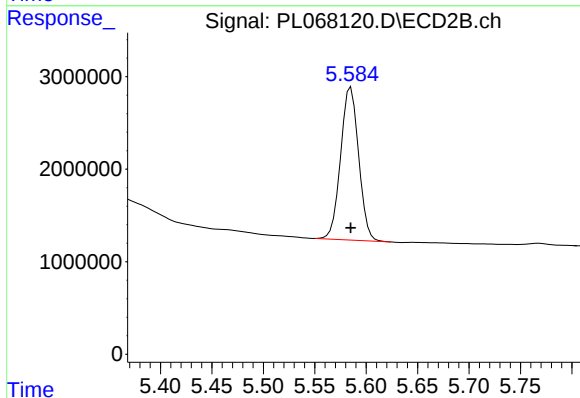


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 20131682
Conc: 19.52 ng/ml

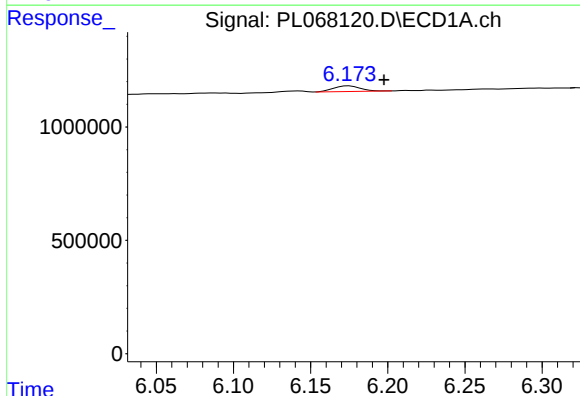


#4 Heptachlor

R.T.: 6.175 min
Delta R.T.: -0.023 min
Response: 300904
Conc: 0.54 ng/ml

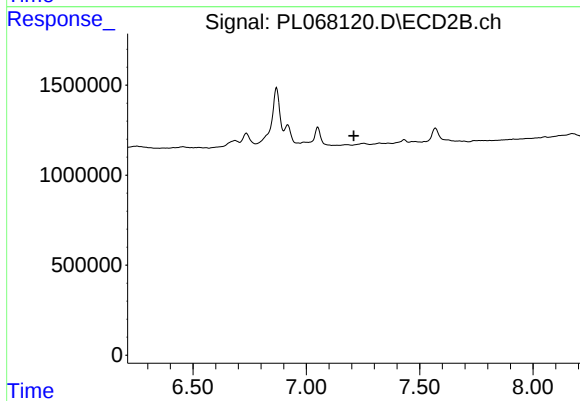

#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 7.210 min
Response: 0
Conc: N.D.

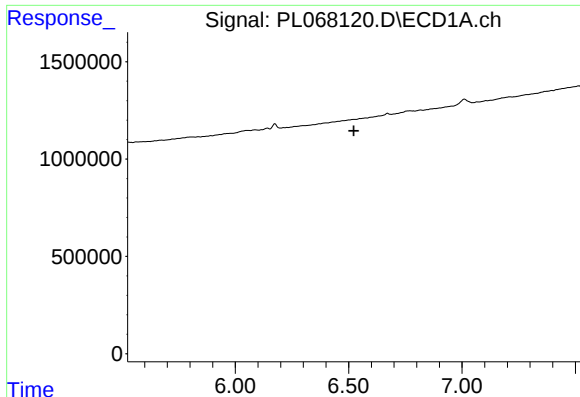


#5 Aldrin

R.T.: 0.000 min

Exp R.T. : 6.523 min

Response: 0

Conc: N.D.

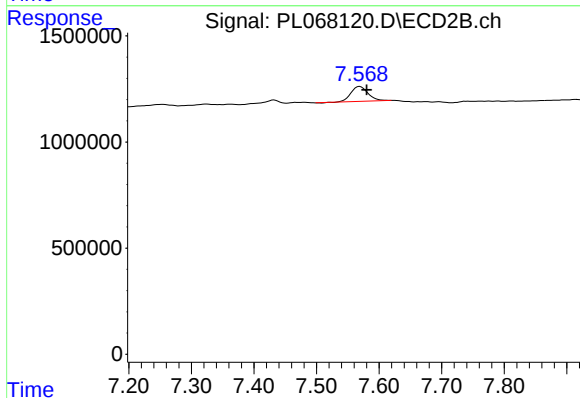


#5 Aldrin

R.T.: 7.569 min

Delta R.T.: -0.011 min

Response: 1362721

Conc: 1.13 ng/ml

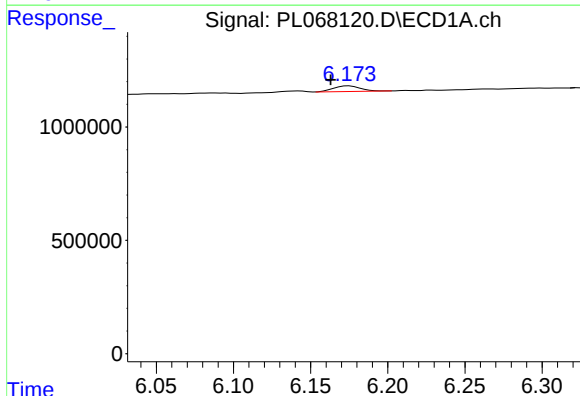


#6 beta-BHC

R.T.: 6.175 min

Delta R.T.: 0.012 min

Response: 300904

Conc: 1.16 ng/ml

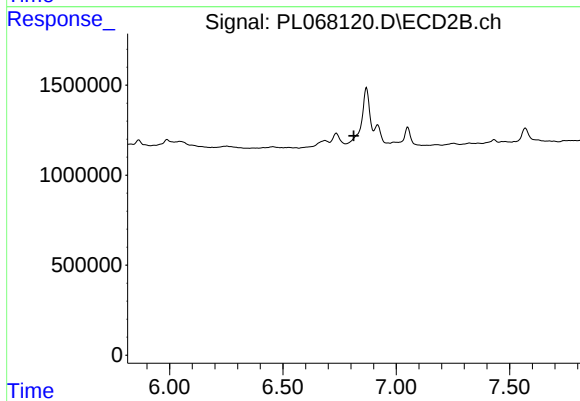


#6 beta-BHC

R.T.: 0.000 min

Exp R.T. : 6.812 min


Response: 0

Conc: N.D.

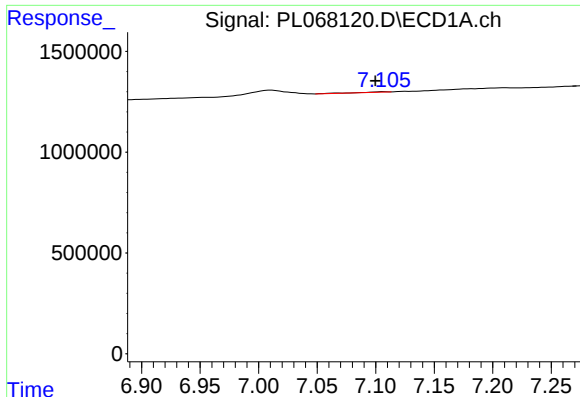


#8 Heptachlor epoxide

R.T.: 7.107 min
Delta R.T.: 0.007 min
Response: 39015
Conc: 0.08 ng/ml

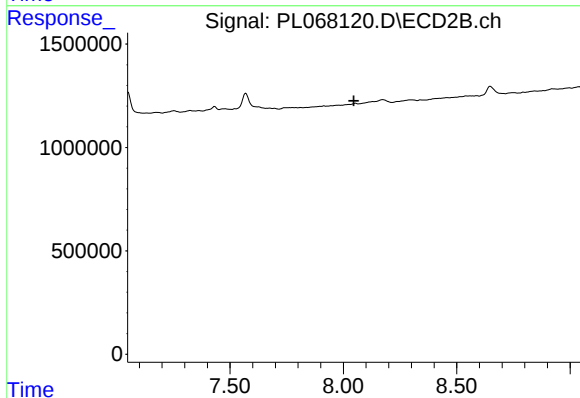


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 8.047 min
Response: 0
Conc: N.D.

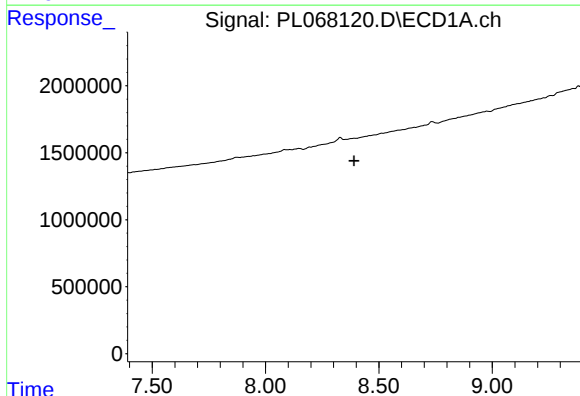


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.391 min
Response: 0
Conc: N.D.

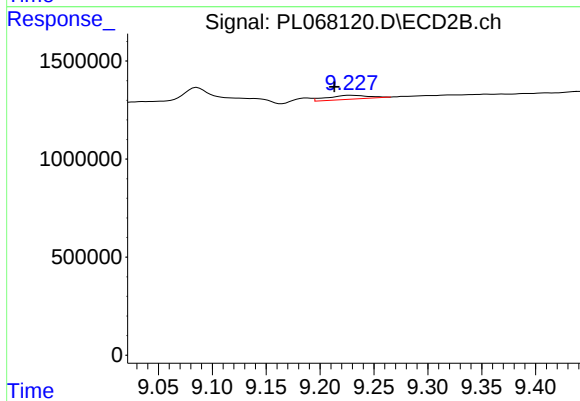


#15 Endosulfan II

R.T.: 9.228 min
Delta R.T.: 0.015 min
Response: 531965
Conc: 0.60 ng/ml

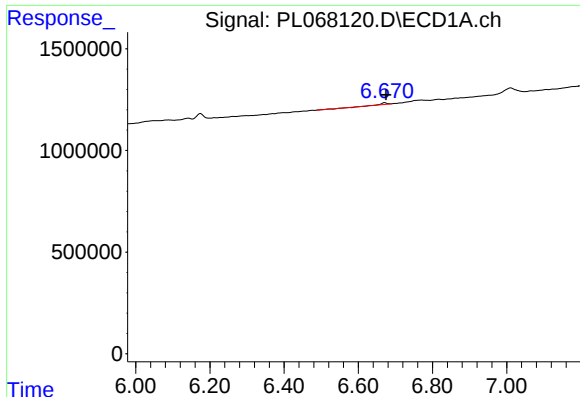


#24 Chlordane-2

R.T.: 6.671 min
Delta R.T.: -0.003 min
Response: 31513
Conc: 1.62 ng/ml

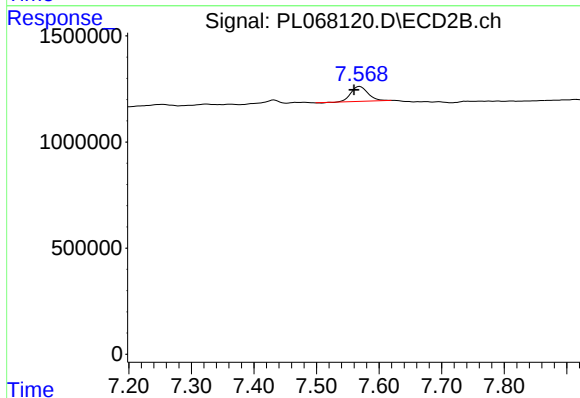


#24 Chlordane-2

R.T.: 7.569 min
Delta R.T.: 0.009 min
Response: 1362721
Conc: 29.73 ng/ml

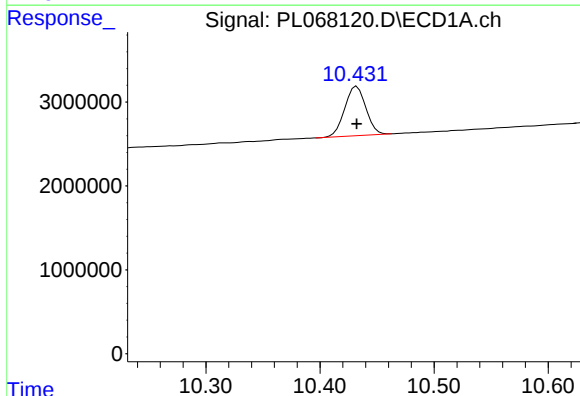

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 7559930
Conc: 18.32 ng/ml

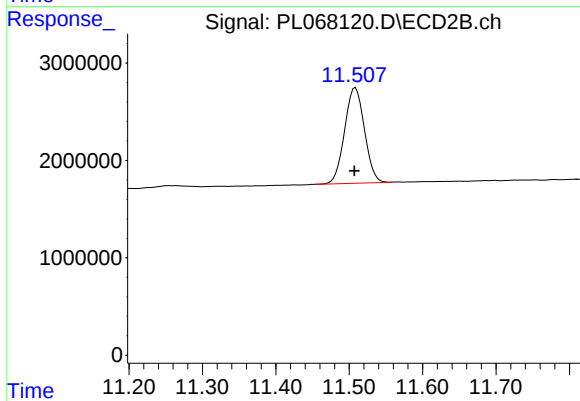

#28 Decachlorobiphenyl

R.T.: 11.509 min
Delta R.T.: 0.001 min
Response: 18445832
Conc: 20.50 ng/ml