

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2021 22:40
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 04:01:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:01:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	27694273	55758099	51.181	49.715
28)	SA Decachlor...	10.432	11.509	19218057	46904799	45.647	49.184
Target Compounds							
23)	Chlordane-1	5.986	6.969	7512325	19047526	507.661	494.835
24)	Chlordane-2	6.676	7.559	9885643	22261160	507.210	485.685
25)	Chlordane-3	7.378	8.317	23659164	80186886	465.555	496.763
26)	Chlordane-4	7.447	8.399	24383658	98036438	460.250	496.841
27)	Chlordane-5	8.397	9.287	7754812	18166841	431.280	500.402


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2021 22:40
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 04:01:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:01:15 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

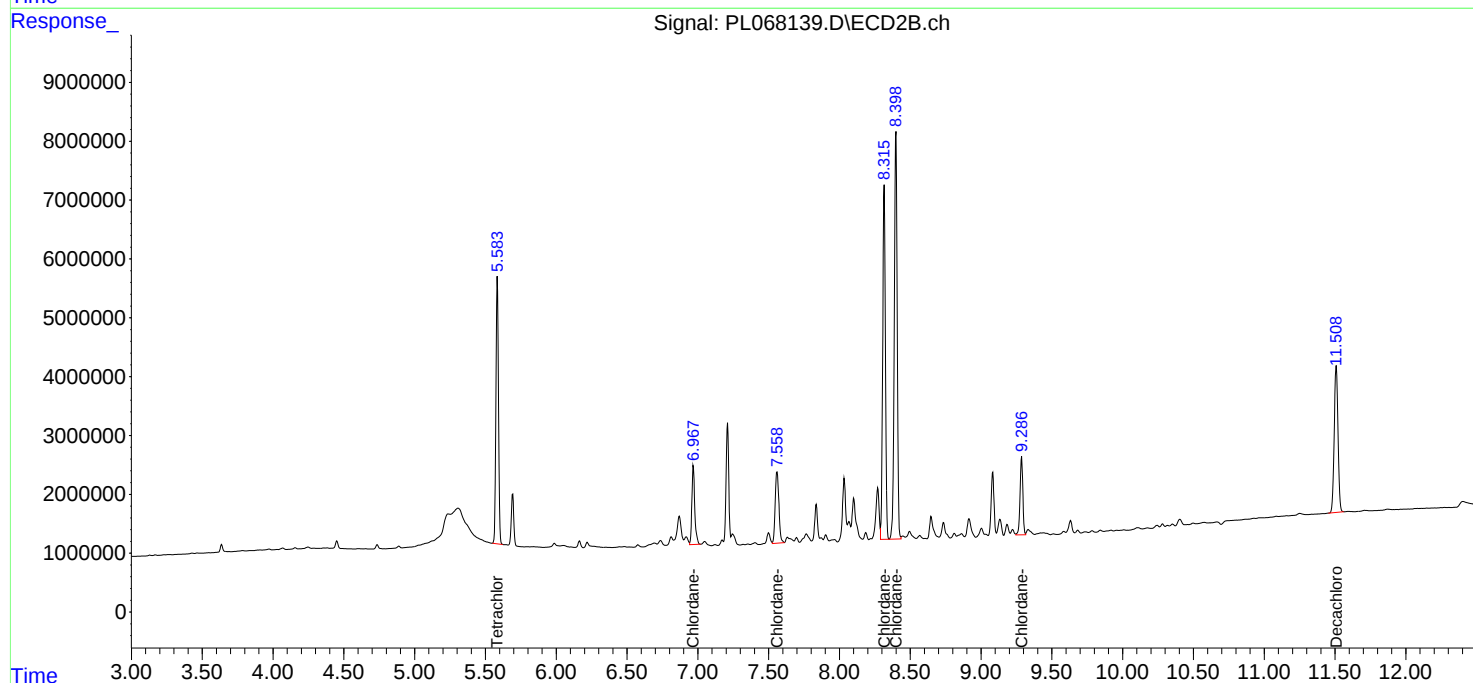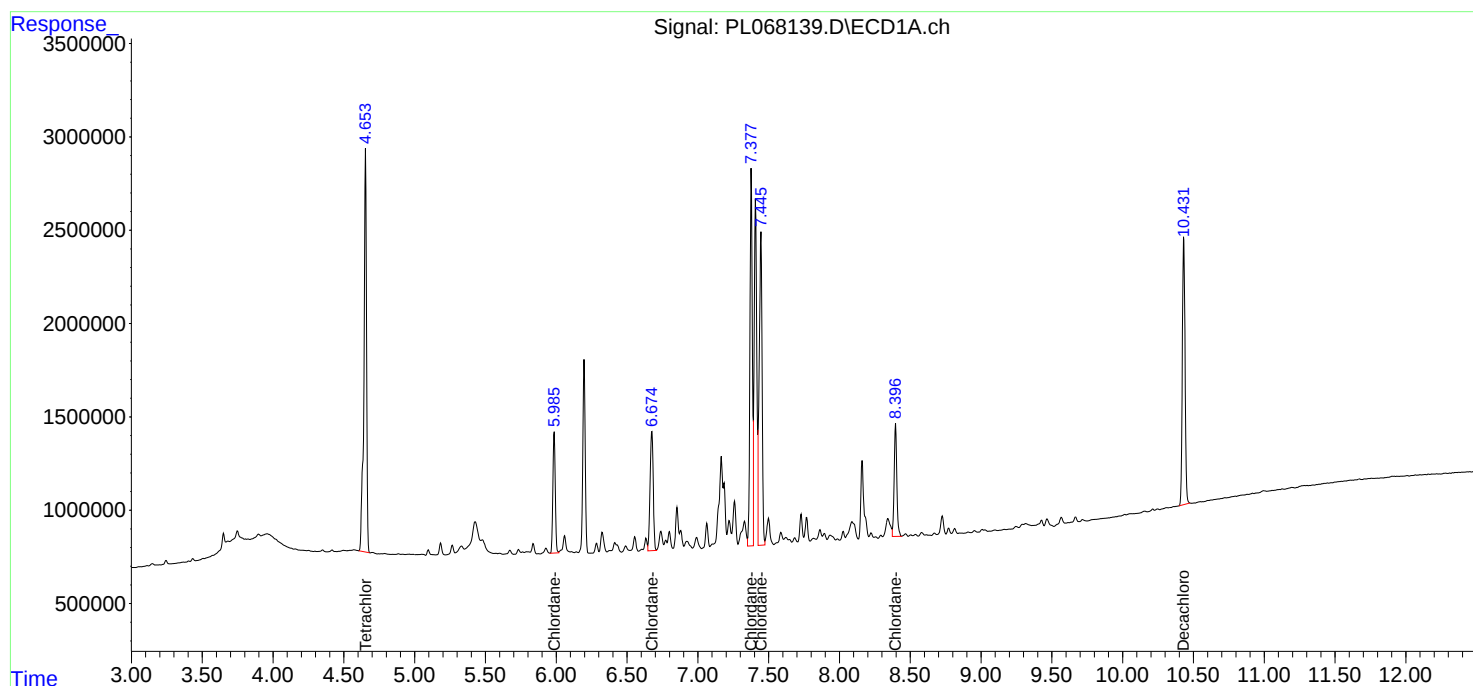

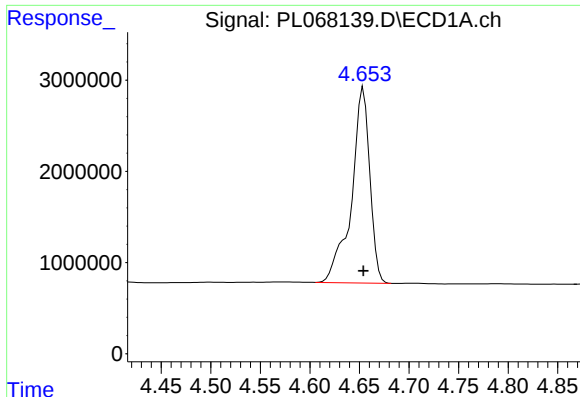


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 27694273
Conc: 51.18 ng/ml

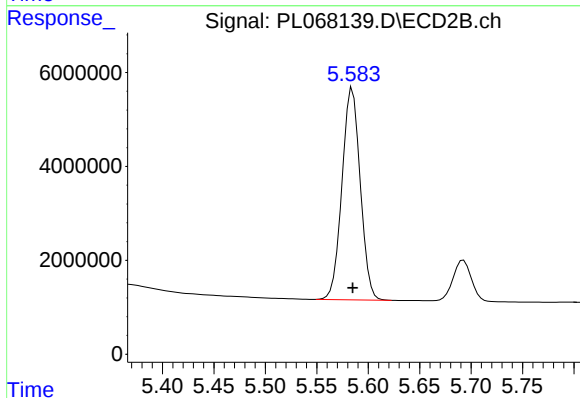


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 55758099
Conc: 49.71 ng/ml

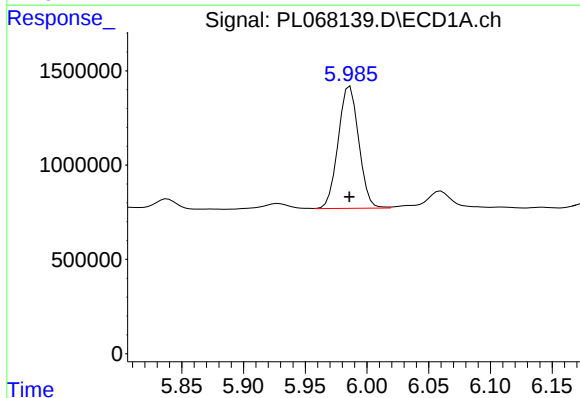


#23 Chlordane-1

R.T.: 5.986 min
Delta R.T.: 0.000 min
Response: 7512325
Conc: 507.66 ng/ml

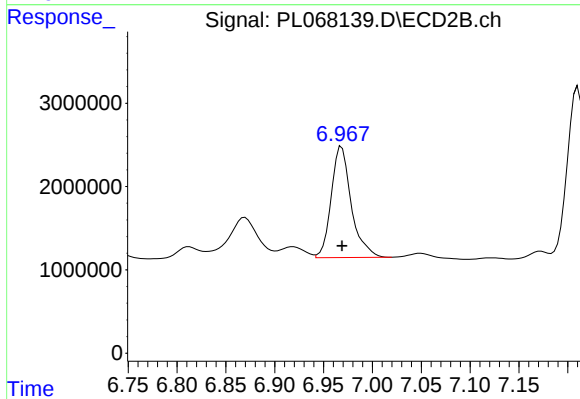


#23 Chlordane-1

R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 19047526
Conc: 494.83 ng/ml

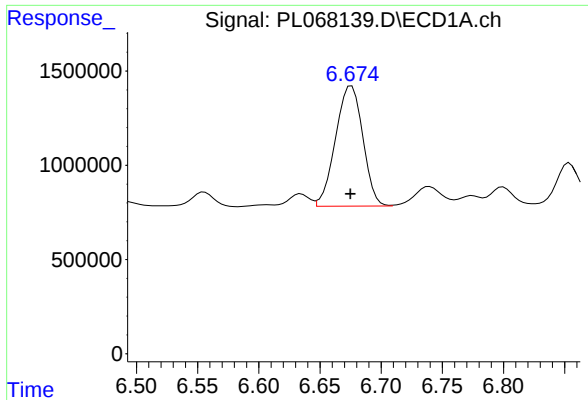


#24 Chlordane-2

R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 9885643
Conc: 507.21 ng/ml

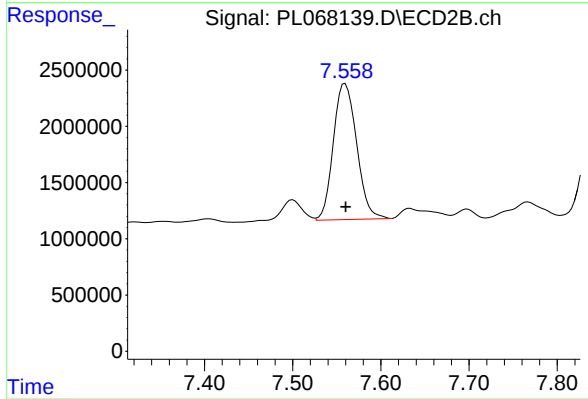


#24 Chlordane-2

R.T.: 7.559 min
Delta R.T.: 0.000 min
Response: 22261160
Conc: 485.68 ng/ml

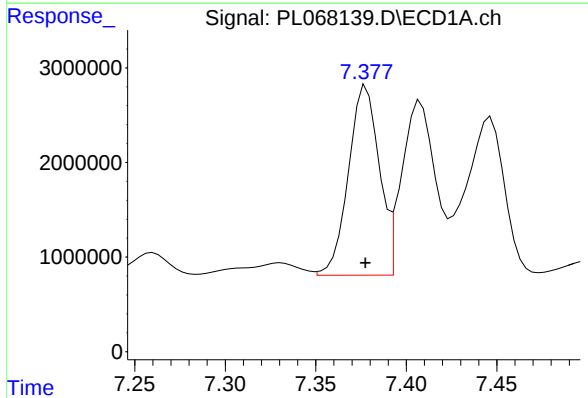


#25 Chlordane-3

R.T.: 7.378 min
Delta R.T.: 0.000 min
Response: 23659164
Conc: 465.56 ng/ml

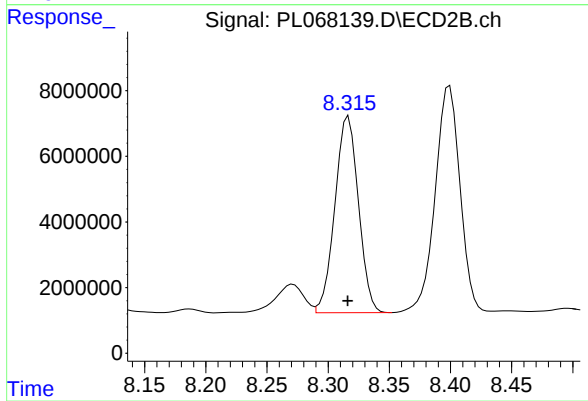


#25 Chlordane-3

R.T.: 8.317 min
Delta R.T.: 0.000 min
Response: 80186886
Conc: 496.76 ng/ml

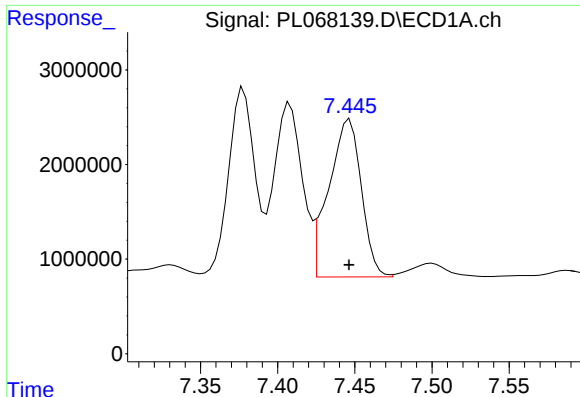


#26 Chlordane-4

R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 24383658
Conc: 460.25 ng/ml

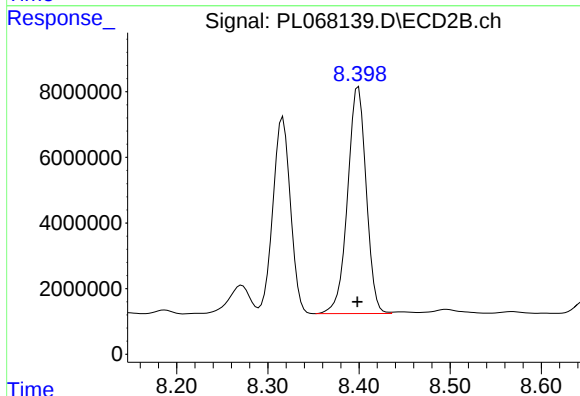


#26 Chlordane-4

R.T.: 8.399 min
Delta R.T.: 0.000 min
Response: 98036438
Conc: 496.84 ng/ml

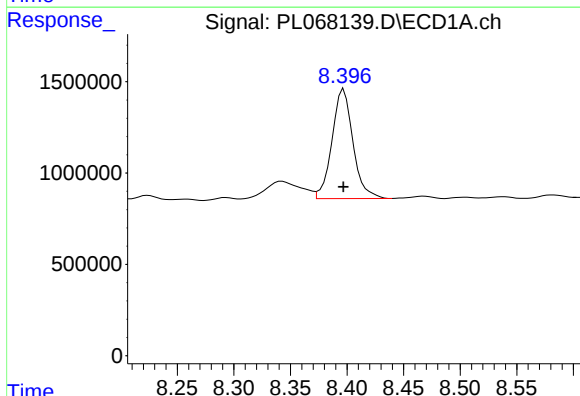


#27 Chlordane-5

R.T.: 8.397 min
Delta R.T.: 0.000 min
Response: 7754812
Conc: 431.28 ng/ml

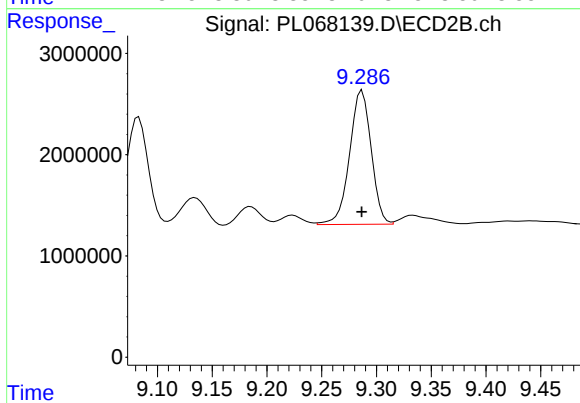

#27 Chlordane-5

R.T.: 9.287 min
Delta R.T.: 0.000 min
Response: 18166841
Conc: 500.40 ng/ml

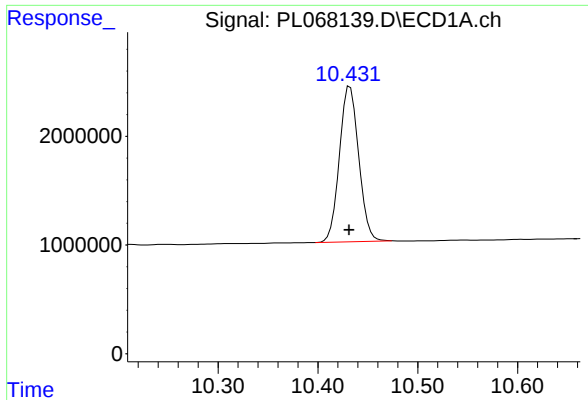


#28 Decachlorobiphenyl

R.T.: 10.432 min

Delta R.T.: 0.000 min

Response: 19218057

Conc: 45.65 ng/ml

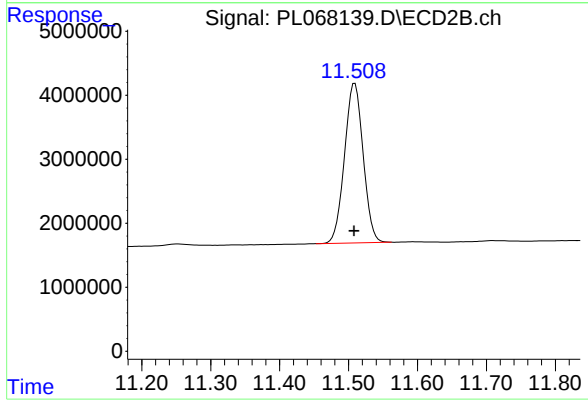

#28 Decachlorobiphenyl

R.T.: 11.509 min

Delta R.T.: 0.000 min

Response: 46904799

Conc: 49.18 ng/ml