

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 01:59
 Operator : AR\AJ
 Sample : M3012-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 04:49:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.586	8443626	19350875	20.946	18.764
28)	SA Decachlor...	10.432	11.509	9092442	18970678	22.034	21.085
Target Compounds							
2)	A alpha-BHC	0.000	6.142f	0	1263684	N.D.	0.923 #
10)	B gamma-Chl...	0.000	8.309	0	468640	N.D.	0.422 #
15)	B Endosulfa...	0.000	9.228	0	599543	N.D.	0.677 #
25)	Chlordane-3	0.000	8.309	0	468640	N.D.	2.903 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 01:59
Operator : AR\AJ
Sample : M3012-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 04:49:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

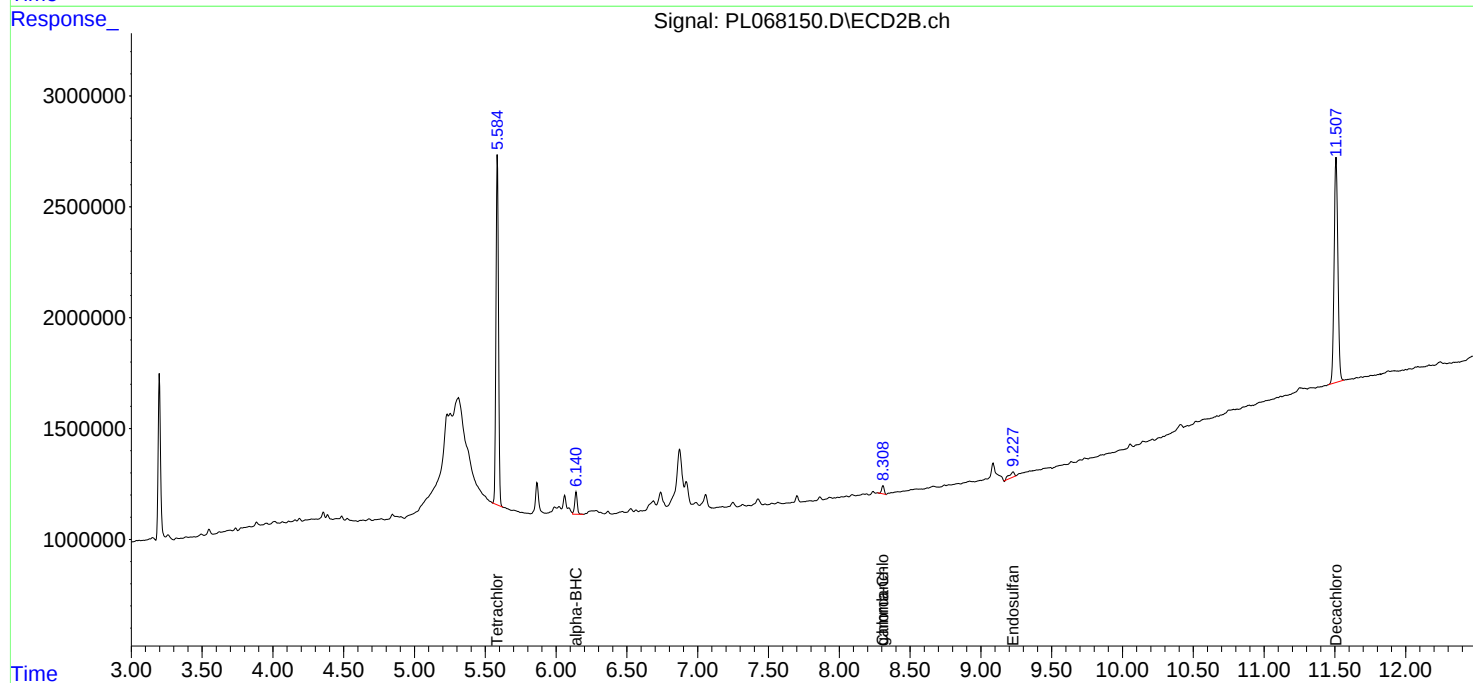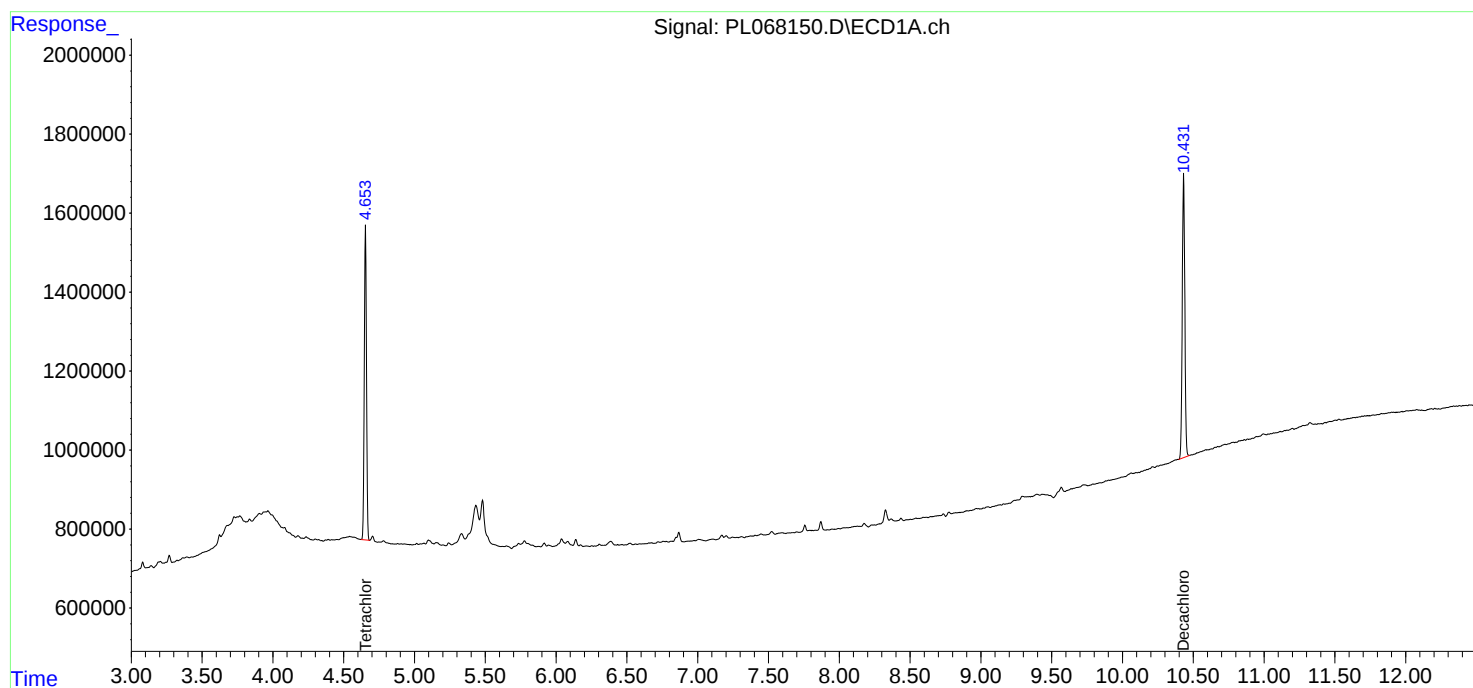

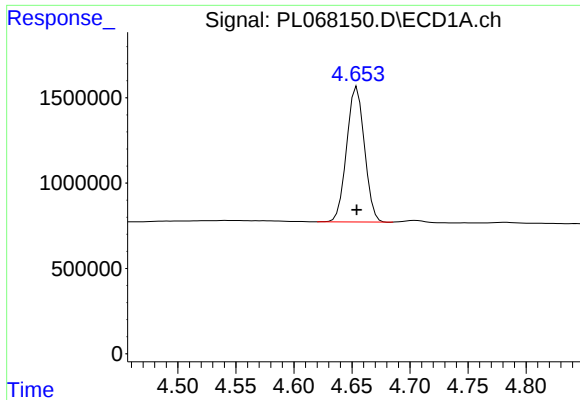


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 8443626
Conc: 20.95 ng/ml

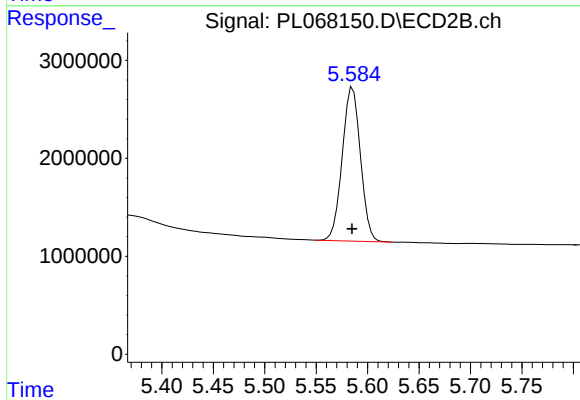


#1 Tetrachloro-m-xylene

R.T.: 5.586 min
Delta R.T.: 0.000 min
Response: 19350875
Conc: 18.76 ng/ml

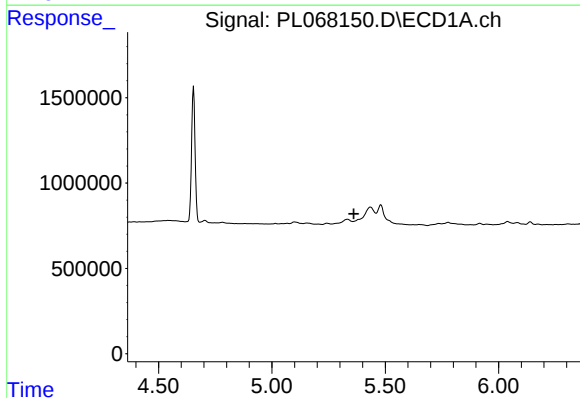


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.361 min
Response: 0
Conc: N.D.

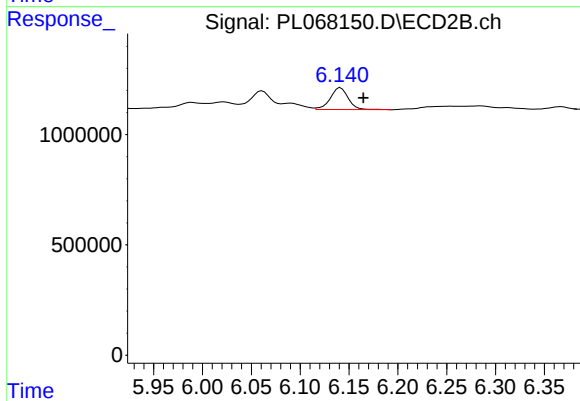


#2 alpha-BHC

R.T.: 6.142 min
Delta R.T.: -0.023 min
Response: 1263684
Conc: 0.92 ng/ml

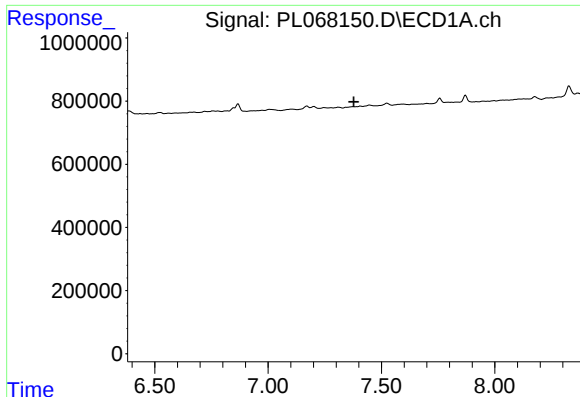


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.377 min
Response: 0
Conc: N.D.

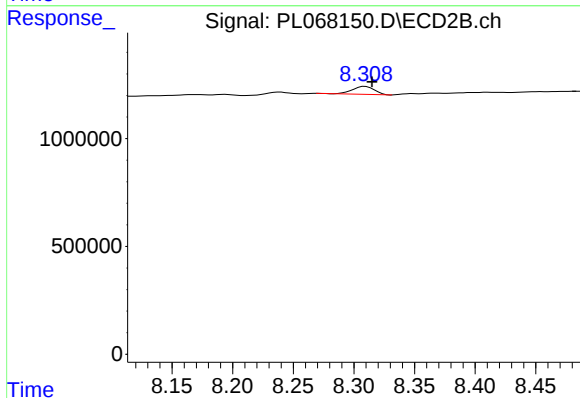


#10 gamma-Chlordane

R.T.: 8.309 min
Delta R.T.: -0.006 min
Response: 468640
Conc: 0.42 ng/ml

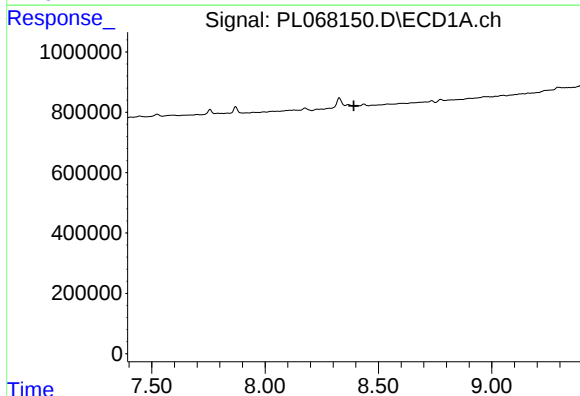


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.391 min
Response: 0
Conc: N.D.

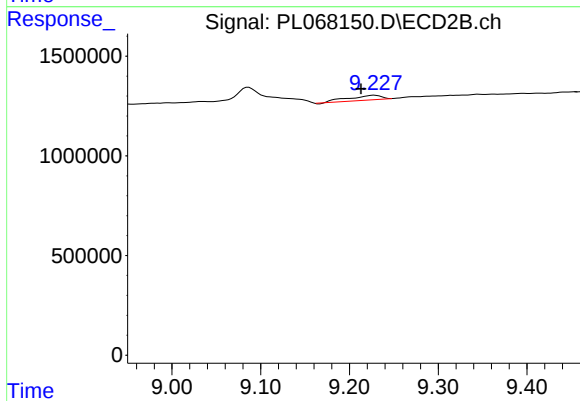


#15 Endosulfan II

R.T.: 9.228 min
Delta R.T.: 0.015 min
Response: 599543
Conc: 0.68 ng/ml

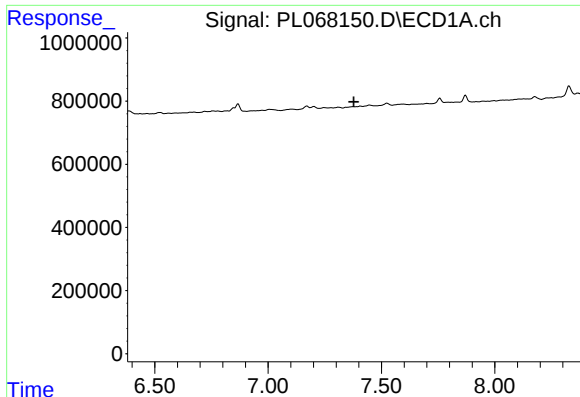


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.378 min
Response: 0
Conc: N.D.

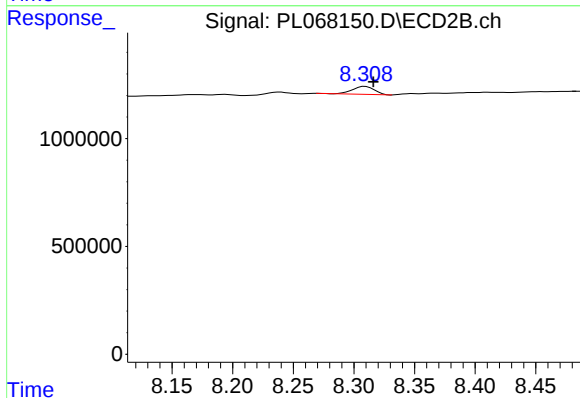


#25 Chlordane-3

R.T.: 8.309 min
Delta R.T.: -0.007 min
Response: 468640
Conc: 2.90 ng/ml

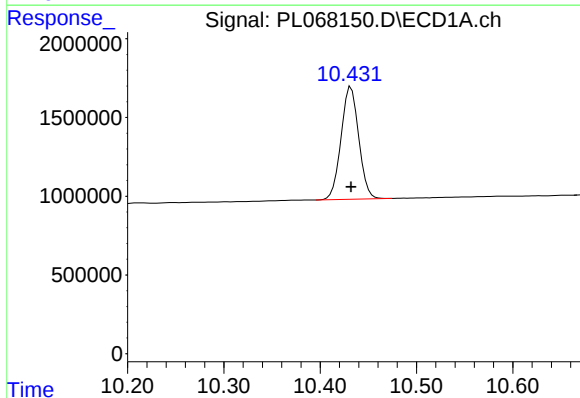

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 9092442
Conc: 22.03 ng/ml

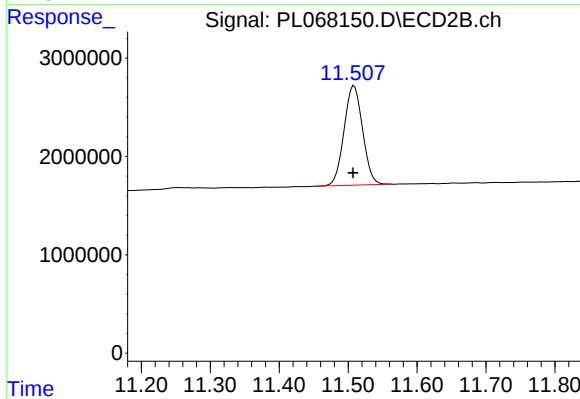

#28 Decachlorobiphenyl

R.T.: 11.509 min
Delta R.T.: 0.002 min
Response: 18970678
Conc: 21.09 ng/ml