

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
 Data File : PL068151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2021 02:16
 Operator : AR\AJ
 Sample : M3013-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 04:50:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 15 04:04:16 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	5.585	8759355	20242992	21.729	19.629
28)	SA Decachlor...	10.432	11.508	9229551	19226468	22.366	21.370
Target Compounds							
2)	A alpha-BHC	0.000	6.140f	0	1001545	N.D.	0.731 #
4)	MA Heptachlor	0.000	7.218	0	72444	N.D.	0.056 #
6)	B beta-BHC	6.141f	0.000	717890	0	2.761	N.D. #
7)	B delta-BHC	0.000	7.058f	0	766037	N.D.	0.629 #
10)	B gamma-Chl...	0.000	8.308	0	472114	N.D.	0.425 #
15)	B Endosulfa...	0.000	9.229f	0	427707	N.D.	0.483 #
25)	Chlordane-3	0.000	8.308	0	472114	N.D.	2.925 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL071521\
Data File : PL068151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2021 02:16
Operator : AR\AJ
Sample : M3013-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 04:50:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071521.M
Quant Title : GC Extractables
QLast Update : Thu Jul 15 04:04:16 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

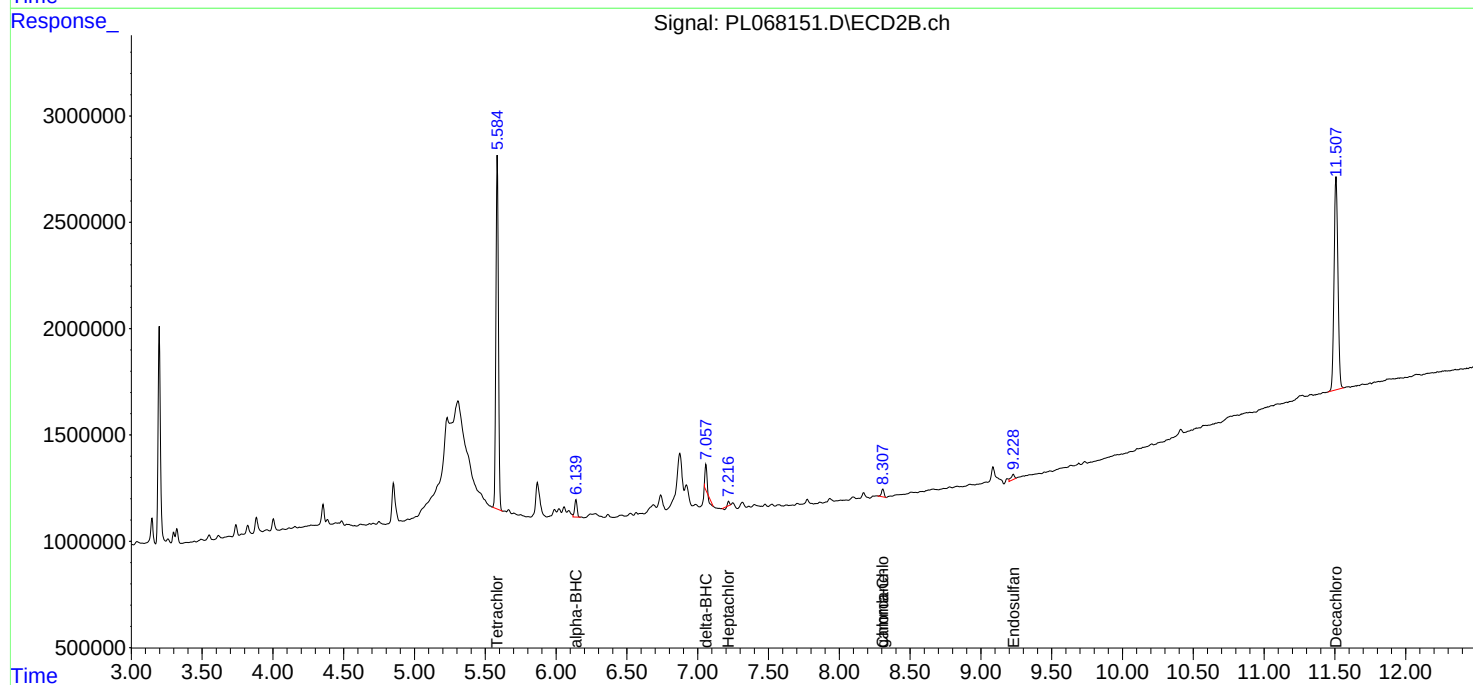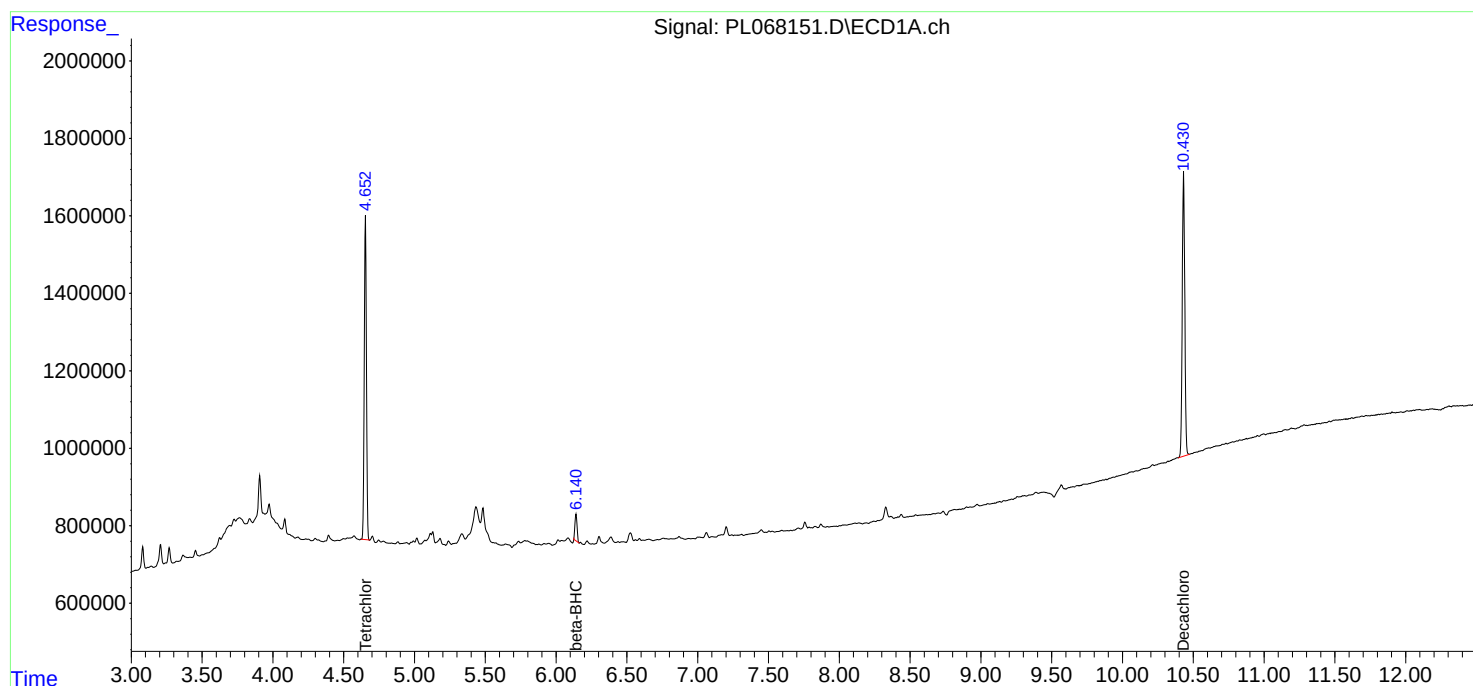

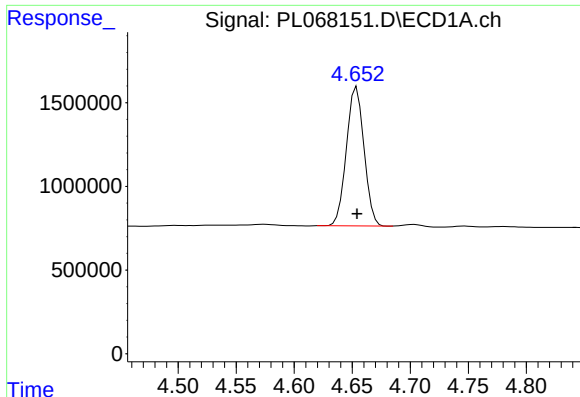


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.000 min
Response: 8759355
Conc: 21.73 ng/ml

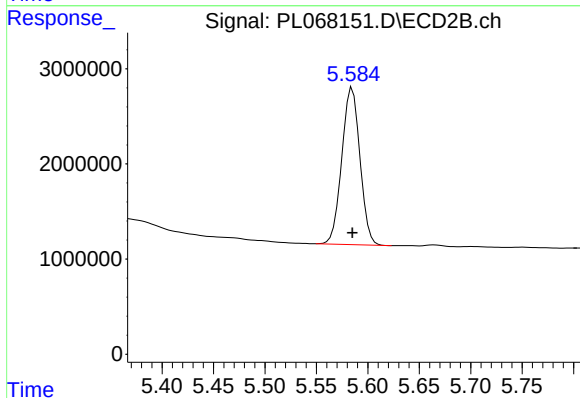


#1 Tetrachloro-m-xylene

R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 20242992
Conc: 19.63 ng/ml

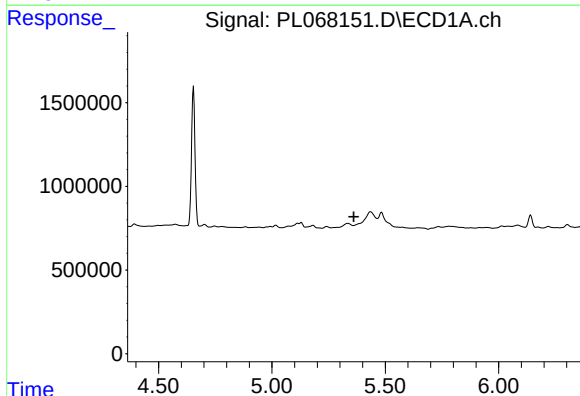


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.361 min
Response: 0
Conc: N.D.

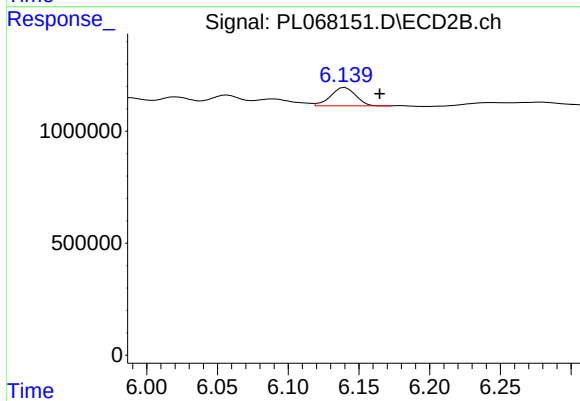


#2 alpha-BHC

R.T.: 6.140 min
Delta R.T.: -0.024 min
Response: 1001545
Conc: 0.73 ng/ml

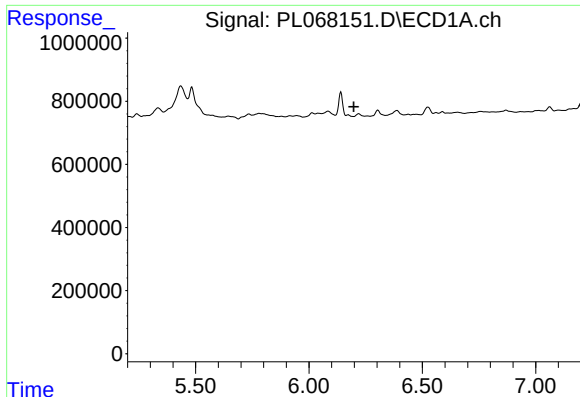


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

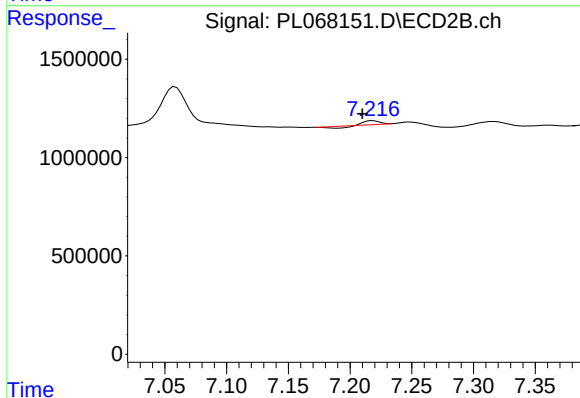


#4 Heptachlor

R.T.: 7.218 min
Delta R.T.: 0.008 min
Response: 72444
Conc: 0.06 ng/ml

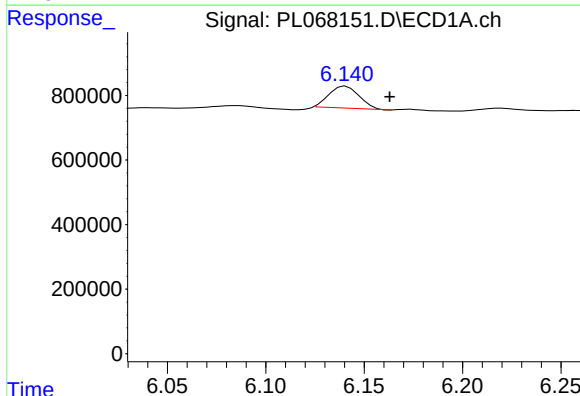


#6 beta-BHC

R.T.: 6.141 min
Delta R.T.: -0.022 min
Response: 717890
Conc: 2.76 ng/ml

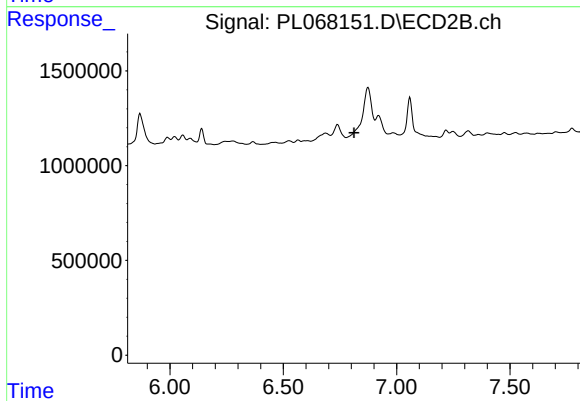


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.812 min
Response: 0
Conc: N.D.

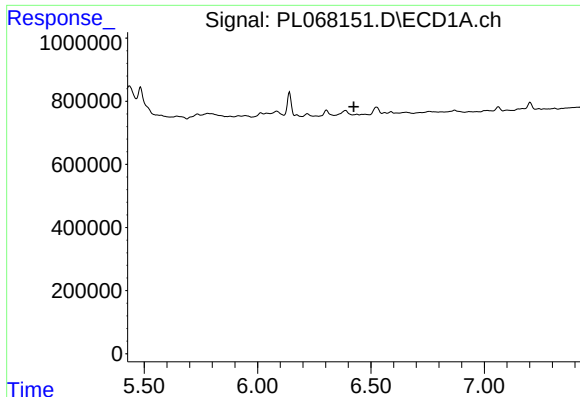


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

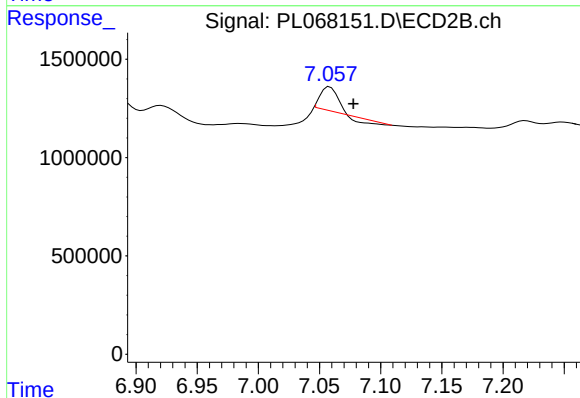


#7 delta-BHC

R.T.: 7.058 min
Delta R.T.: -0.019 min
Response: 766037
Conc: 0.63 ng/ml

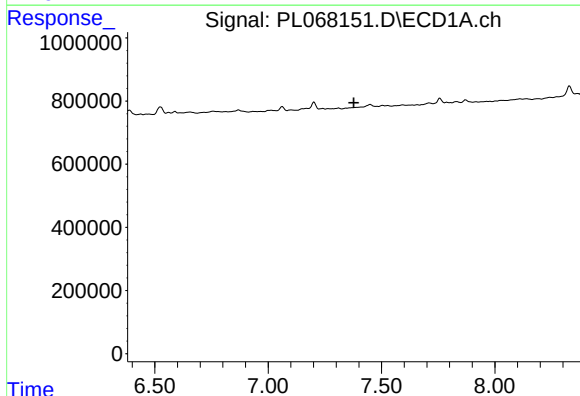


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

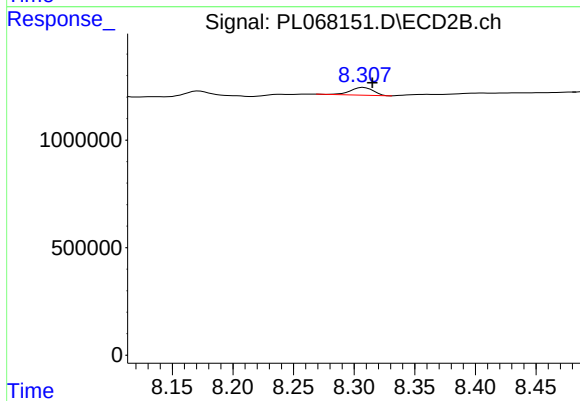


#10 gamma-Chlordane

R.T.: 8.308 min
Delta R.T.: -0.007 min
Response: 472114
Conc: 0.42 ng/ml

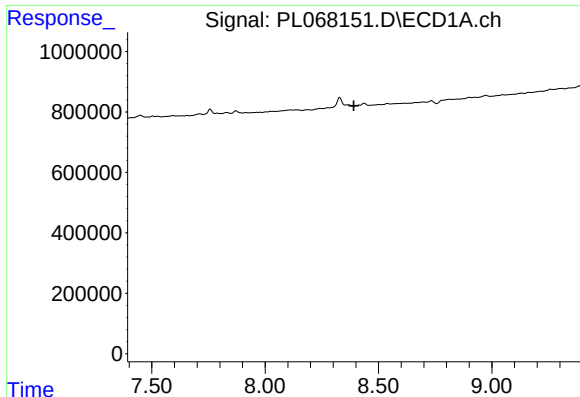


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.391 min
Response: 0
Conc: N.D.

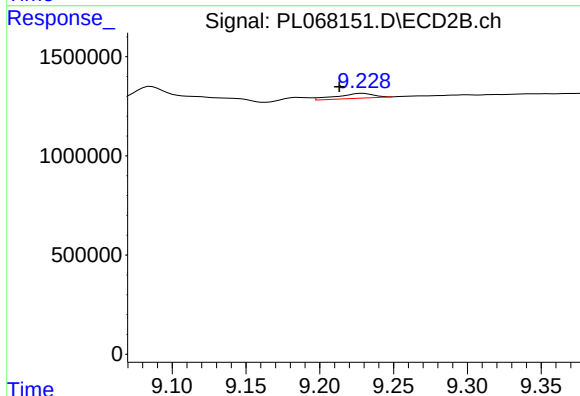


#15 Endosulfan II

R.T.: 9.229 min
Delta R.T.: 0.016 min
Response: 427707
Conc: 0.48 ng/ml

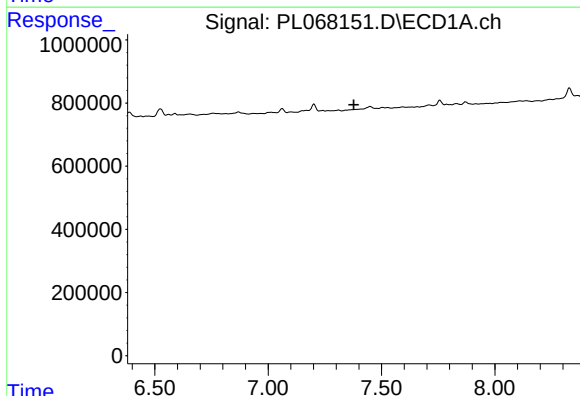


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.378 min
Response: 0
Conc: N.D.

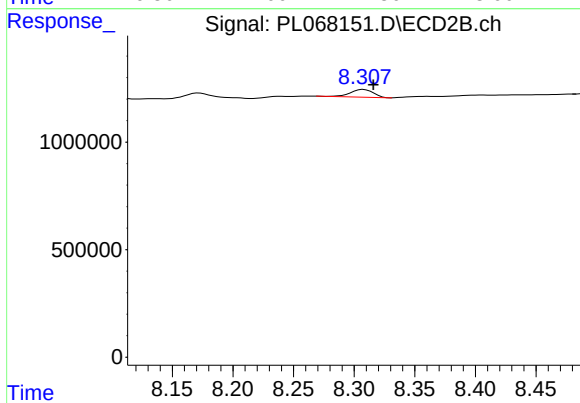


#25 Chlordane-3

R.T.: 8.308 min
Delta R.T.: -0.008 min
Response: 472114
Conc: 2.92 ng/ml

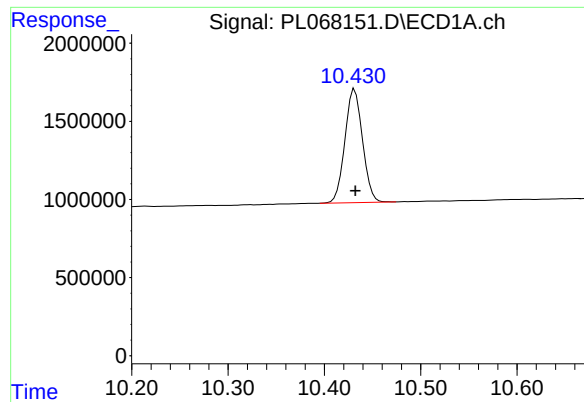

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 9229551
Conc: 22.37 ng/ml

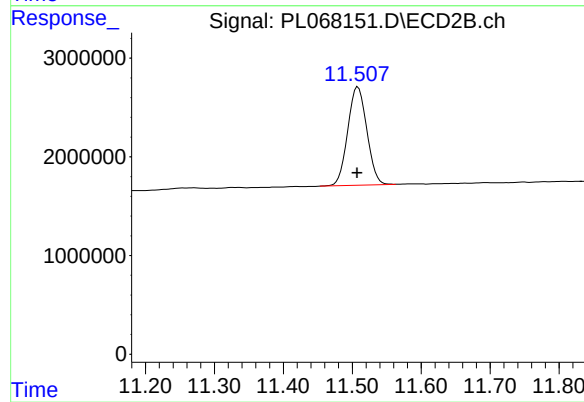

#28 Decachlorobiphenyl

R.T.: 11.508 min
Delta R.T.: 0.001 min
Response: 19226468
Conc: 21.37 ng/ml